

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
 Data File : PR068165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 17:15
 Operator : AJ\MA
 Sample : PB162655BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PB162655BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:07:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 08 22:24:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.676	3.009	50045146	113.8E6	20.148	22.862
2) SA Decachlor...	9.581	8.326	107.9E6	119.3E6	24.029	22.739m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
Data File : PR068165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 17:15
Operator : AJ\MA
Sample : PB162655BL
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PB162655BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:07:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 08 22:24:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

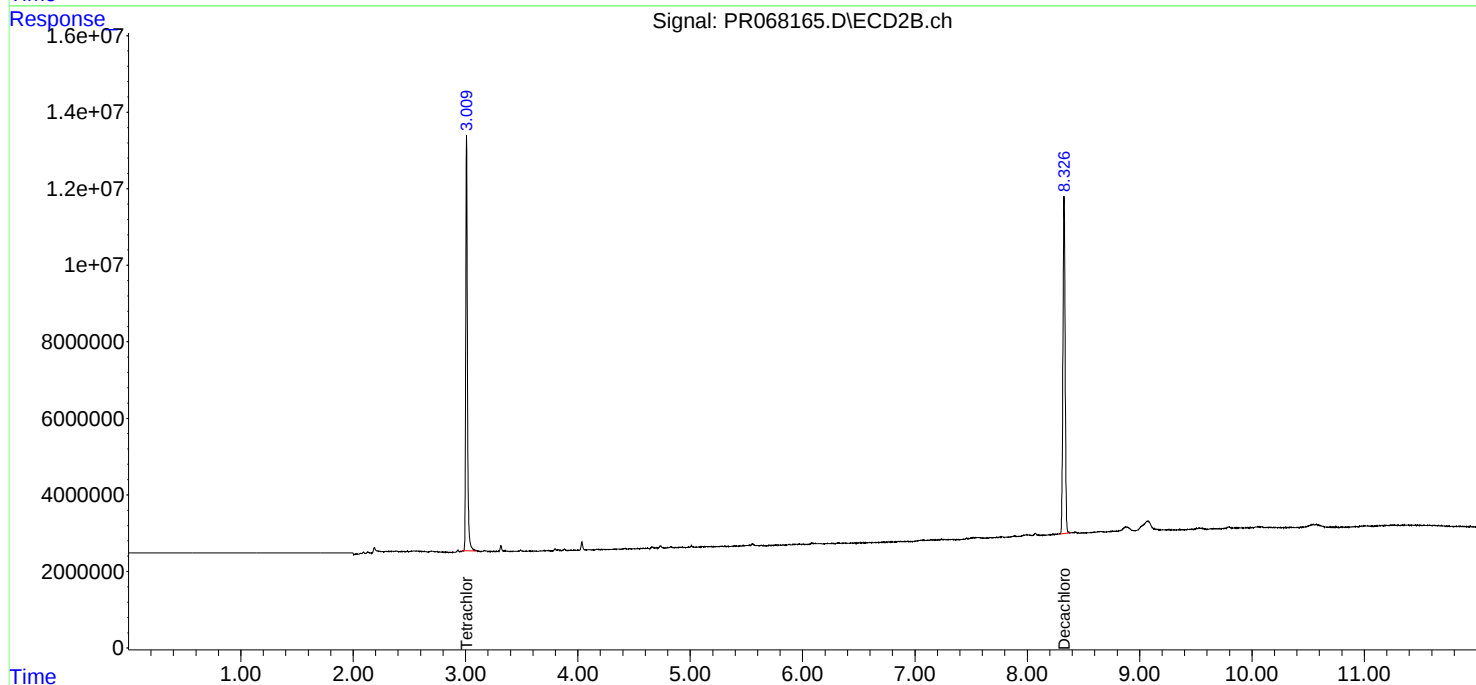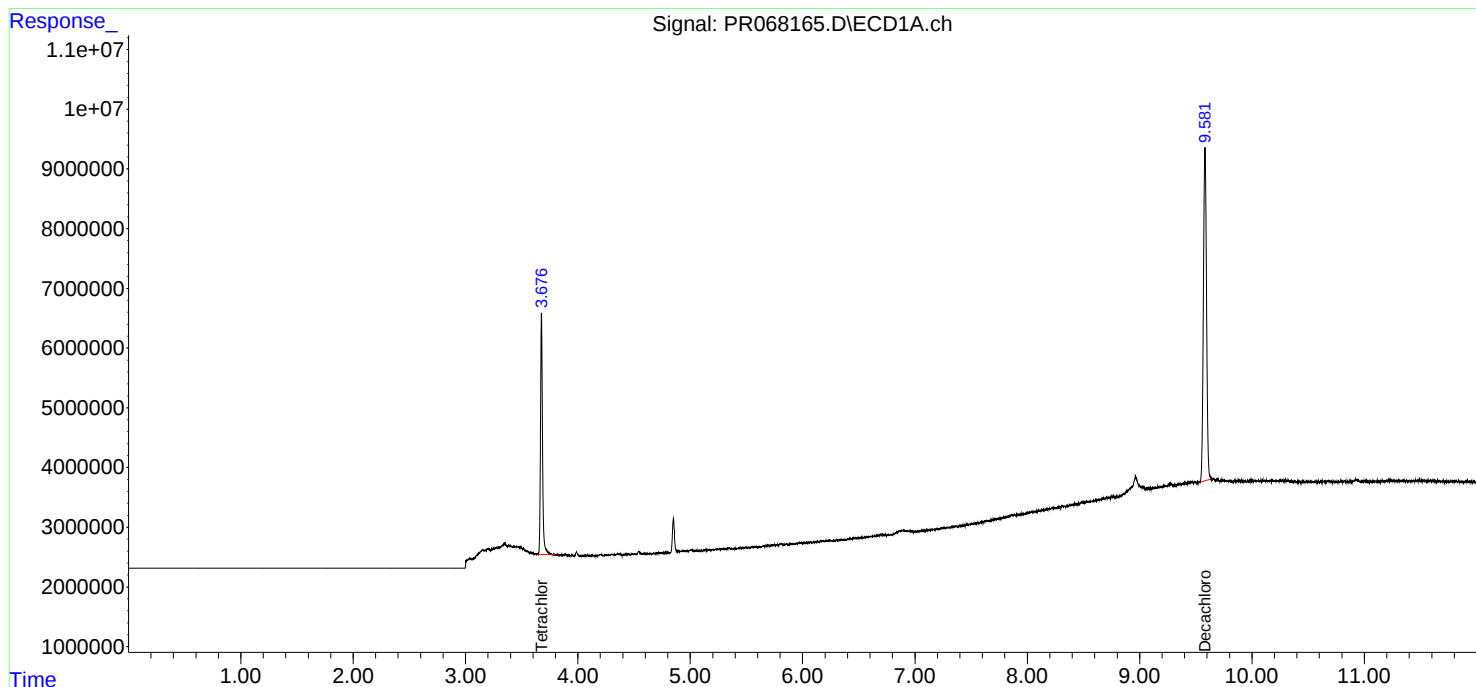

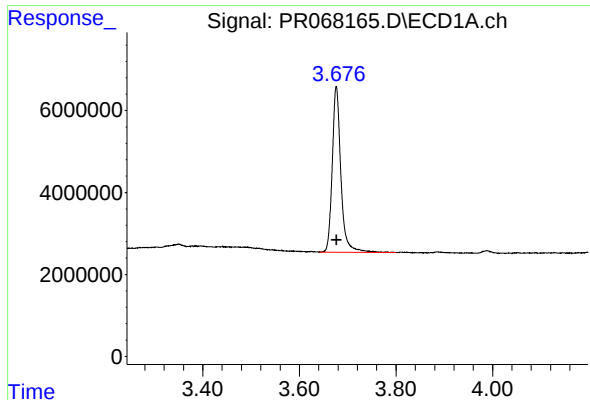

#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 50045146
Conc: 20.15 ng/ml

Instrument :

ECD_R


ClientSampleId :

PB162655BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

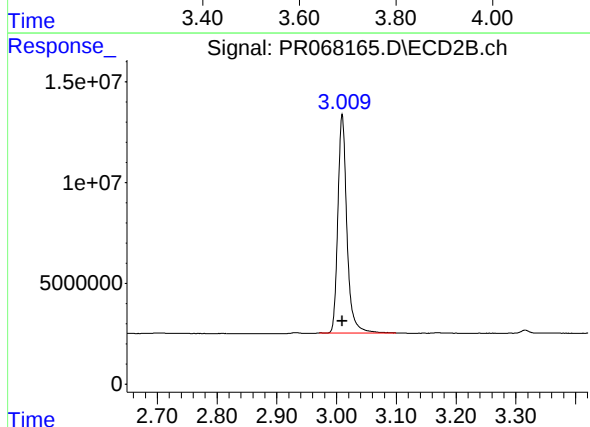


#1 Tetrachloro-m-xylene

R.T.: 3.009 min
Delta R.T.: 0.000 min
Response: 113758841
Conc: 22.86 ng/ml

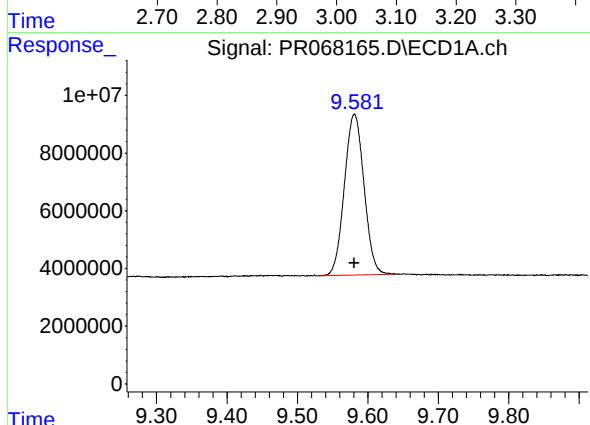

#2 Decachlorobiphenyl

R.T.: 9.581 min
Delta R.T.: 0.000 min
Response: 107890679
Conc: 24.03 ng/ml

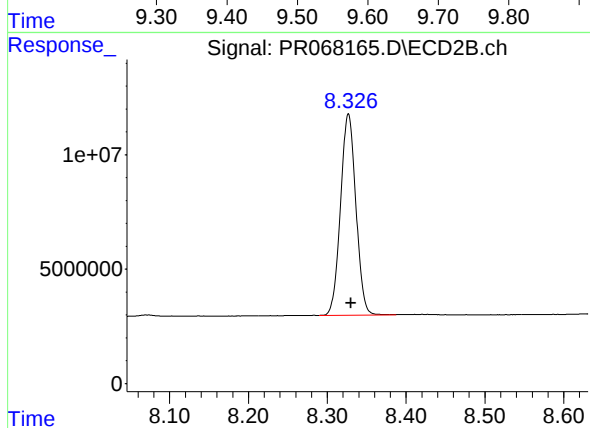

#2 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.004 min
Response: 119259725
Conc: 22.74 ng/ml m