

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
 Data File : PR068185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 23:37
 Operator : AJ\MA
 Sample : P3520-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 OU4-57S-01-080624

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:25:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 08 22:24:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.676	3.009	48299229	112.6E6	19.445	22.632
2) SA Decachlor...	9.581	8.325	106.1E6	115.6E6	23.633	22.035m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081224\
Data File : PR068185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 23:37
Operator : AJ\MA
Sample : P3520-17
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
OU4-57S-01-080624


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:25:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080824.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 08 22:24:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

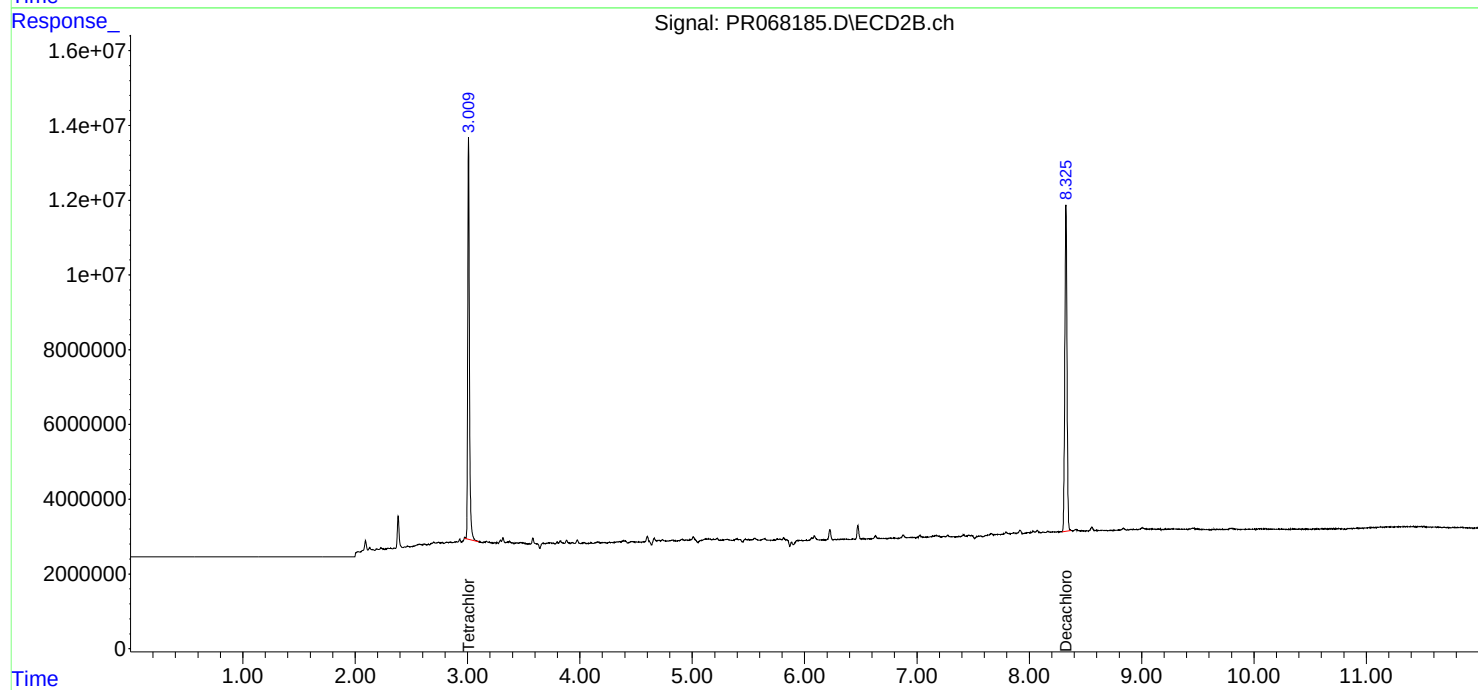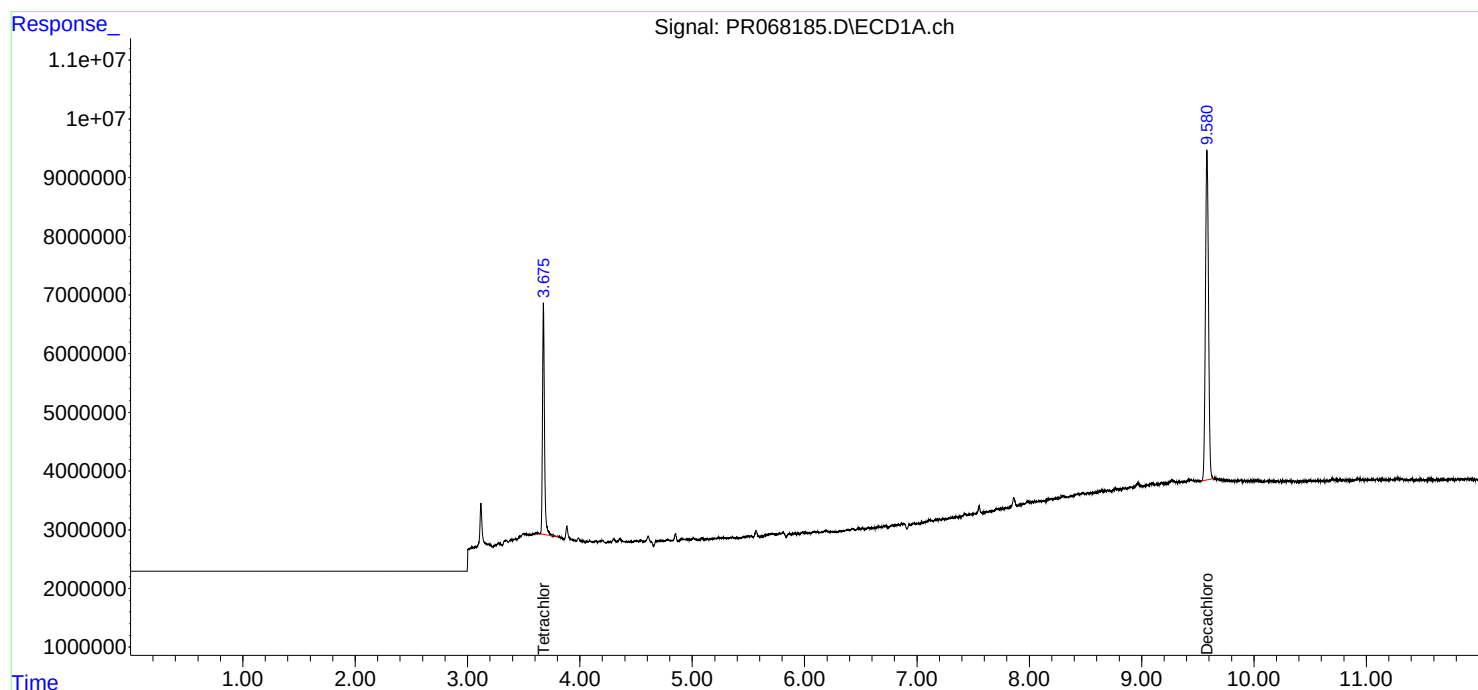

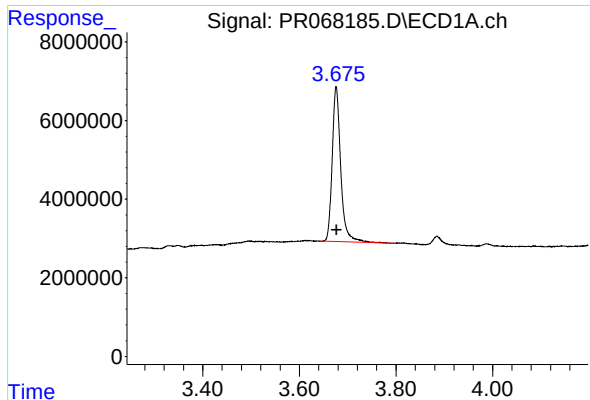


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 48299229
Conc: 19.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
OU4-57S-01-080624


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

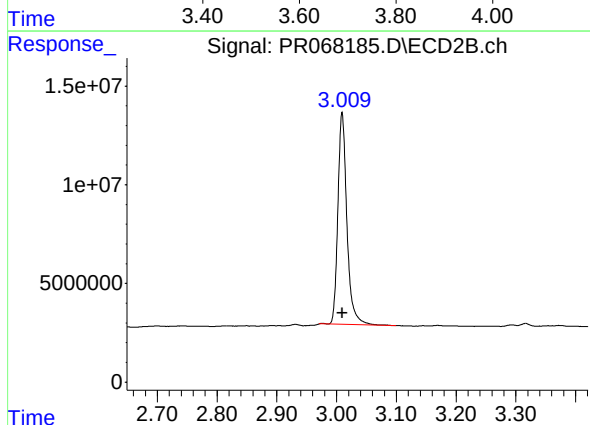


#1 Tetrachloro-m-xylene

R.T.: 3.009 min
Delta R.T.: 0.000 min
Response: 112617191
Conc: 22.63 ng/ml

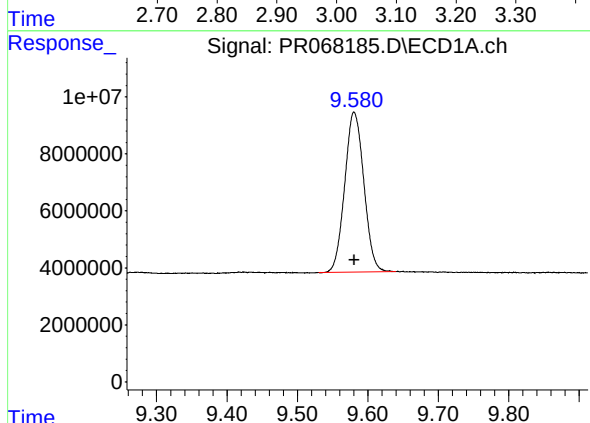

#2 Decachlorobiphenyl

R.T.: 9.581 min
Delta R.T.: 0.000 min
Response: 106115517
Conc: 23.63 ng/ml

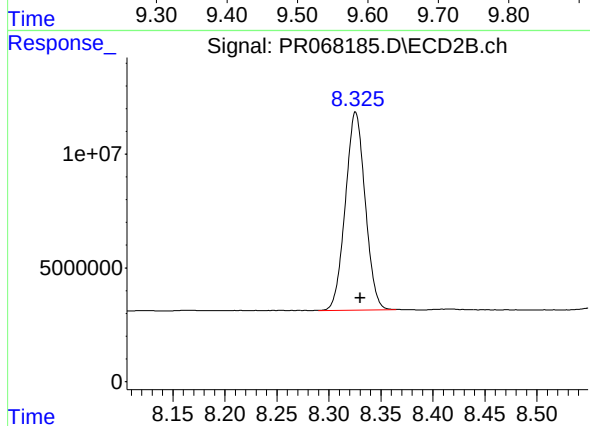

#2 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.005 min
Response: 115568218
Conc: 22.03 ng/ml m