

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081519\
 Data File : PR040378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 20:03
 Operator : SM\AJ
 Sample : K3591-01
 Misc : AR1221 LOD WATER 25PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 05:14:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 15:16:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.756	4.600	14963011	72791833	12.177	11.802
2) SA Decachlor...	8.679	10.317	60463823	239.0E6	20.989	20.595
Target Compounds						
10) L2 AR-1221-3	4.125	0.000	732047	0	17.310	N.D. #
11) L3 AR-1232-1	4.125	0.000	732047	0	16.017	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081519\
Data File : PR040378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 20:03
Operator : SM\AJ
Sample : K3591-01
Misc : AR1221 LOD WATER 25PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 05:14:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081519.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 15:16:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

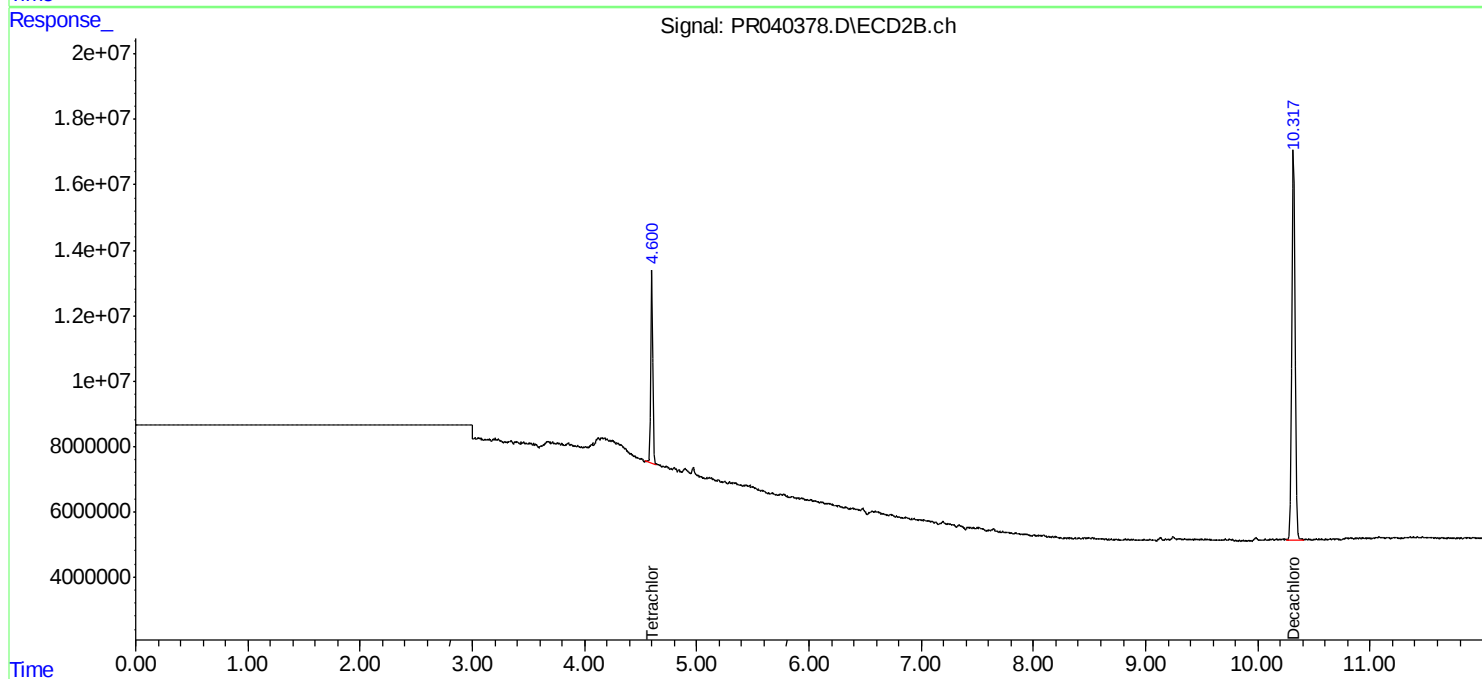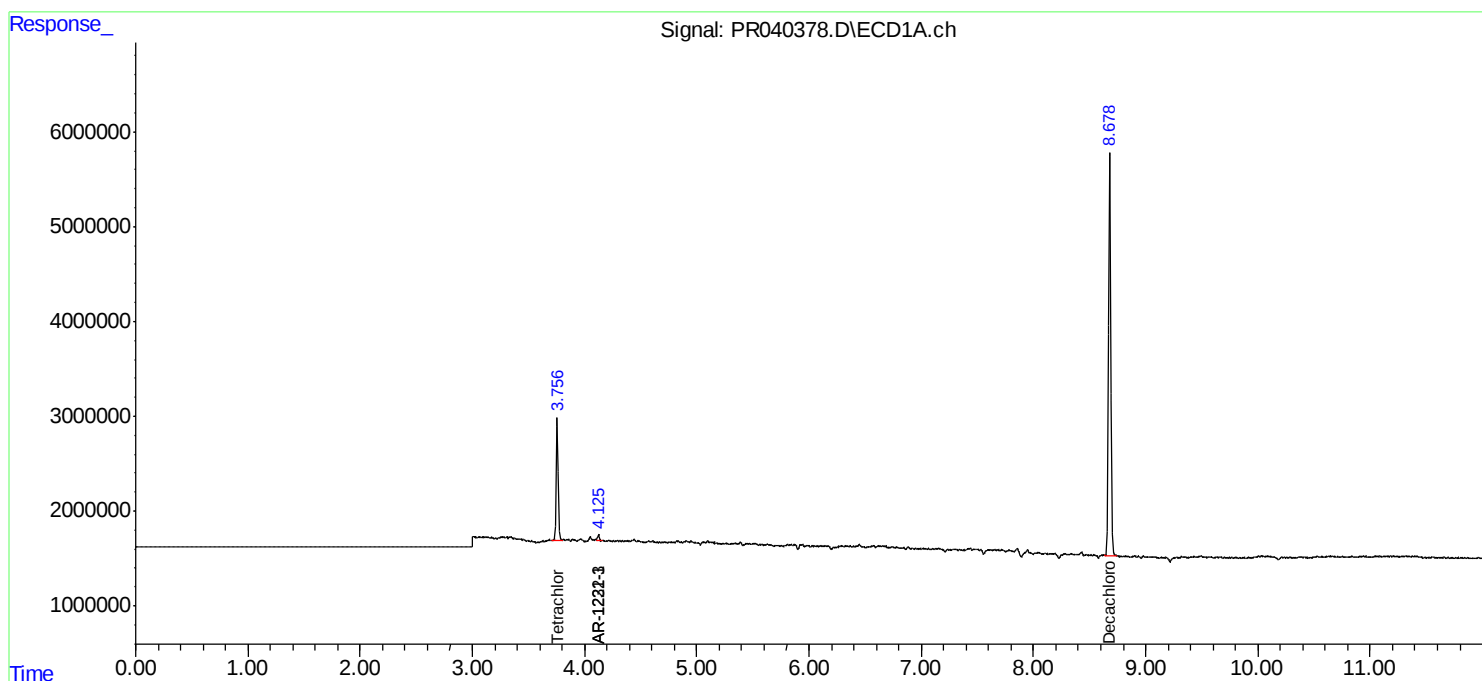


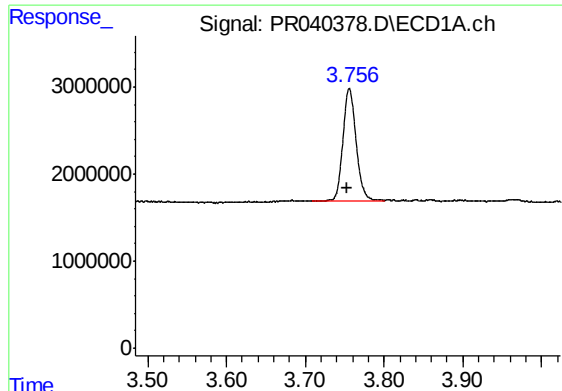

#1 Tetrachloro-m-xylene


R.T.: 3.756 min
Delta R.T.: 0.002 min
Response: 14963011
Conc: 12.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2019

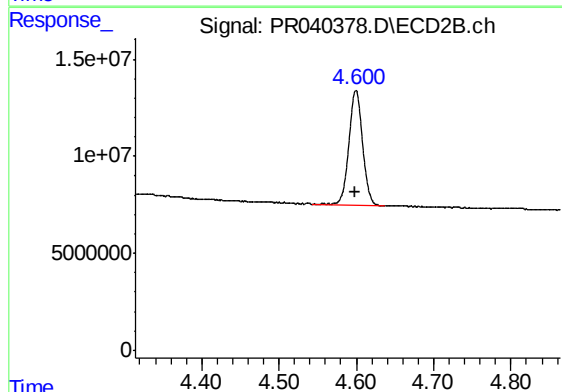


#1 Tetrachloro-m-xylene

R.T.: 4.600 min
Delta R.T.: 0.001 min
Response: 72791833
Conc: 11.80 ng/ml

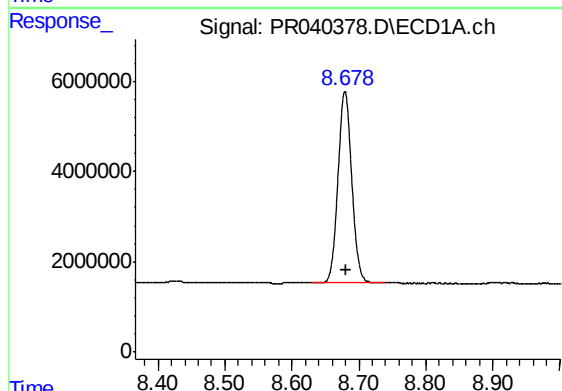


#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: 0.000 min
Response: 60463823
Conc: 20.99 ng/ml

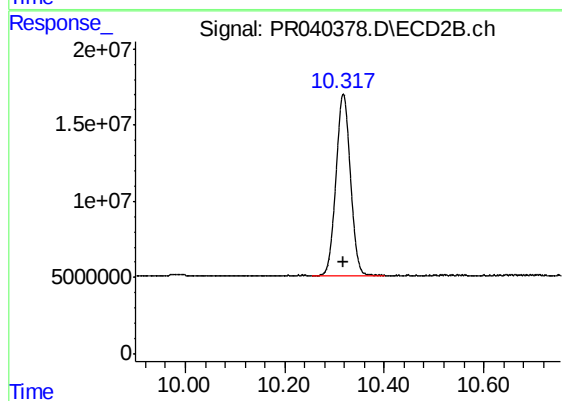

#2 Decachlorobiphenyl


R.T.: 10.317 min
Delta R.T.: -0.002 min
Response: 239030818
Conc: 20.59 ng/ml

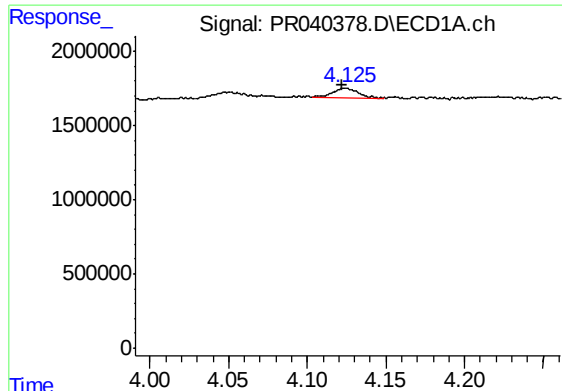

#10 AR-1221-3


R.T.: 4.125 min
Delta R.T.: 0.003 min
Response: 732047
Conc: 17.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT3-2019

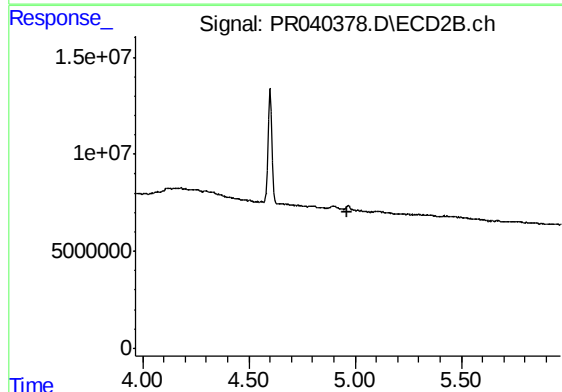


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

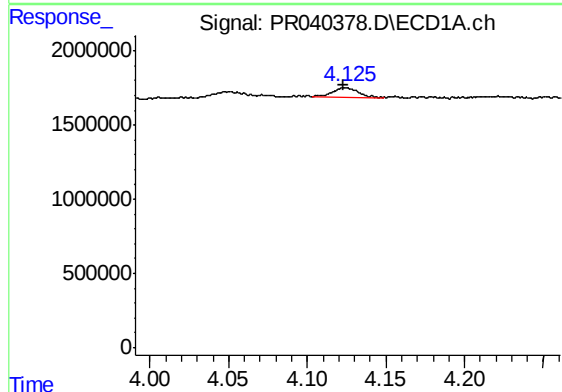

#11 AR-1232-1

R.T.: 4.125 min
Delta R.T.: 0.002 min
Response: 732047
Conc: 16.02 ng/ml

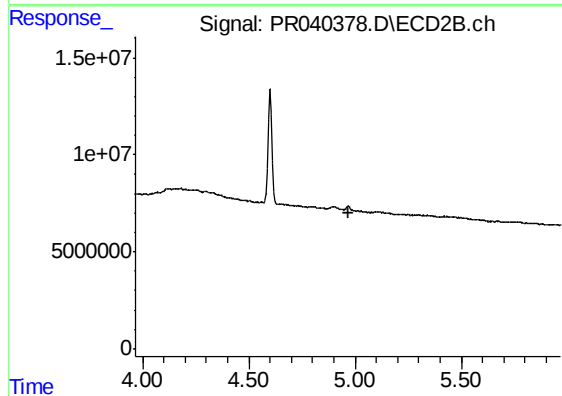

#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.