

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081619\
 Data File : PR040416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 12:38
 Operator : SM\AJ
 Sample : K3591-09
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 23:50:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 15:16:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	4.612	0	79230	N.D.	0.013 #
Target Compounds							
3)	L1 AR-1016-1	0.000	5.783	0	187488	N.D.	0.751 #
4)	L1 AR-1016-2	0.000	5.783	0	187488	N.D.	0.481 #
5)	L1 AR-1016-3	0.000	5.783	0	187488	N.D.	0.765 #
9)	L2 AR-1221-2	0.000	4.943	0	147006	N.D.	2.342 #
10)	L2 AR-1221-3	0.000	4.943	0	147006	N.D.	0.734 #
11)	L3 AR-1232-1	0.000	4.943	0	147006	N.D.	0.707 #
13)	L3 AR-1232-3	0.000	5.783	0	187488	N.D.	0.735 #
16)	L4 AR-1242-1	0.000	5.783	0	187488	N.D.	0.776 #
17)	L4 AR-1242-2	0.000	5.783	0	187488	N.D.	0.506 #
18)	L4 AR-1242-3	0.000	5.783	0	187488	N.D.	0.825 #
21)	L5 AR-1248-1	0.000	5.783	0	187488	N.D.	1.120 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR081619\
Data File : PR040416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 12:38
Operator : SM\AJ
Sample : K3591-09
Misc : AR1660 MDL 25 PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 23:50:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR081519.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 15:16:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

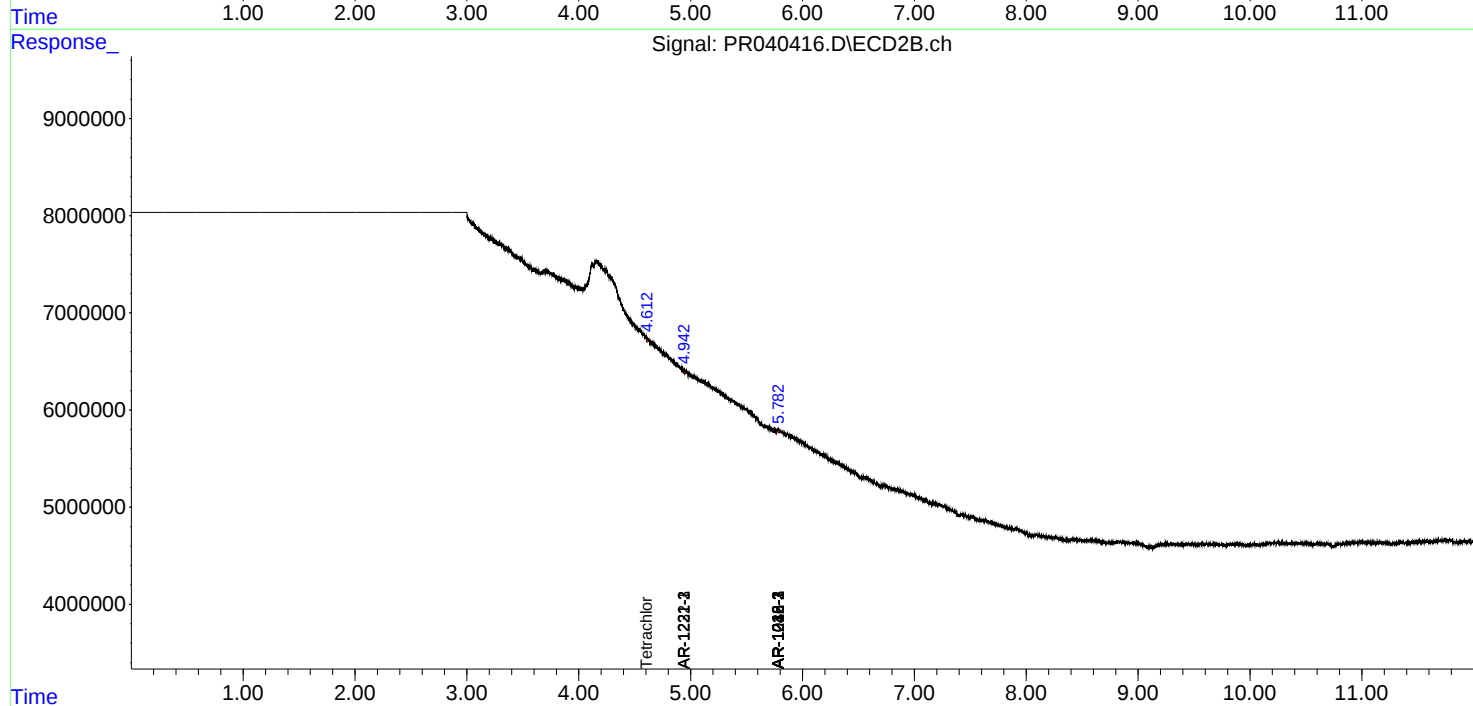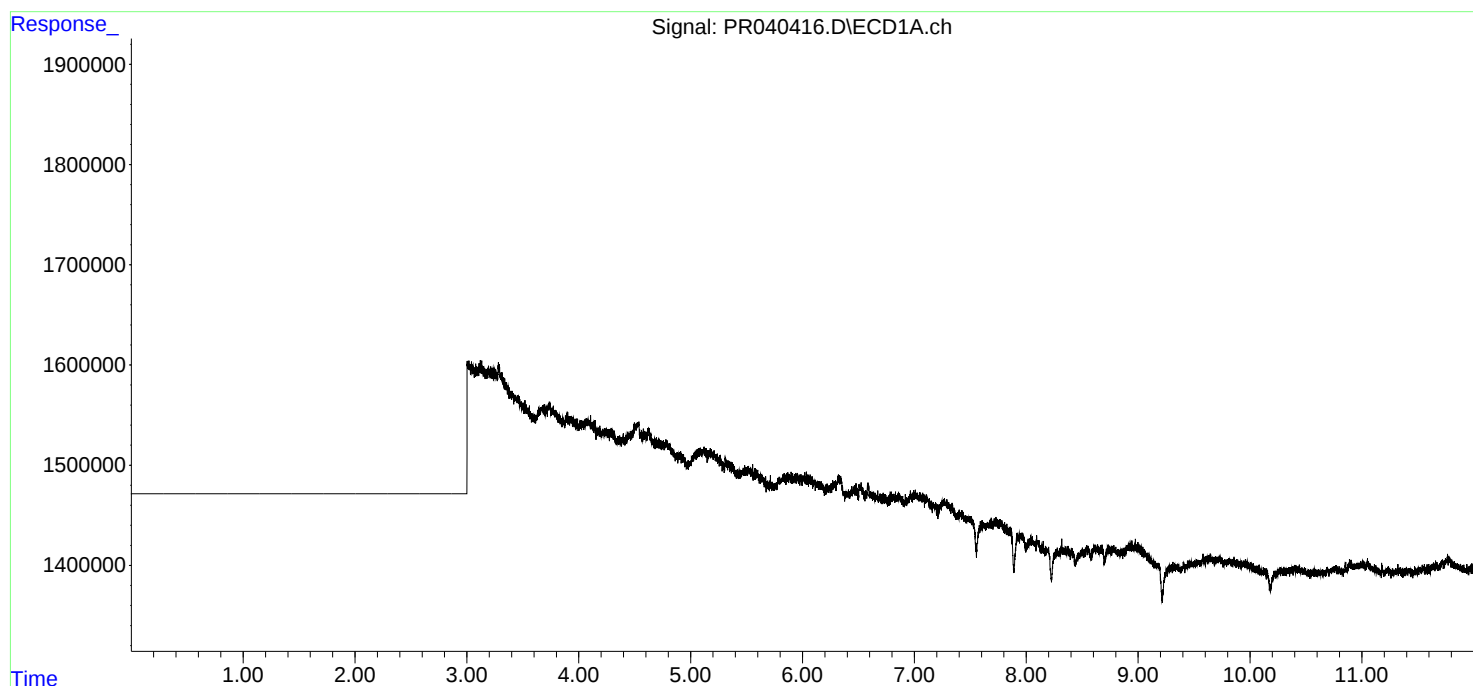


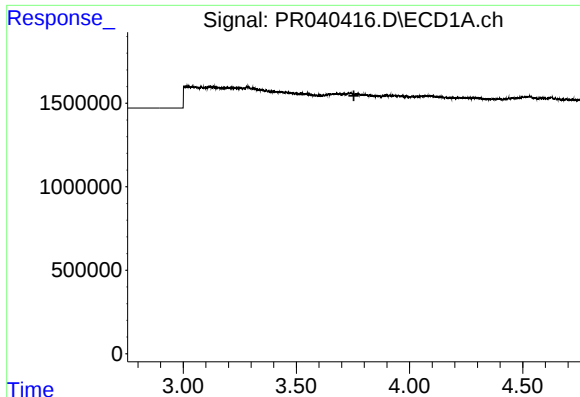

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.754 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

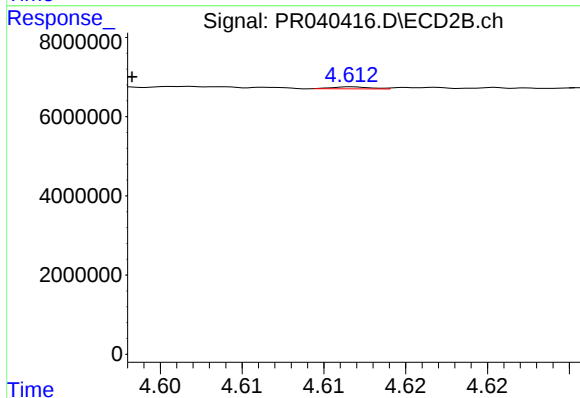


#1 Tetrachloro-m-xylene

R.T.: 4.612 min
Delta R.T.: 0.014 min
Response: 79230
Conc: 0.01 ng/ml

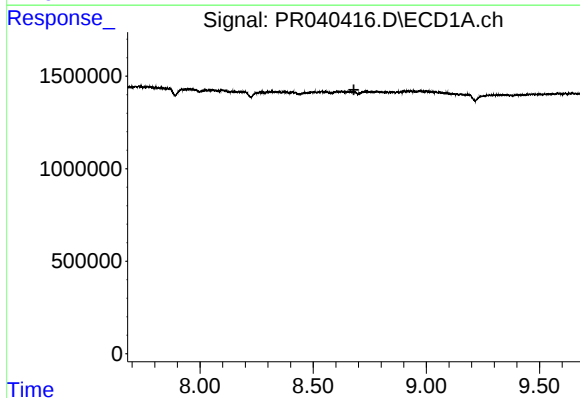


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.680 min
Response: 0
Conc: N.D.

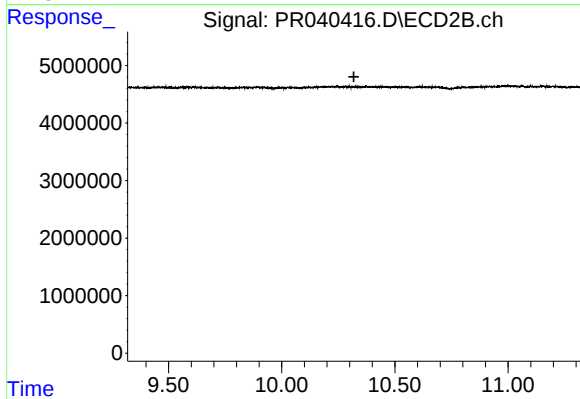

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 10.319 min
Response: 0
Conc: N.D.

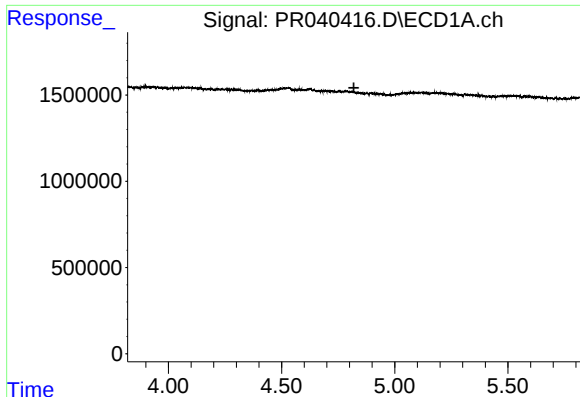

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 4.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

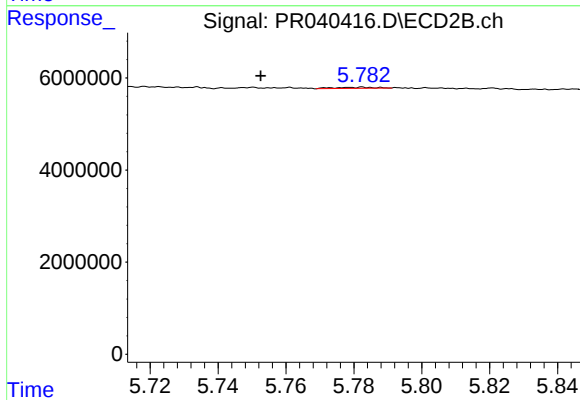


#3 AR-1016-1

R.T.: 5.783 min
Delta R.T.: 0.030 min
Response: 187488
Conc: 0.75 ng/ml

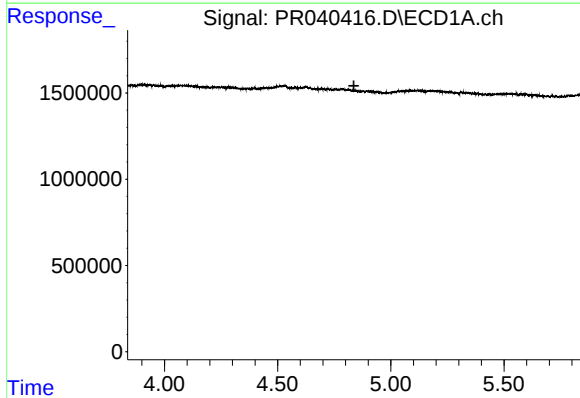


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 4.837 min
Response: 0
Conc: N.D.

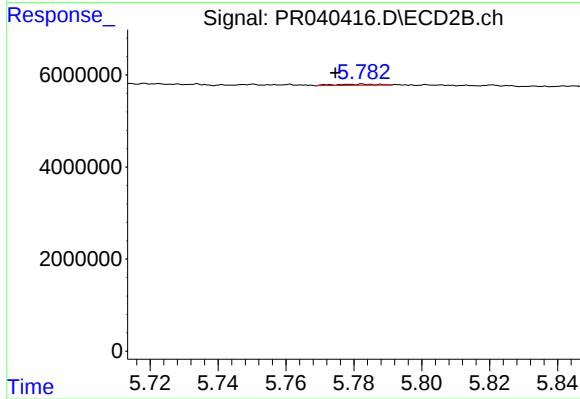

#4 AR-1016-2


R.T.: 5.783 min
Delta R.T.: 0.008 min
Response: 187488
Conc: 0.48 ng/ml

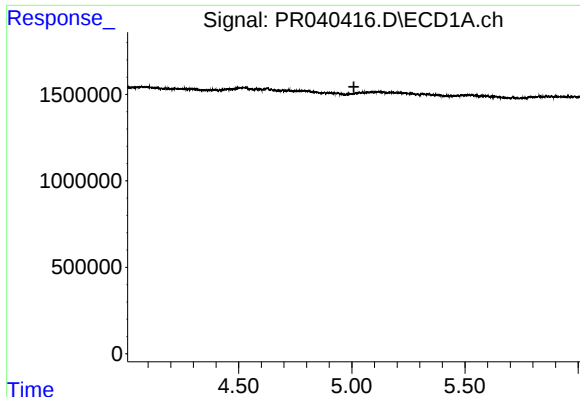

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

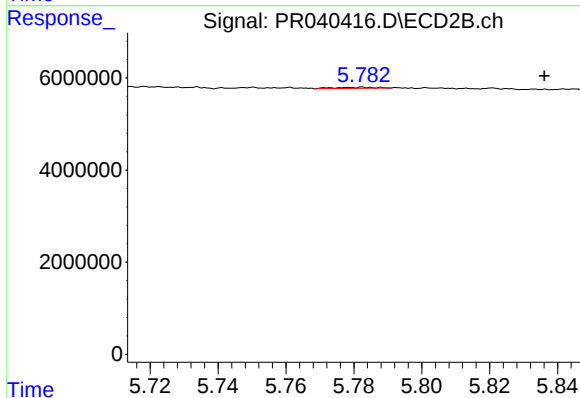


#5 AR-1016-3

R.T.: 5.783 min
Delta R.T.: -0.053 min
Response: 187488
Conc: 0.77 ng/ml

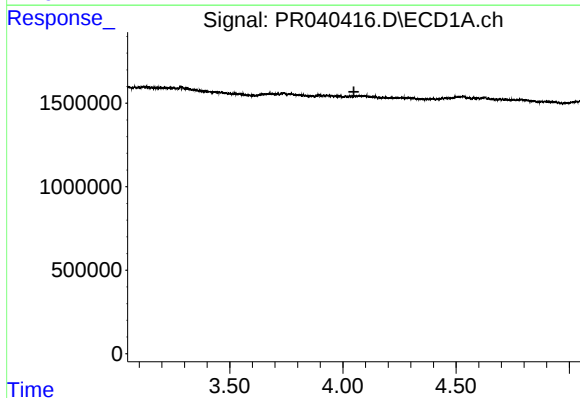


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.048 min
Response: 0
Conc: N.D.

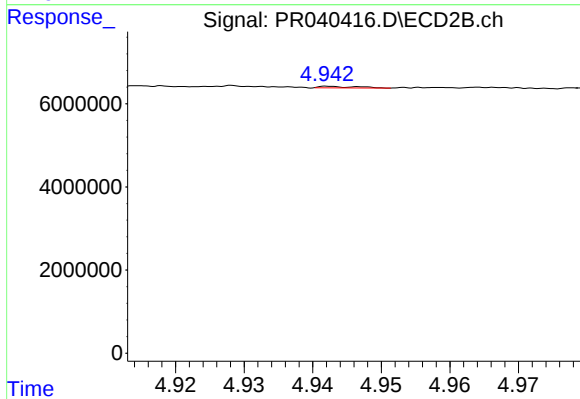

#9 AR-1221-2


R.T.: 4.943 min
Delta R.T.: 0.053 min
Response: 147006
Conc: 2.34 ng/ml

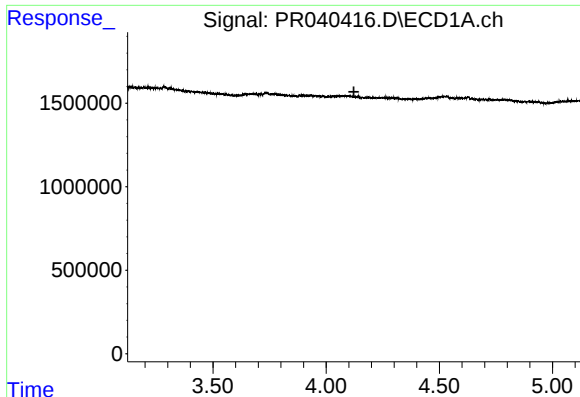

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

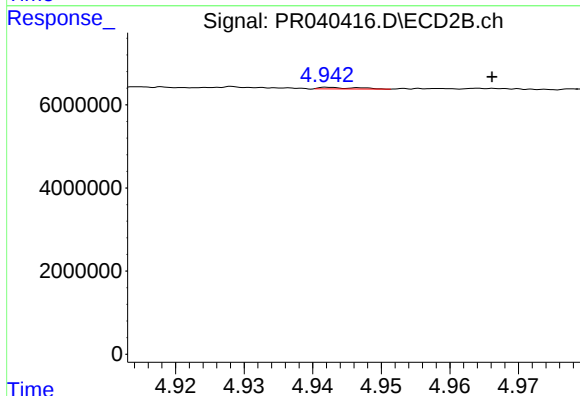


#10 AR-1221-3

R.T.: 4.943 min
Delta R.T.: -0.024 min
Response: 147006
Conc: 0.73 ng/ml

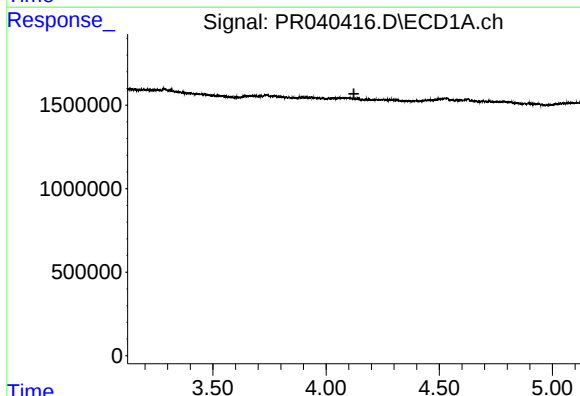


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 4.123 min
Response: 0
Conc: N.D.

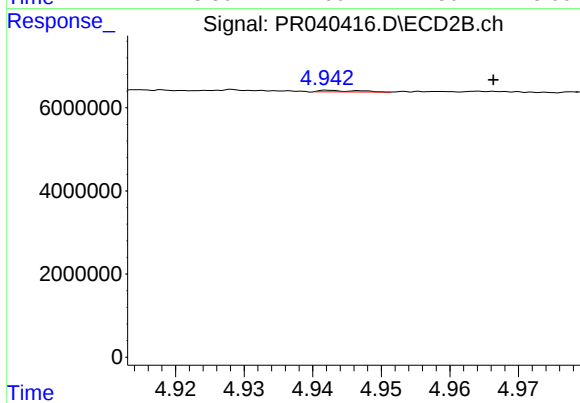

#11 AR-1232-1


R.T.: 4.943 min
Delta R.T.: -0.024 min
Response: 147006
Conc: 0.71 ng/ml

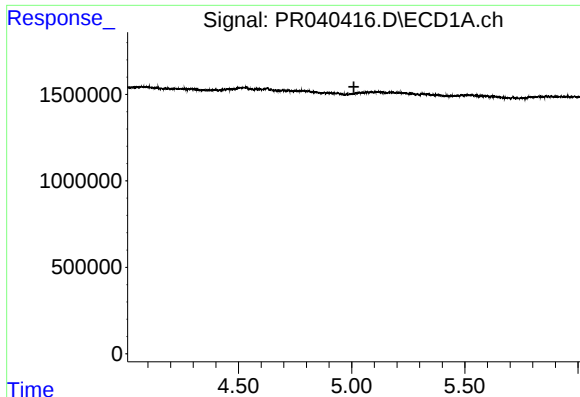

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

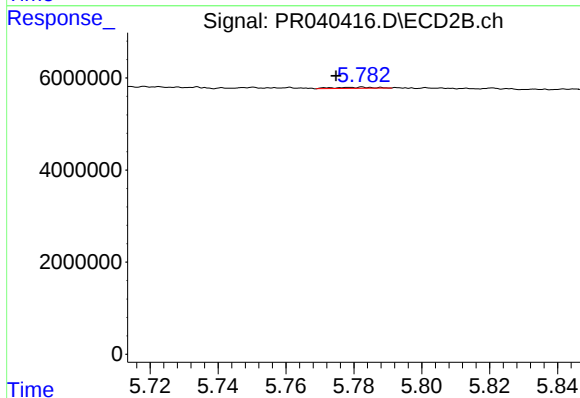


#13 AR-1232-3

R.T.: 5.783 min
Delta R.T.: 0.008 min
Response: 187488
Conc: 0.74 ng/ml

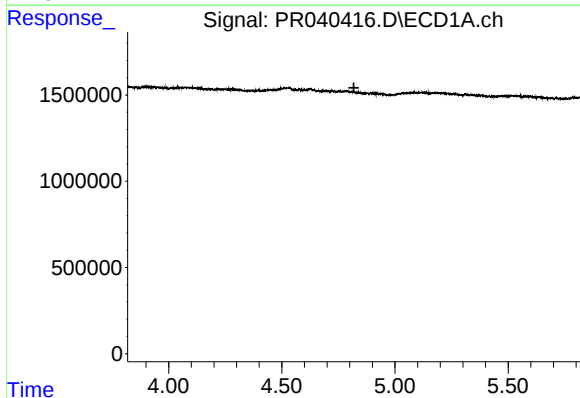


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 4.819 min
Response: 0
Conc: N.D.

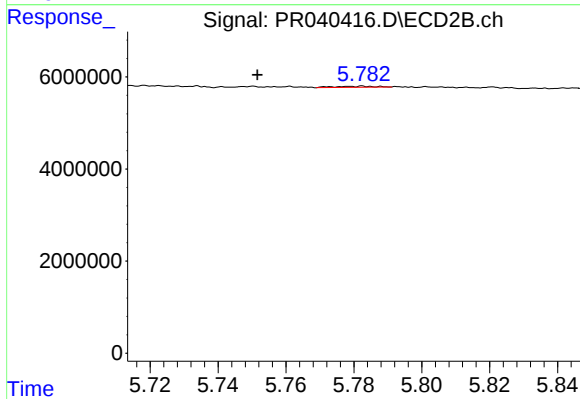

#16 AR-1242-1


R.T.: 5.783 min
Delta R.T.: 0.031 min
Response: 187488
Conc: 0.78 ng/ml

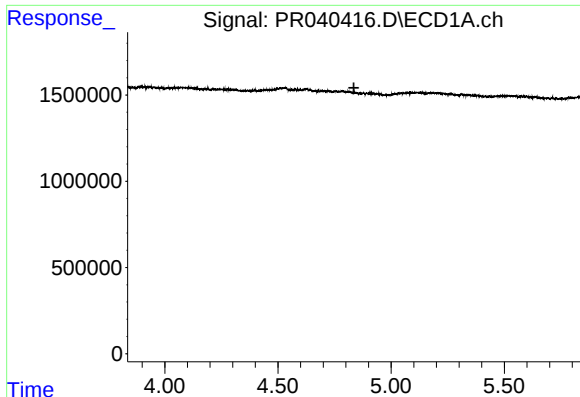

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 4.836 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

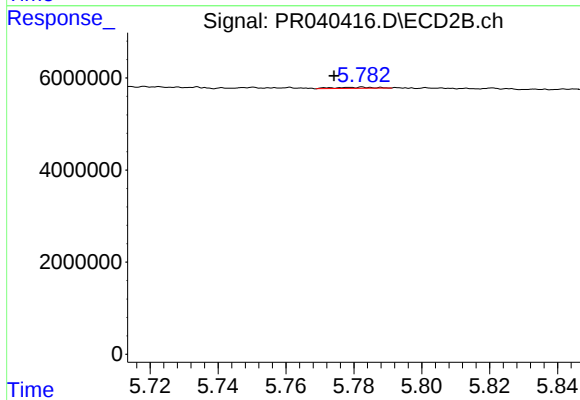


#17 AR-1242-2

R.T.: 5.783 min
Delta R.T.: 0.008 min
Response: 187488
Conc: 0.51 ng/ml

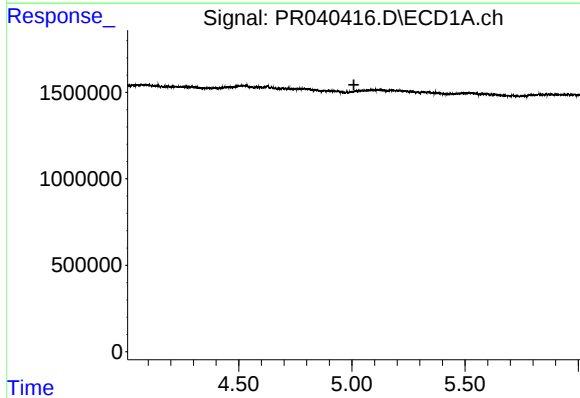


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

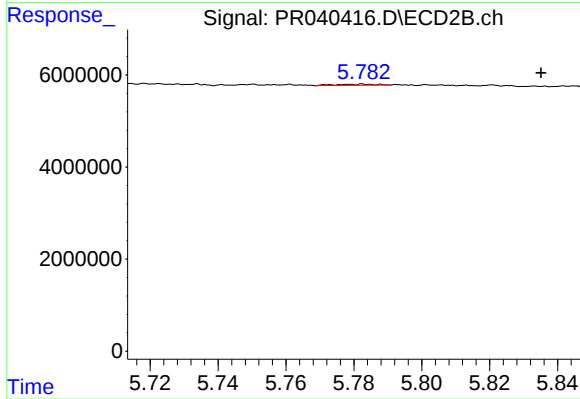

#18 AR-1242-3


R.T.: 5.783 min
Delta R.T.: -0.053 min
Response: 187488
Conc: 0.82 ng/ml

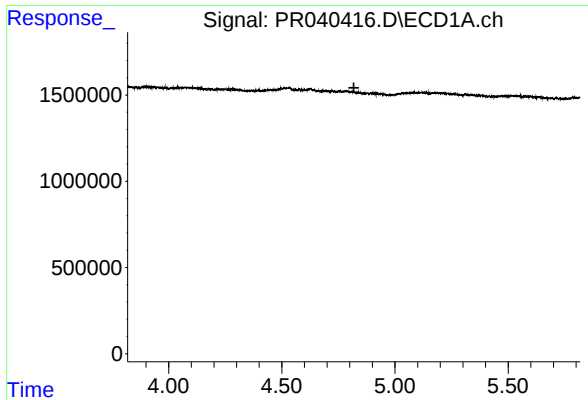

#21 AR-1248-1

R.T.: 0.000 min
Exp R.T.: 4.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

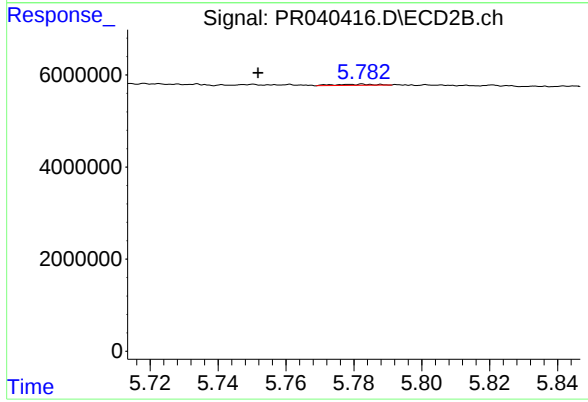

#21 AR-1248-1

R.T.: 5.783 min
Delta R.T.: 0.031 min
Response: 187488
Conc: 1.12 ng/ml