

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR081619\  
Data File : PR040416.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Aug 2019 12:38  
Operator : SM\AJ  
Sample : K3591-09  
Misc : AR1660 MDL 25 PPB  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 16 23:50:09 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR081519.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Aug 15 15:16:04 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR081619\  
Data File : PR040416.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Aug 2019 12:38  
Operator : SM\AJ  
Sample : K3591-09  
Misc : AR1660 MDL 25 PPB  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 16 23:50:09 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR081519.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Aug 15 15:16:04 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

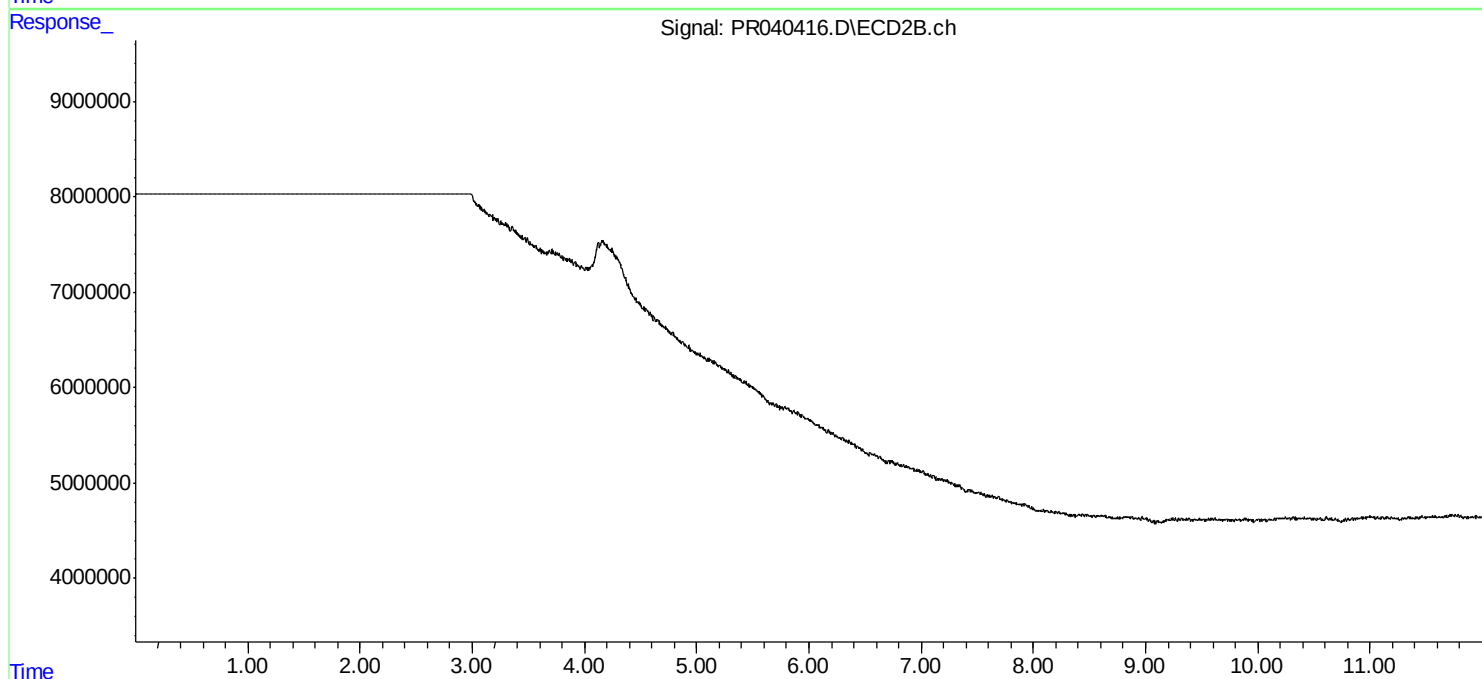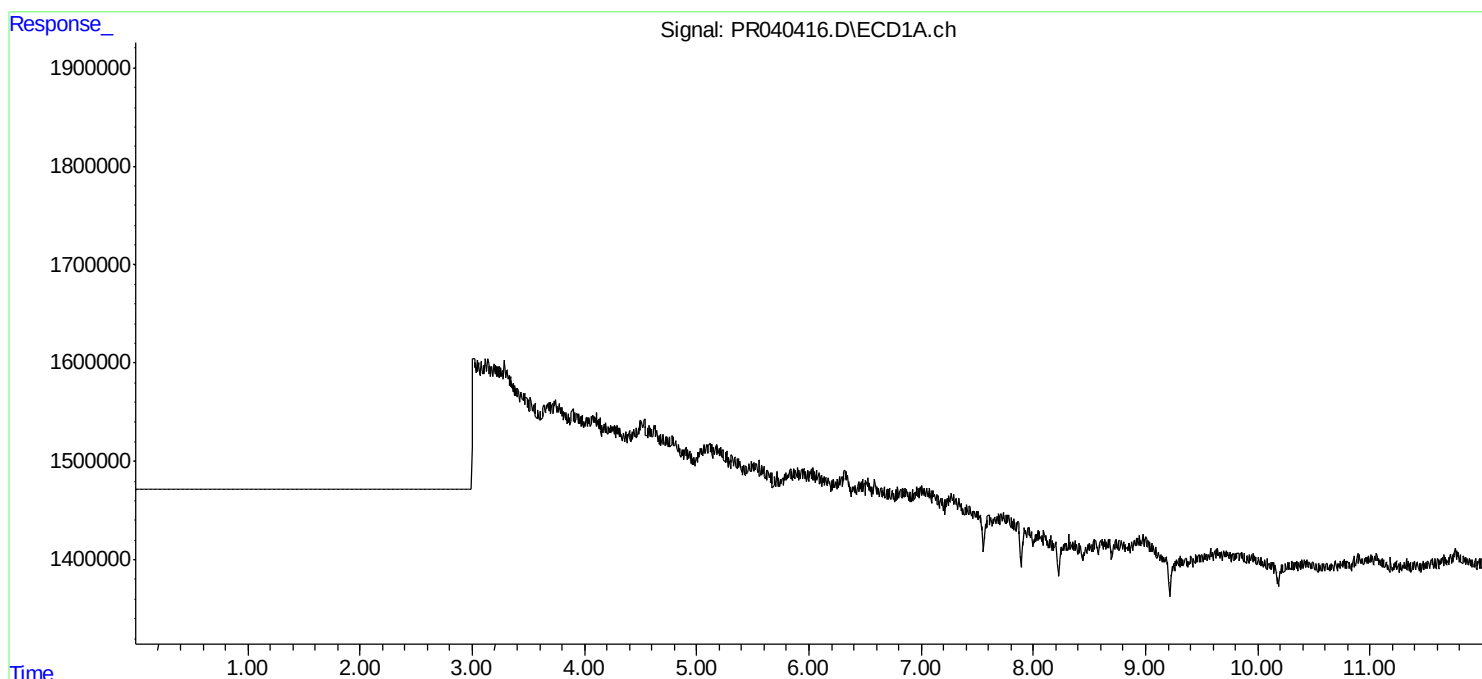


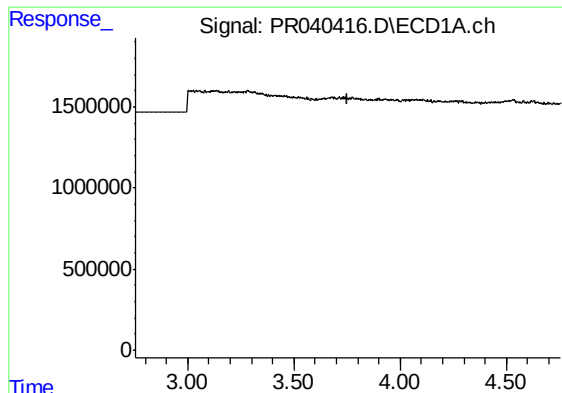

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.754 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_R  
ClientSampleId :  
MDL-MDL-WATER-03-QT3-2019

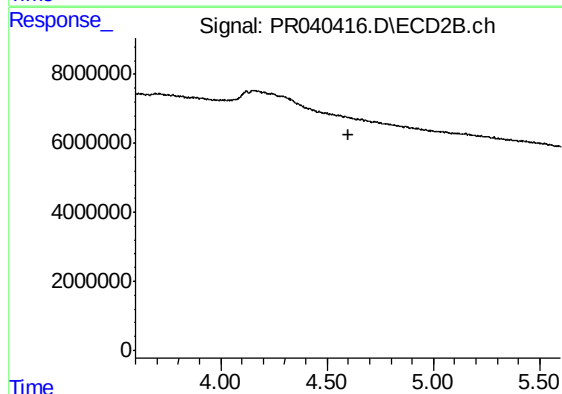


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 4.598 min  
Response: 0  
Conc: N.D.

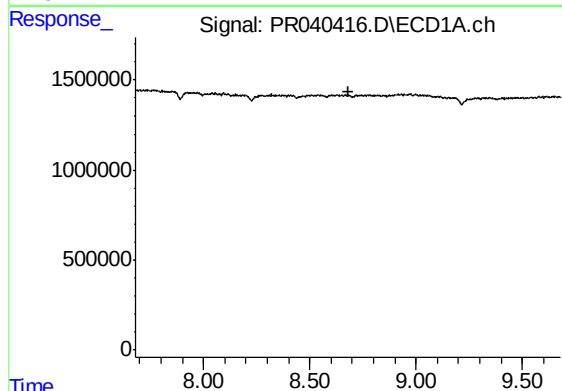

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.680 min  
Response: 0  
Conc: N.D.

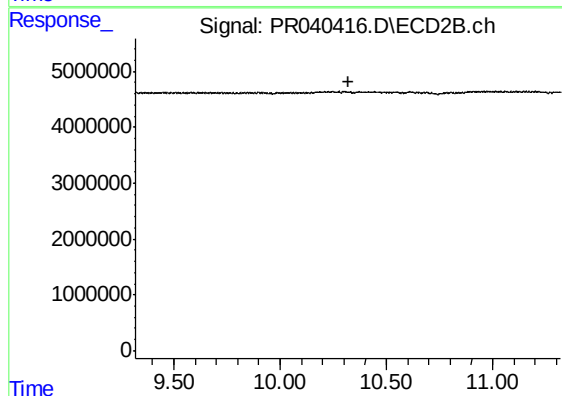

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 10.319 min  
Response: 0  
Conc: N.D.