

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082321\
 Data File : PR051698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 13:01
 Operator : DD\AJ
 Sample : M3474-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 01:19:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072921CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 30 04:51:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	3.815	125.3E6	125.7E6	17.710	20.324
2)	SA Decachlor...	10.503	8.831	218.2E6	168.6E6	22.256	22.643
Target Compounds							
9)	L2 AR-1221-2	4.946	0.000	1213325	0	18.283	N.D. #
10)	L2 AR-1221-3	4.946f	0.000	1213325	0	5.831	N.D. #
11)	L3 AR-1232-1	4.946f	0.000	1213325	0	7.051	N.D. #
12)	L3 AR-1232-2	5.526	0.000	2801607	0	30.198	N.D. #
27)	L6 AR-1254-2	6.892	0.000	2239441	0	4.684	N.D. #
28)	L6 AR-1254-3	7.279	0.000	4687647	0	9.106	N.D. #
29)	L6 AR-1254-4	7.562	0.000	1417413	0	3.244	N.D. #
31)	L7 AR-1260-1	7.385	0.000	2385946	0	5.672	N.D. #
45)	L9 AR-1268-5	10.154	0.000	2016209	0	0.336	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082321\
Data File : PR051698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 13:01
Operator : DD\AJ
Sample : M3474-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 01:19:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072921CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 30 04:51:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

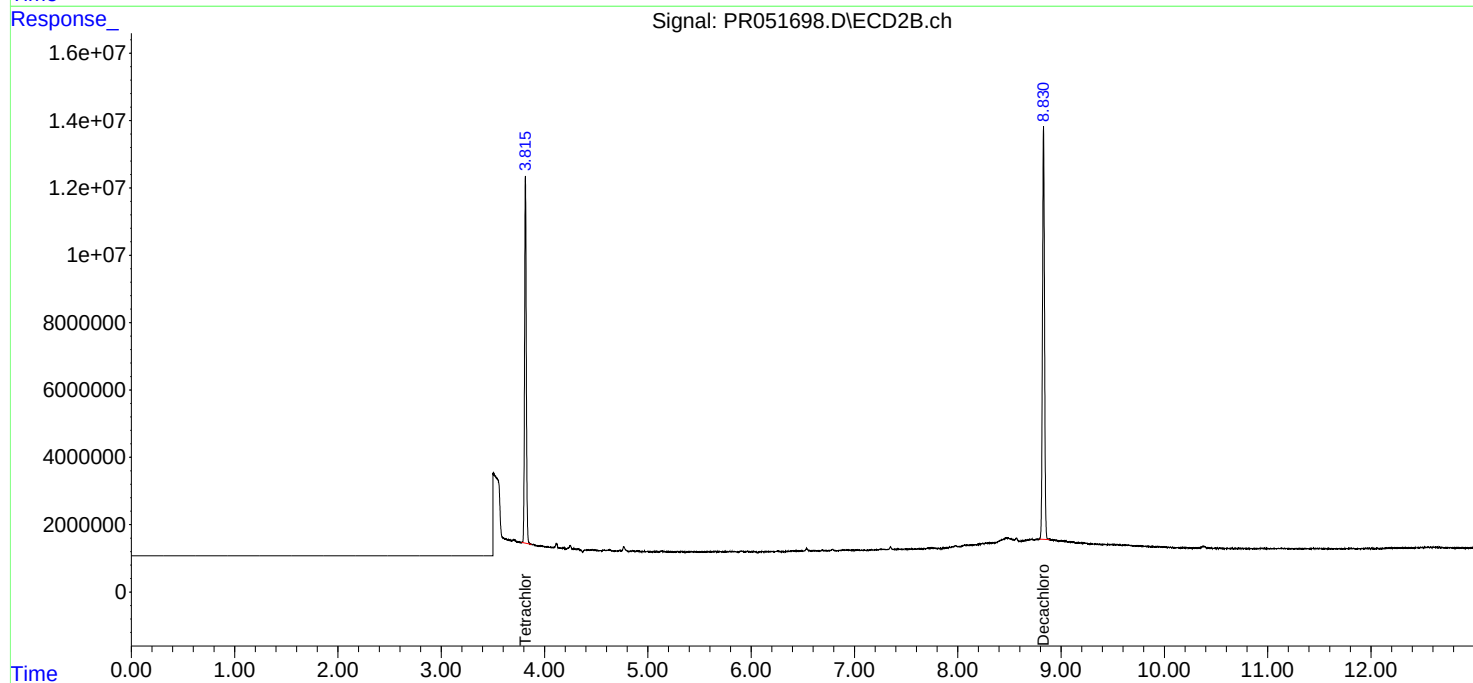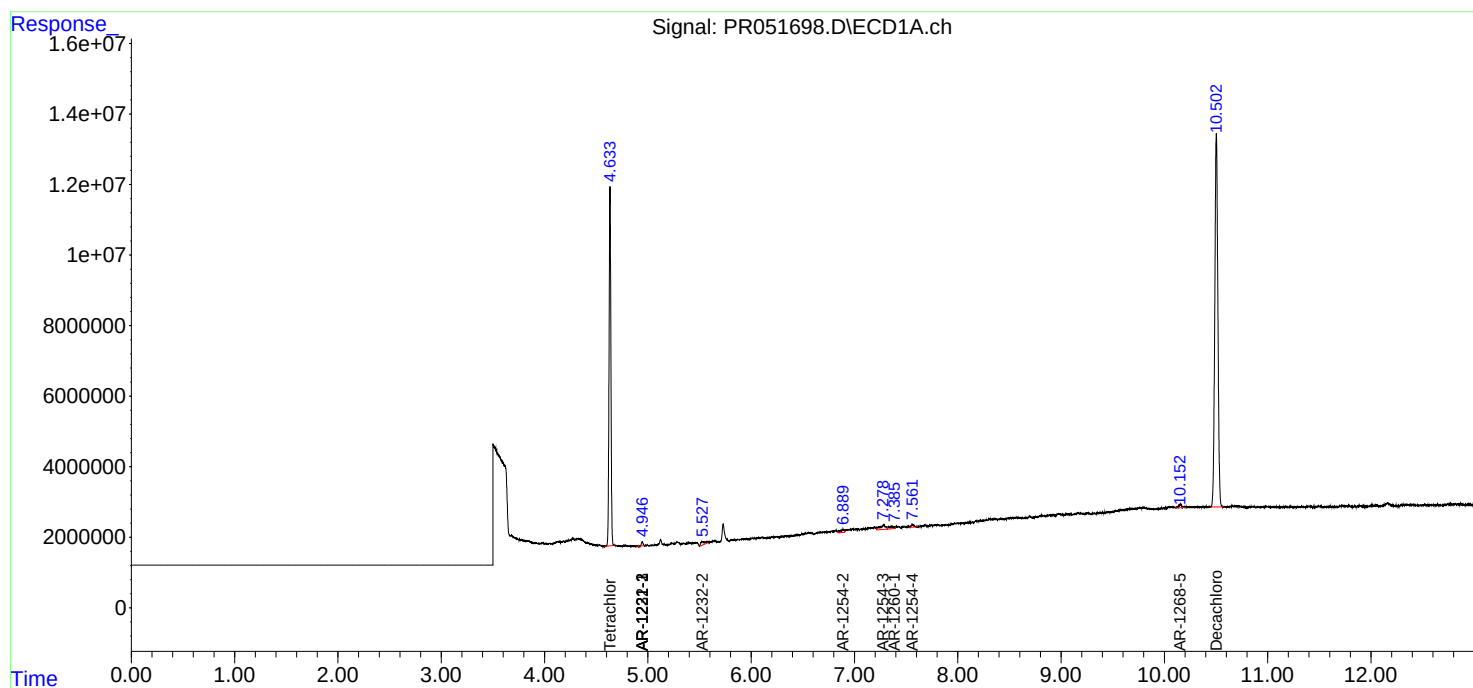


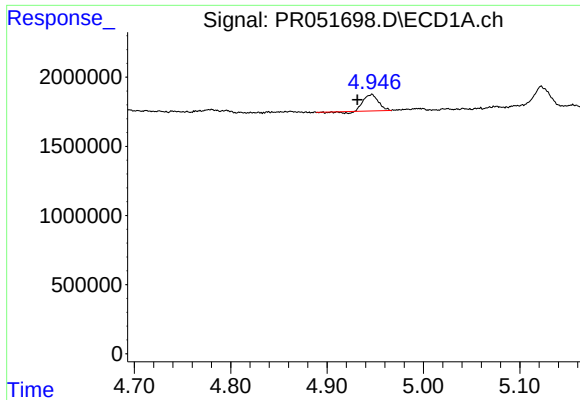

#9 AR-1221-2


R.T.: 4.946 min
Delta R.T.: 0.014 min
Response: 1213325
Conc: 18.28 ng/ml

Instrument :
ECD_R
ClientSampleId :

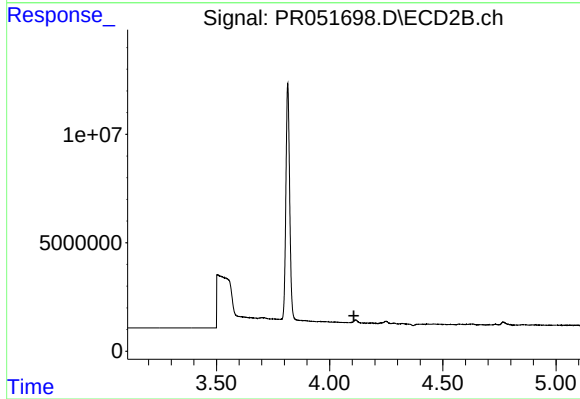


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

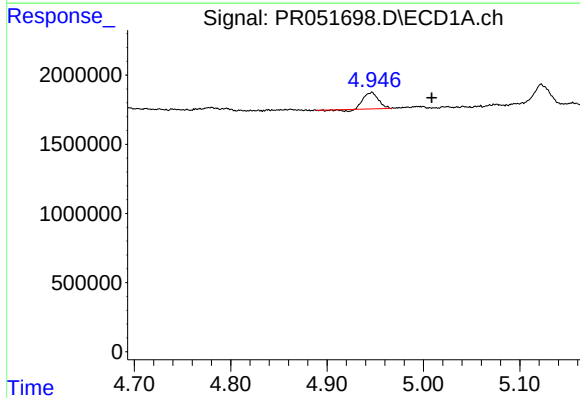


#10 AR-1221-3

R.T.: 4.946 min
Delta R.T.: -0.063 min
Response: 1213325
Conc: 5.83 ng/ml

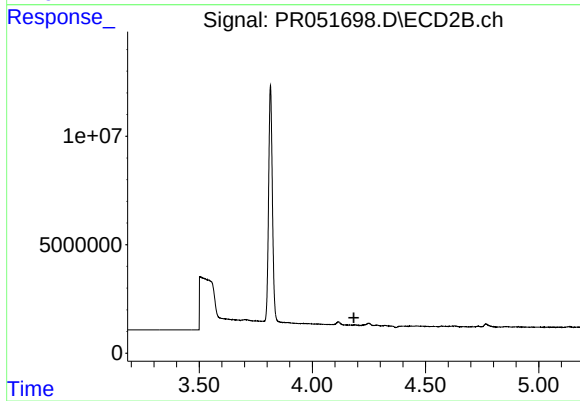

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.184 min
Response: 0
Conc: N.D.

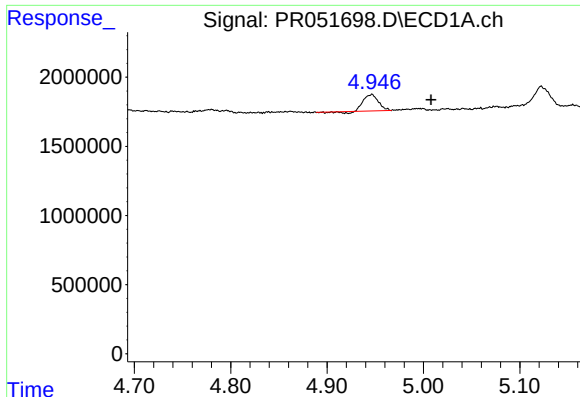

#11 AR-1232-1


R.T.: 4.946 min
Delta R.T.: -0.062 min
Response: 1213325
Conc: 7.05 ng/ml

Instrument :
ECD_R
ClientSampleId :

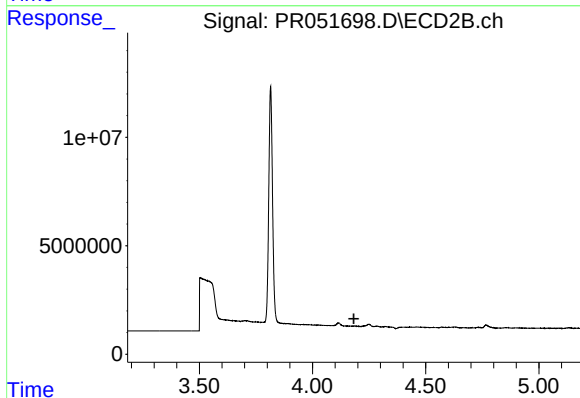


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.183 min
Response: 0
Conc: N.D.

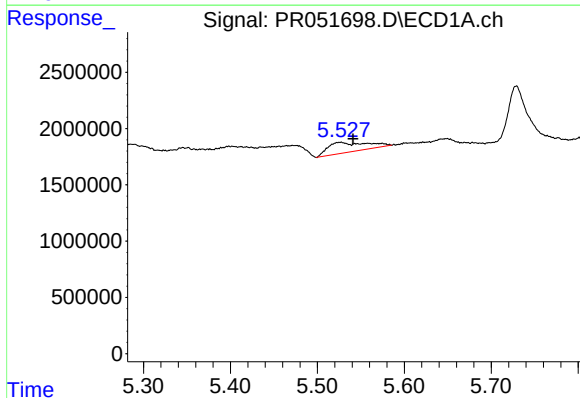


#12 AR-1232-2

R.T.: 5.526 min
Delta R.T.: -0.015 min
Response: 2801607
Conc: 30.20 ng/ml

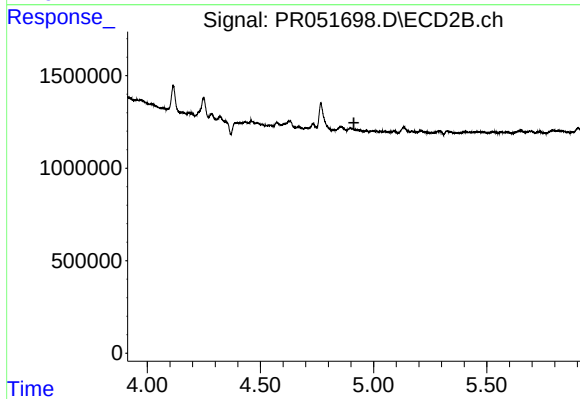

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.913 min
Response: 0
Conc: N.D.

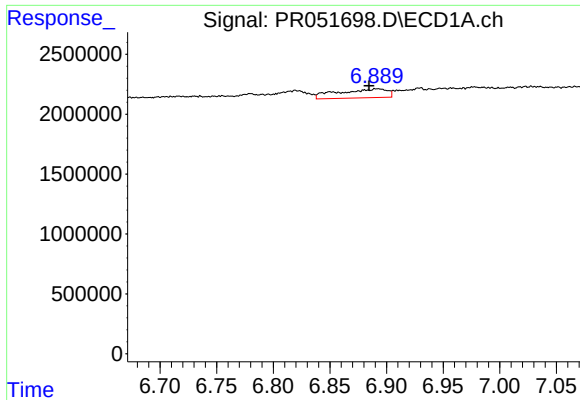

#27 AR-1254-2


R.T.: 6.892 min
Delta R.T.: 0.008 min
Response: 2239441
Conc: 4.68 ng/ml

Instrument :
ECD_R
ClientSampleId :

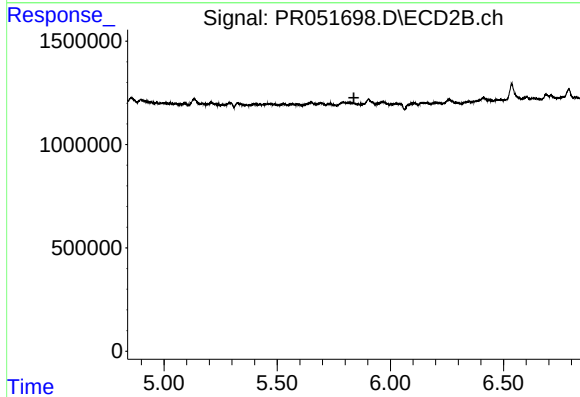


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.839 min
Response: 0
Conc: N.D.

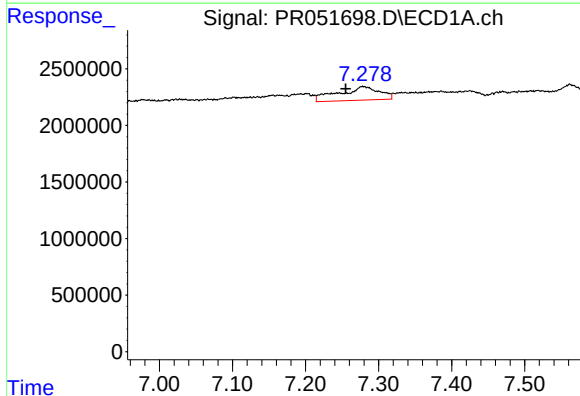


#28 AR-1254-3

R.T.: 7.279 min
Delta R.T.: 0.024 min
Response: 4687647
Conc: 9.11 ng/ml

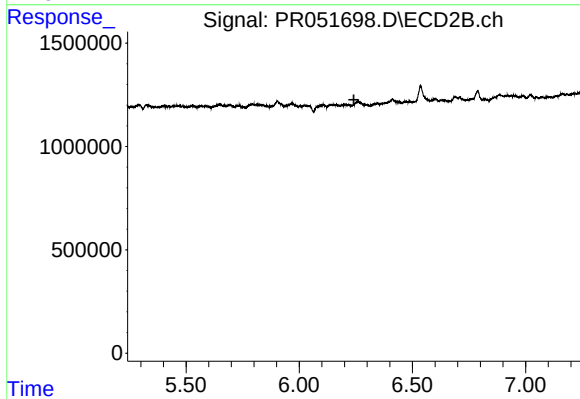

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

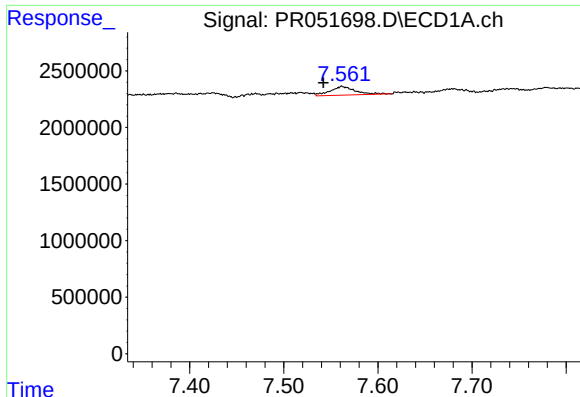

#29 AR-1254-4


R.T.: 7.562 min
Delta R.T.: 0.020 min
Response: 1417413
Conc: 3.24 ng/ml

Instrument :
ECD_R
ClientSampleId :

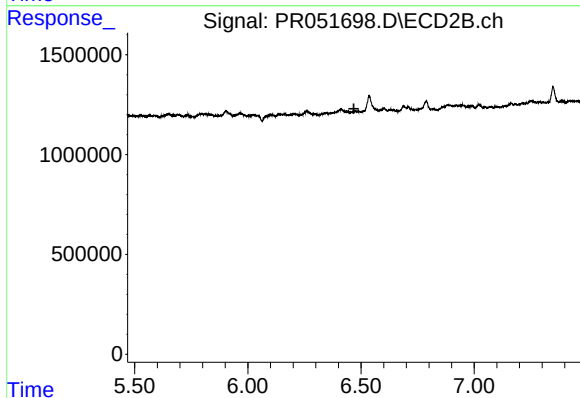


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.469 min
Response: 0
Conc: N.D.

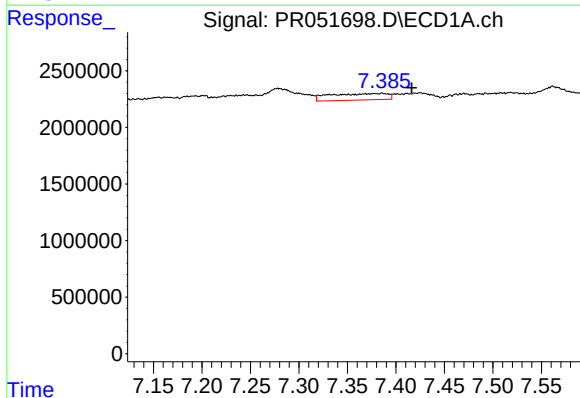


#31 AR-1260-1

R.T.: 7.385 min
Delta R.T.: -0.032 min
Response: 2385946
Conc: 5.67 ng/ml

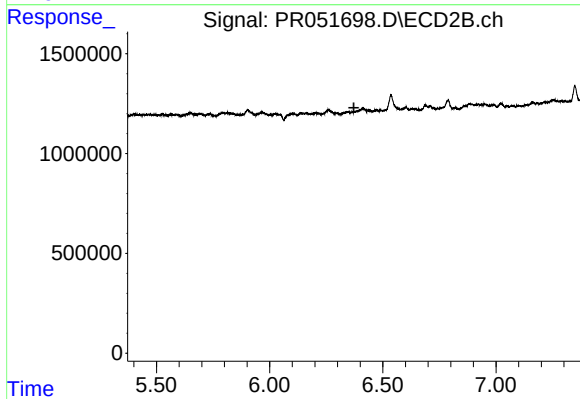

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

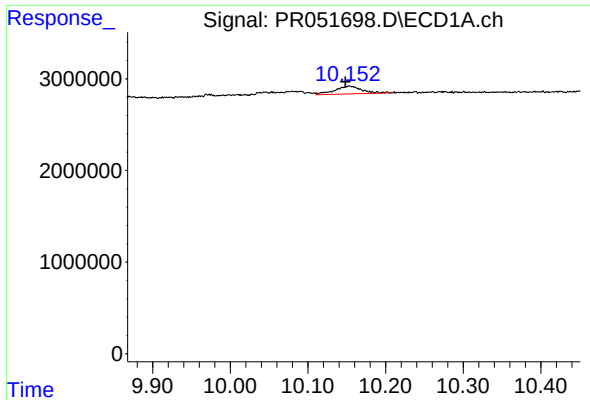

#45 AR-1268-5

R.T.: 10.154 min
Delta R.T.: 0.006 min
Response: 2016209
Conc: 0.34 ng/ml

Instrument :
ECD_R
ClientSampleId :

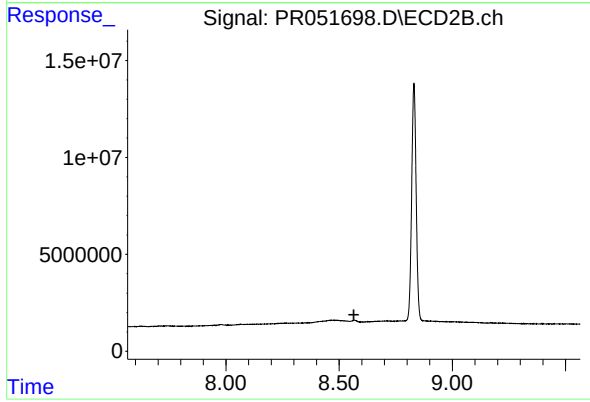

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.565 min
Response: 0
Conc: N.D.