

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082321\
 Data File : PR051700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 13:32
 Operator : DD\AJ
 Sample : M3474-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 01:20:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072921CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 30 04:51:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	3.816	108.7E6	109.5E6	15.363	17.701
2)	SA Decachlor...	10.501	8.829	256.6E6	195.4E6	26.174	26.253
Target Compounds							
9)	L2 AR-1221-2	4.946	0.000	1628151	0	24.534	N.D. #
10)	L2 AR-1221-3	4.946f	0.000	1628151	0	7.824	N.D. #
11)	L3 AR-1232-1	4.946f	0.000	1628151	0	9.461	N.D. #
12)	L3 AR-1232-2	5.527	0.000	1488188	0	16.041	N.D. #
28)	L6 AR-1254-3	7.279	0.000	2636819	0	5.122	N.D. #
29)	L6 AR-1254-4	0.000	6.537f	0 36968388	0	N.D.	116.685 #
30)	L6 AR-1254-5	7.923f	0.000	19054205	0	44.303	N.D. #
32)	L7 AR-1260-2	0.000	6.537	0 36968388	0	N.D.	80.044 #
45)	L9 AR-1268-5	10.152	0.000	2222083	0	0.370	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082321\
Data File : PR051700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 13:32
Operator : DD\AJ
Sample : M3474-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 01:20:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR072921CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 30 04:51:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

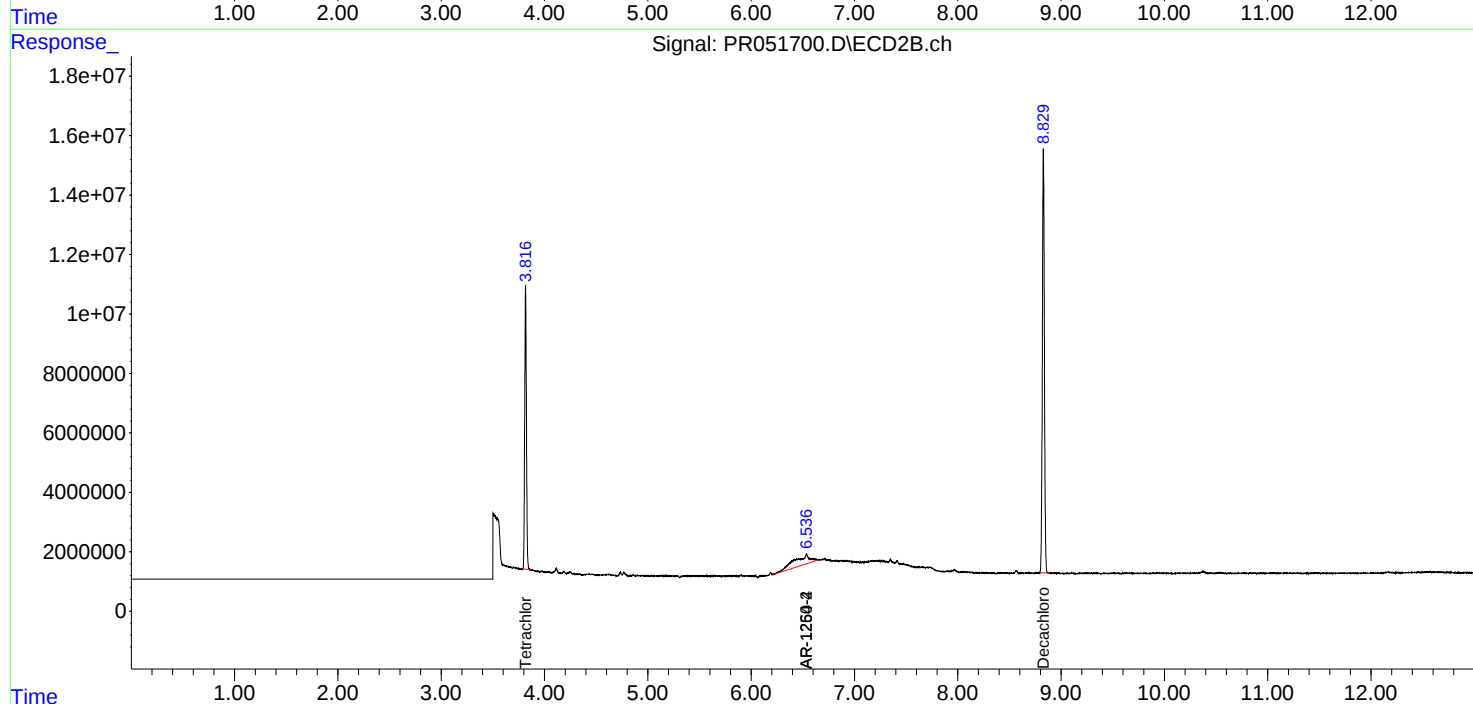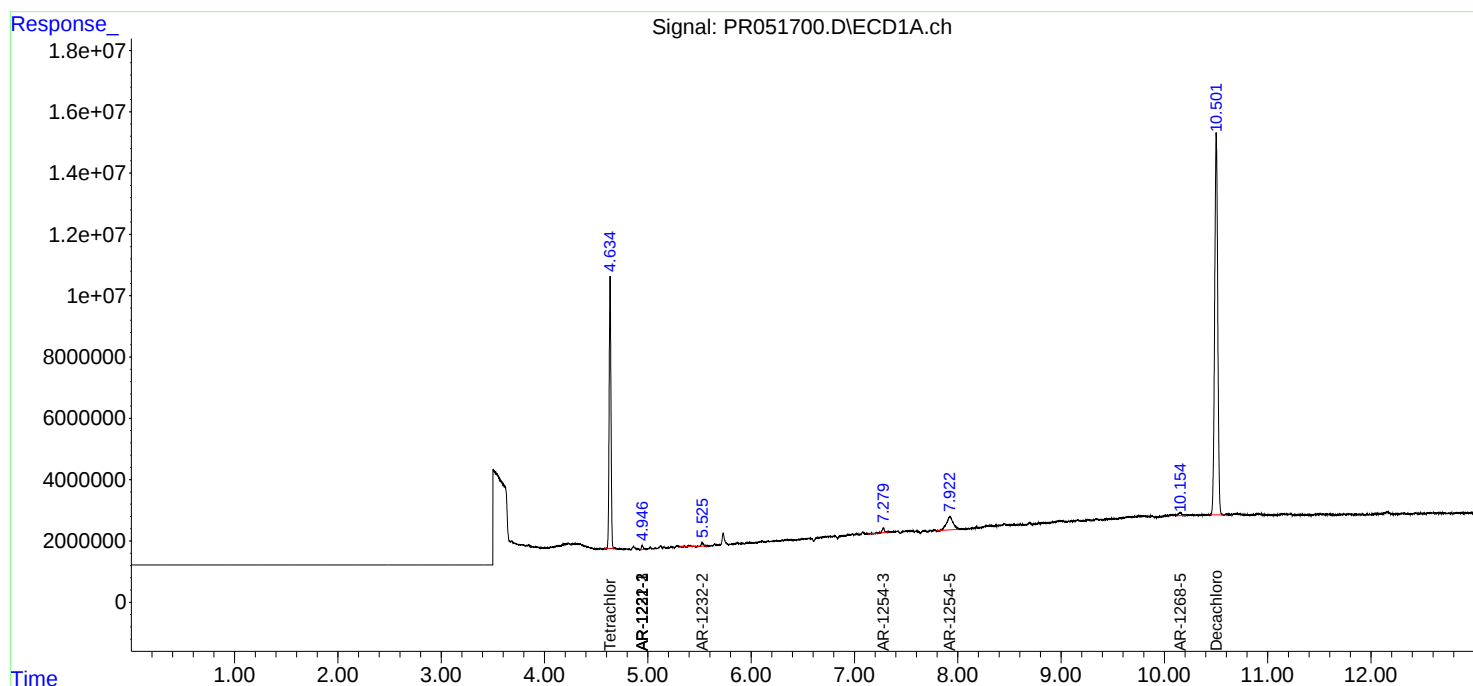


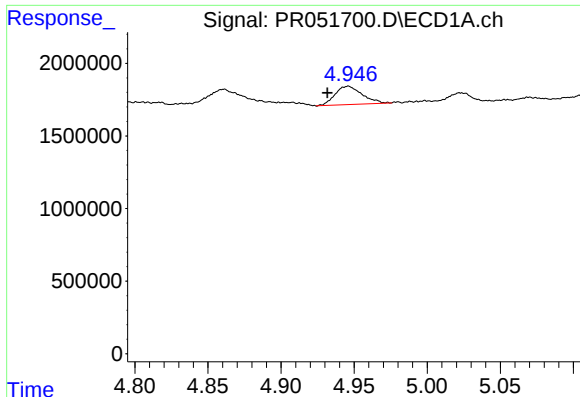

#9 AR-1221-2


R.T.: 4.946 min
Delta R.T.: 0.014 min
Response: 1628151
Conc: 24.53 ng/ml

Instrument :
ECD_R
ClientSampleId :

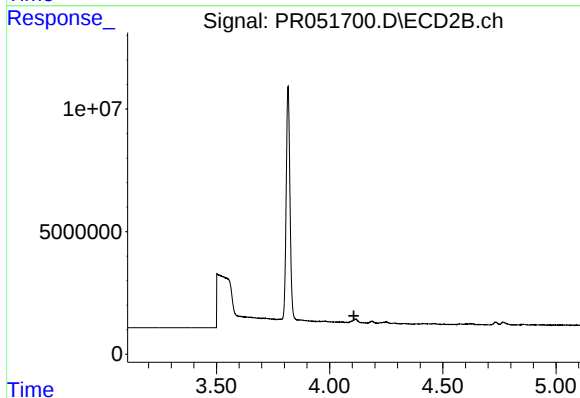


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

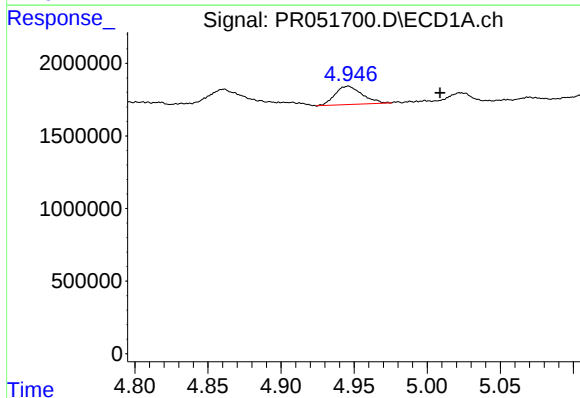


#10 AR-1221-3

R.T.: 4.946 min
Delta R.T.: -0.063 min
Response: 1628151
Conc: 7.82 ng/ml

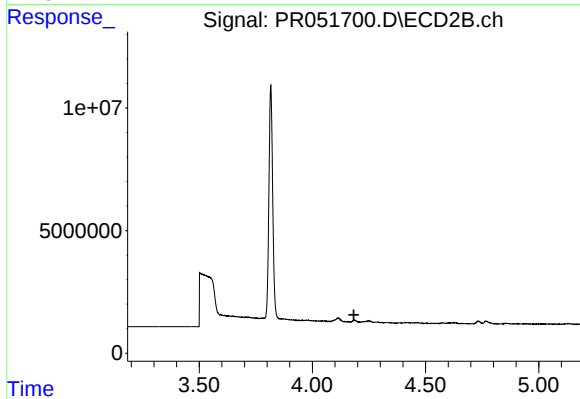

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.184 min
Response: 0
Conc: N.D.

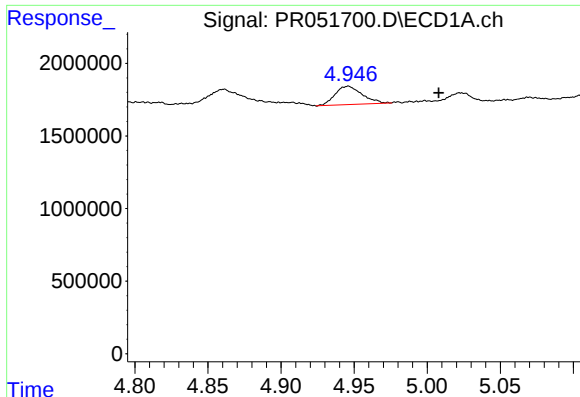

#11 AR-1232-1


R.T.: 4.946 min
Delta R.T.: -0.062 min
Response: 1628151
Conc: 9.46 ng/ml

Instrument :
ECD_R
ClientSampleId :

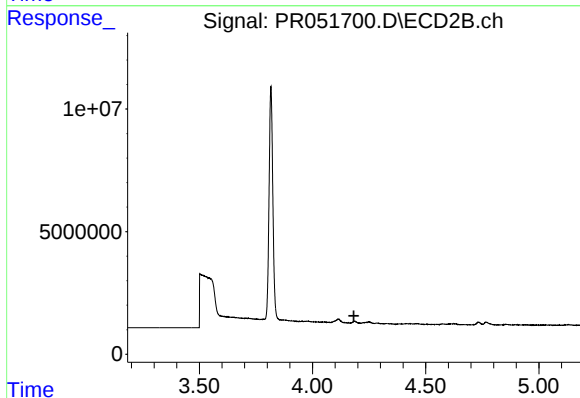


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.183 min
Response: 0
Conc: N.D.

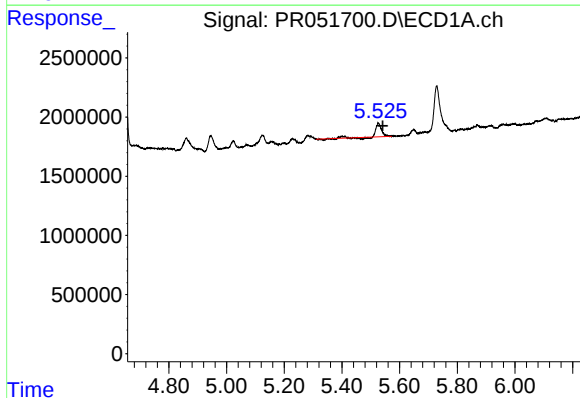


#12 AR-1232-2

R.T.: 5.527 min
Delta R.T.: -0.015 min
Response: 1488188
Conc: 16.04 ng/ml

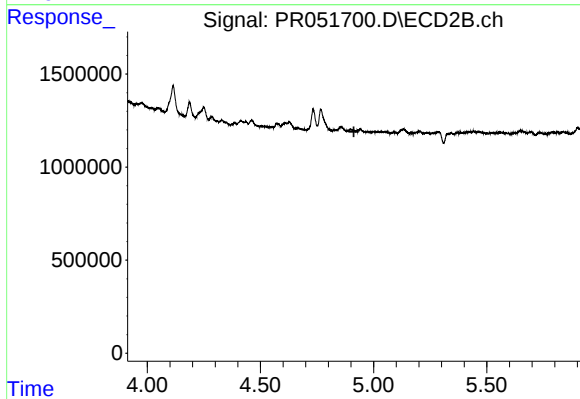

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.913 min
Response: 0
Conc: N.D.

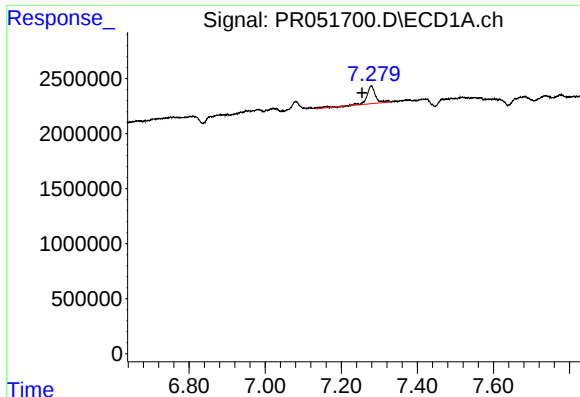

#28 AR-1254-3


R.T.: 7.279 min
Delta R.T.: 0.024 min
Response: 2636819
Conc: 5.12 ng/ml

Instrument :
ECD_R
ClientSampleId :

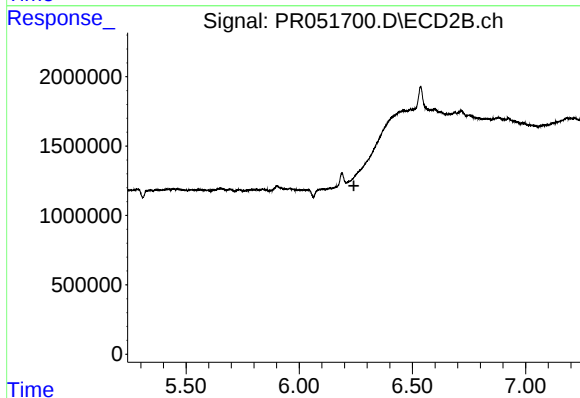


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

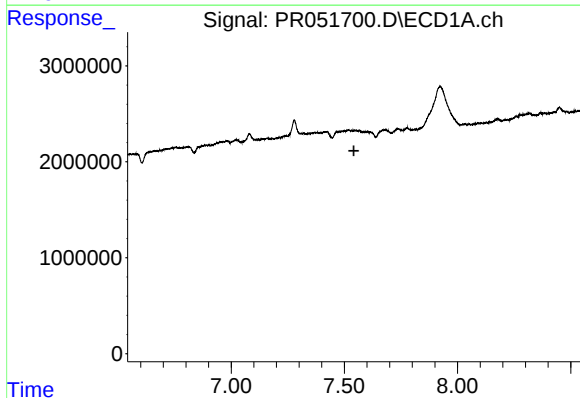


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.542 min
Response: 0
Conc: N.D.

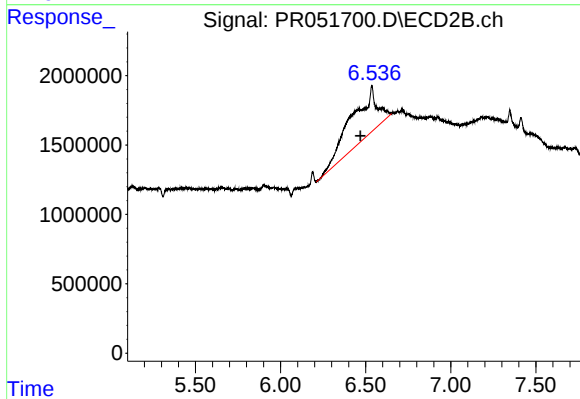

#29 AR-1254-4


R.T.: 6.537 min
Delta R.T.: 0.068 min
Response: 36968388
Conc: 116.69 ng/ml

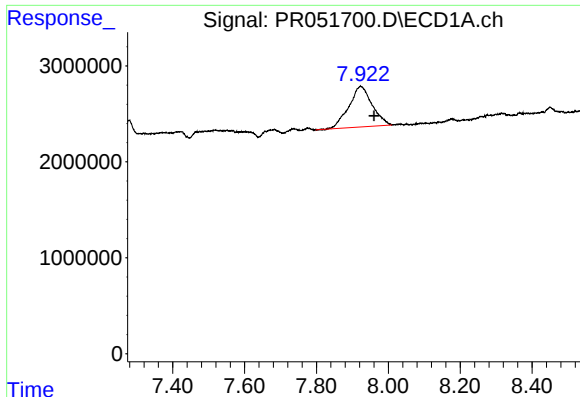

#30 AR-1254-5


R.T.: 7.923 min
Delta R.T.: -0.038 min
Response: 19054205
Conc: 44.30 ng/ml

Instrument :
ECD_R
ClientSampleId :

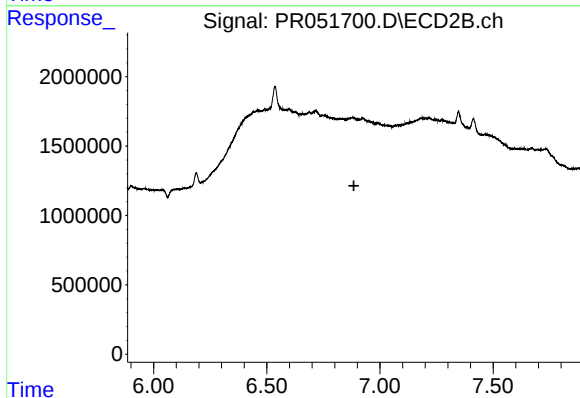


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.885 min
Response: 0
Conc: N.D.

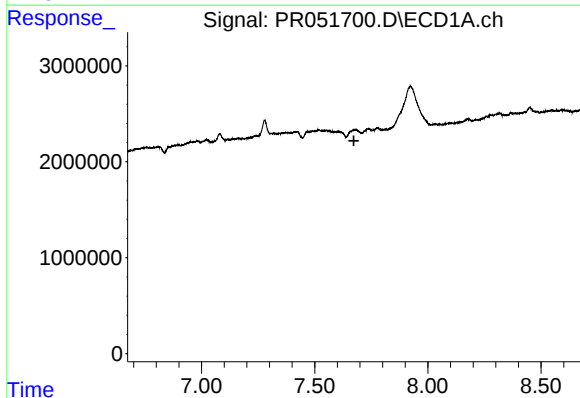


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.673 min
Response: 0
Conc: N.D.

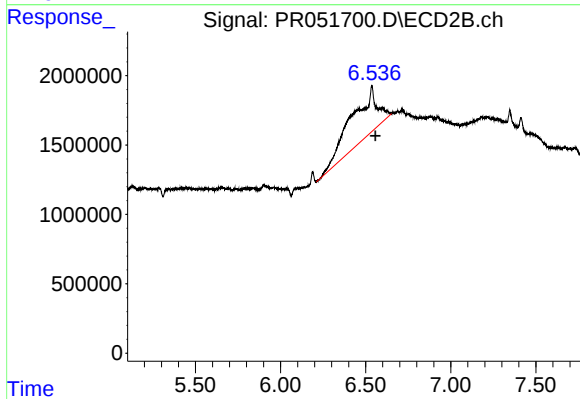

#32 AR-1260-2


R.T.: 6.537 min
Delta R.T.: -0.022 min
Response: 36968388
Conc: 80.04 ng/ml

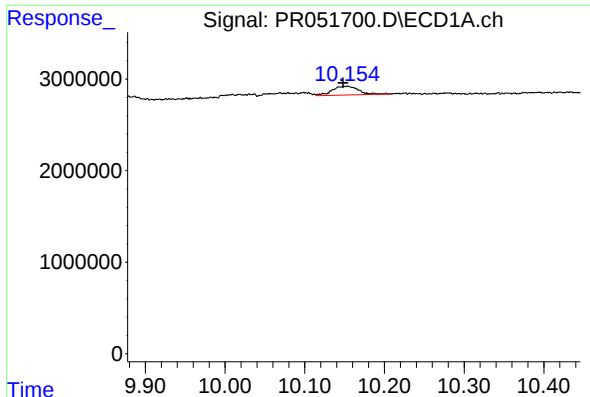

#45 AR-1268-5

R.T.: 10.152 min
Delta R.T.: 0.004 min
Response: 2222083
Conc: 0.37 ng/ml

Instrument :
ECD_R
ClientSampleId :

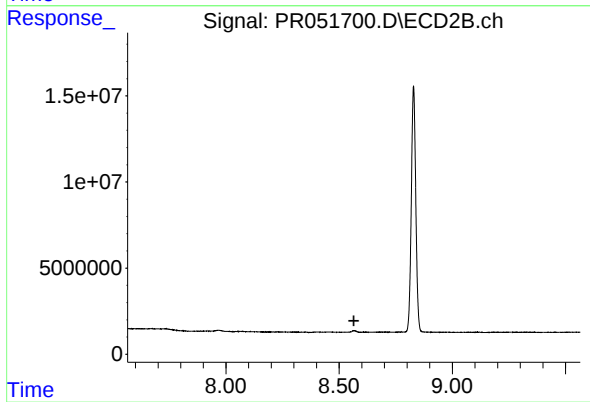

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.565 min
Response: 0
Conc: N.D.