

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082322\
 Data File : PR056104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2022 19:09
 Operator : AJ\MA
 Sample : PB147202BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PB147202BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/24/2022
 Supervised By :Ankita Jodhani 08/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 00:00:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 12:39:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.627	2.898	107.0E6	45659070	25.071	22.741
2) SA Decachlor...	9.517	8.110	45394547	42051955	25.531	23.117m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082322\
Data File : PR056104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2022 19:09
Operator : AJ\MA
Sample : PB147202BL
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PB147202BL


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 08/24/2022
Supervised By : Ankita Jodhani 08/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 00:00:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 12:39:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

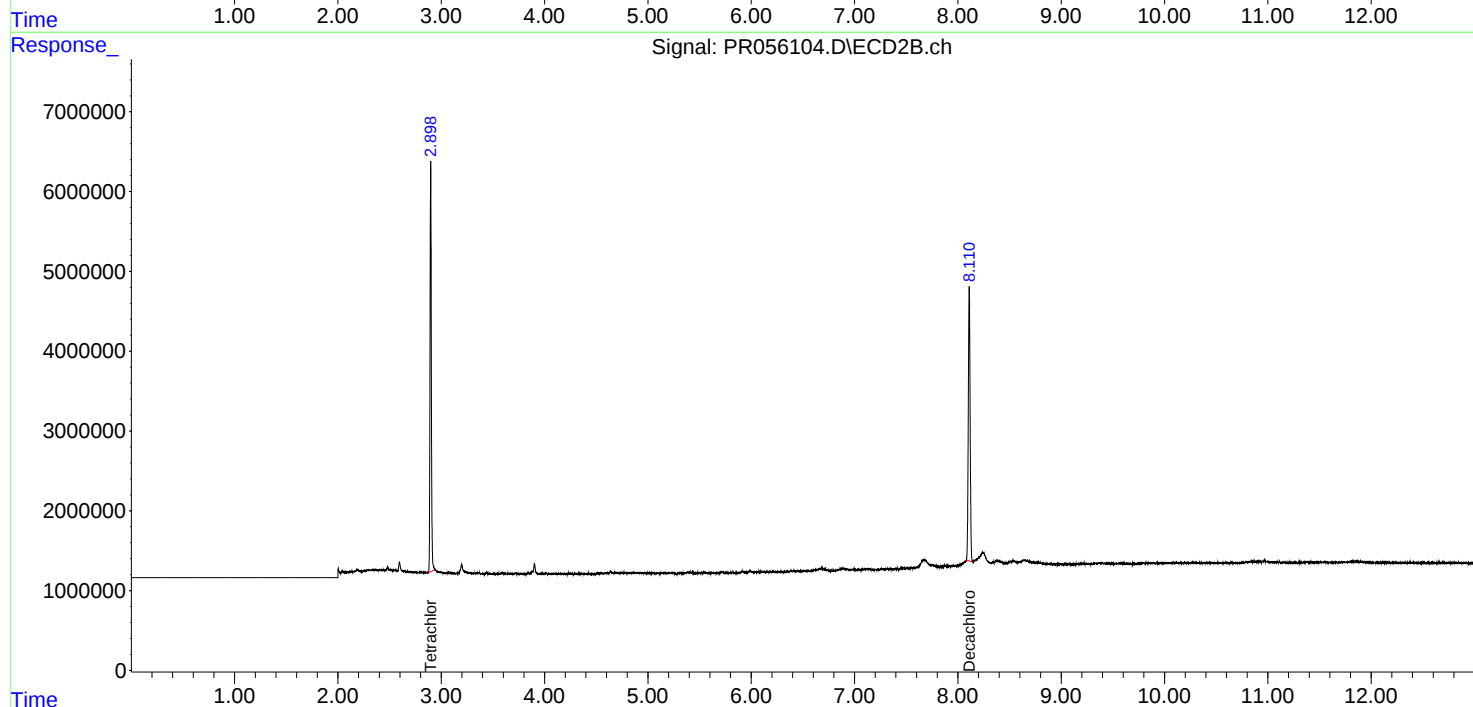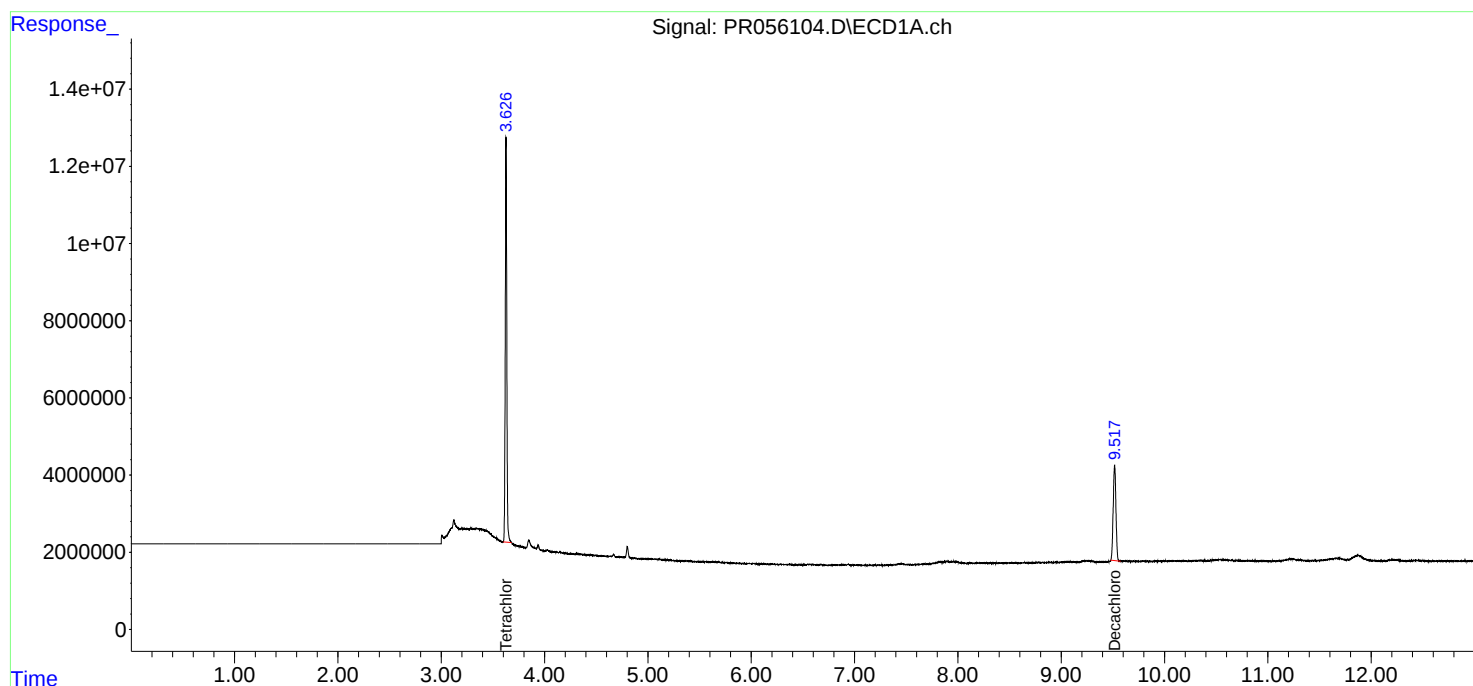

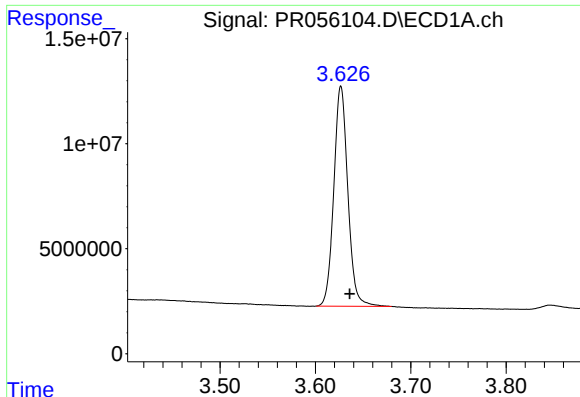

#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: -0.009 min
Response: 106977237
Conc: 25.07 ng/ml

Instrument :

ECD_R


ClientSampleId :

PB147202BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 08/24/2022
Supervised By :Ankita Jodhani 08/24/2022

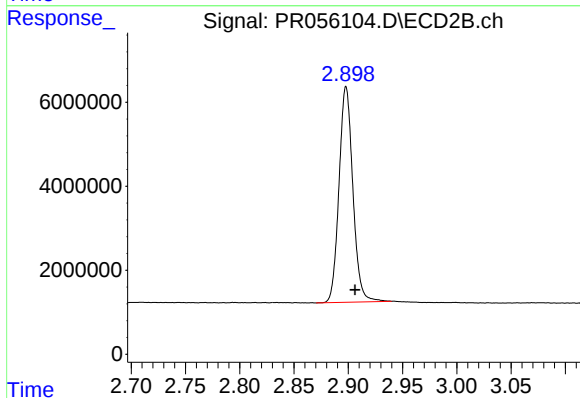


#1 Tetrachloro-m-xylene

R.T.: 2.898 min
Delta R.T.: -0.008 min
Response: 45659070
Conc: 22.74 ng/ml

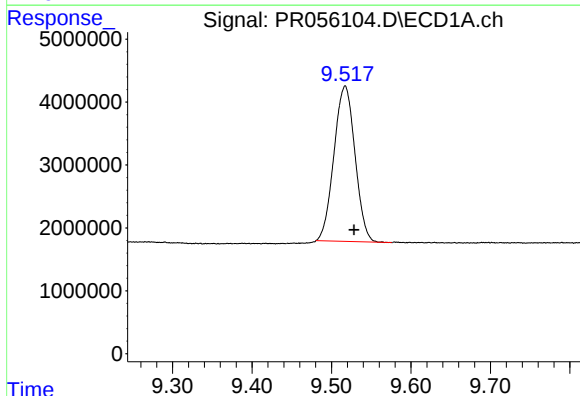

#2 Decachlorobiphenyl

R.T.: 9.517 min
Delta R.T.: -0.011 min
Response: 45394547
Conc: 25.53 ng/ml

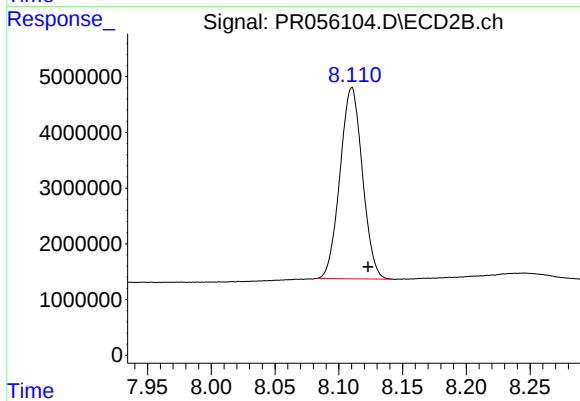

#2 Decachlorobiphenyl

R.T.: 8.110 min
Delta R.T.: -0.013 min
Response: 42051955
Conc: 23.12 ng/ml m