

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082422\
 Data File : PR056121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2022 12:59
 Operator : AJ\MA
 Sample : PB147204BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PB147204BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/25/2022
 Supervised By :Ankita Jodhani 08/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 04:38:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 12:39:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.628	2.898	87489120	33828910	20.504	16.849
2) SA Decachlor...	9.517	8.109	38386512	34585648	21.589	19.013m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082422\
Data File : PR056121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2022 12:59
Operator : AJ\MA
Sample : PB147204BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PB147204BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2022
Supervised By :Ankita Jodhani 08/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 04:38:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 12:39:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

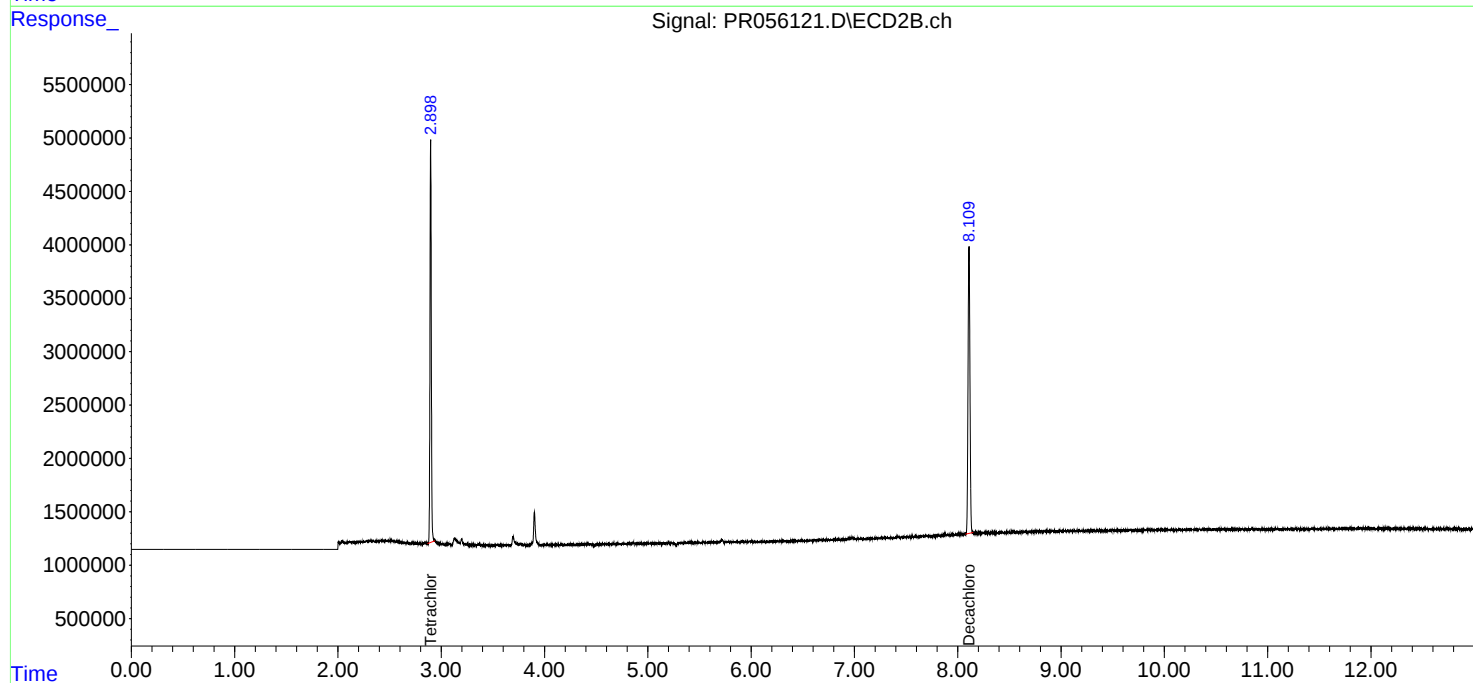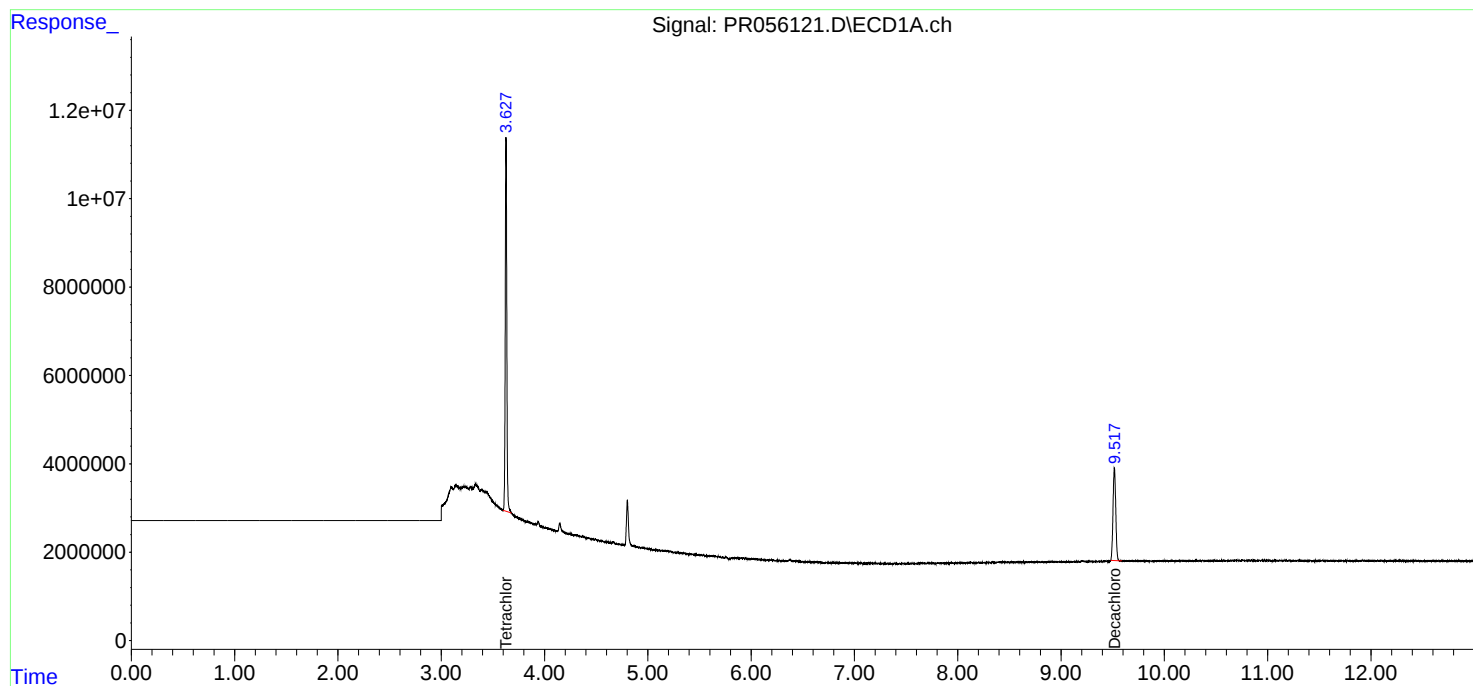

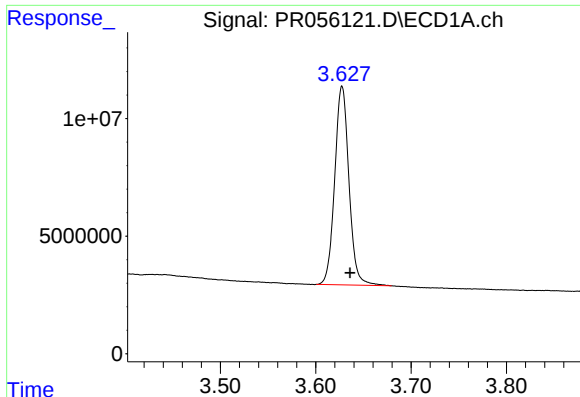

#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.008 min
Response: 87489120
Conc: 20.50 ng/ml

Instrument :

ECD_R


ClientSampleId :

PB147204BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 08/25/2022
Supervised By :Ankita Jodhani 08/25/2022

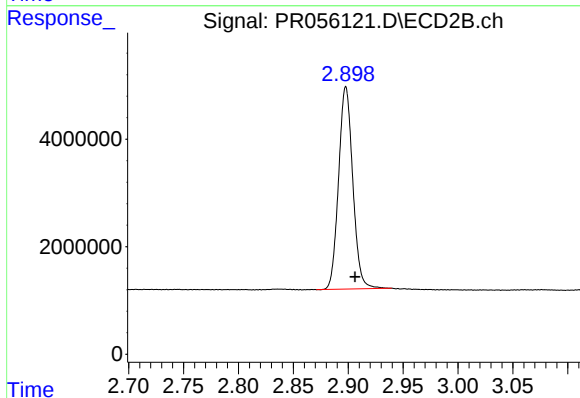


#1 Tetrachloro-m-xylene

R.T.: 2.898 min
Delta R.T.: -0.008 min
Response: 33828910
Conc: 16.85 ng/ml

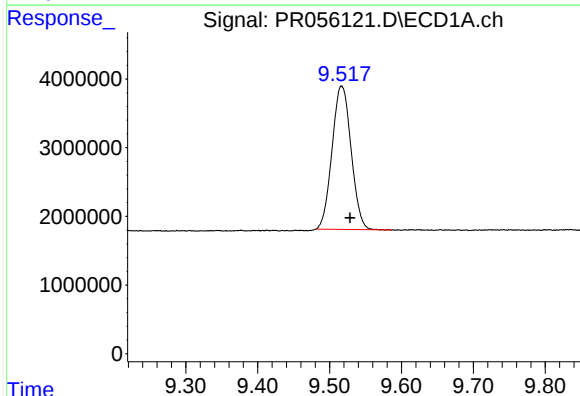

#2 Decachlorobiphenyl

R.T.: 9.517 min
Delta R.T.: -0.011 min
Response: 38386512
Conc: 21.59 ng/ml

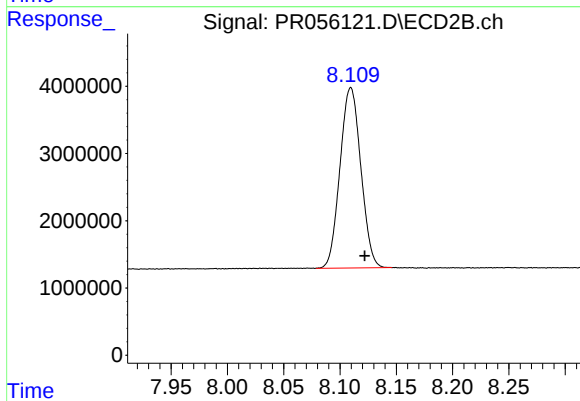

#2 Decachlorobiphenyl

R.T.: 8.109 min
Delta R.T.: -0.013 min
Response: 34585648
Conc: 19.01 ng/ml m