

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082422\
 Data File : PR056128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2022 14:49
 Operator : AJ\MA
 Sample : N4279-02RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TT-050-IDWGW-20220819RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/25/2022
 Supervised By :Ankita Jodhani 08/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 15:52:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 12:39:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.627	2.898	61688810	25220472	14.457	12.561
2) SA Decachlor...	9.517	8.110	10702724	10515668	6.019	5.781m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR082422\
Data File : PR056128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2022 14:49
Operator : AJ\MA
Sample : N4279-02RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
TT-050-IDWGW-20220819RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2022
Supervised By :Ankita Jodhani 08/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 15:52:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR080522.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 12:39:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

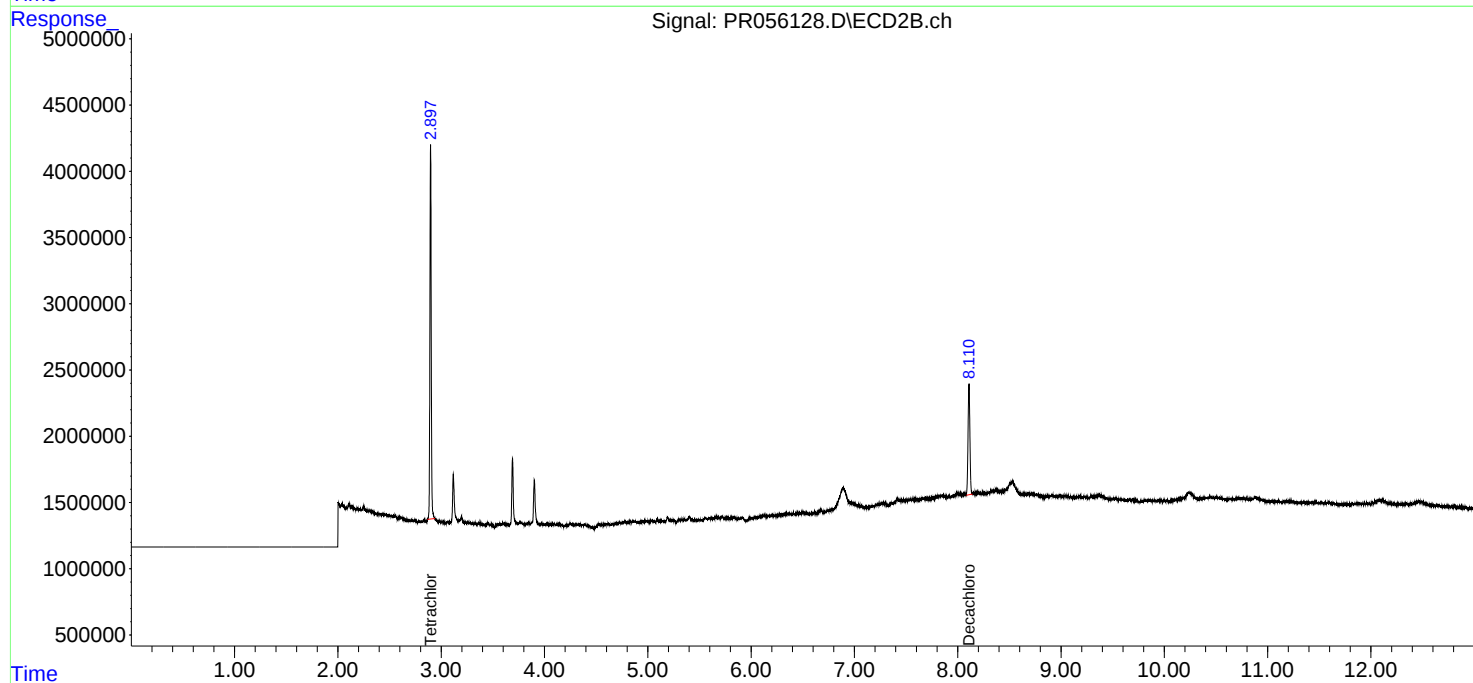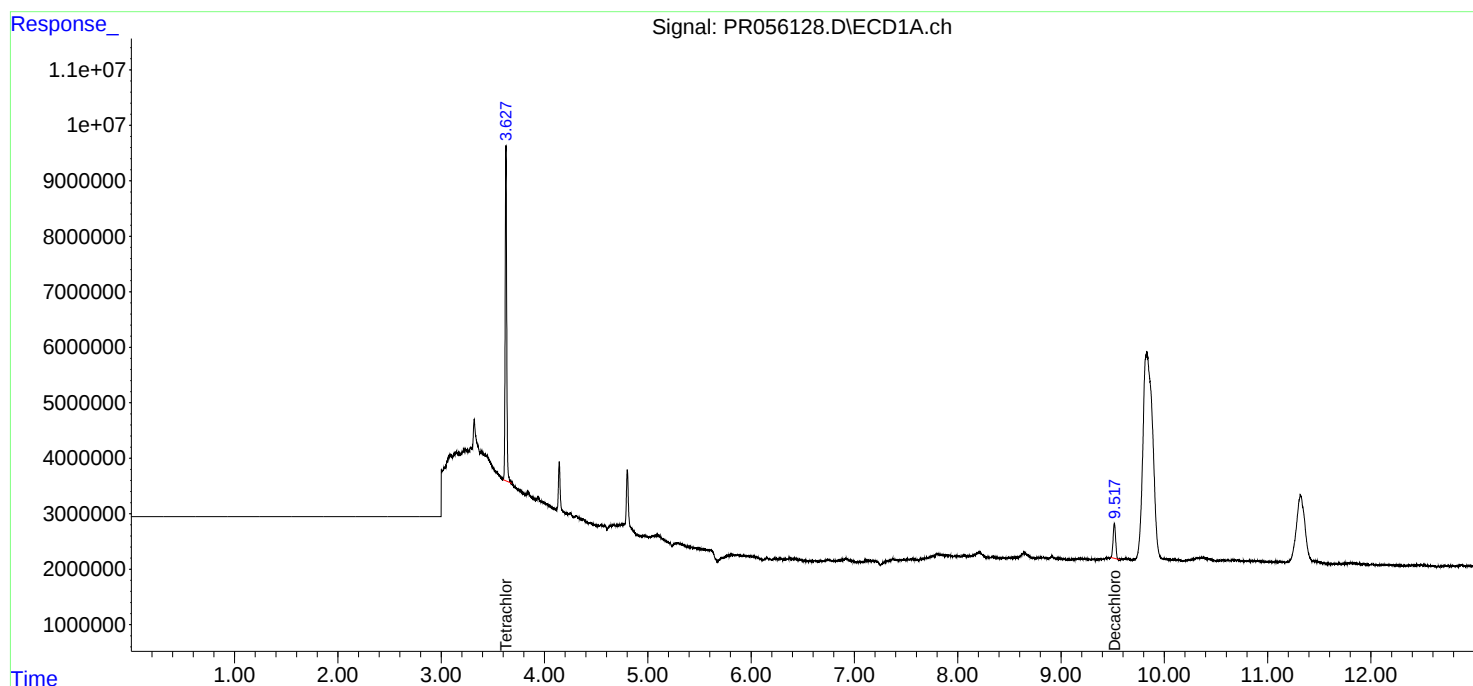

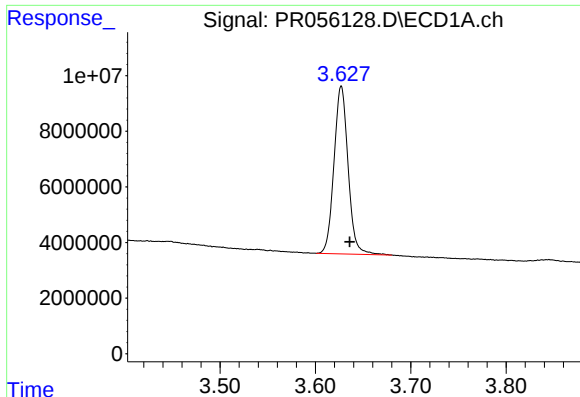


#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: -0.009 min
Response: 61688810
Conc: 14.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
TT-050-IDWGW-20220819RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2022
Supervised By :Ankita Jodhani 08/25/2022

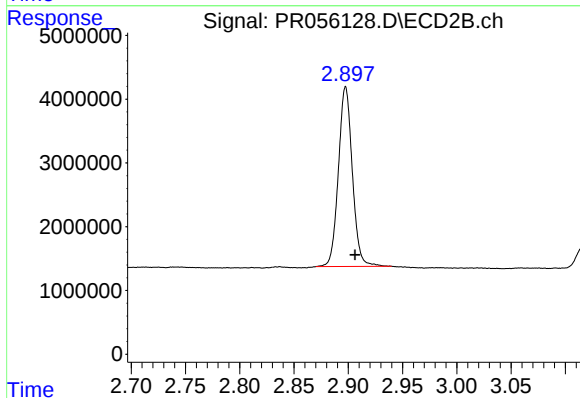


#1 Tetrachloro-m-xylene

R.T.: 2.898 min
Delta R.T.: -0.009 min
Response: 25220472
Conc: 12.56 ng/ml

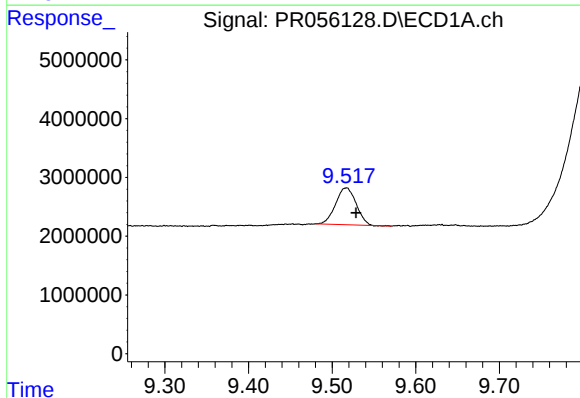

#2 Decachlorobiphenyl

R.T.: 9.517 min
Delta R.T.: -0.012 min
Response: 10702724
Conc: 6.02 ng/ml

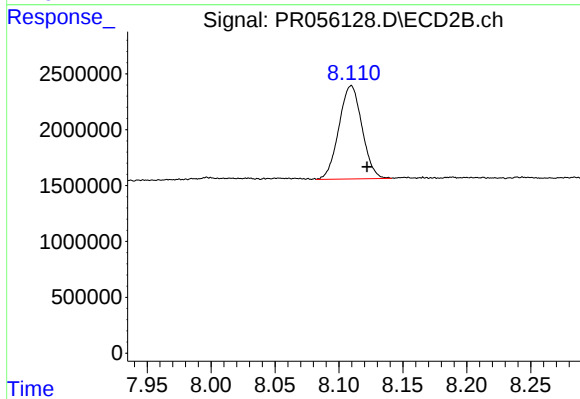

#2 Decachlorobiphenyl

R.T.: 8.110 min
Delta R.T.: -0.012 min
Response: 10515668
Conc: 5.78 ng/ml m