

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR083018\
 Data File : PR031681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 23:50
 Operator : SM\SJ
 Sample : J4700-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 082818-SIDI-F-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 08:37:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR083018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 31 07:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.660	240.8E6	487.4E6	17.664	19.603
2) SA Decachlor...	10.276	8.523	391.8E6	295.4E6	15.776	18.521

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR083018\
Data File : PR031681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 23:50
Operator : SM\SJ
Sample : J4700-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
082818-SIDI-F-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 08:37:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR083018.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 31 07:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

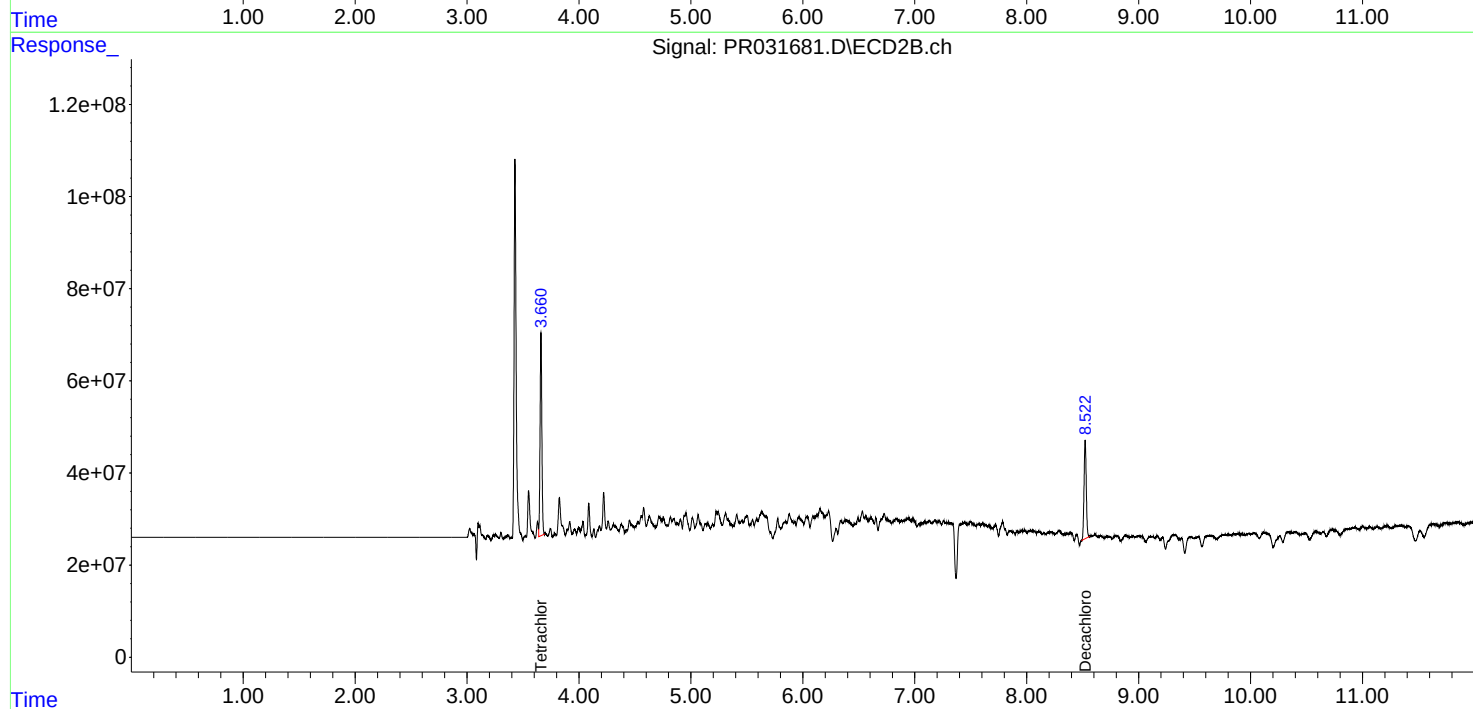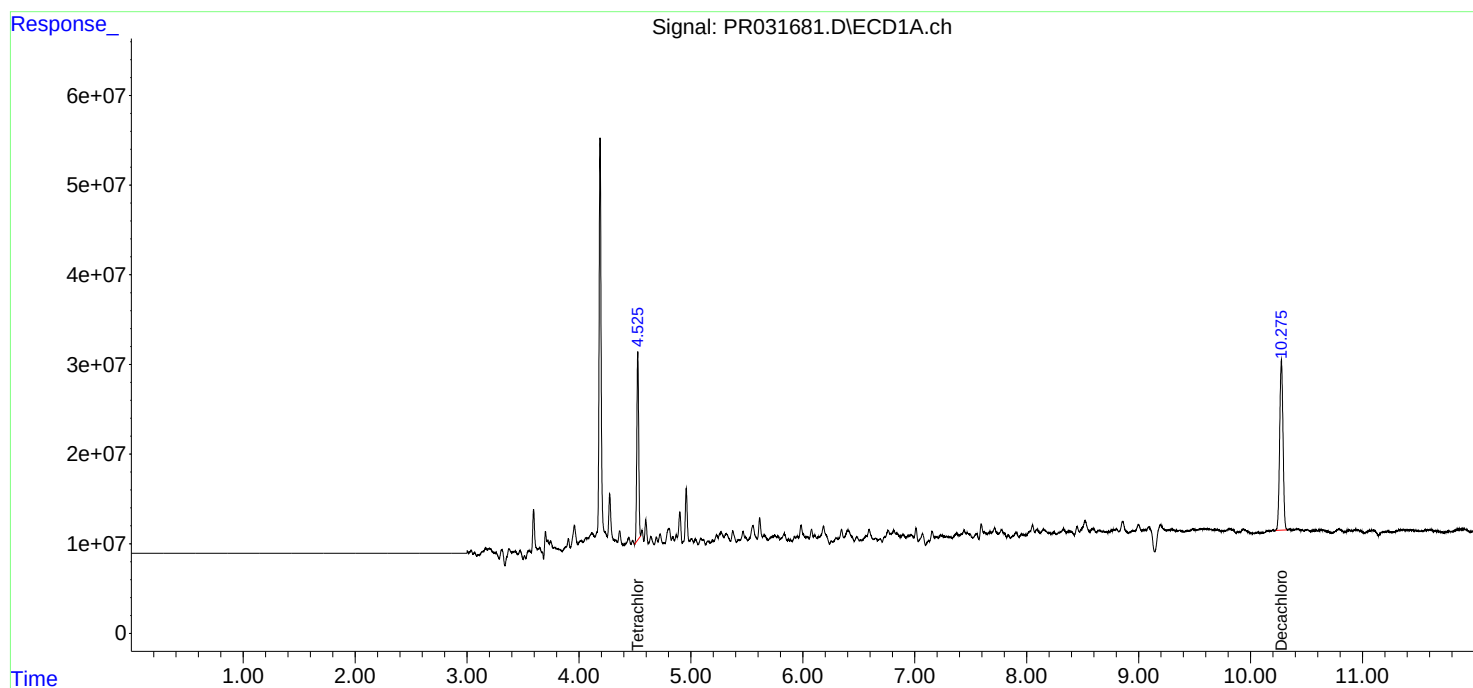


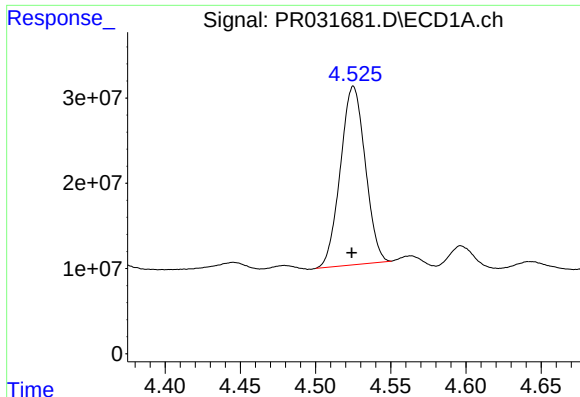

#1 Tetrachloro-m-xylene


R.T.: 4.525 min
Delta R.T.: 0.001 min
Response: 240773825
Conc: 17.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
082818-SIDI-F-D-S

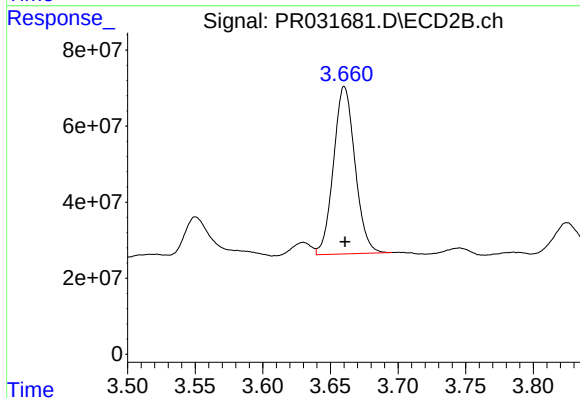


#1 Tetrachloro-m-xylene

R.T.: 3.660 min
Delta R.T.: 0.000 min
Response: 487354389
Conc: 19.60 ng/ml

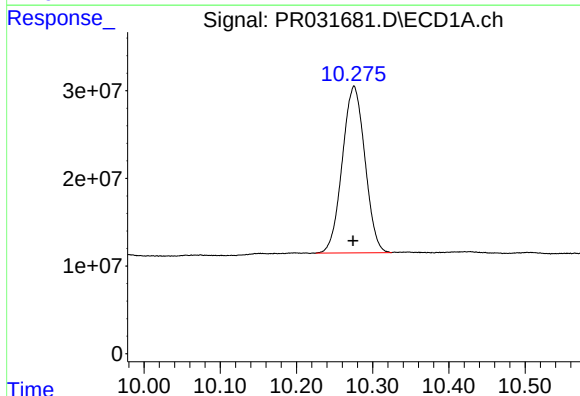

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: 0.001 min
Response: 391788856
Conc: 15.78 ng/ml

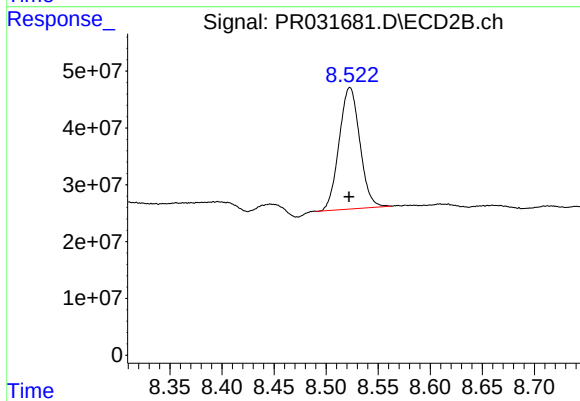

#2 Decachlorobiphenyl

R.T.: 8.523 min
Delta R.T.: 0.000 min
Response: 295374550
Conc: 18.52 ng/ml