

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR083021\
 Data File : PR051916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 03:59
 Operator : DD\AJ
 Sample : AIBLK86
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 05:30:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR083021CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 31 05:27:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	3.806	76956233	109.4E6	16.684	19.202
2)	SA Decachlor...	10.546	8.838	264.2E6	285.3E6	30.475	38.536 #
Target Compounds							
3)	L1 AR-1016-1	5.777	0.000	1095747	0	10.223	N.D. #
4)	L1 AR-1016-2	5.777f	0.000	1095747	0	5.907	N.D. #
9)	L2 AR-1221-2	0.000	4.106	0	1431230	N.D.	30.630 #
13)	L3 AR-1232-3	5.777f	0.000	1095747	0	16.569	N.D. #
16)	L4 AR-1242-1	5.777	0.000	1095747	0	16.412	N.D. #
17)	L4 AR-1242-2	5.777f	0.000	1095747	0	9.176	N.D. #
21)	L5 AR-1248-1	5.777	0.000	1095747	0	21.262	N.D. #
29)	L6 AR-1254-4	7.531	0.000	843729	0	1.865	N.D. #
45)	L9 AR-1268-5	0.000	8.576	0	1951709	N.D.	0.704 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR083021\
Data File : PR051916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 03:59
Operator : DD\AJ
Sample : AIBLK86
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 05:30:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR083021CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 31 05:27:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

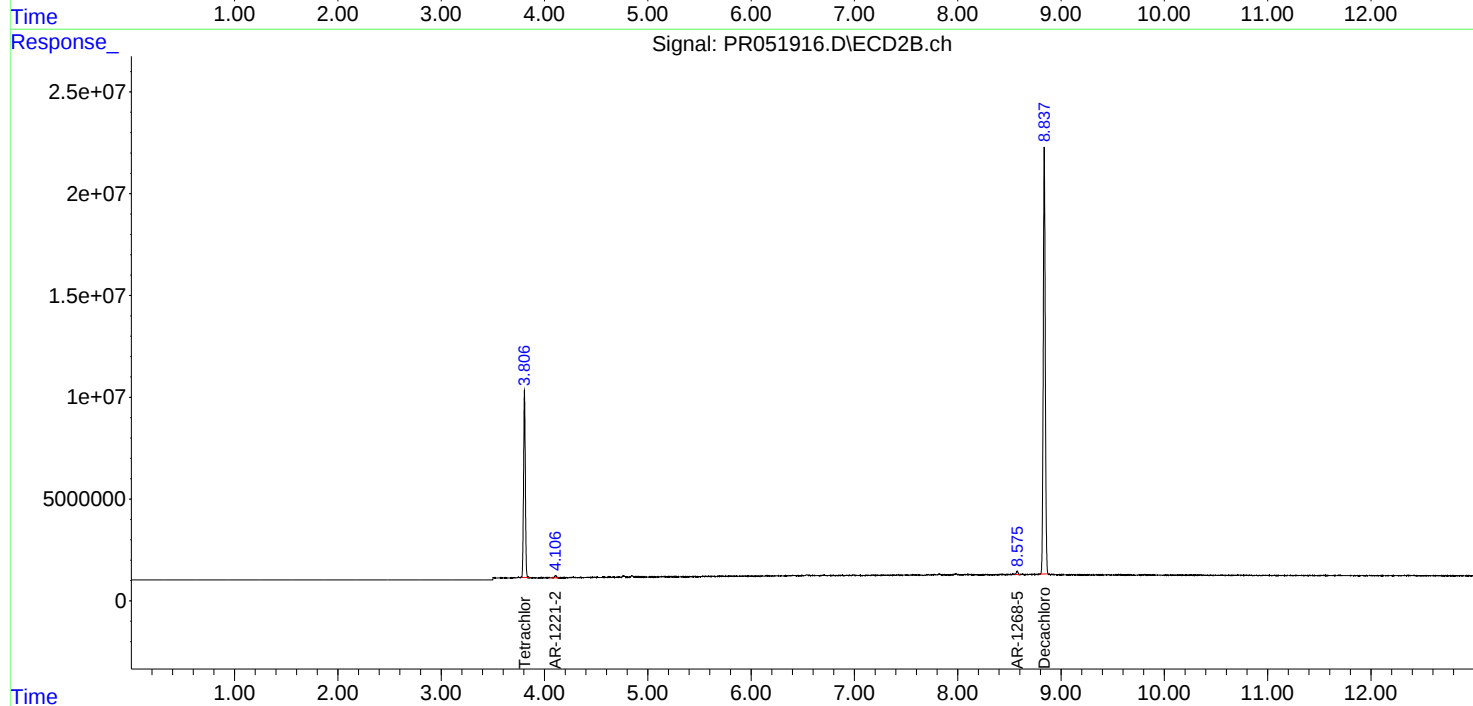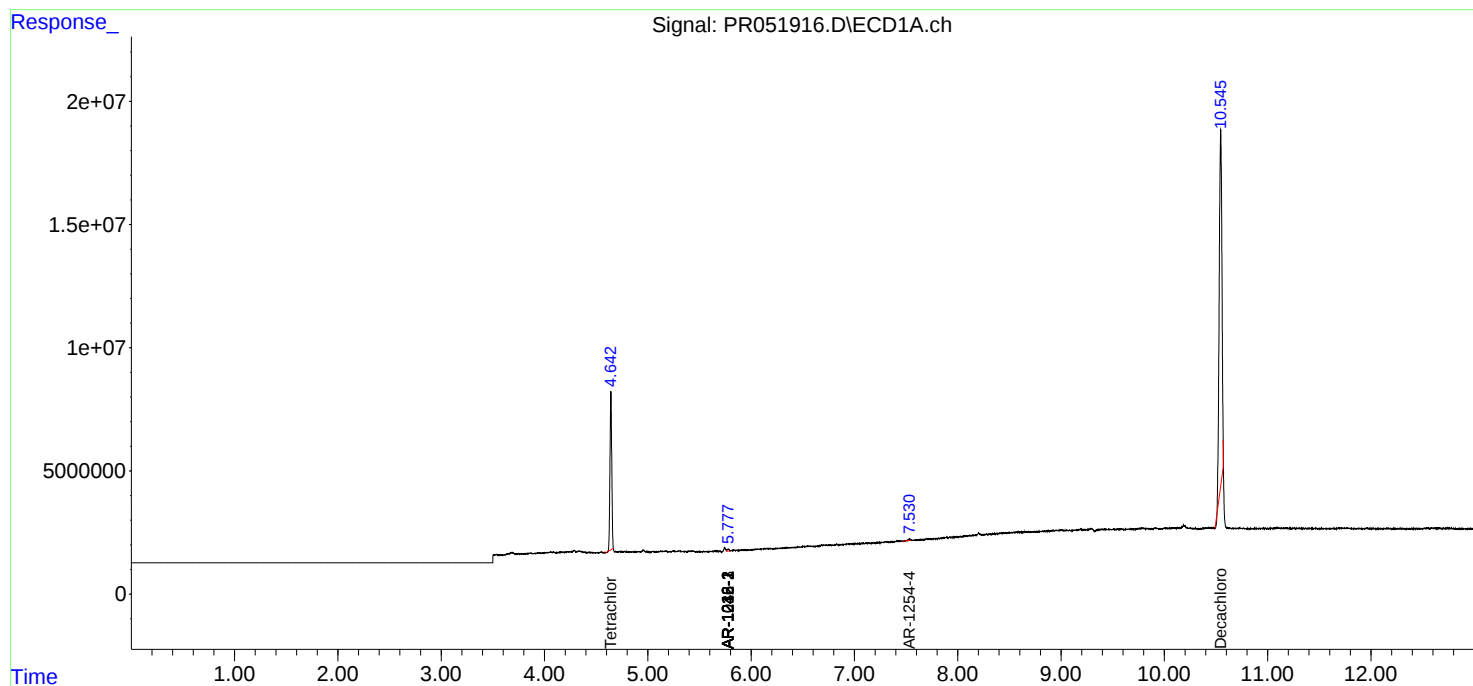


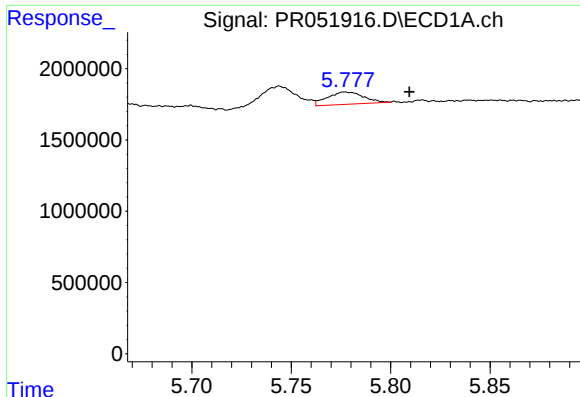

#3 AR-1016-1


R.T.: 5.777 min
Delta R.T.: -0.033 min
Response: 1095747
Conc: 10.22 ng/ml

Instrument :
ECD_R
ClientSampleId :

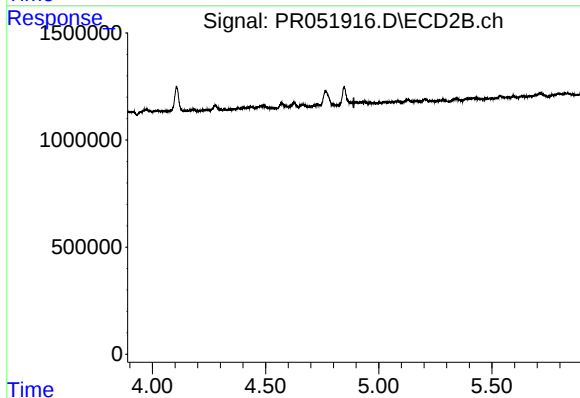


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.890 min
Response: 0
Conc: N.D.

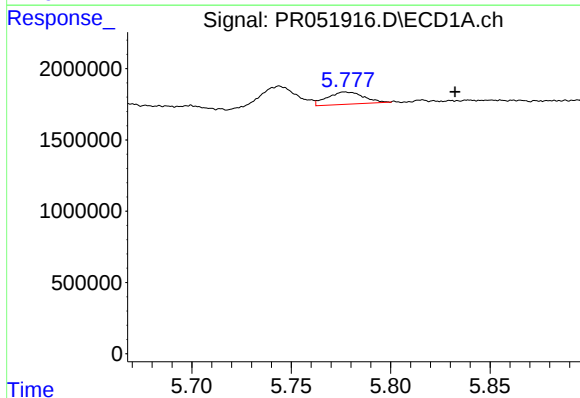


#4 AR-1016-2

R.T.: 5.777 min
Delta R.T.: -0.056 min
Response: 1095747
Conc: 5.91 ng/ml

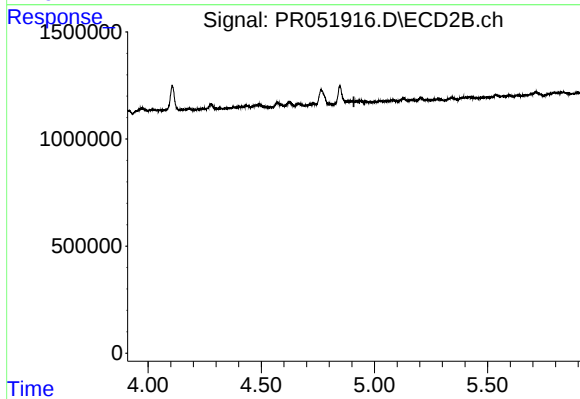

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

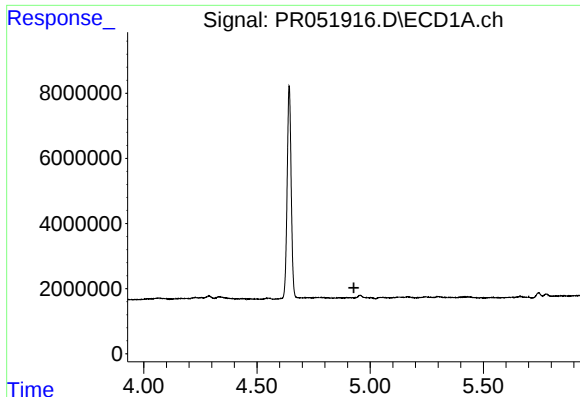

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.928 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

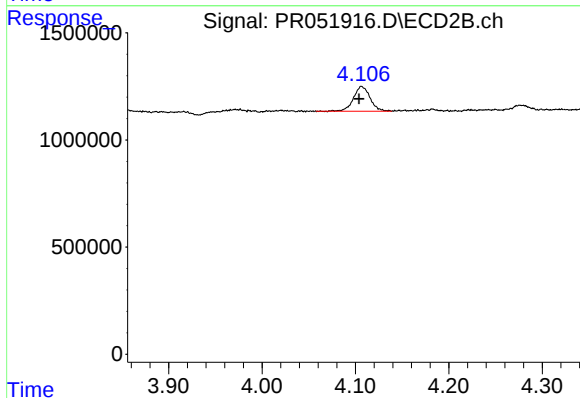


#9 AR-1221-2

R.T.: 4.106 min
Delta R.T.: 0.003 min
Response: 1431230
Conc: 30.63 ng/ml

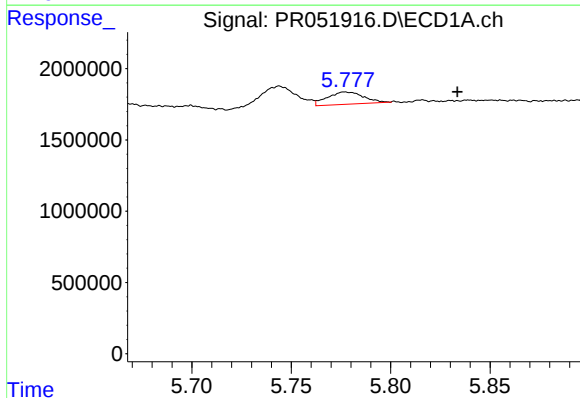


#13 AR-1232-3

R.T.: 5.777 min
Delta R.T.: -0.057 min
Response: 1095747
Conc: 16.57 ng/ml

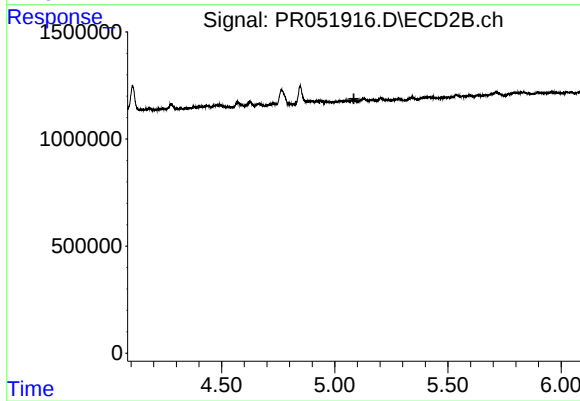

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.085 min
Response: 0
Conc: N.D.

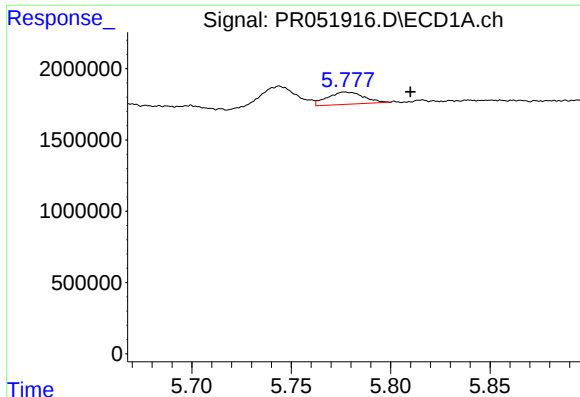

#16 AR-1242-1


R.T.: 5.777 min
Delta R.T.: -0.033 min
Response: 1095747
Conc: 16.41 ng/ml

Instrument :
ECD_R
ClientSampleId :

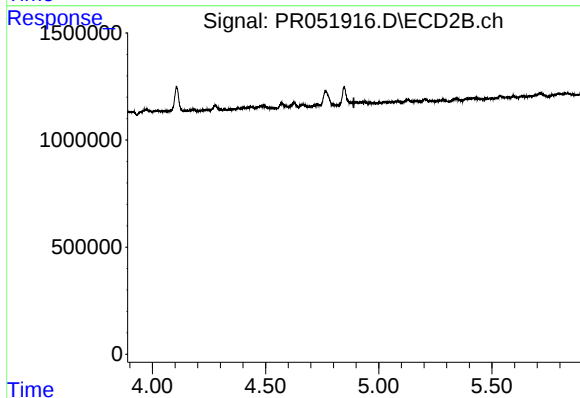


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.890 min
Response: 0
Conc: N.D.

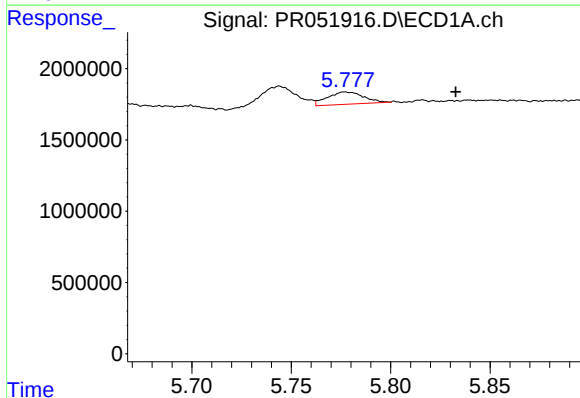


#17 AR-1242-2

R.T.: 5.777 min
Delta R.T.: -0.056 min
Response: 1095747
Conc: 9.18 ng/ml

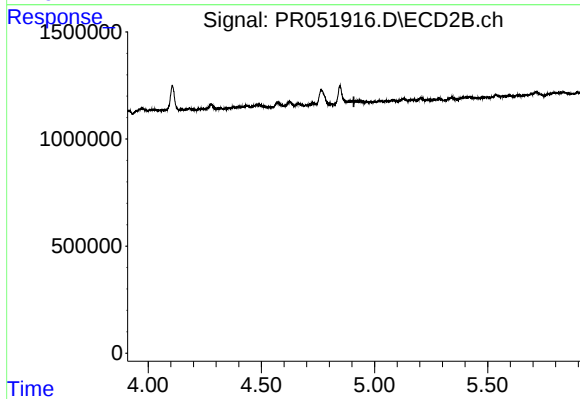

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

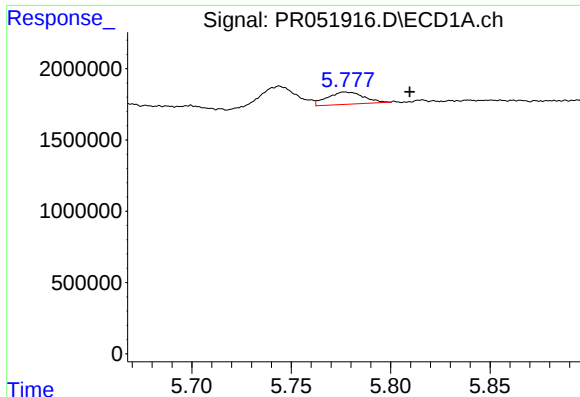

#21 AR-1248-1


R.T.: 5.777 min
Delta R.T.: -0.033 min
Response: 1095747
Conc: 21.26 ng/ml

Instrument :
ECD_R
ClientSampleId :

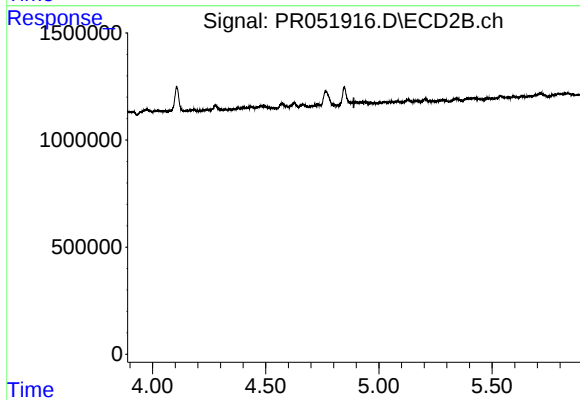


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.890 min
Response: 0
Conc: N.D.

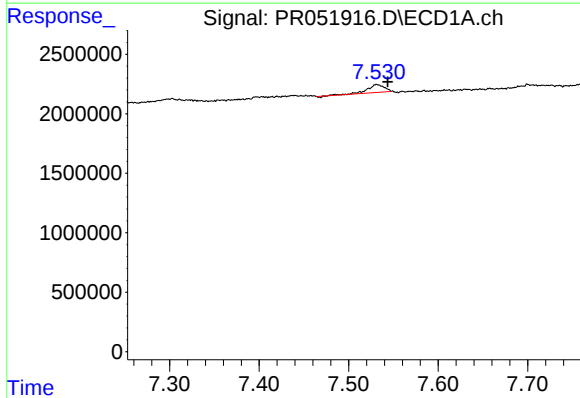


#29 AR-1254-4

R.T.: 7.531 min
Delta R.T.: -0.012 min
Response: 843729
Conc: 1.87 ng/ml

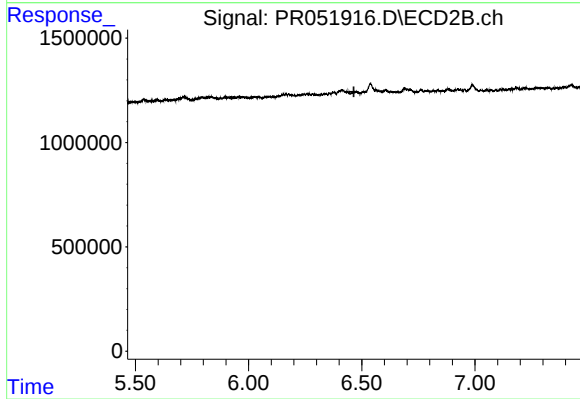

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.465 min
Response: 0
Conc: N.D.

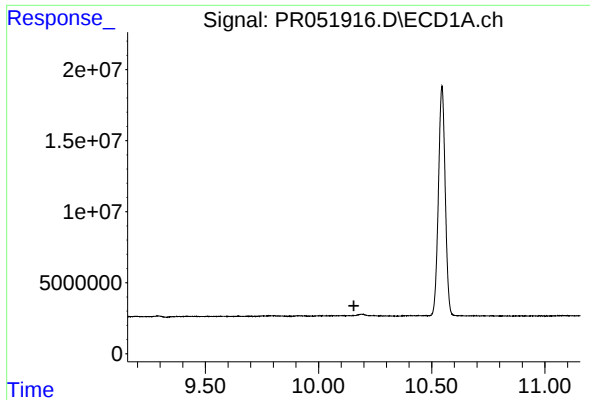

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.156 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

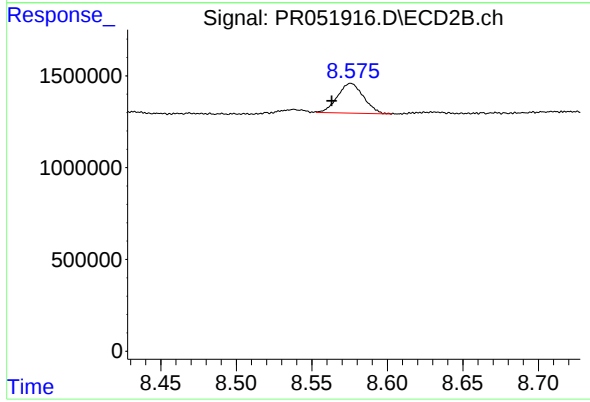

#45 AR-1268-5

R.T.: 8.576 min
Delta R.T.: 0.013 min
Response: 1951709
Conc: 0.70 ng/ml