

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR083118\
 Data File : PR031710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2018 17:53
 Operator : SM\SJ
 Sample : J4735-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 KG-BASELINE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 03:33:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR083018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 31 07:21:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.533	3.672	200.4E6	377.0E6	14.702	15.164
2) SA Decachlor...	10.275	8.522	327.5E6	239.6E6	13.185	15.027

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR083118\
Data File : PR031710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2018 17:53
Operator : SM\SJ
Sample : J4735-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
KG-BASELINE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 03:33:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR083018.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 31 07:21:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

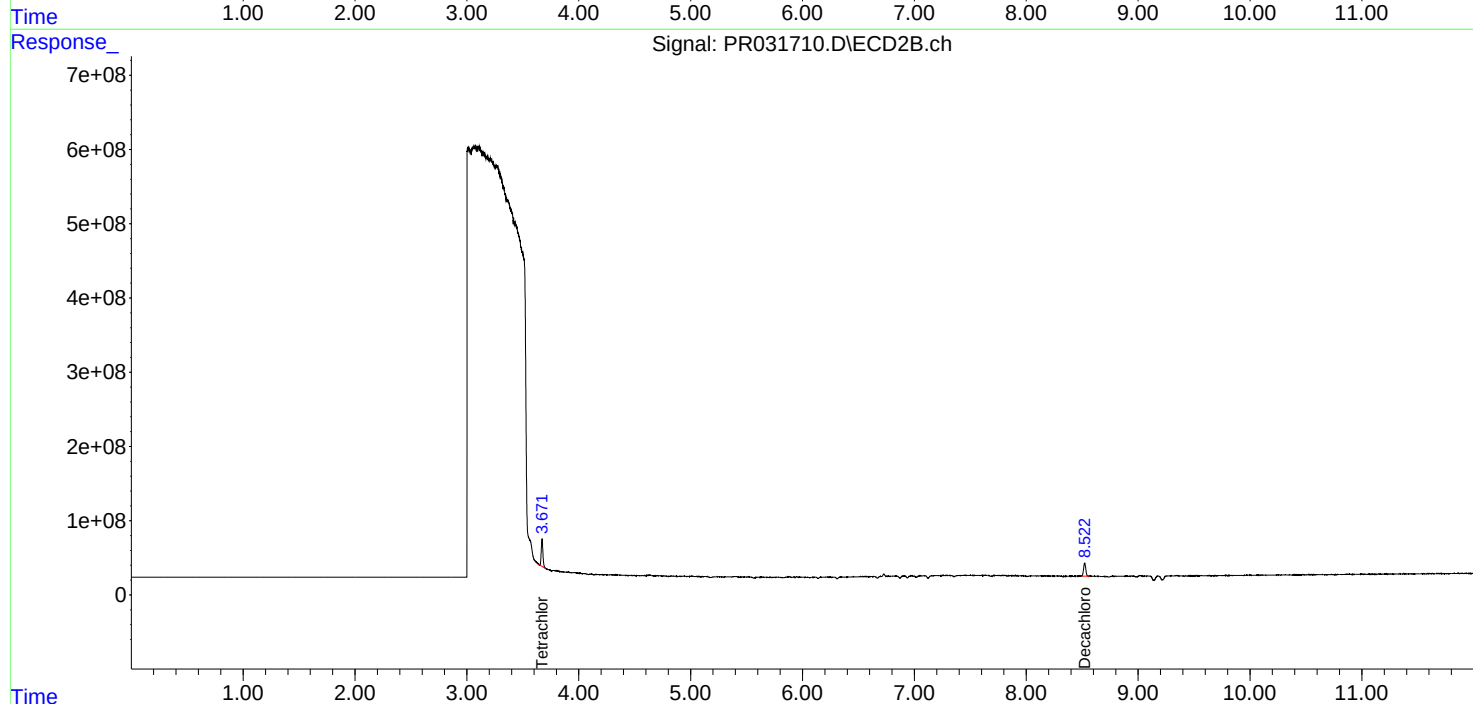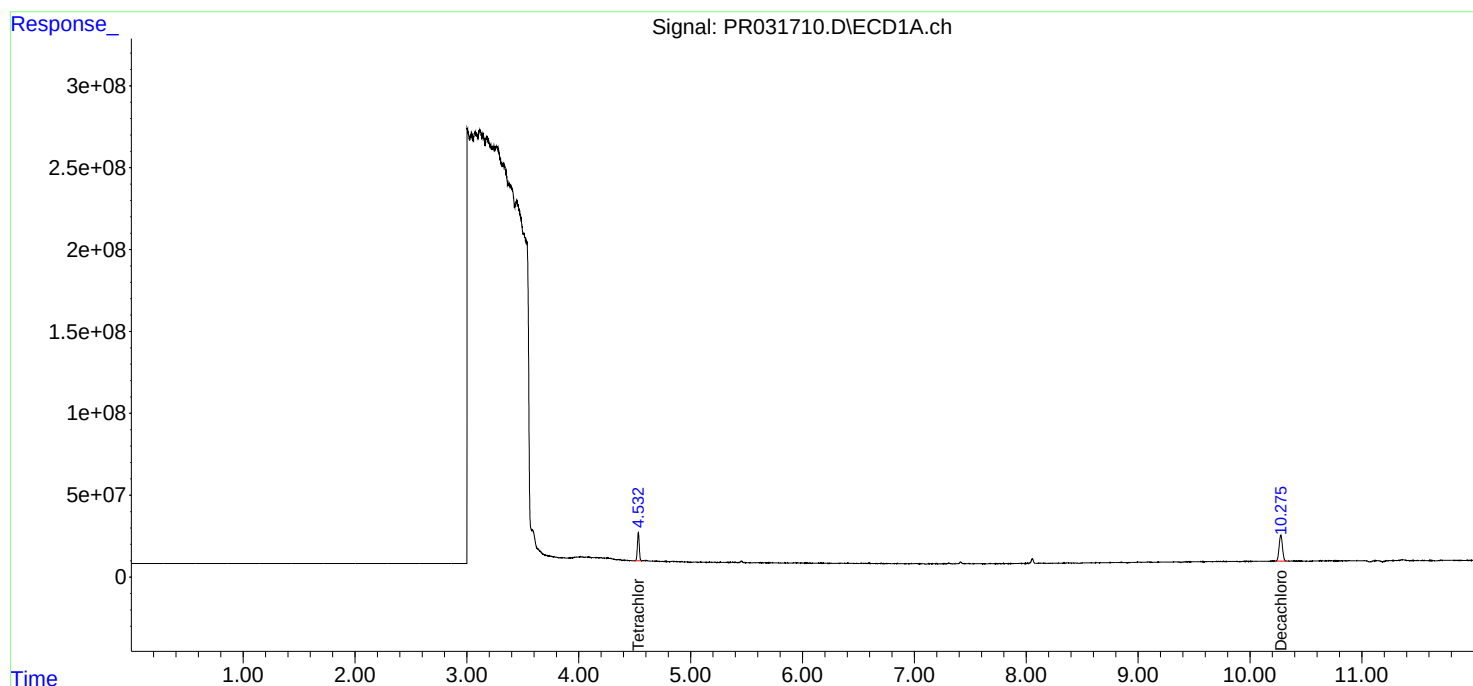


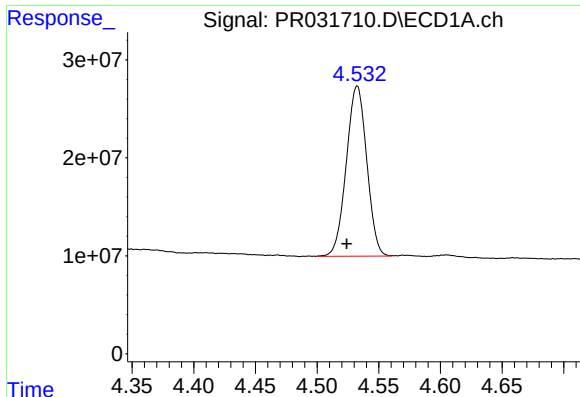

#1 Tetrachloro-m-xylene


R.T.: 4.533 min
Delta R.T.: 0.009 min
Response: 200406103
Conc: 14.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
KG-BASELINE-WATER

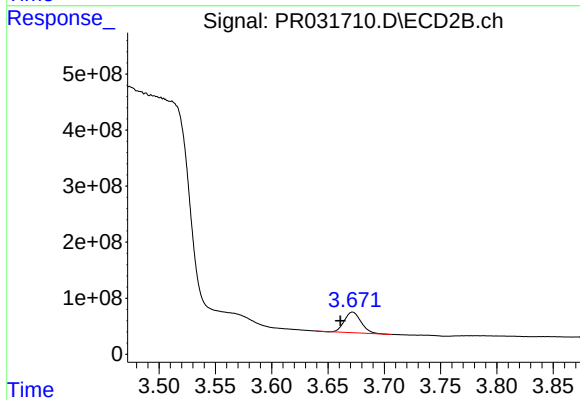


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.011 min
Response: 376994775
Conc: 15.16 ng/ml

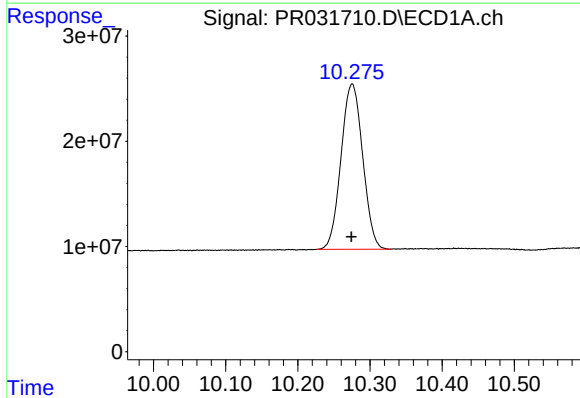

#2 Decachlorobiphenyl

R.T.: 10.275 min
Delta R.T.: 0.001 min
Response: 327457355
Conc: 13.19 ng/ml

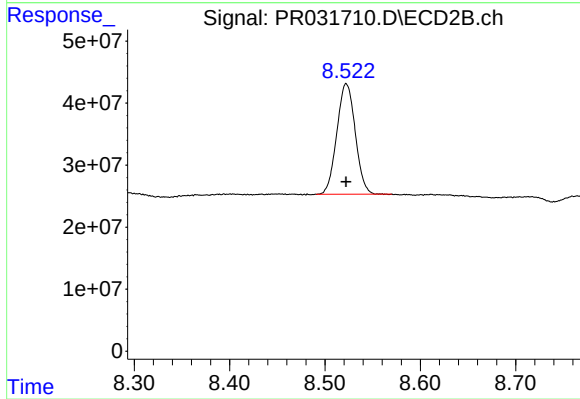

#2 Decachlorobiphenyl

R.T.: 8.522 min
Delta R.T.: 0.000 min
Response: 239643091
Conc: 15.03 ng/ml