

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090322\
 Data File : PS020445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 22:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 01:25:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 03 01:09:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.177	6.757	1324.9E6	432.6E6	375.903	402.566
Target Compounds							
1) T	Dalapon	3.043f	0.000	865812	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.440	0.000	4545395	0	<MDL	N.D. #
7) T	MCPA	7.709	7.151f	10200623	55415399	<MDL	10.218 #
8) T	DICHLORPROP	8.083	7.606f	3002007	2044906	<MDL	1.636 #
9) T	2,4-D	8.360f	0.000	130.2E6	0	27.756	N.D. #
10) T	Pentachlo...	8.634f	0.000	473128	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.088f	0.000	8341434	0	<MDL	N.D. #
12) T	2,4,5-T	9.462	0.000	1936308	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.568f	0	5521157	N.D.	6.098
14) T	DINOSEB	11.132	9.838	14596280	1263764	<MDL	<MDL #
15) T	Picloram	10.947	10.838	22331126	20784977	<MDL	2.024 #
16) T	DCPA	11.406	10.745	10491083	9923270	<MDL	1.114 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS090322\
Data File : PS020445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 22:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 01:25:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090222.M
Quant Title : 8080.M
QLast Update : Sat Sep 03 01:09:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

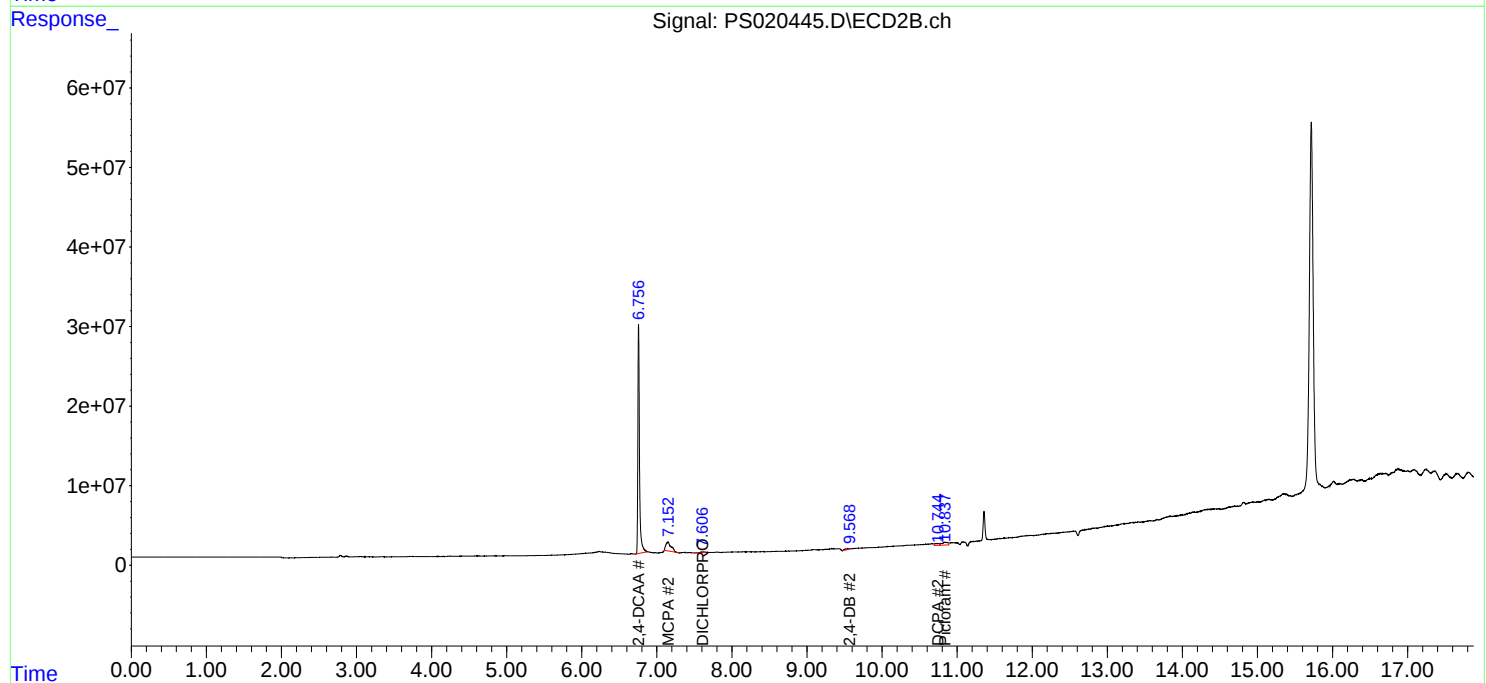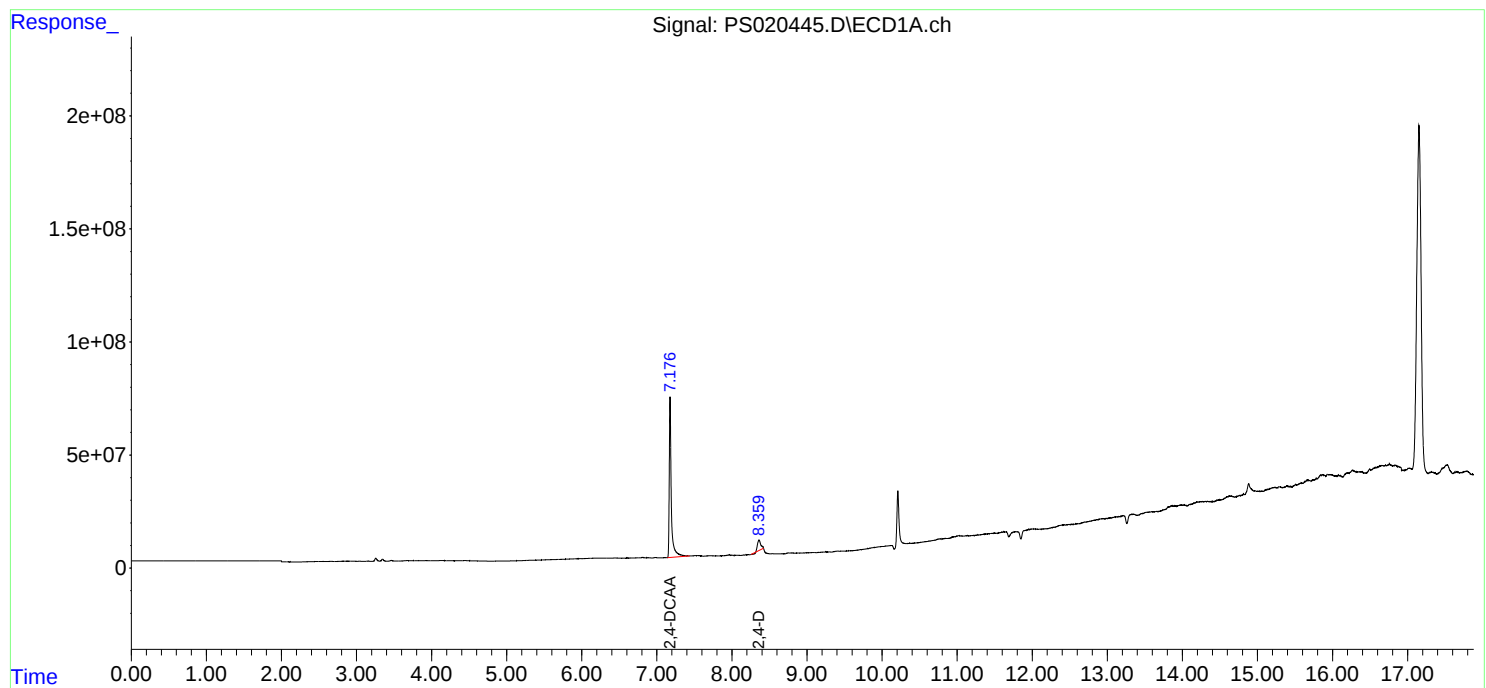


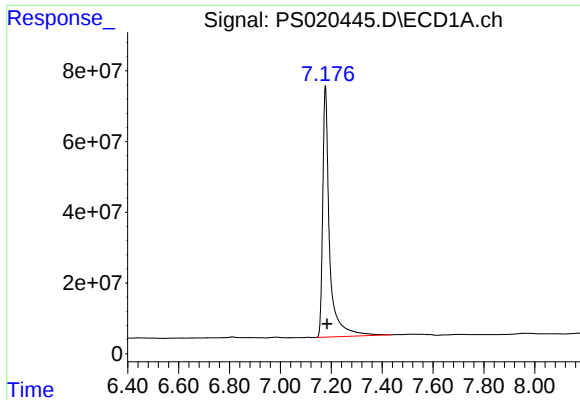

#4 2,4-DCAA


R.T.: 7.177 min
Delta R.T.: -0.006 min
Response: 1324931486
Conc: 375.90 ng/ml

Instrument :
ECD_R
ClientSampleId :

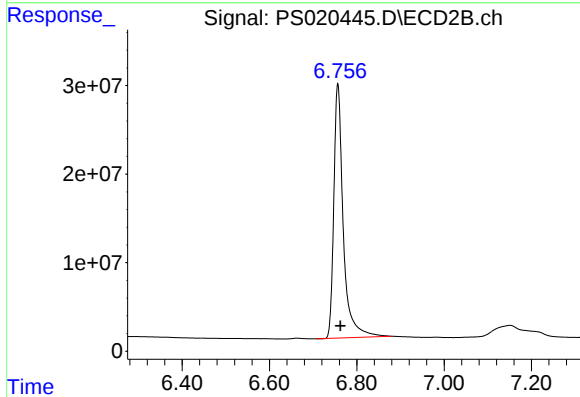


#4 2,4-DCAA

R.T.: 6.757 min
Delta R.T.: -0.006 min
Response: 432565666
Conc: 402.57 ng/ml

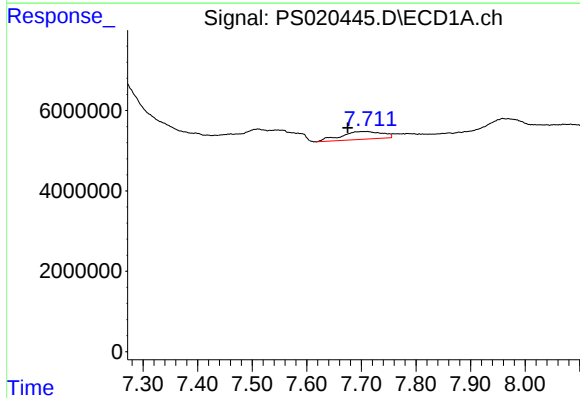


#7 MCPA

R.T.: 7.709 min
Delta R.T.: 0.034 min
Response: 10200623
Conc: N.D.

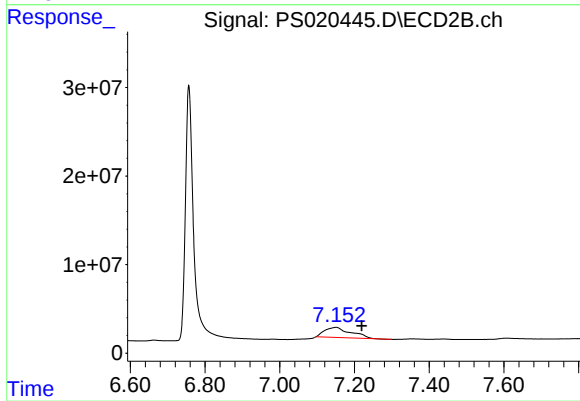

#7 MCPA


R.T.: 7.151 min
Delta R.T.: -0.068 min
Response: 55415399
Conc: 10.22 ug/ml

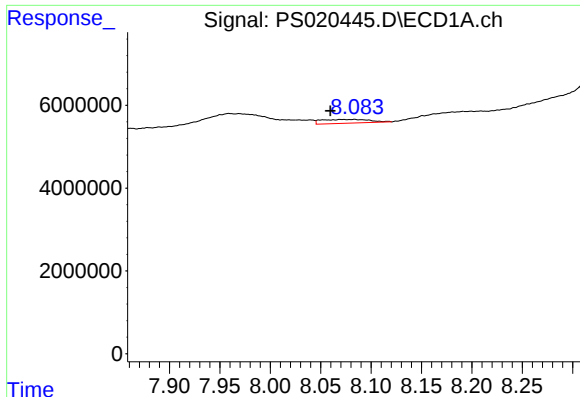

#8 DICHLORPROP


R.T.: 8.083 min
Delta R.T.: 0.023 min
Response: 3002007
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

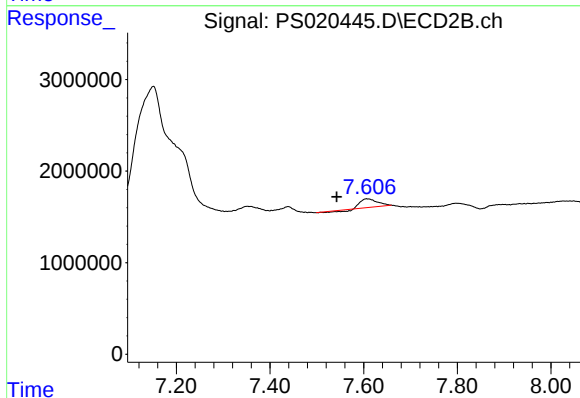


#8 DICHLORPROP

R.T.: 7.606 min
Delta R.T.: 0.064 min
Response: 2044906
Conc: 1.64 ng/ml

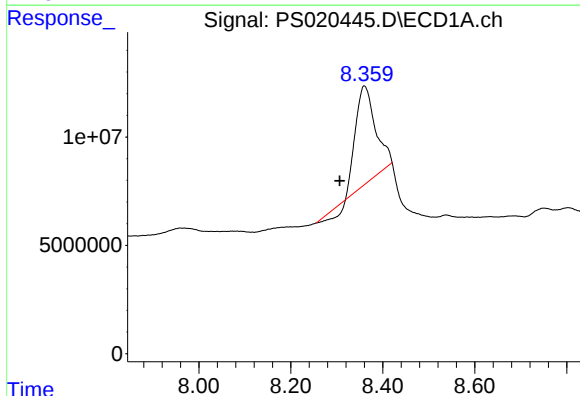


#9 2,4-D

R.T.: 8.360 min
Delta R.T.: 0.054 min
Response: 130216553
Conc: 27.76 ng/ml

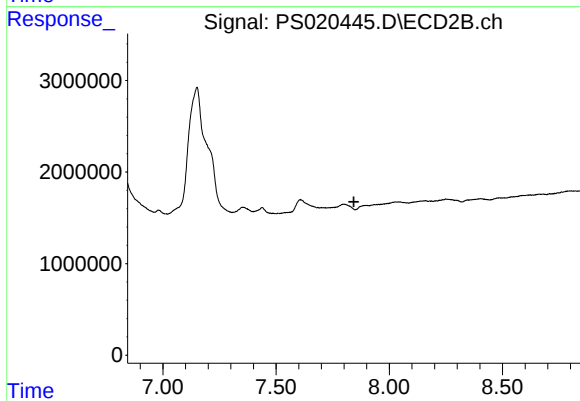

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.844 min
Response: 0
Conc: N.D.

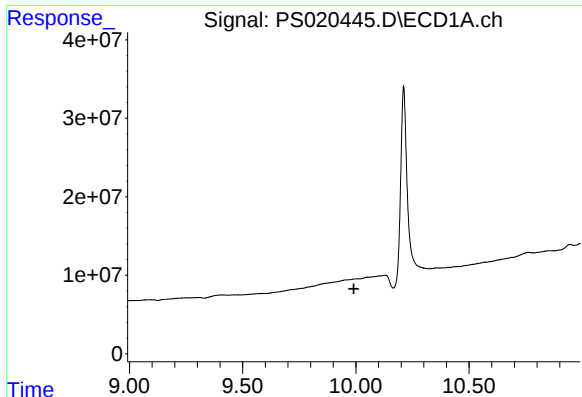

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.991 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

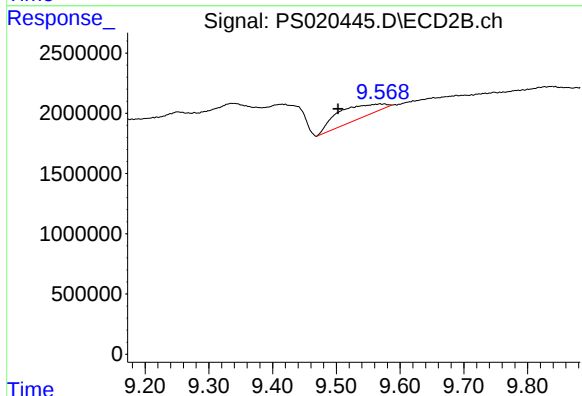


#13 2,4-DB

R.T.: 9.568 min
Delta R.T.: 0.066 min
Response: 5521157
Conc: 6.10 ng/ml

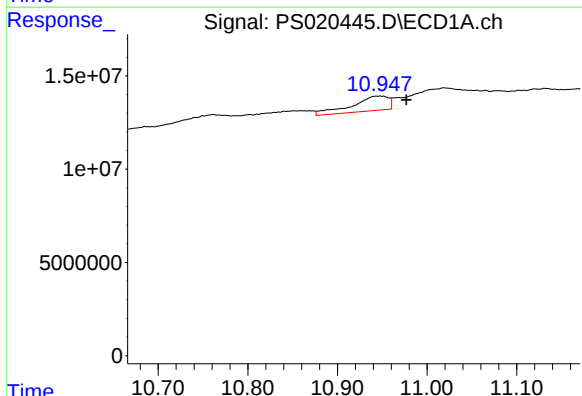


#15 Picloram

R.T.: 10.947 min
Delta R.T.: -0.030 min
Response: 22331126
Conc: N.D.

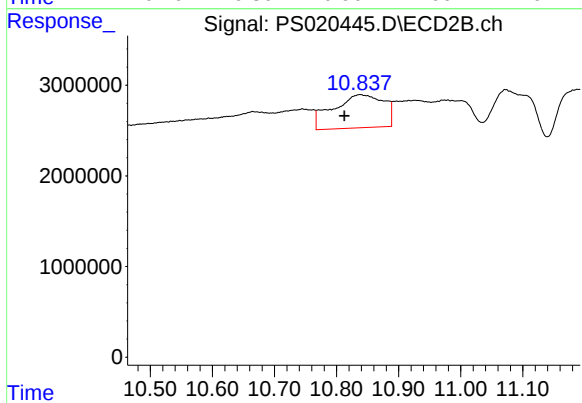

#15 Picloram


R.T.: 10.838 min
Delta R.T.: 0.026 min
Response: 20784977
Conc: 2.02 ng/ml

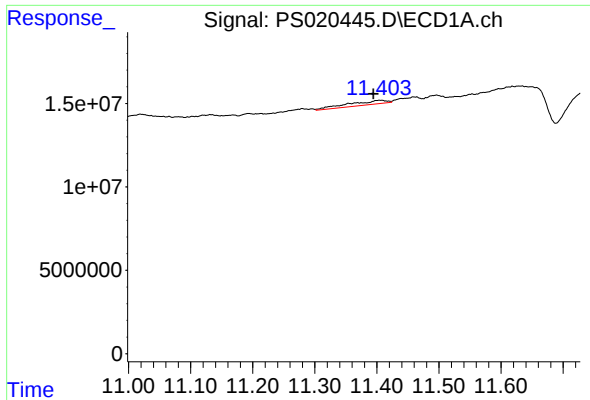

#16 DCPA

R.T.: 11.406 min
Delta R.T.: 0.011 min
Response: 10491083
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

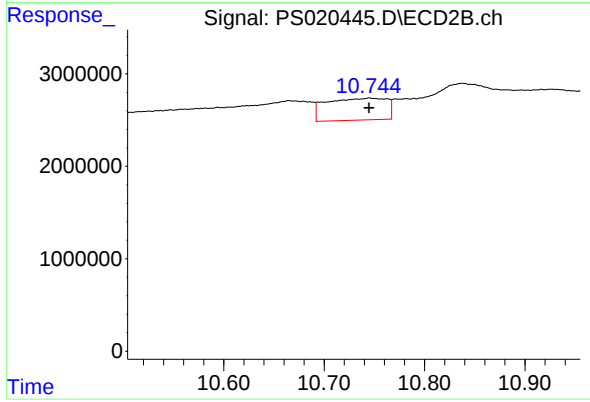

#16 DCPA

R.T.: 10.745 min
Delta R.T.: 0.000 min
Response: 9923270
Conc: 1.11 ng/ml