

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR090822\
 Data File : PR056418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2022 03:19
 Operator : AJ\MA
 Sample : N4502-02RE
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 DEACON-WATER-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/08/2022
 Supervised By :Ankita Jodhani 09/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 03:52:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.623	2.895	70512664	28943786	14.676m	16.513
2) SA Decachlor...	9.509	8.101	15545516	12804042	7.834	7.696

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR090822\
Data File : PR056418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2022 03:19
Operator : AJ\MA
Sample : N4502-02RE
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
DEACON-WATER-COMPRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2022
Supervised By :Ankita Jodhani 09/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 03:52:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

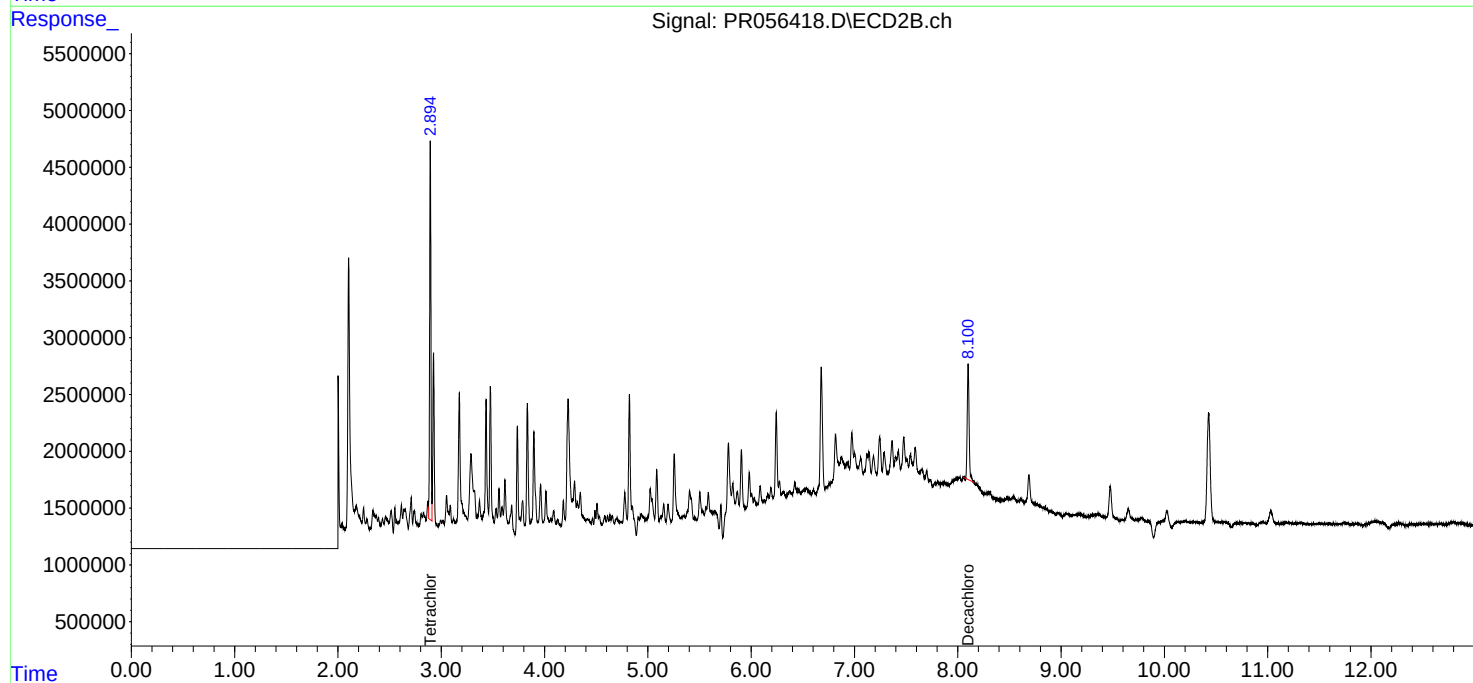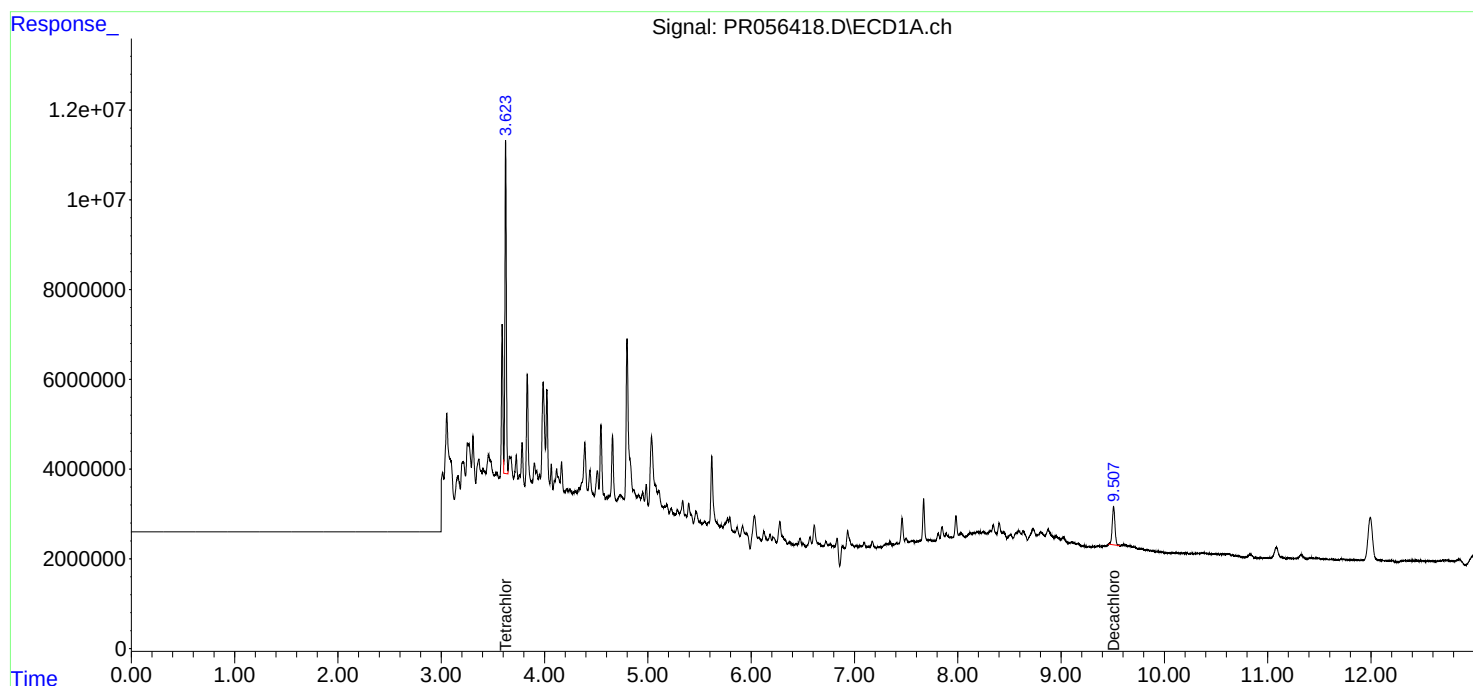

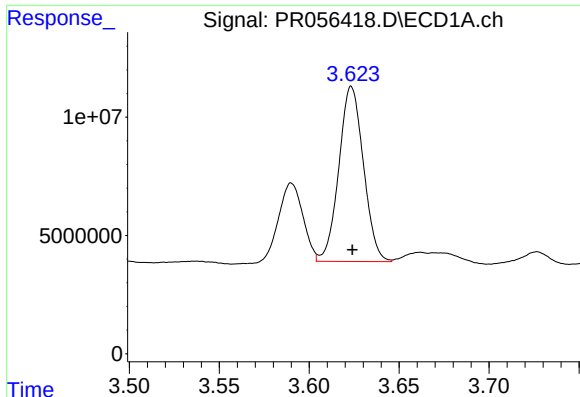


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.001 min
Response: 70512664
Conc: 14.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
DEACON-WATER-COMPRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/08/2022
Supervised By :Ankita Jodhani 09/08/2022

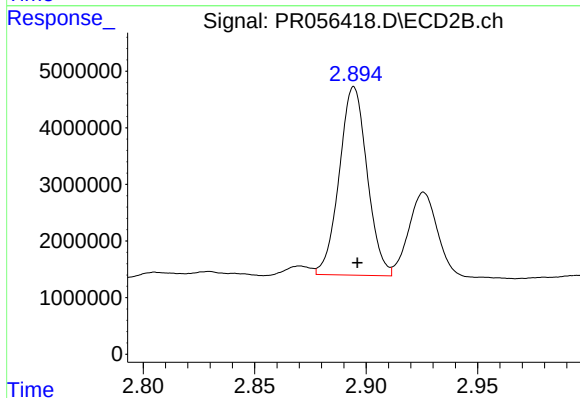


#1 Tetrachloro-m-xylene

R.T.: 2.895 min
Delta R.T.: -0.002 min
Response: 28943786
Conc: 16.51 ng/ml

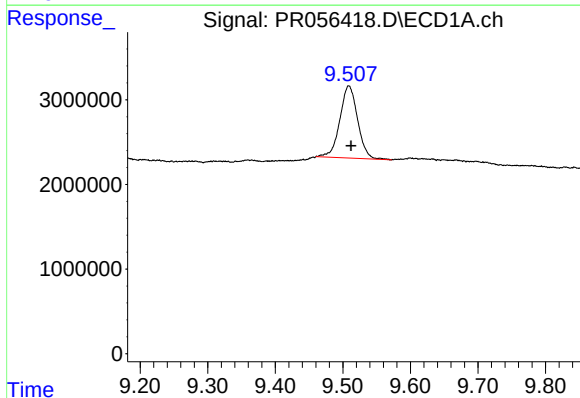

#2 Decachlorobiphenyl

R.T.: 9.509 min
Delta R.T.: -0.003 min
Response: 15545516
Conc: 7.83 ng/ml

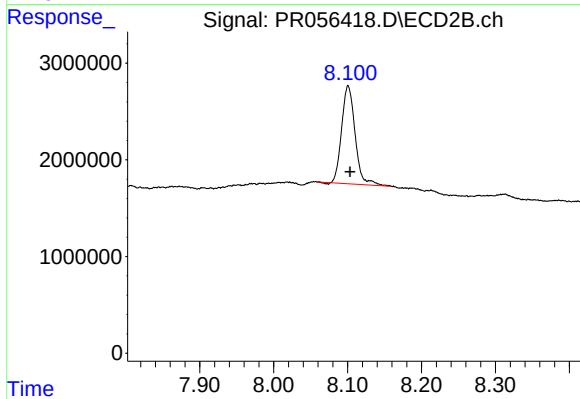

#2 Decachlorobiphenyl

R.T.: 8.101 min
Delta R.T.: -0.003 min
Response: 12804042
Conc: 7.70 ng/ml