

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091019\
 Data File : PR040911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 21:39
 Operator : SM\AJ
 Sample : K4731-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 C0AE6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 03:48:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:01:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.725	3.994	42766878	180.5E6	13.916	13.555
2) SA Decachlor...	10.643	9.120	84415087	258.5E6	30.331	26.444
Target Compounds						
9) L2 AR-1221-2	0.000	4.300	0	1483330	N.D.	19.316 #
20) L4 AR-1242-5	0.000	5.910	0	1482893	N.D.	6.466 #
25) L5 AR-1248-5	0.000	5.910f	0	1482893	N.D.	4.692 #
26) L6 AR-1254-1	0.000	5.910	0	1482893	N.D.	3.097 #
28) L6 AR-1254-3	0.000	6.457	0	11111793	N.D.	14.771 #
29) L6 AR-1254-4	0.000	6.683	0	3364980	N.D.	6.435 #
31) L7 AR-1260-1	0.000	6.594	0	6972792	N.D.	13.687 #
32) L7 AR-1260-2	0.000	6.780	0	3122566	N.D.	4.912 #
45) L9 AR-1268-5	0.000	8.835	0	2406529	N.D.	0.652 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091019\
Data File : PR040911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 21:39
Operator : SM\AJ
Sample : K4731-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
C0AE6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:48:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:01:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

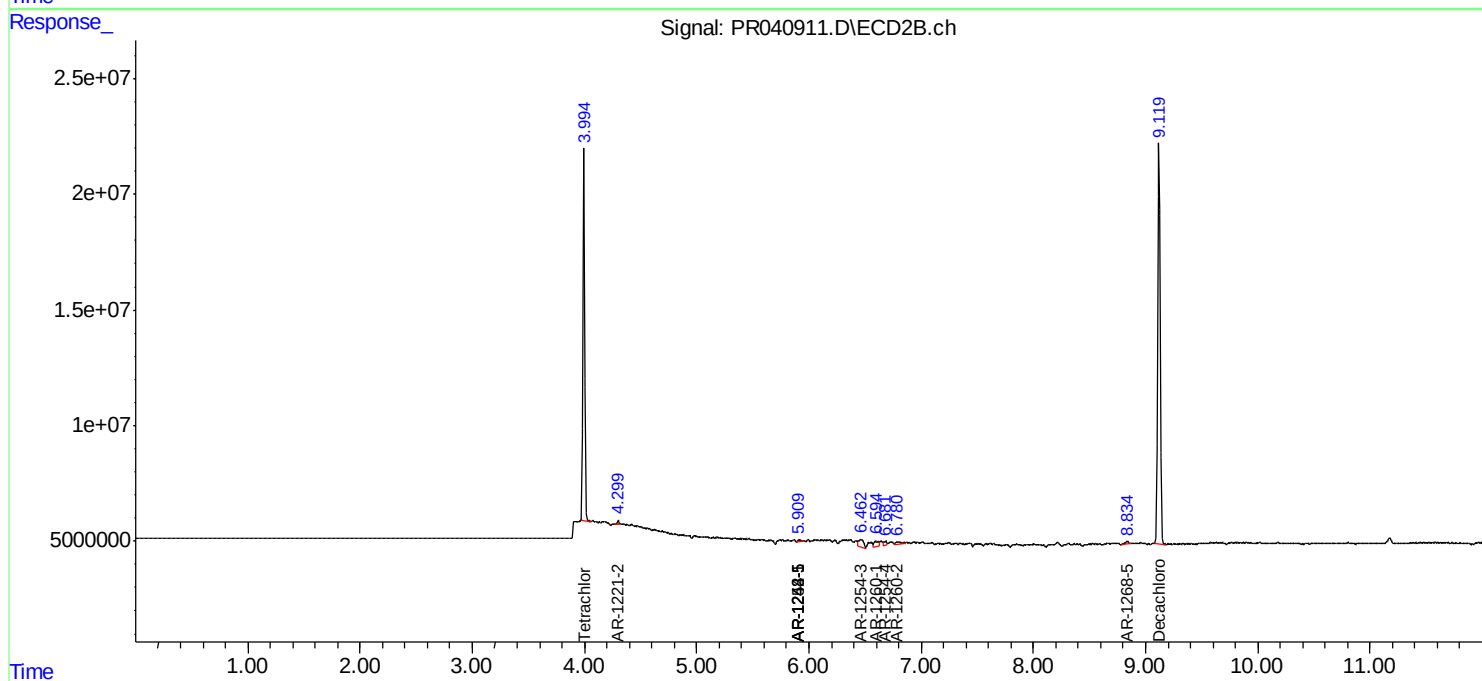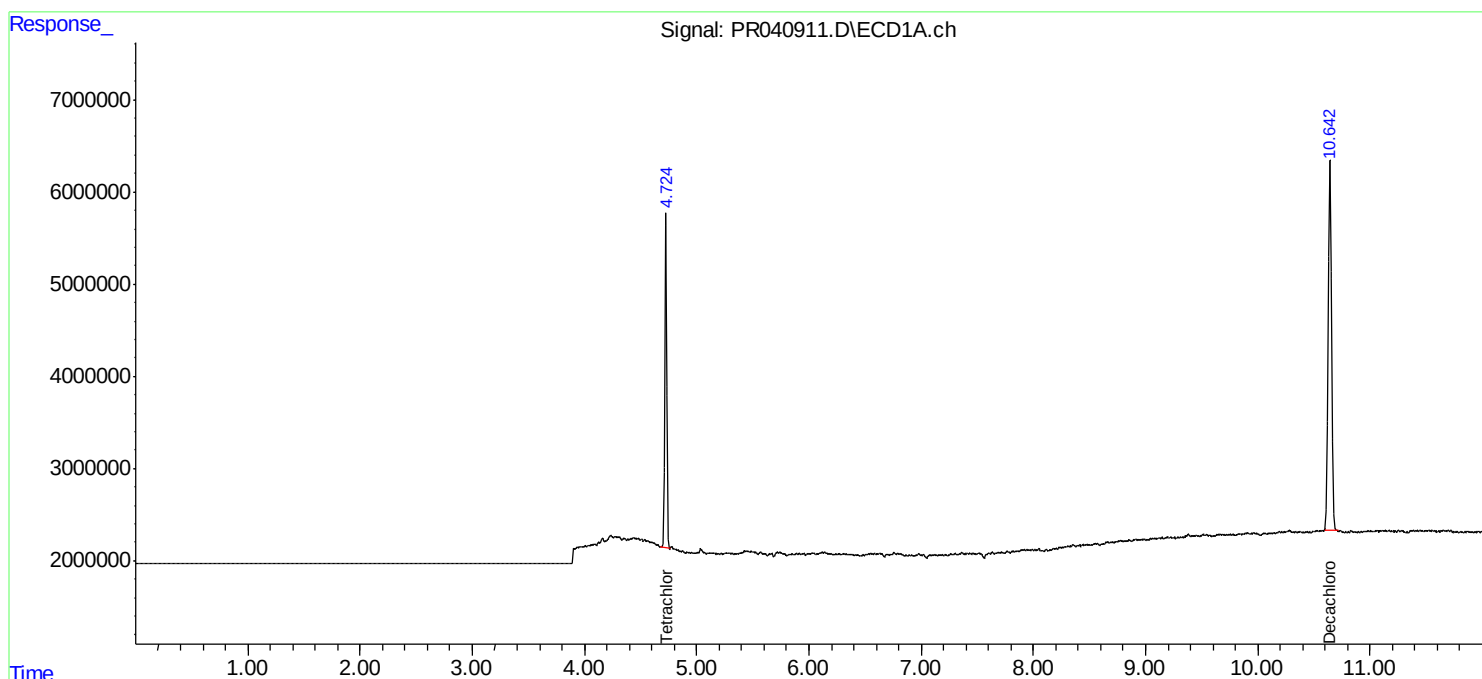


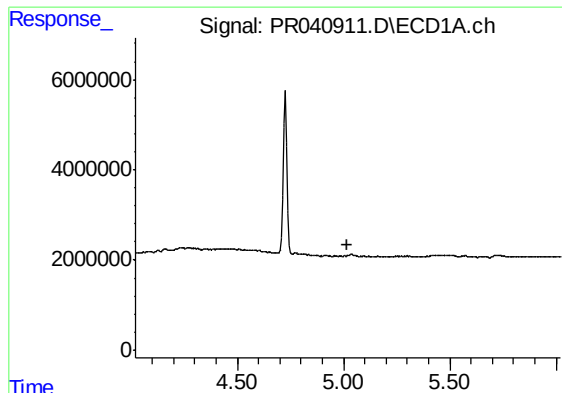

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AE6

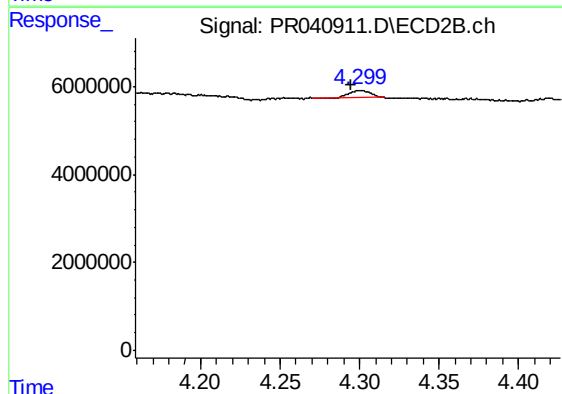


#9 AR-1221-2

R.T.: 4.300 min
Delta R.T.: 0.006 min
Response: 1483330
Conc: 19.32 ng/ml

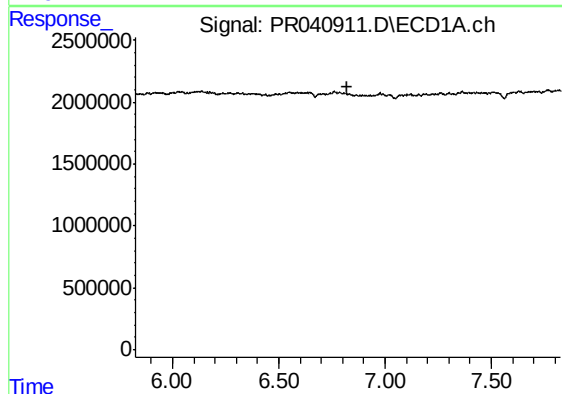


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.825 min
Response: 0
Conc: N.D.

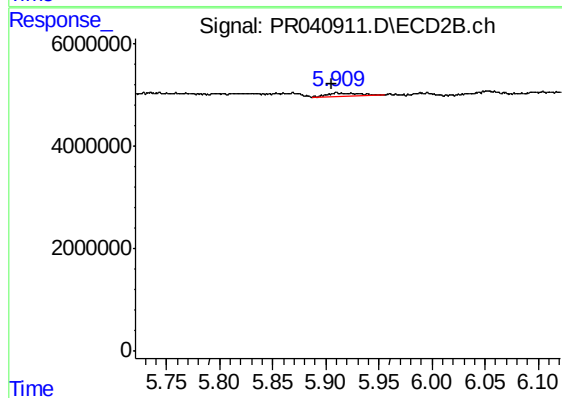

#20 AR-1242-5


R.T.: 5.910 min
Delta R.T.: 0.005 min
Response: 1482893
Conc: 6.47 ng/ml

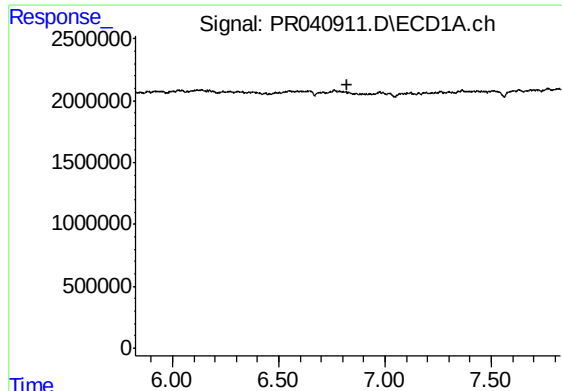

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.825 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AE6

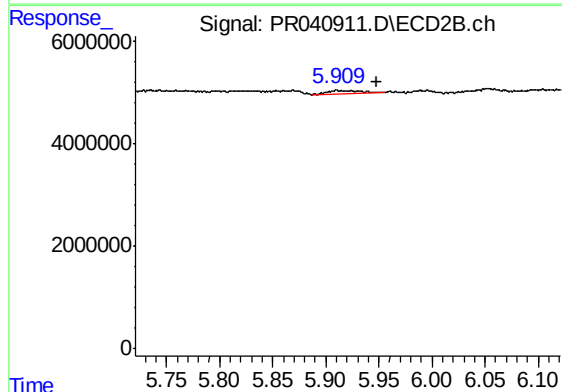


#25 AR-1248-5

R.T.: 5.910 min
Delta R.T.: -0.037 min
Response: 1482893
Conc: 4.69 ng/ml

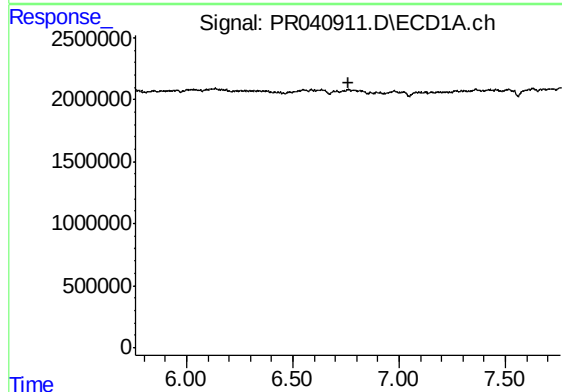


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

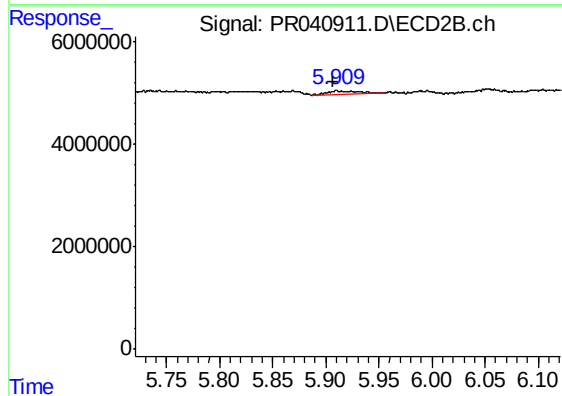

#26 AR-1254-1


R.T.: 5.910 min
Delta R.T.: 0.003 min
Response: 1482893
Conc: 3.10 ng/ml

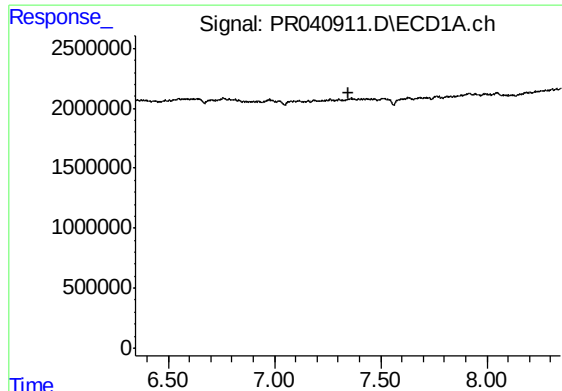

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AE6

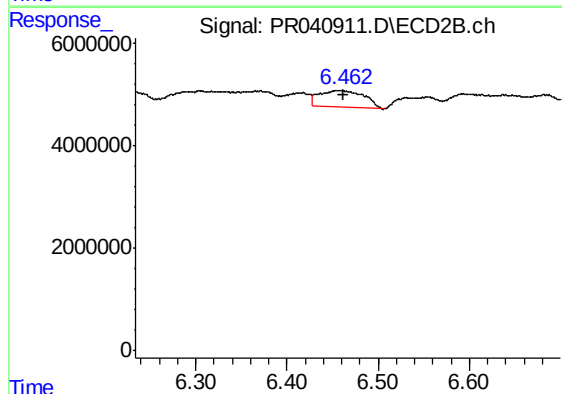


#28 AR-1254-3

R.T.: 6.457 min
Delta R.T.: -0.004 min
Response: 11111793
Conc: 14.77 ng/ml

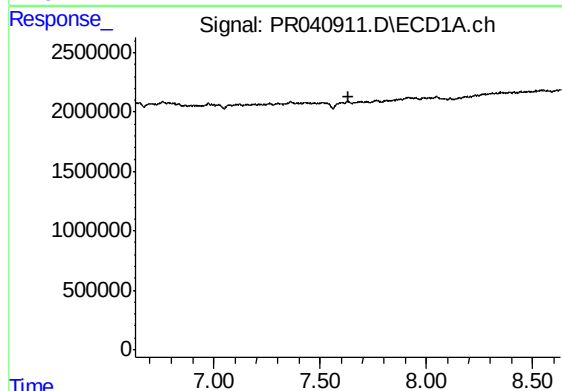


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.631 min
Response: 0
Conc: N.D.

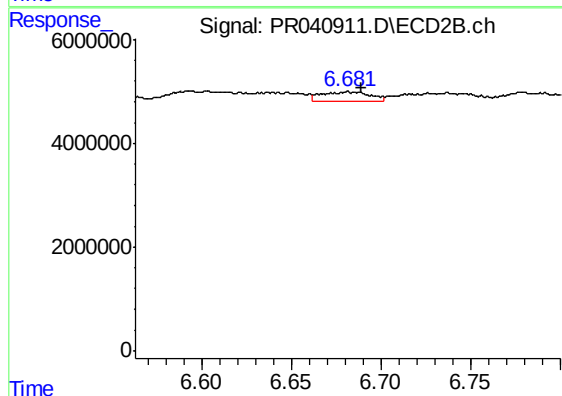

#29 AR-1254-4


R.T.: 6.683 min
Delta R.T.: -0.006 min
Response: 3364980
Conc: 6.44 ng/ml

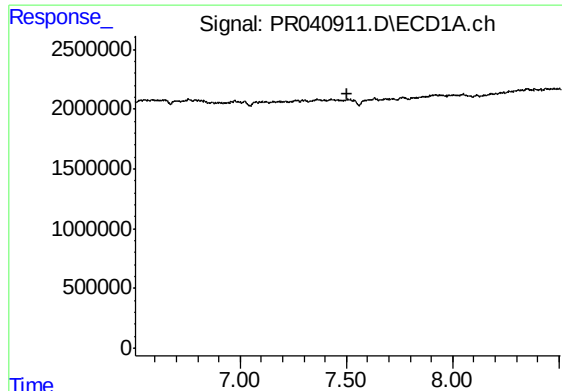

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AE6

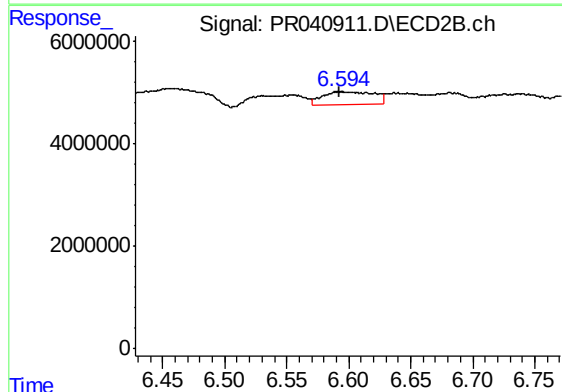


#31 AR-1260-1

R.T.: 6.594 min
Delta R.T.: 0.001 min
Response: 6972792
Conc: 13.69 ng/ml

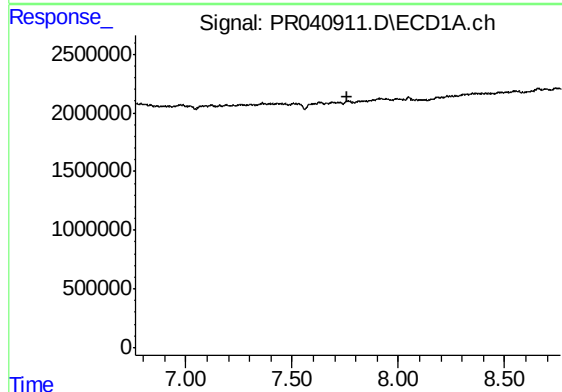


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.762 min
Response: 0
Conc: N.D.

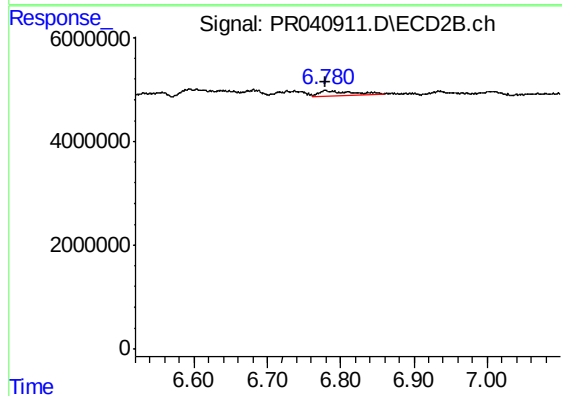

#32 AR-1260-2


R.T.: 6.780 min
Delta R.T.: 0.001 min
Response: 3122566
Conc: 4.91 ng/ml

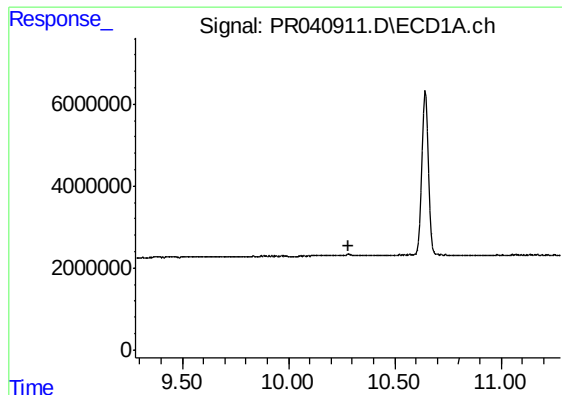

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AE6

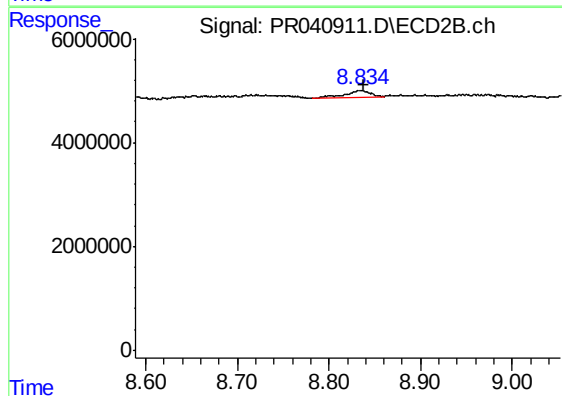

#45 AR-1268-5

R.T.: 8.835 min
Delta R.T.: -0.004 min
Response: 2406529
Conc: 0.65 ng/ml