

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091022\
 Data File : PR056525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2022 19:25
 Operator : AJ\MA
 Sample : N4530-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 SB-19-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/12/2022
 Supervised By :Ankita Jodhani 09/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 02:29:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.623	2.894	102.1E6	36058860	21.259m	20.573
2) SA Decachlor...	9.506	8.097	40317999	31303711	20.318m	18.815m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091022\
Data File : PR056525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2022 19:25
Operator : AJ\MA
Sample : N4530-06
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
SB-19-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2022
Supervised By :Ankita Jodhani 09/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 02:29:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

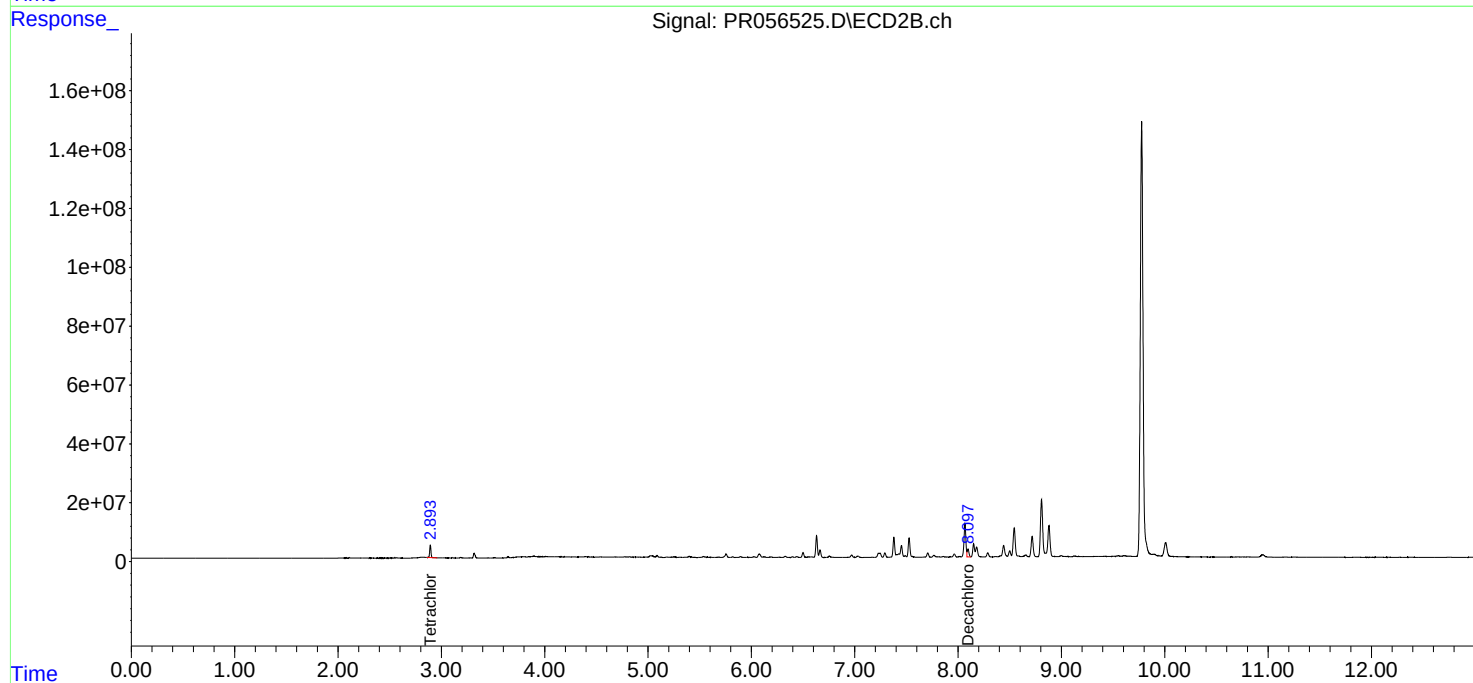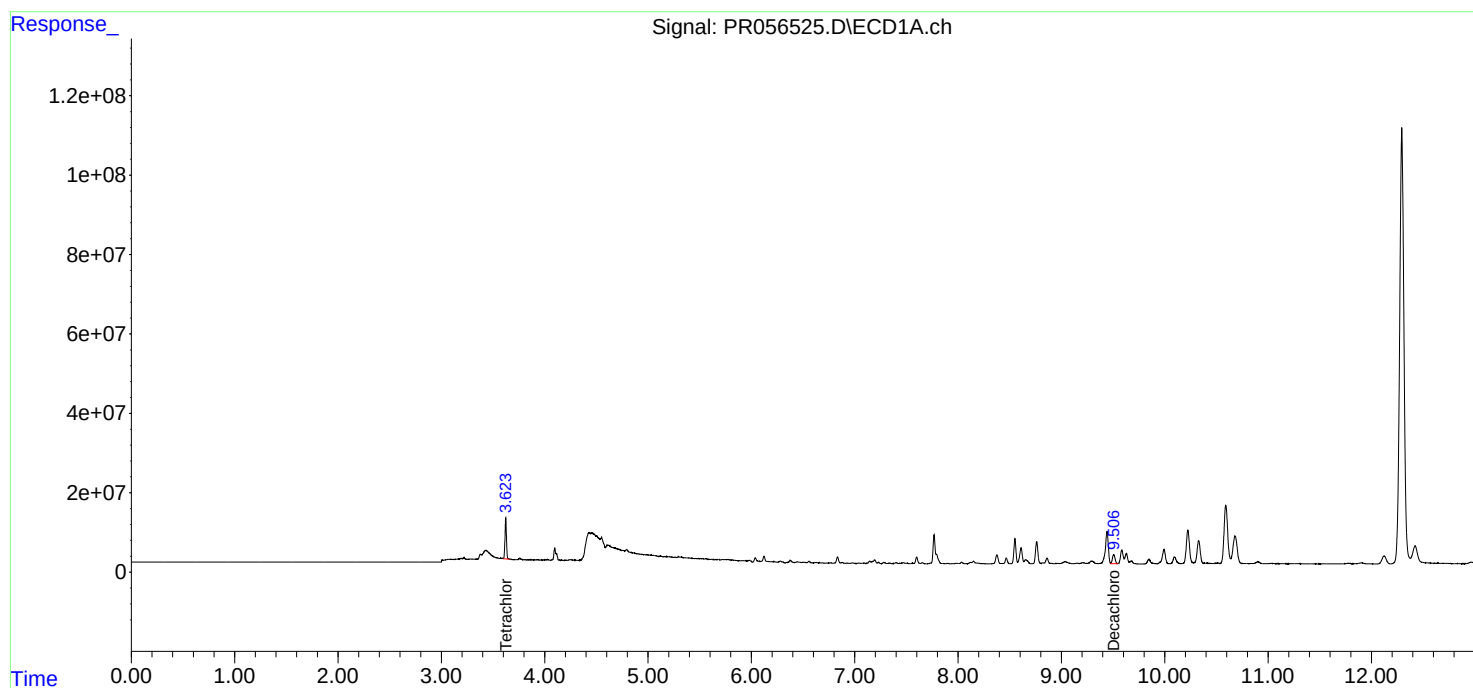

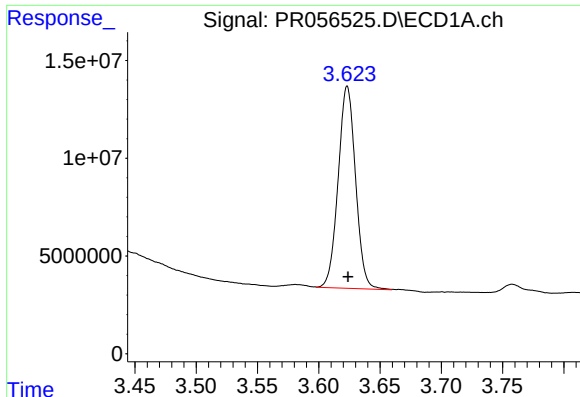


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.001 min
Response: 102143367
Conc: 21.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
SB-19-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2022
Supervised By :Ankita Jodhani 09/12/2022

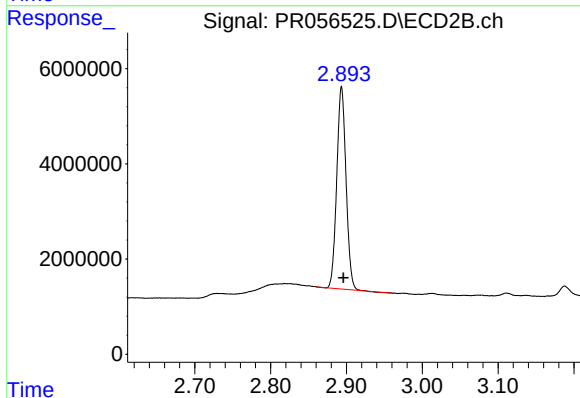


#1 Tetrachloro-m-xylene

R.T.: 2.894 min
Delta R.T.: -0.002 min
Response: 36058860
Conc: 20.57 ng/ml

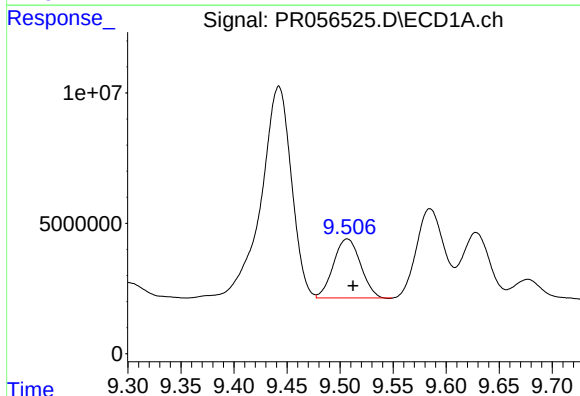

#2 Decachlorobiphenyl

R.T.: 9.506 min
Delta R.T.: -0.006 min
Response: 40317999
Conc: 20.32 ng/ml m

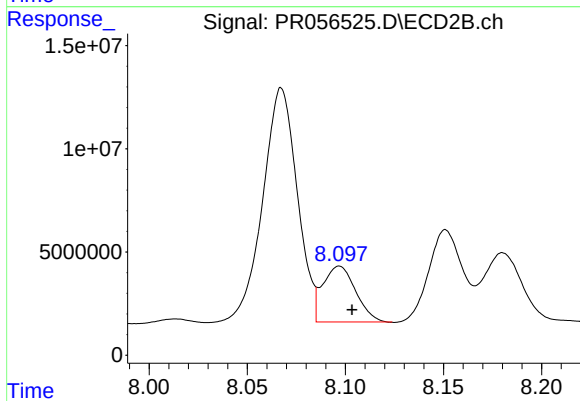

#2 Decachlorobiphenyl

R.T.: 8.097 min
Delta R.T.: -0.007 min
Response: 31303711
Conc: 18.81 ng/ml m