

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091119\
 Data File : PR040981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2019 18:24
 Operator : SM\AJ
 Sample : K4718-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 C0AD6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:44:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:01:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.724	3.992	2689907	11554135	0.875	0.868
2)	SA Decachlor...	10.645	9.120	2192318	7259642	0.788	0.743
Target Compounds							
28)	L6 AR-1254-3	0.000	6.457	0	16330535	N.D.	21.709 #
29)	L6 AR-1254-4	0.000	6.682	0	7285175	N.D.	13.932 #
31)	L7 AR-1260-1	0.000	6.599	0	10010542	N.D.	19.650 #
32)	L7 AR-1260-2	0.000	6.777	0	4977647	N.D.	7.830 #
33)	L7 AR-1260-3	0.000	6.936	0	2062358	N.D.	3.576 #
39)	L8 AR-1262-4	0.000	8.024	0	3559288	N.D.	3.192 #
40)	L8 AR-1262-5	0.000	8.507	0	3932535	N.D.	7.526 #
42)	L9 AR-1268-2	0.000	8.024	0	3559288	N.D.	2.382 #
44)	L9 AR-1268-4	0.000	8.507	0	3932535	N.D.	7.551 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091119\
Data File : PR040981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2019 18:24
Operator : SM\AJ
Sample : K4718-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
C0AD6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:44:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:01:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

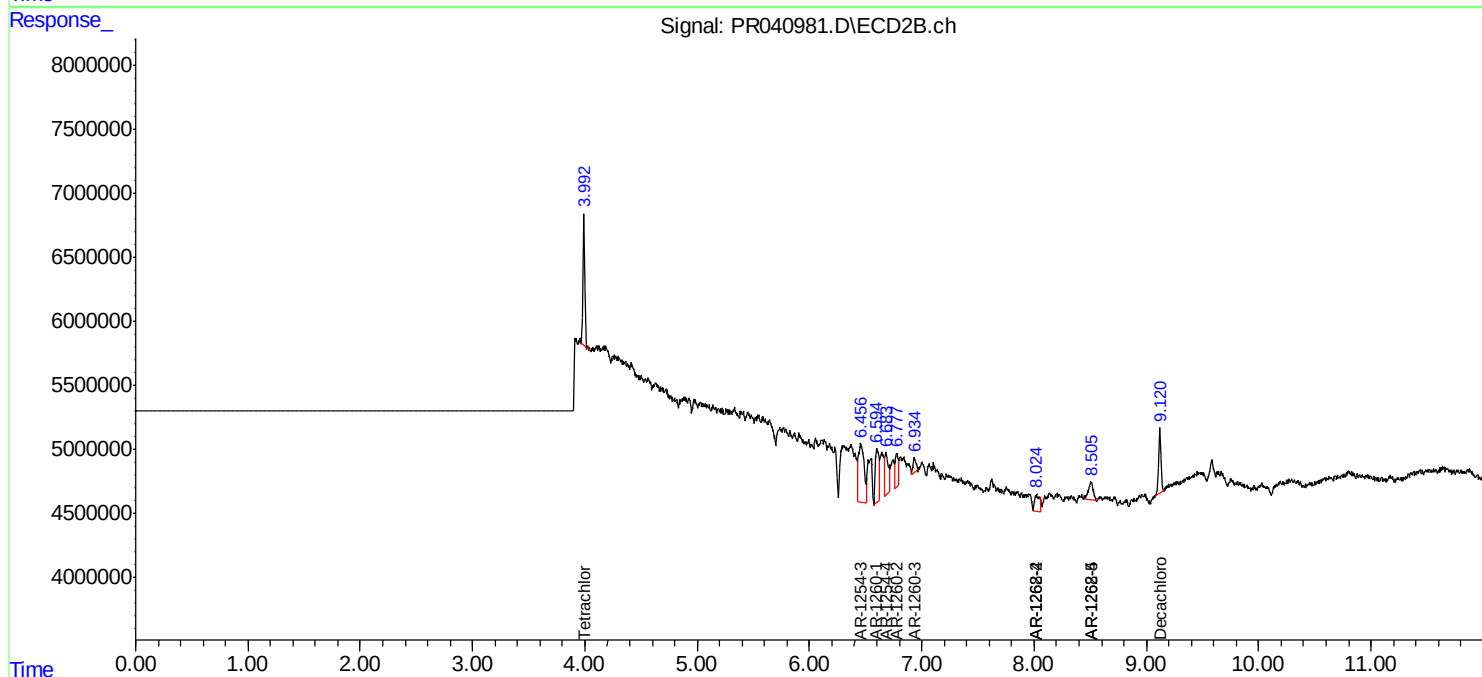


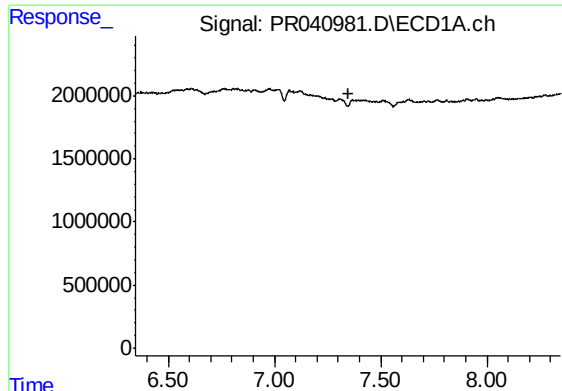

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AD6

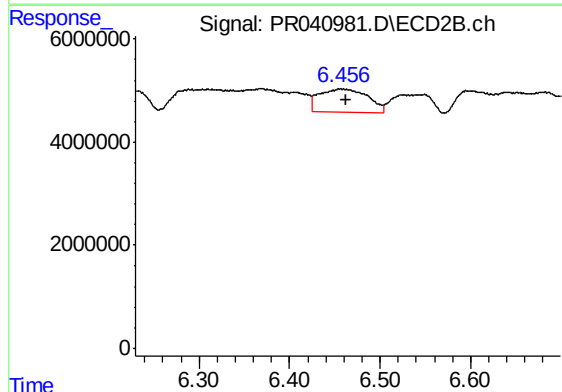


#28 AR-1254-3

R.T.: 6.457 min
Delta R.T.: -0.005 min
Response: 16330535
Conc: 21.71 ng/ml

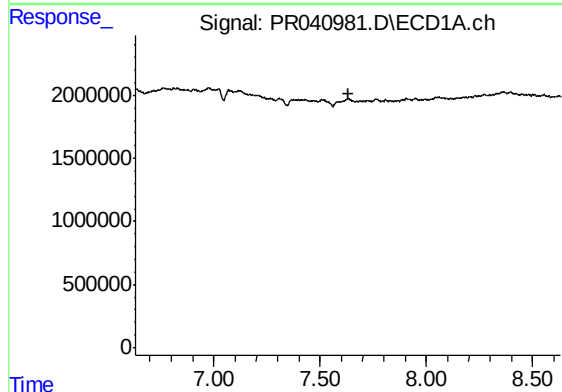


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.631 min
Response: 0
Conc: N.D.

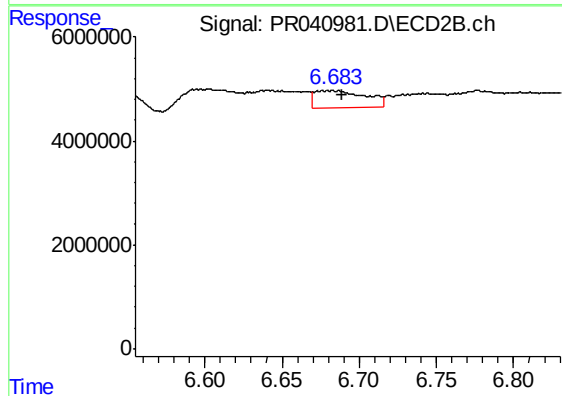

#29 AR-1254-4


R.T.: 6.682 min
Delta R.T.: -0.007 min
Response: 7285175
Conc: 13.93 ng/ml

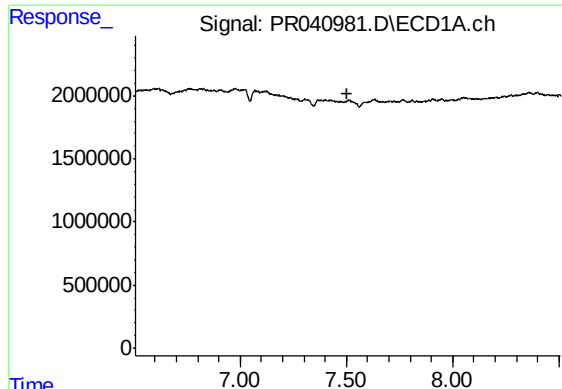

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AD6

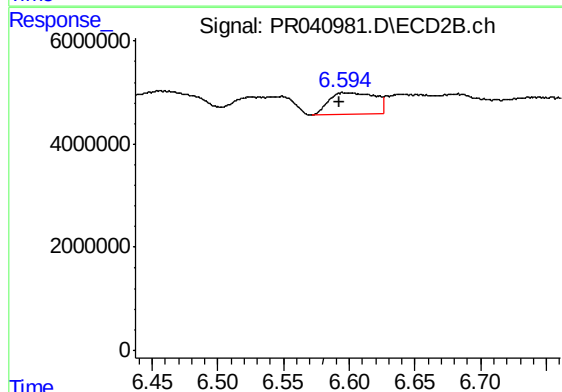


#31 AR-1260-1

R.T.: 6.599 min
Delta R.T.: 0.007 min
Response: 10010542
Conc: 19.65 ng/ml

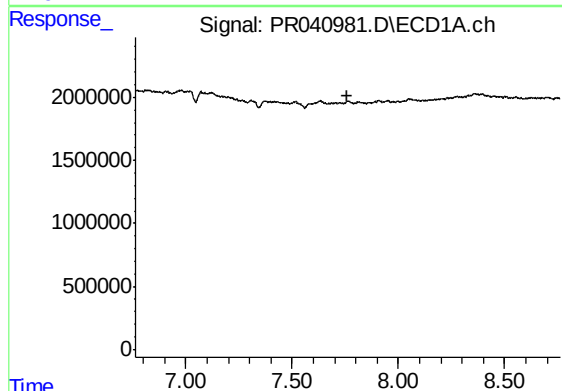


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.762 min
Response: 0
Conc: N.D.

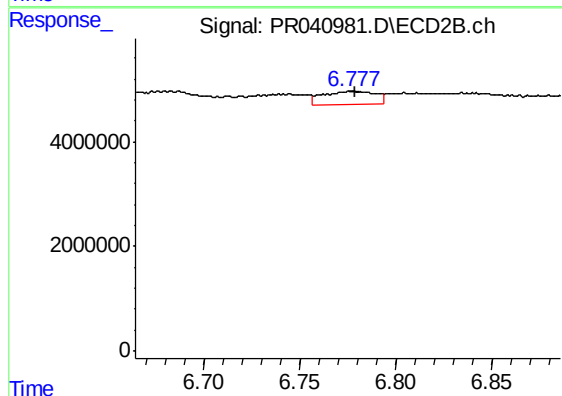

#32 AR-1260-2


R.T.: 6.777 min
Delta R.T.: -0.002 min
Response: 4977647
Conc: 7.83 ng/ml

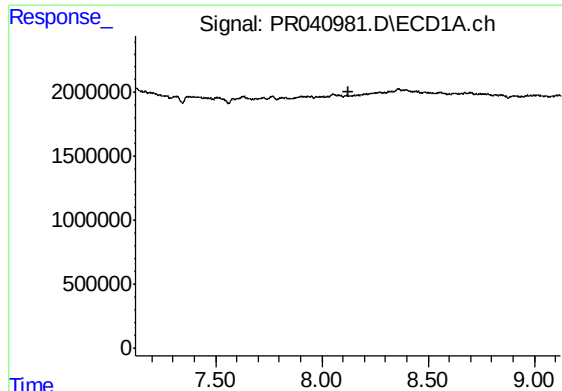

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 8.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AD6

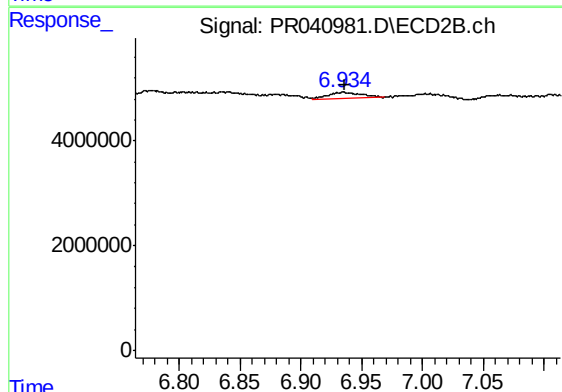


#33 AR-1260-3

R.T.: 6.936 min
Delta R.T.: 0.000 min
Response: 2062358
Conc: 3.58 ng/ml

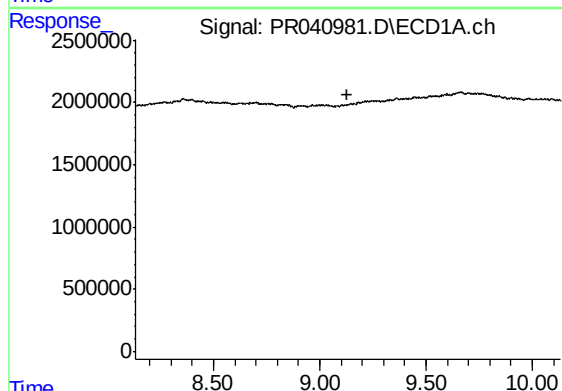


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.132 min
Response: 0
Conc: N.D.

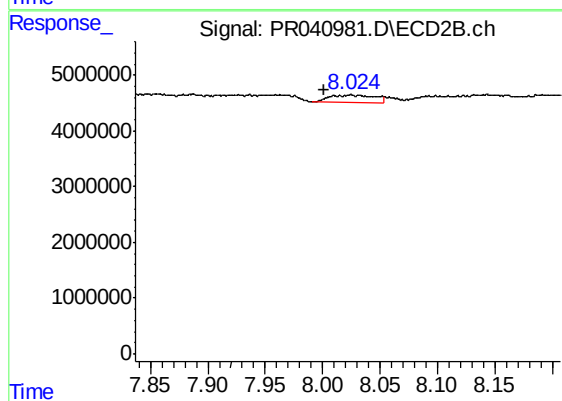

#39 AR-1262-4


R.T.: 8.024 min
Delta R.T.: 0.022 min
Response: 3559288
Conc: 3.19 ng/ml

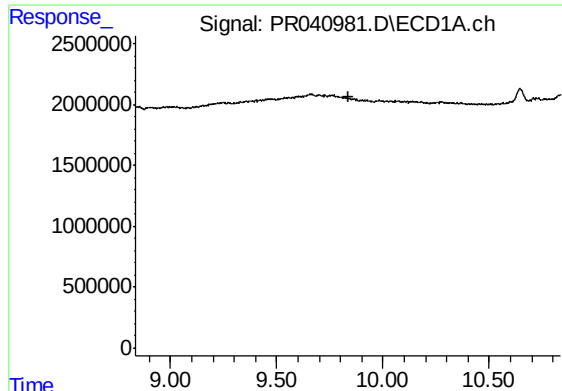

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AD6

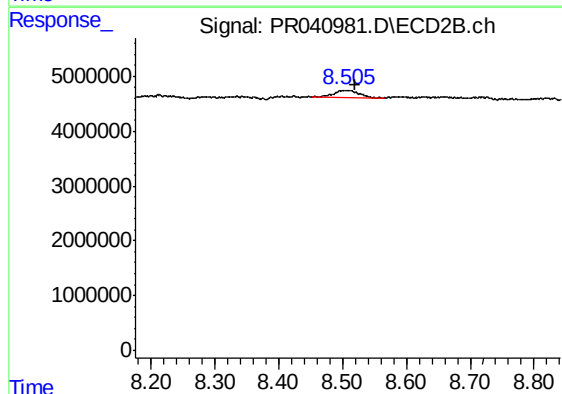


#40 AR-1262-5

R.T.: 8.507 min
Delta R.T.: -0.013 min
Response: 3932535
Conc: 7.53 ng/ml

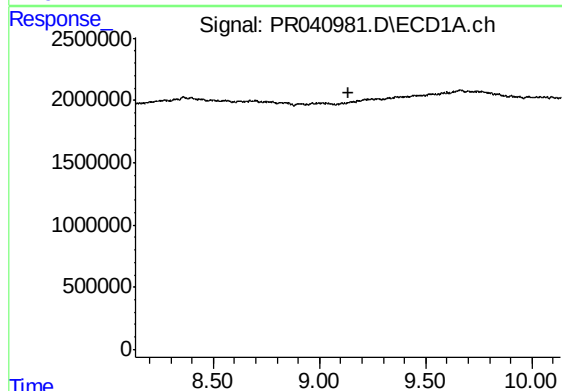


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.134 min
Response: 0
Conc: N.D.

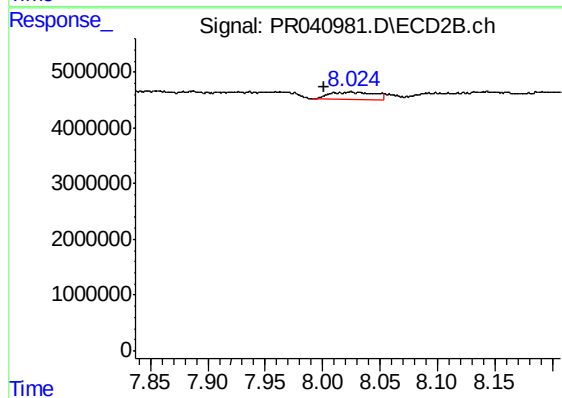

#42 AR-1268-2


R.T.: 8.024 min
Delta R.T.: 0.023 min
Response: 3559288
Conc: 2.38 ng/ml

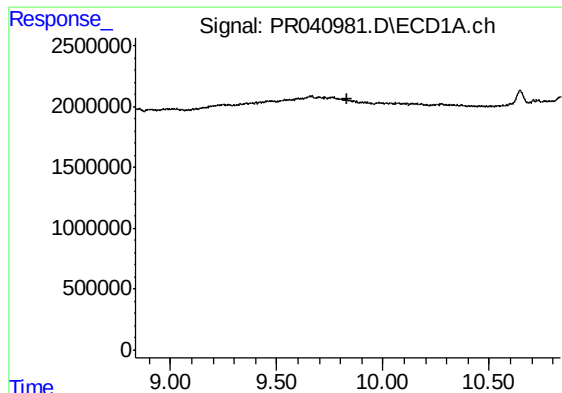

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AD6

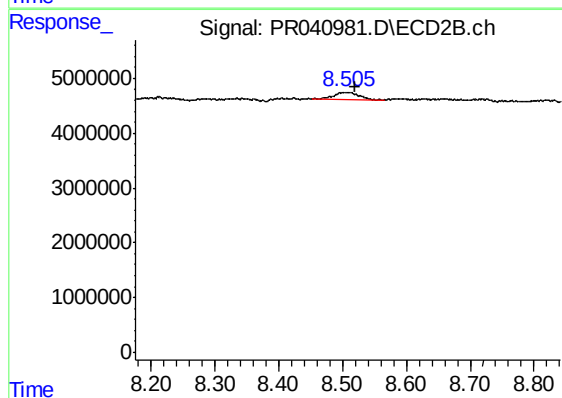

#44 AR-1268-4

R.T.: 8.507 min
Delta R.T.: -0.012 min
Response: 3932535
Conc: 7.55 ng/ml