

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091222\
 Data File : PR056564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2022 14:35
 Operator : AJ\MA
 Sample : N4550-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 D-CRTE-SLAB-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/13/2022
 Supervised By :Ankita Jodhani 09/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 00:59:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.625	2.896	74846925	27835133	15.578m	15.881
2) SA Decachlor...	9.517	8.106	41256636	29341231	20.791	17.635

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091222\
Data File : PR056564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2022 14:35
Operator : AJ\MA
Sample : N4550-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
D-CRTE-SLAB-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/13/2022
Supervised By :Ankita Jodhani 09/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 00:59:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

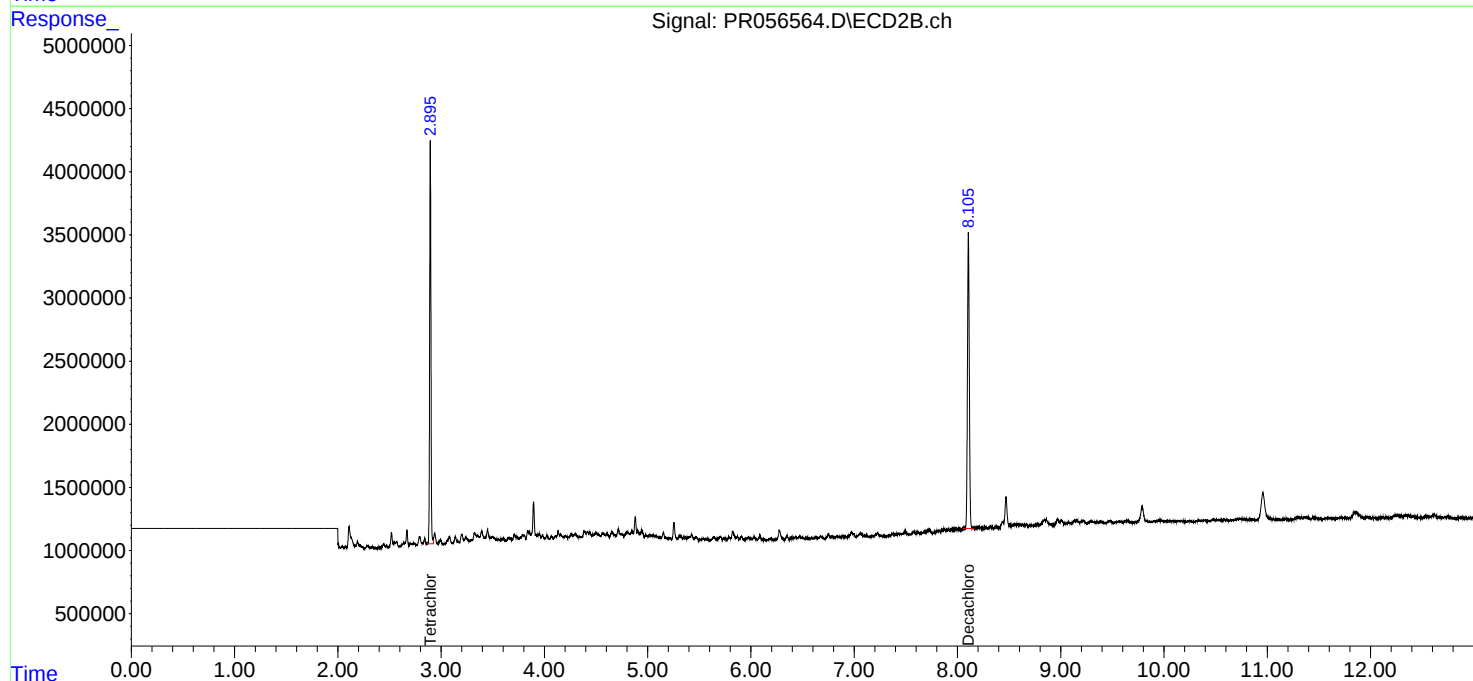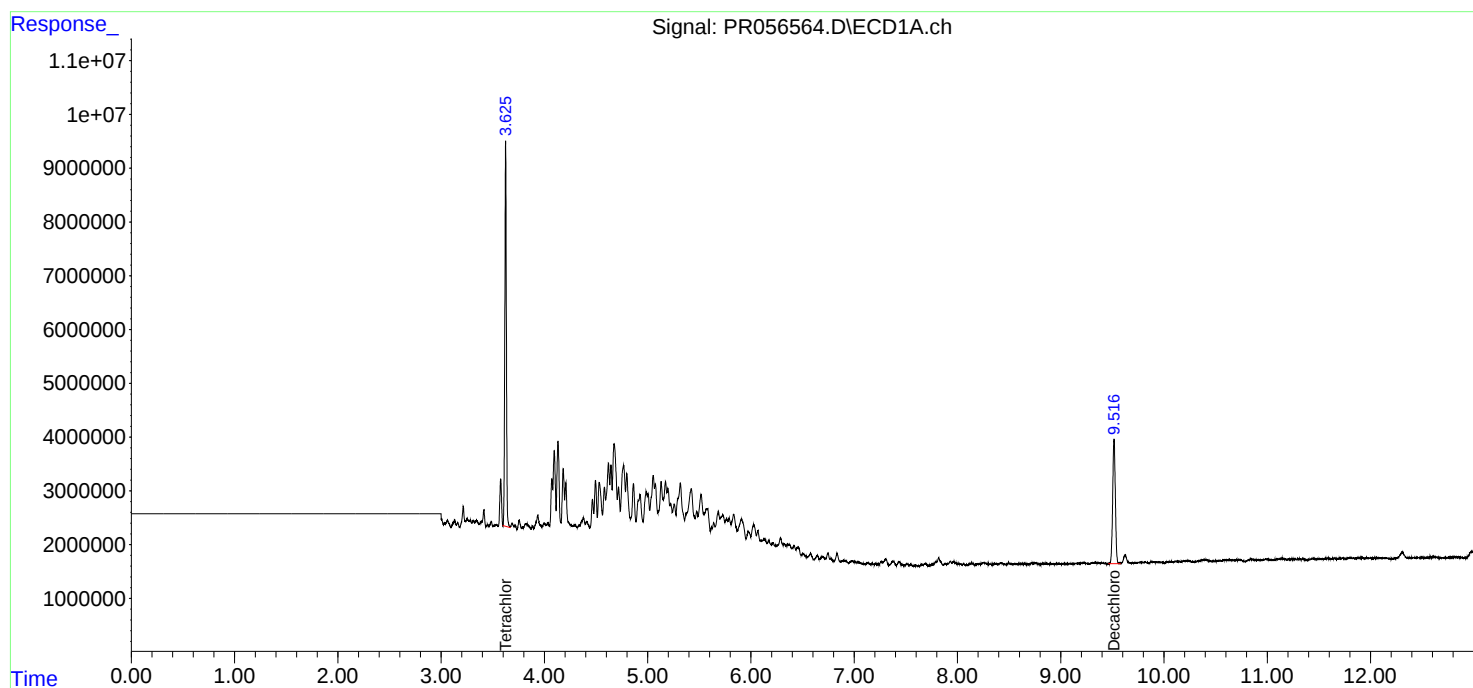

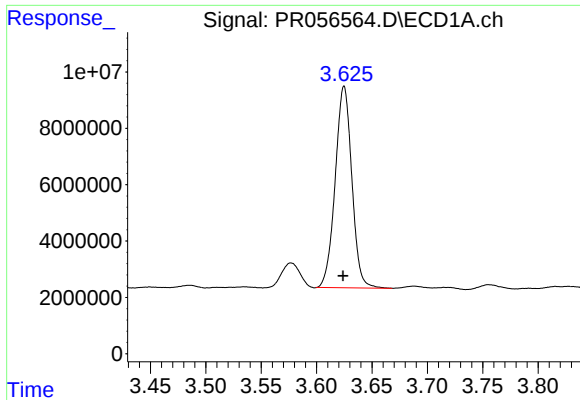


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: 0.000 min
Response: 74846925
Conc: 15.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
D-CRTE-SLAB-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/13/2022
Supervised By :Ankita Jodhani 09/13/2022

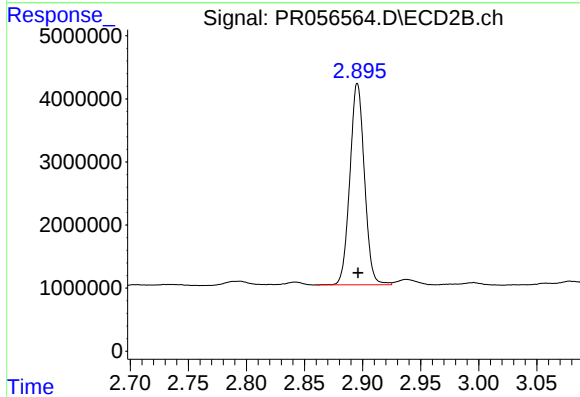


#1 Tetrachloro-m-xylene

R.T.: 2.896 min
Delta R.T.: 0.000 min
Response: 27835133
Conc: 15.88 ng/ml

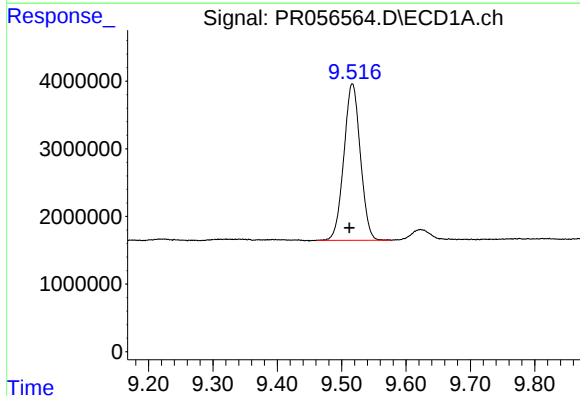

#2 Decachlorobiphenyl

R.T.: 9.517 min
Delta R.T.: 0.004 min
Response: 41256636
Conc: 20.79 ng/ml

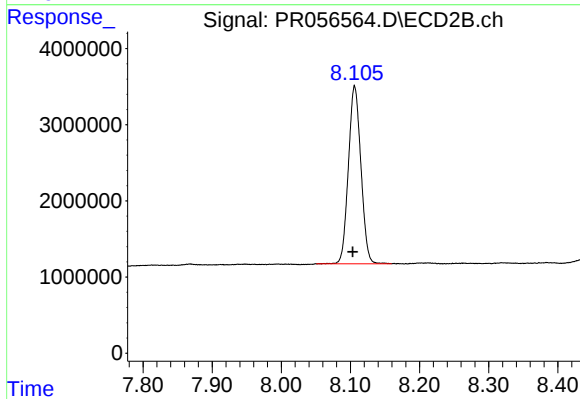

#2 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: 0.003 min
Response: 29341231
Conc: 17.64 ng/ml