

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091222\
 Data File : PR056599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2022 01:55
 Operator : AJ\MA
 Sample : N4573-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 172

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/13/2022
 Supervised By :Ankita Jodhani 09/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 03:13:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.632	2.908	93092595	34177940	19.375m	19.500
2) SA Decachlor...	9.504	8.095	54410748	39990205	27.420	24.036

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091222\
Data File : PR056599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2022 01:55
Operator : AJ\MA
Sample : N4573-01
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
172


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/13/2022
Supervised By :Ankita Jodhani 09/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 03:13:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

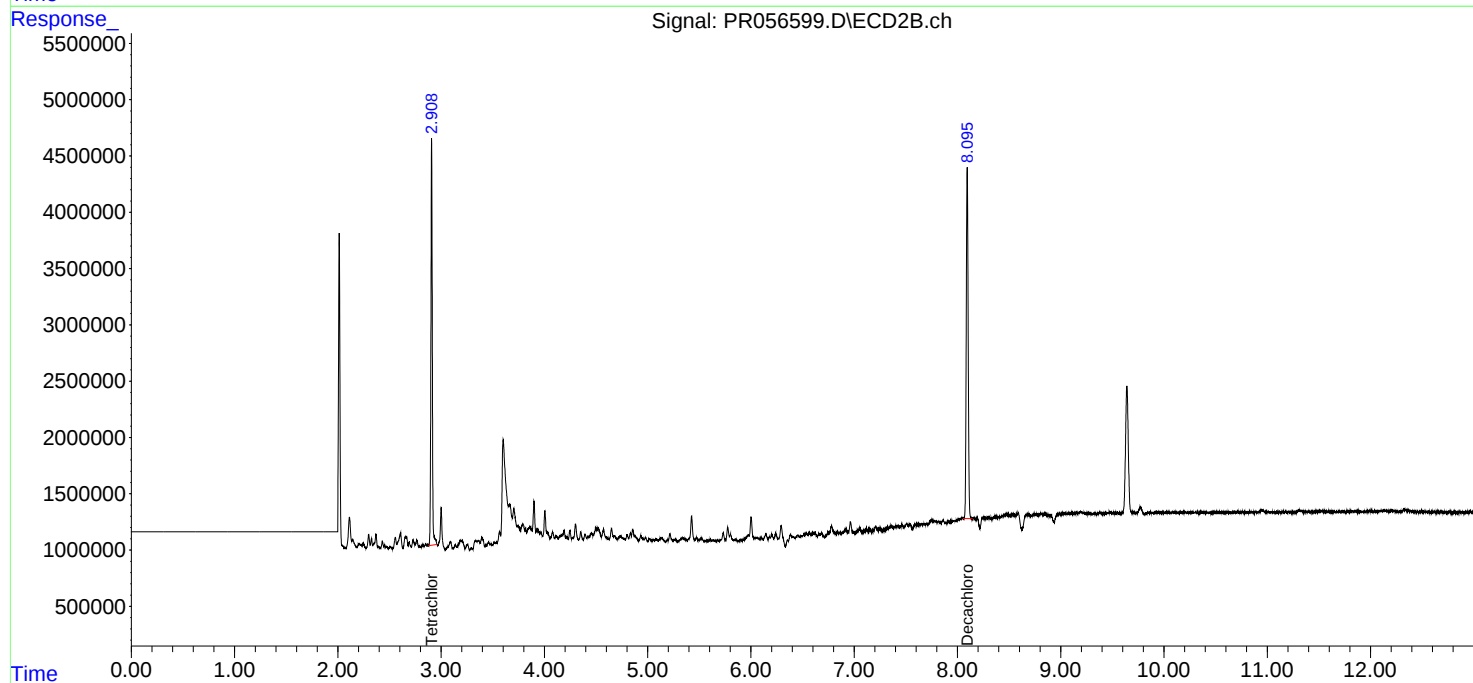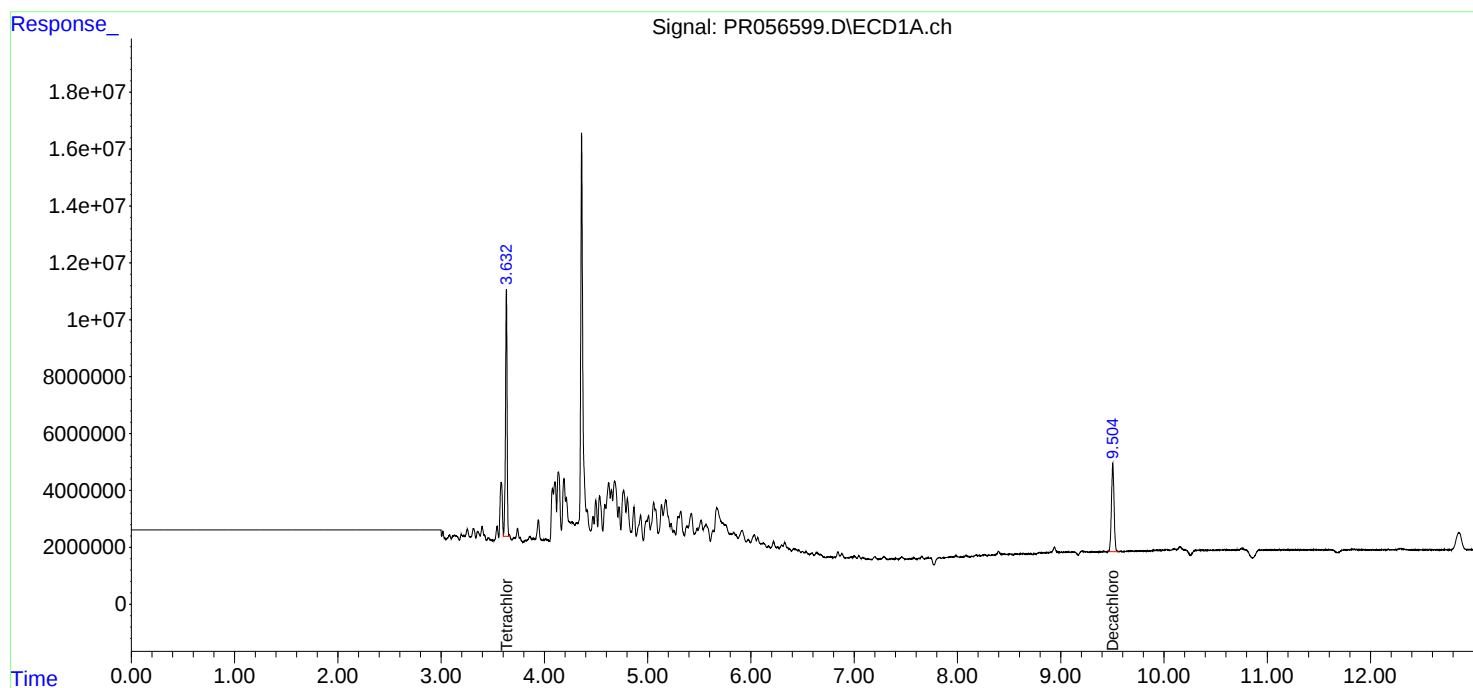

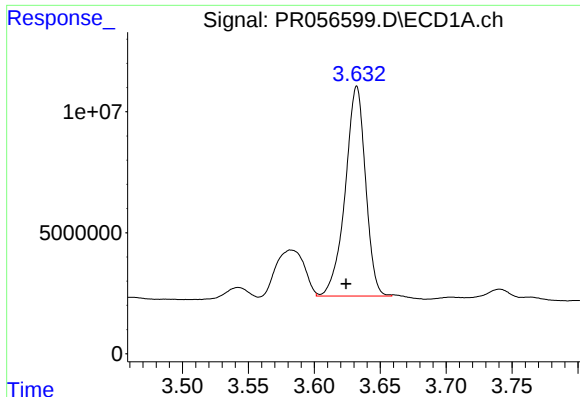


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: 0.008 min
Response: 93092595
Conc: 19.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
172


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/13/2022
Supervised By :Ankita Jodhani 09/13/2022

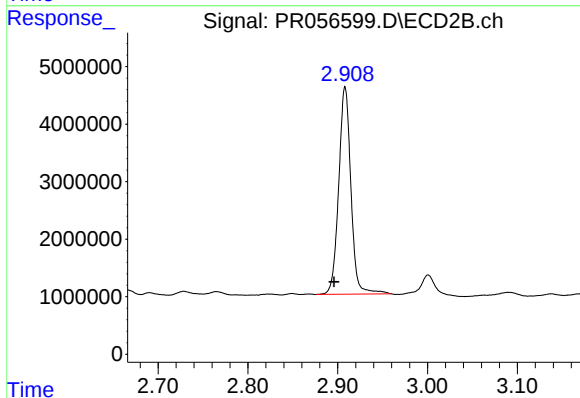


#1 Tetrachloro-m-xylene

R.T.: 2.908 min
Delta R.T.: 0.012 min
Response: 34177940
Conc: 19.50 ng/ml

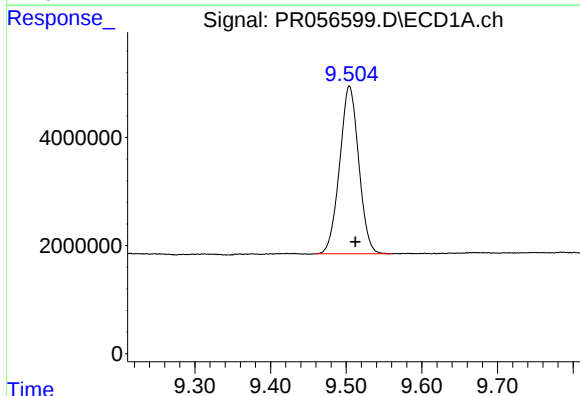

#2 Decachlorobiphenyl

R.T.: 9.504 min
Delta R.T.: -0.008 min
Response: 54410748
Conc: 27.42 ng/ml

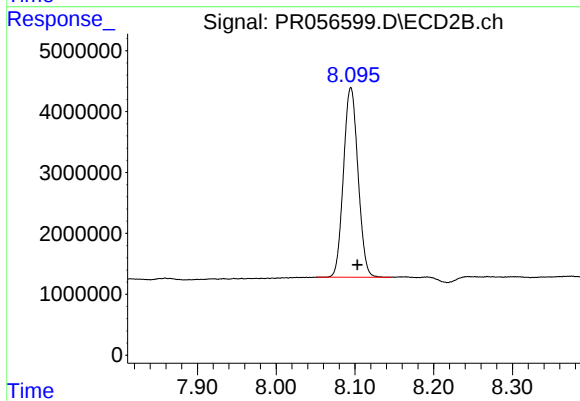

#2 Decachlorobiphenyl

R.T.: 8.095 min
Delta R.T.: -0.009 min
Response: 39990205
Conc: 24.04 ng/ml