

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091322\
 Data File : PR056633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2022 18:30
 Operator : AJ\MA
 Sample : N4579-23
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 CHERRY-HILL-COMP-16

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/14/2022
 Supervised By :Ankita Jodhani 09/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 18:50:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.621	2.892	99294801	36137021	20.666m	20.617
2) SA Decachlor...	9.506	8.097	38839811	30919438	19.573	18.584

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091322\
Data File : PR056633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2022 18:30
Operator : AJ\MA
Sample : N4579-23
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
CHERRY-HILL-COMP-16


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2022
Supervised By :Ankita Jodhani 09/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 18:50:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

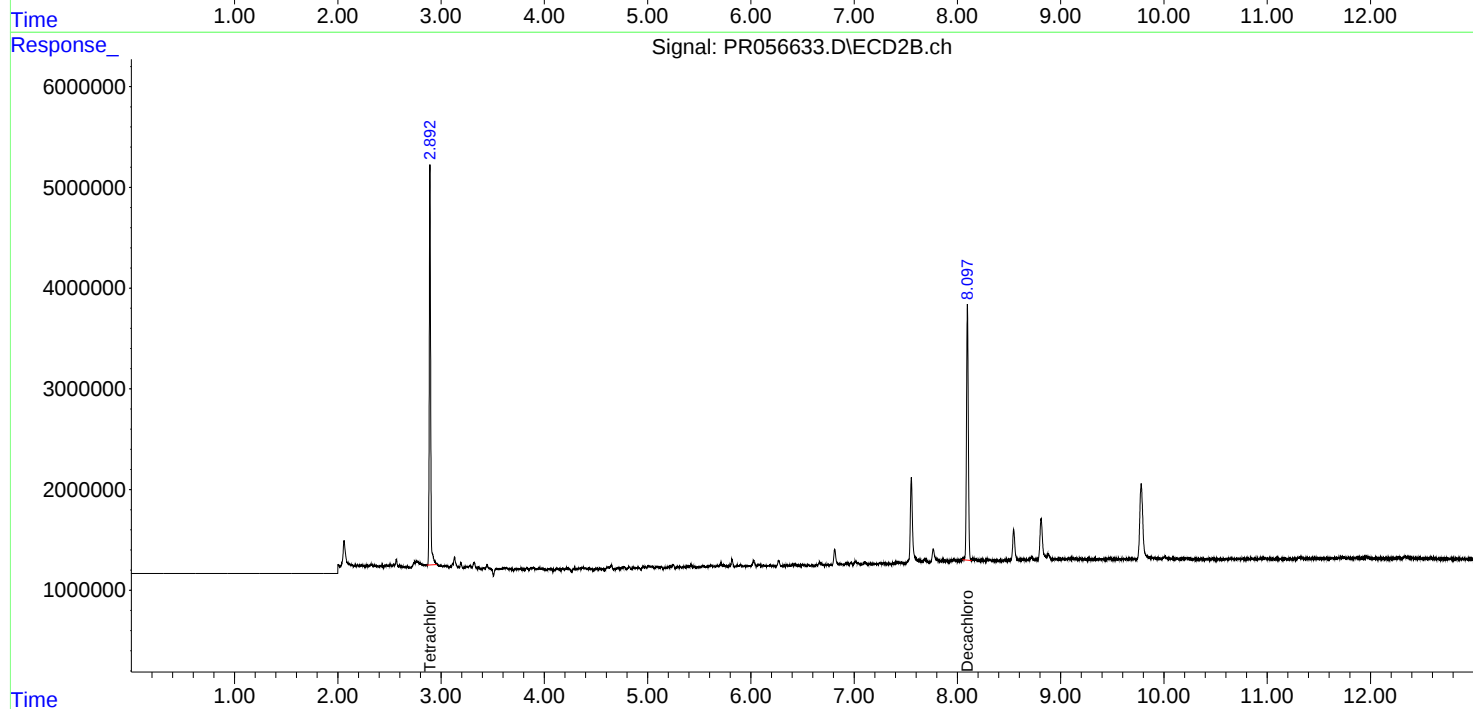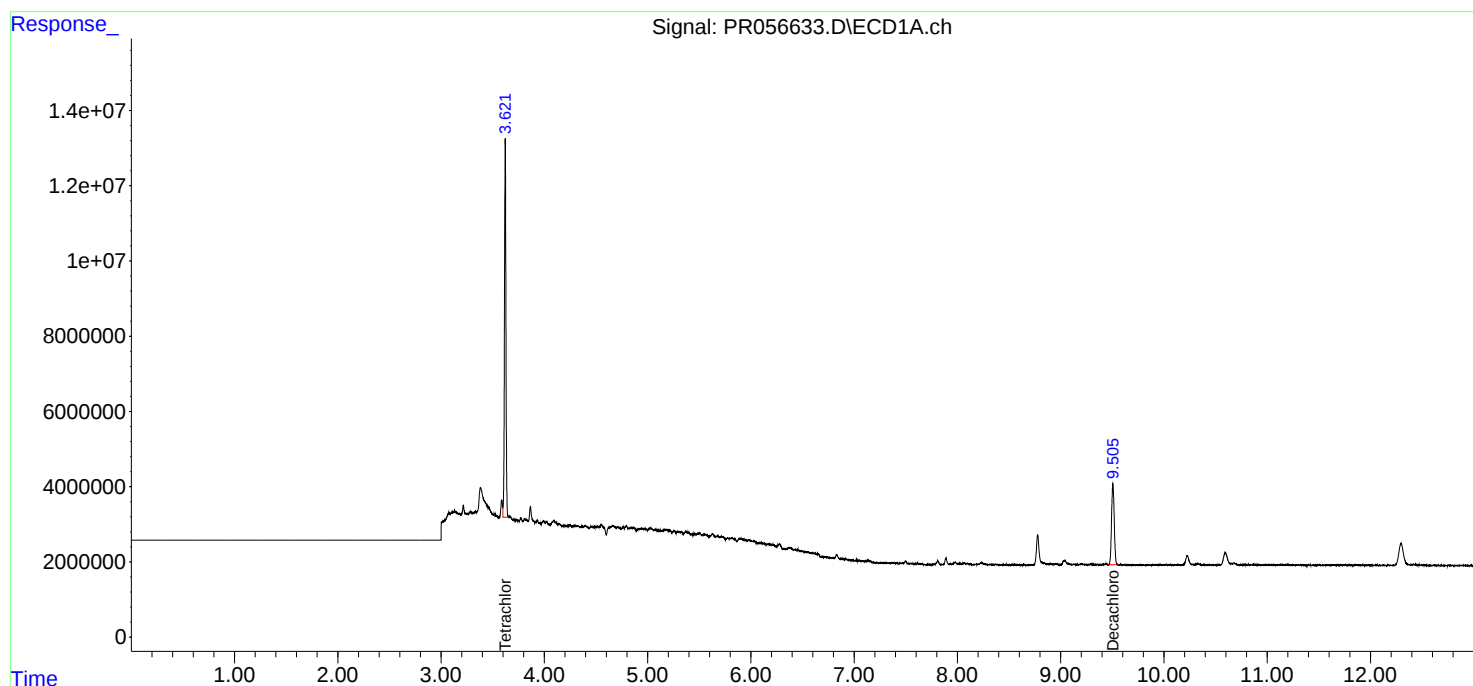

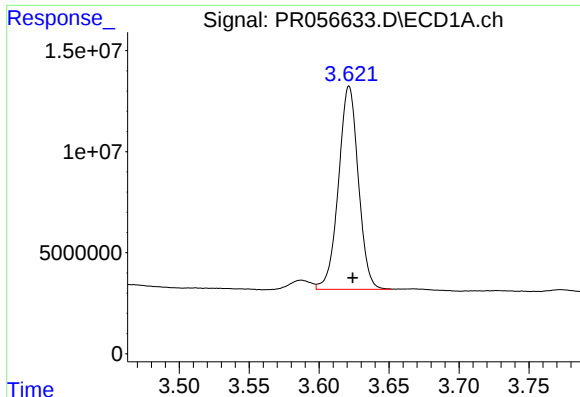


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.003 min
Response: 99294801
Conc: 20.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
CHERRY-HILL-COMP-16


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/14/2022
Supervised By :Ankita Jodhani 09/14/2022

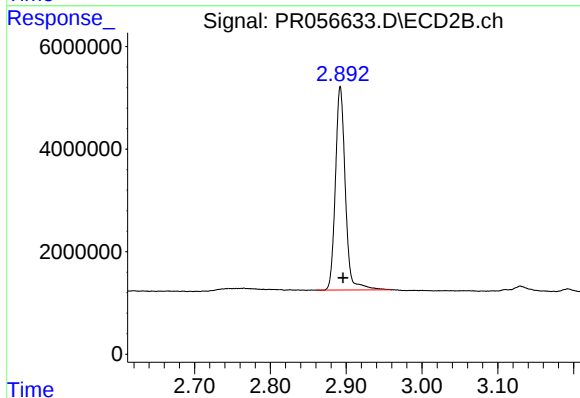


#1 Tetrachloro-m-xylene

R.T.: 2.892 min
Delta R.T.: -0.004 min
Response: 36137021
Conc: 20.62 ng/ml

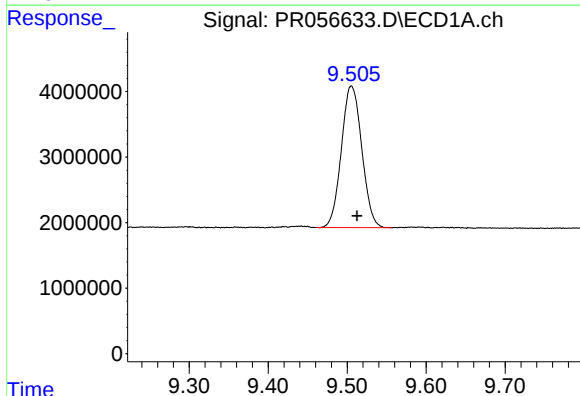

#2 Decachlorobiphenyl

R.T.: 9.506 min
Delta R.T.: -0.007 min
Response: 38839811
Conc: 19.57 ng/ml

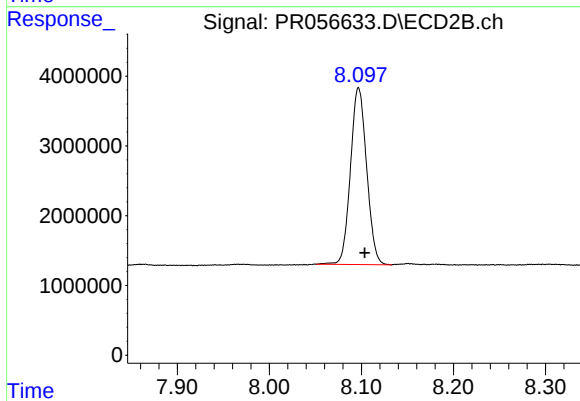

#2 Decachlorobiphenyl

R.T.: 8.097 min
Delta R.T.: -0.006 min
Response: 30919438
Conc: 18.58 ng/ml