

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091323\
Data File : PR063256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 18:18
Operator : YP\AJ
Sample : 04378-02
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
ALCS447

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 22:44:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 13 07:34:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

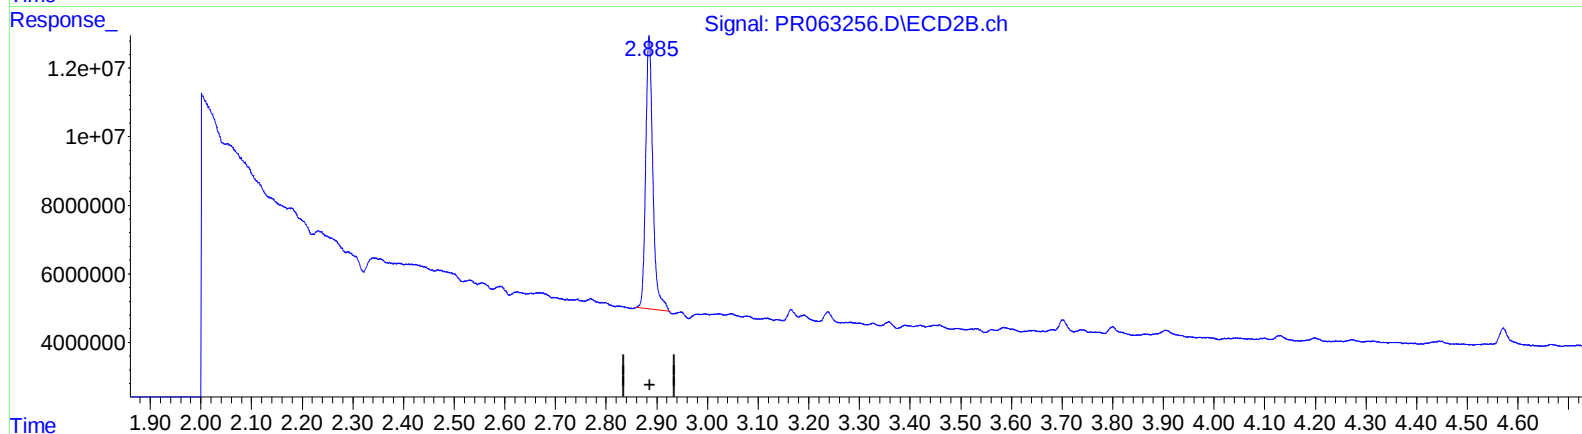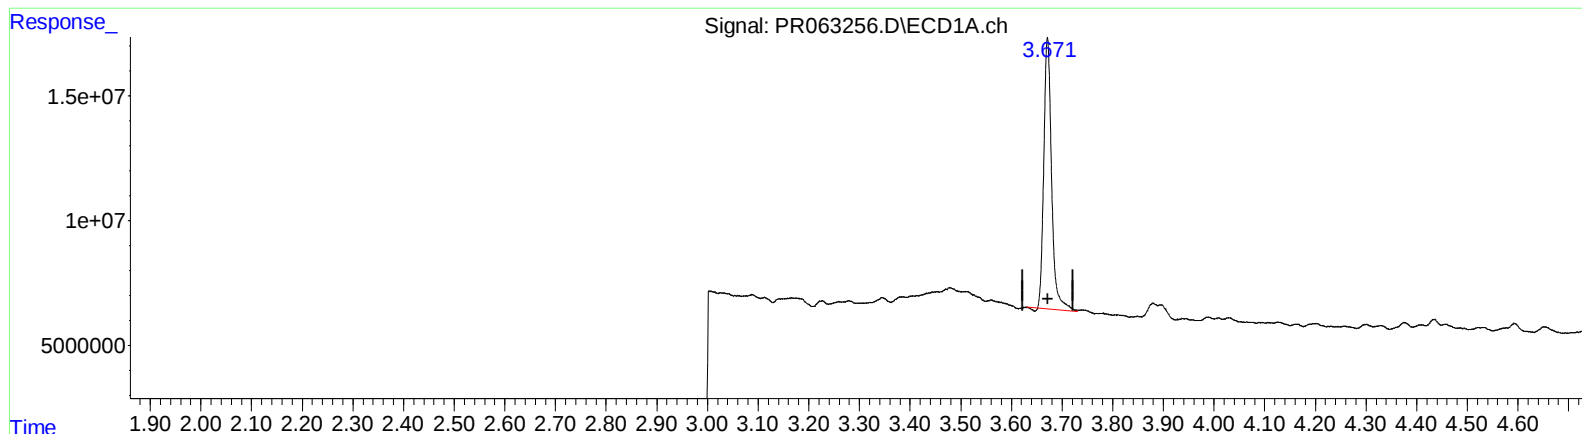

QEdit

(1) Tetrachloro-m-xylene (SA)

3.671min 17.964 ng/ml

response 116586693

(1) Tetrachloro-m-xylene #2 (SA)

2.885min 22.908 ng/ml

response 78316240

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091323\
Data File : PR063256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 18:18
Operator : YP\AJ
Sample : 04378-02
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
ALCS447

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 22:44:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 13 07:34:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

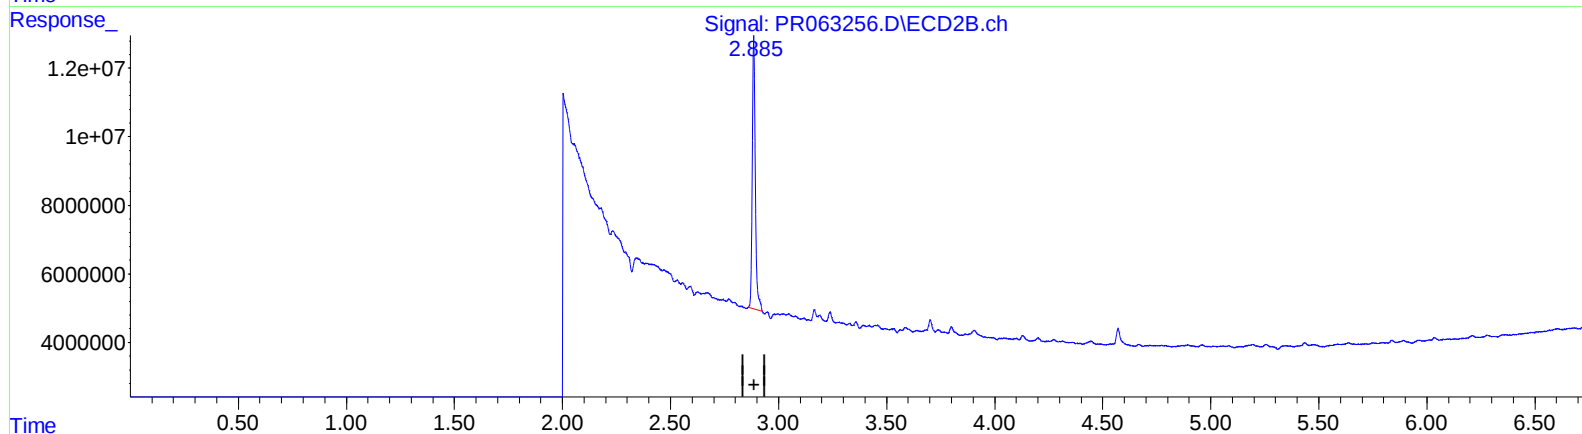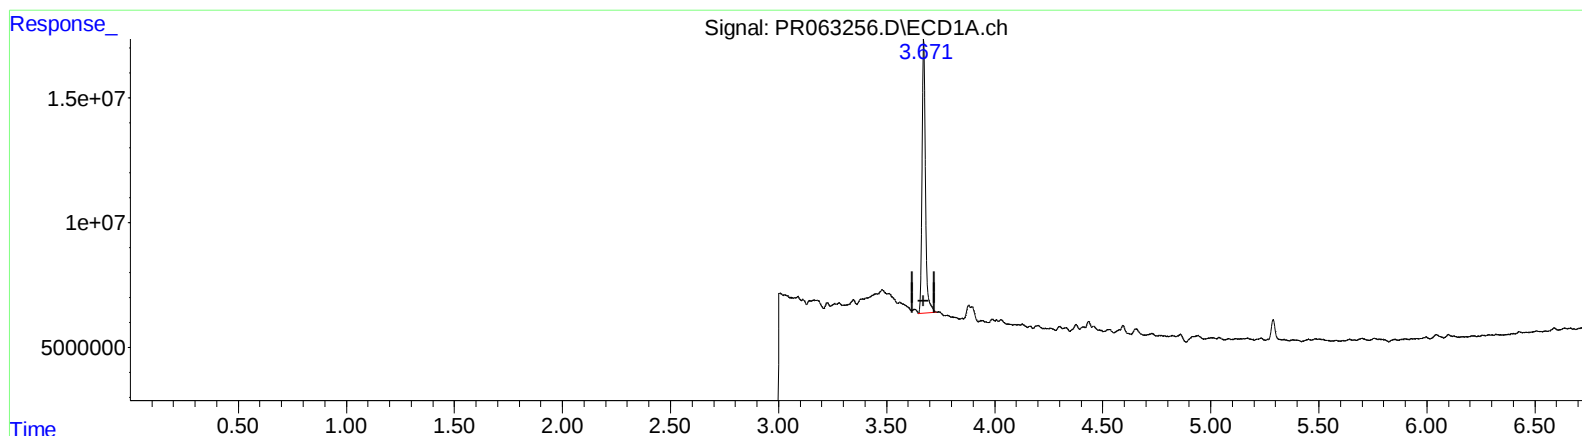

QEdit

(1) Tetrachloro-m-xylene (SA)

3.671min 18.307 ng/ml m

response 118814255

(1) Tetrachloro-m-xylene #2 (SA)

2.885min 22.908 ng/ml

response 78316240

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091323\
Data File : PR063276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 23:41
Operator : YP\AJ
Sample : PB155447BS
Misc :
ALS Vial : 52 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
ALCS447

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 01:46:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 13 07:34:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

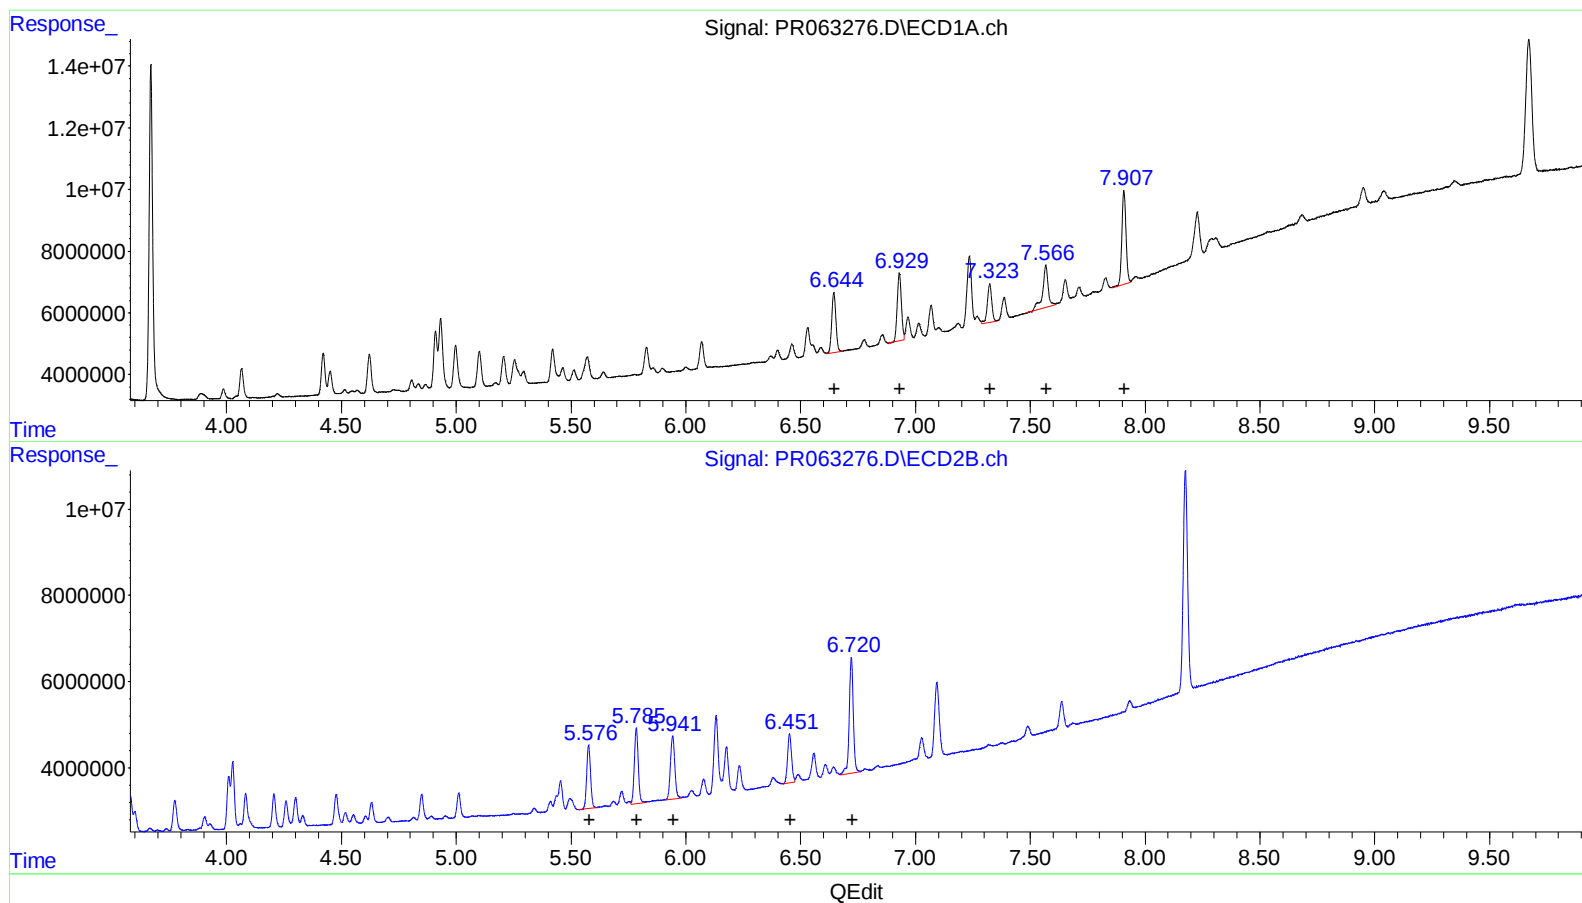

(31) AR-1260-1 (L7)
R.T. Response Conc
6.64 24664245 102.66
6.93 27871546 101.61
7.32 16591872 86.77
7.57 23421666 107.12
7.91 37842510 87.44

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
5.58 17390253 98.02
5.78 20787692 97.66
5.94 19210295 96.45
6.45 13662952 83.44
6.72 33504108 84.64

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091323\
 Data File : PR063276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2023 23:41
 Operator : YP\AJ
 Sample : PB155447BS
 Misc :
 ALS Vial : 52 Sample Multiplier: 1


Instrument :
 ECD_R
 ClientSampleId :
 ALCS447

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/14/2023
 Supervised By :Ankita Jodhani 09/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 01:46:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091223CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 13 07:34:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

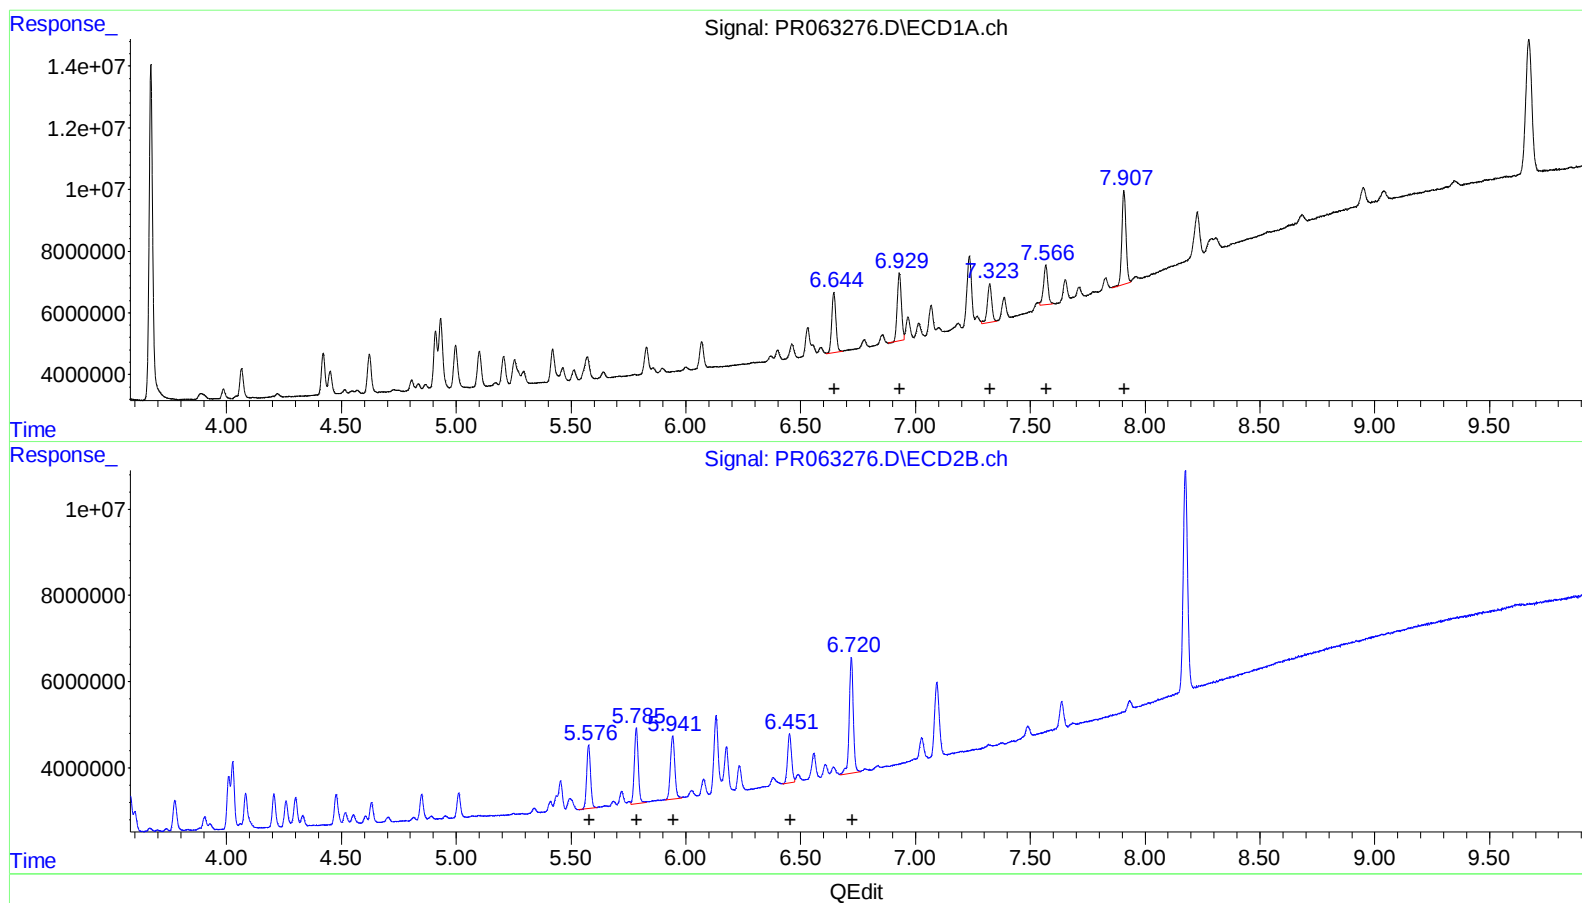

(31) AR-1260-1 #2 (L7)
 R.T. Response Conc
 6.64 24664245 102.66
 6.93 27871546 101.61
 7.32 16591872 86.77
 7.57 16757950 76.64
 7.91 37842510 87.44

(31) AR-1260-1 #2 (L7)
 R.T. Response Conc
 5.58 17390253 98.02
 5.78 20787692 97.66
 5.94 19210295 96.45
 6.45 13662952 83.44
 6.72 33504108 84.64