

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR091523\  
Data File : PR063343.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 15 Sep 2023 14:00  
Operator : YP\AJ  
Sample : 04380-18  
Misc :  
ALS Vial : 25 Sample Multiplier: 1


Instrument :  
ECD\_R  
ClientSampleId :  
BH4N9

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/18/2023  
Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 15 15:00:39 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR091223CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Sep 13 07:34:49 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

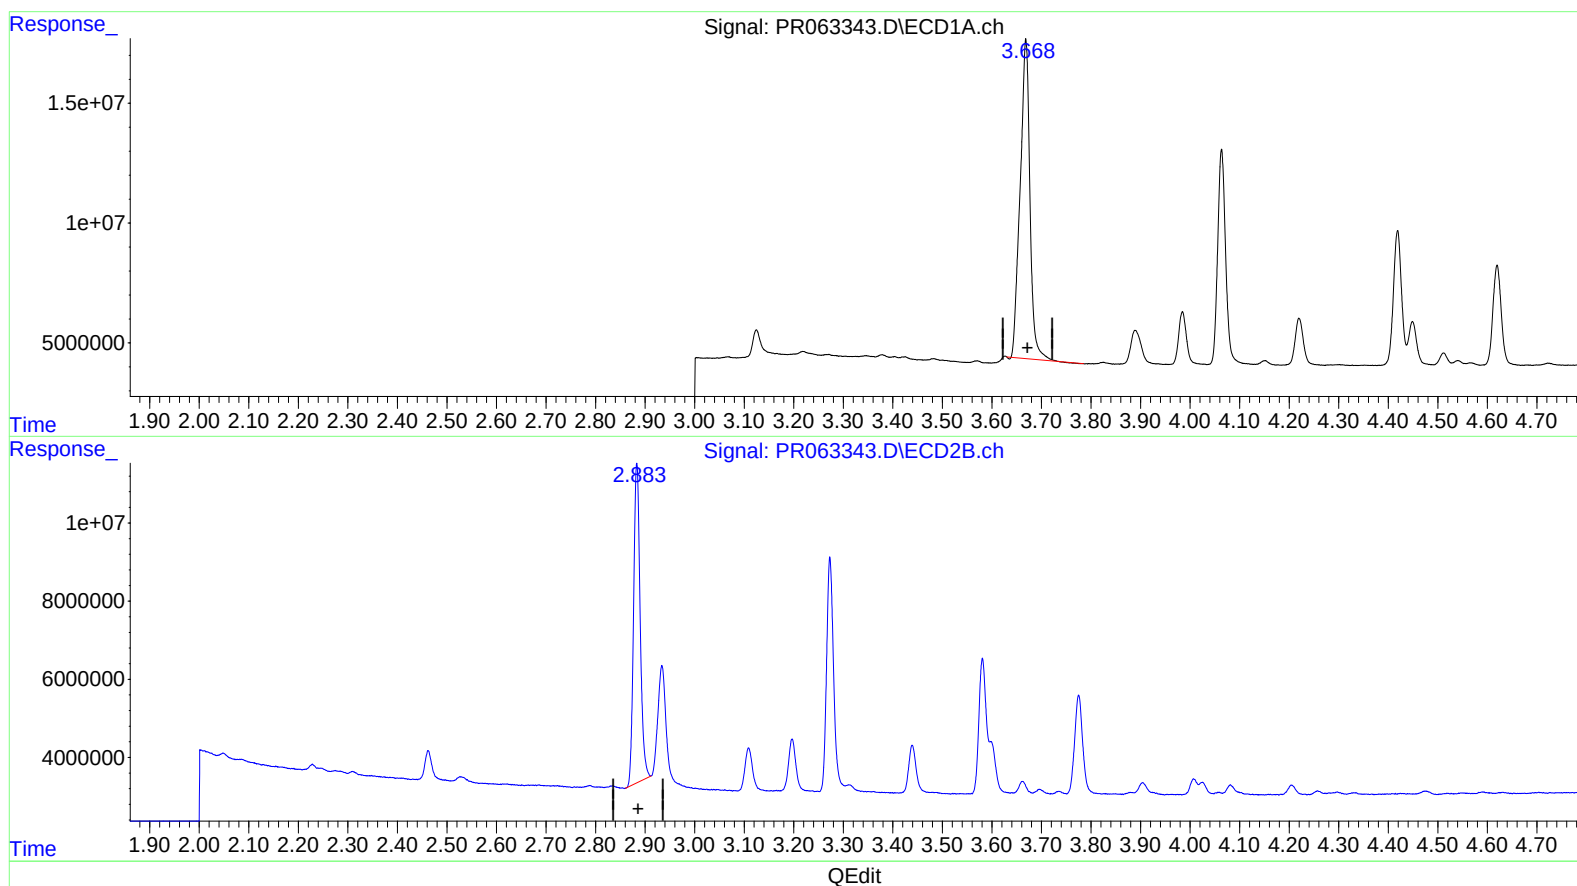

(1) Tetrachloro-m-xylene (SA)

3.669min 28.189 ng/ml

response 182943944

(1) Tetrachloro-m-xylene #2 (SA)

2.884min 22.052 ng/ml

response 75387371

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR091523\  
Data File : PR063343.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 15 Sep 2023 14:00  
Operator : YP\AJ  
Sample : 04380-18  
Misc :  
ALS Vial : 25 Sample Multiplier: 1



Instrument :  
ECD\_R  
ClientSampleId :  
BH4N9

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/18/2023  
Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 15 15:00:39 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR091223CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Sep 13 07:34:49 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

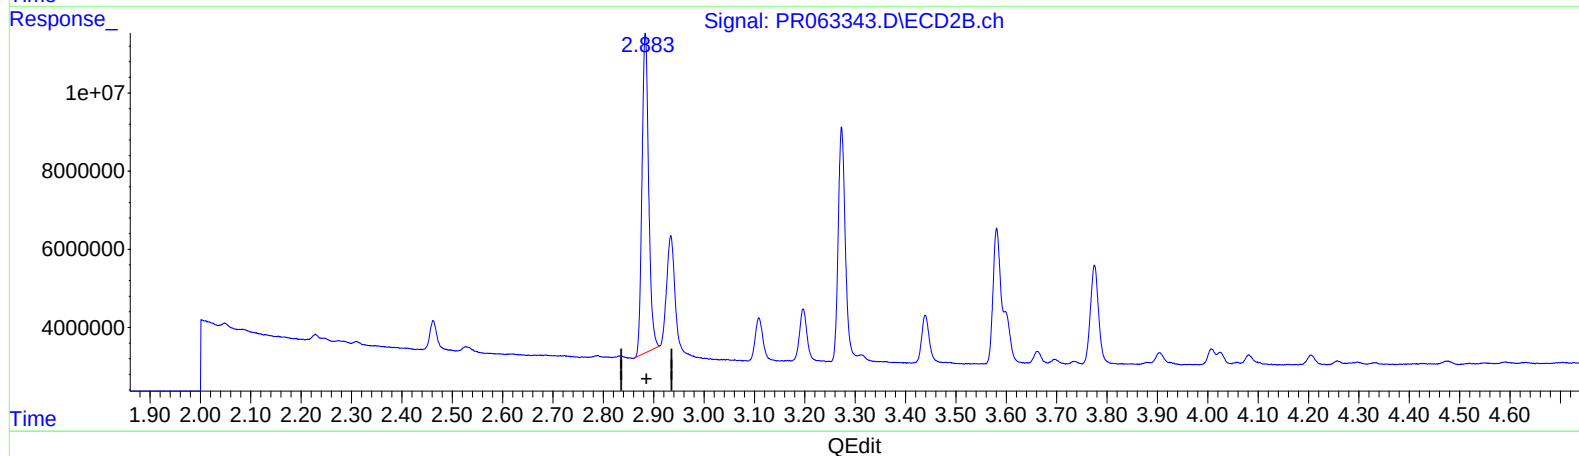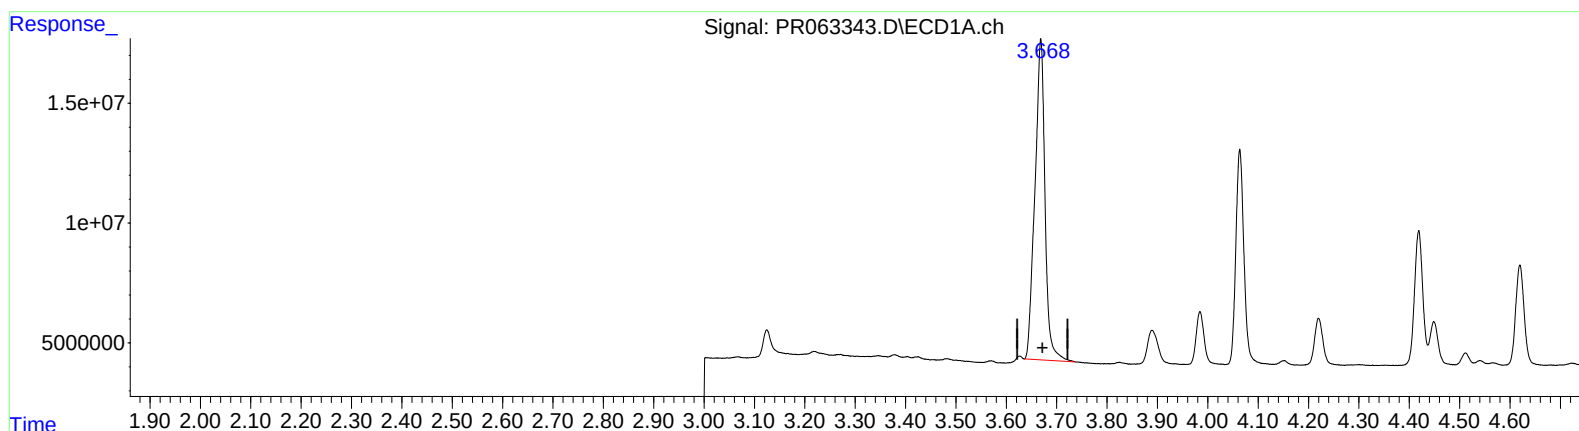

(1) Tetrachloro-m-xylene (SA)

3.668min 28.715 ng/ml m

response 186356837

(1) Tetrachloro-m-xylene #2 (SA)

2.884min 22.052 ng/ml

response 75387371