

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091619\
 Data File : PR041146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 20:04
 Operator : SM\AJ
 Sample : K4875-22
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 C0AR5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:29:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:01:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.724	3.992	44997326	195.6E6	14.642	14.689
2)	SA Decachlor...	10.643	9.116	109.0E6	341.0E6	39.168	34.884
Target Compounds							
9)	L2 AR-1221-2	0.000	4.297	0	1170107	N.D.	15.238 #
20)	L4 AR-1242-5	0.000	5.946f	0	3949031	N.D.	17.219 #
25)	L5 AR-1248-5	0.000	5.946	0	3949031	N.D.	12.496 #
26)	L6 AR-1254-1	0.000	5.946f	0	3949031	N.D.	8.248 #
28)	L6 AR-1254-3	0.000	6.457	0	15675476	N.D.	20.838 #
29)	L6 AR-1254-4	0.000	6.677	0	2056881	N.D.	3.934 #
31)	L7 AR-1260-1	0.000	6.609	0	6058895	N.D.	11.893 #
32)	L7 AR-1260-2	0.000	6.758	0	1548174	N.D.	2.435 #
45)	L9 AR-1268-5	0.000	8.830	0	2000093	N.D.	0.542 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091619\
Data File : PR041146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2019 20:04
Operator : SM\AJ
Sample : K4875-22
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
C0AR5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:29:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:01:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

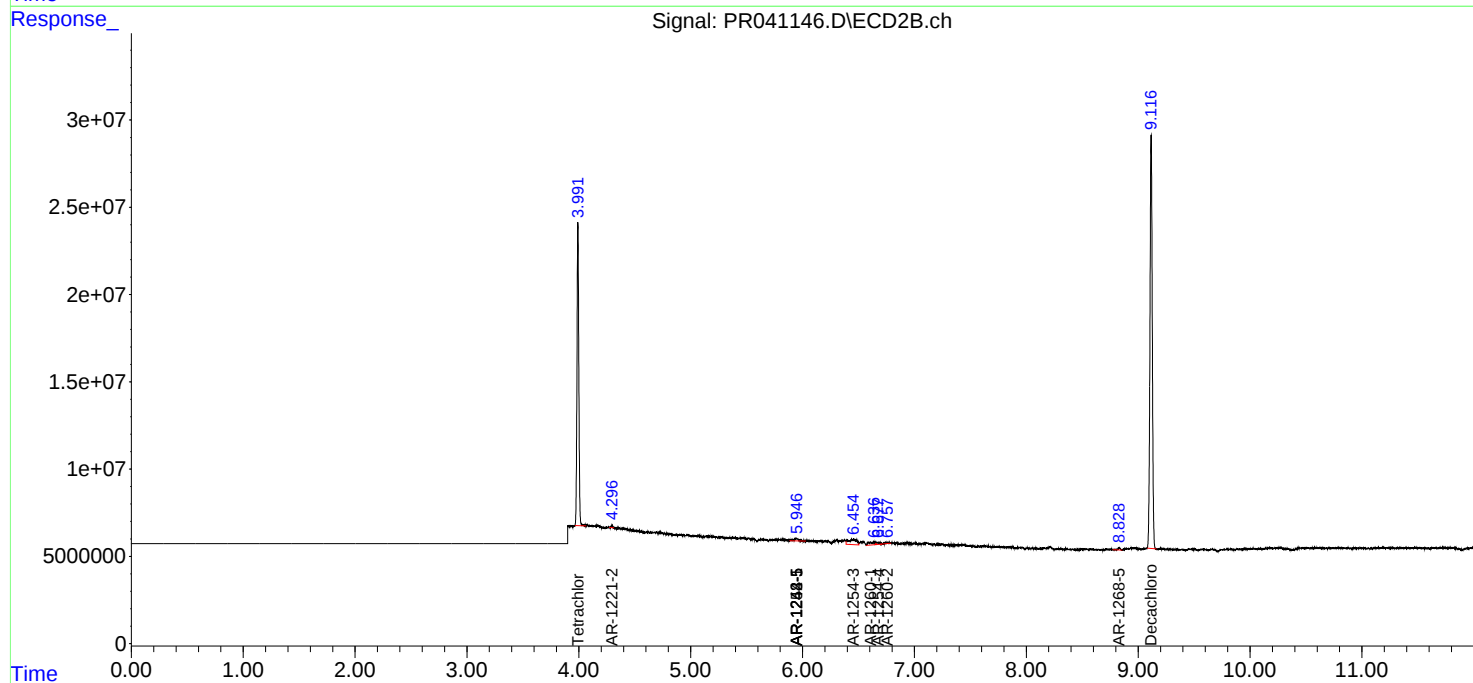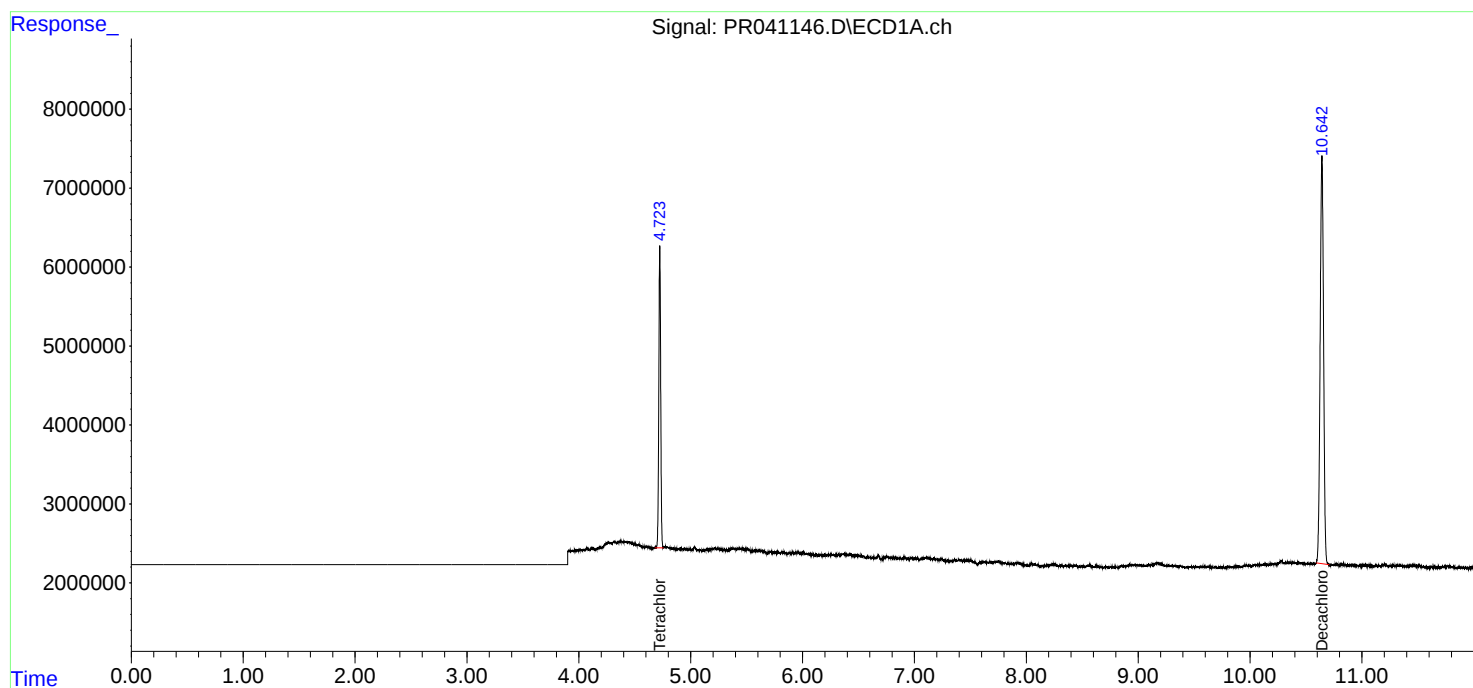


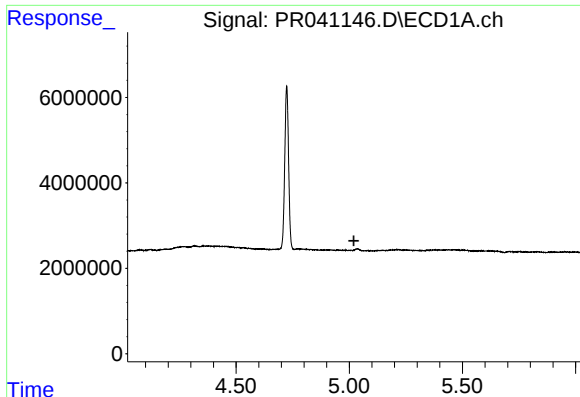

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AR5

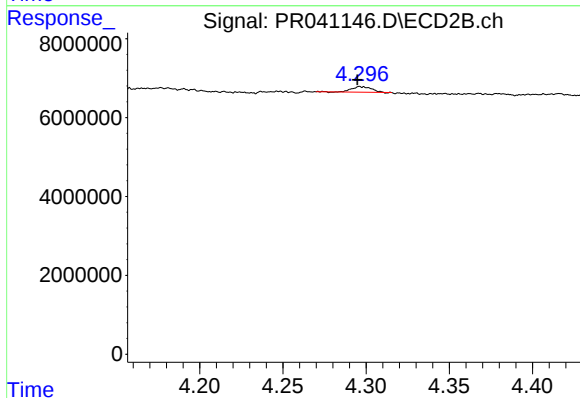


#9 AR-1221-2

R.T.: 4.297 min
Delta R.T.: 0.002 min
Response: 1170107
Conc: 15.24 ng/ml

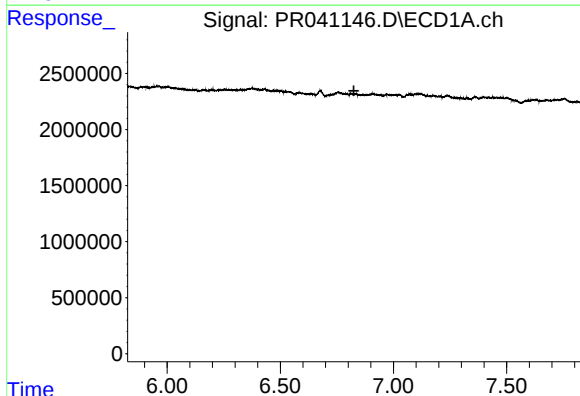


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

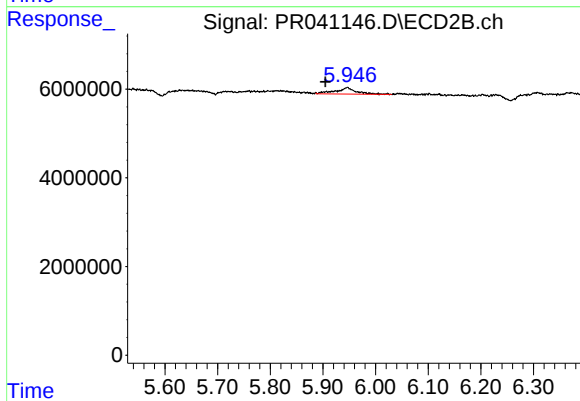

#20 AR-1242-5


R.T.: 5.946 min
Delta R.T.: 0.041 min
Response: 3949031
Conc: 17.22 ng/ml

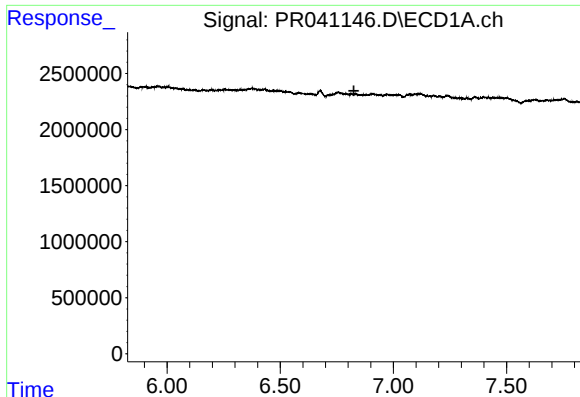

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AR5

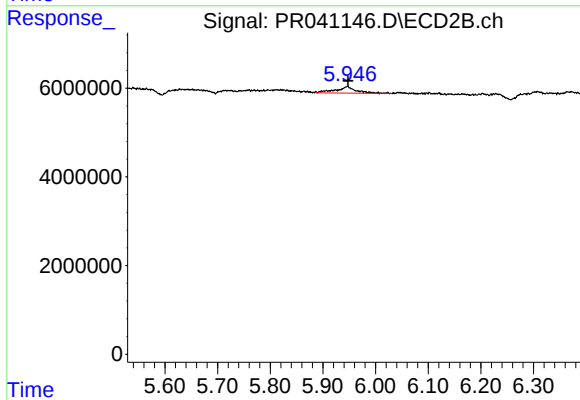


#25 AR-1248-5

R.T.: 5.946 min
Delta R.T.: -0.001 min
Response: 3949031
Conc: 12.50 ng/ml

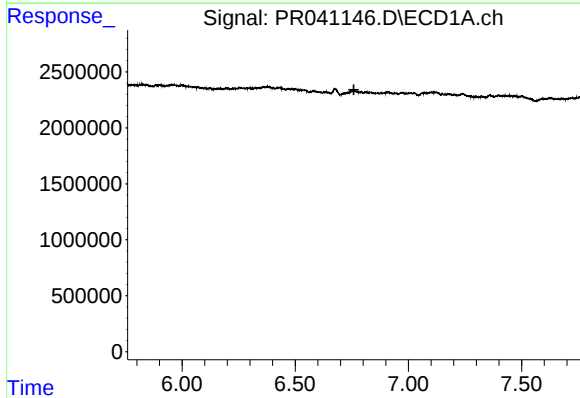


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.759 min
Response: 0
Conc: N.D.

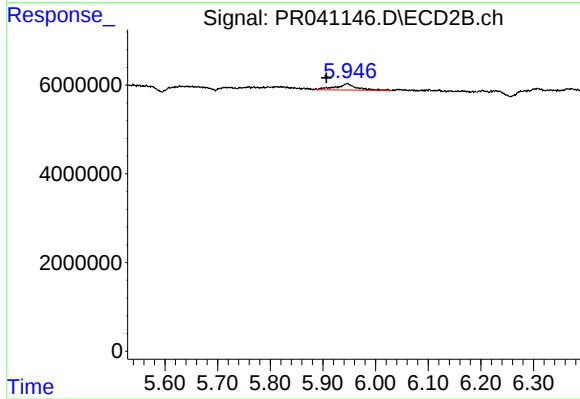

#26 AR-1254-1


R.T.: 5.946 min
Delta R.T.: 0.040 min
Response: 3949031
Conc: 8.25 ng/ml

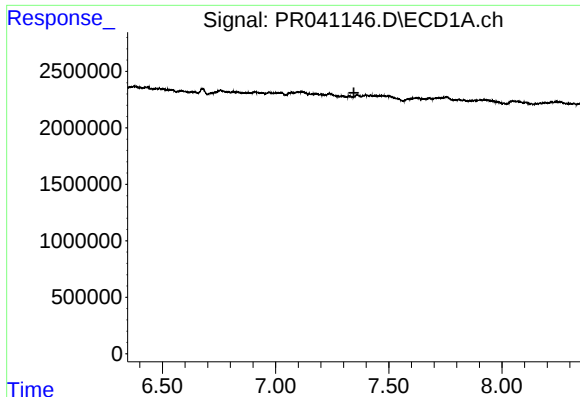

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AR5

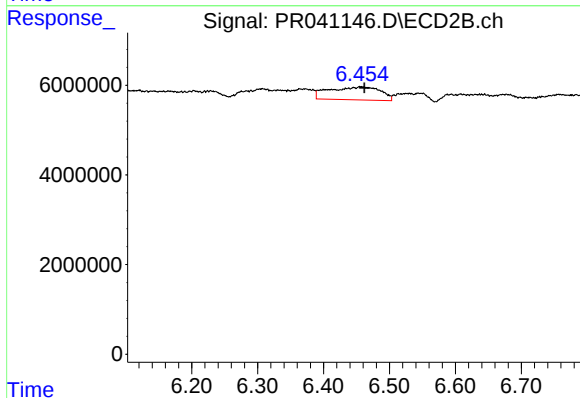


#28 AR-1254-3

R.T.: 6.457 min
Delta R.T.: -0.005 min
Response: 15675476
Conc: 20.84 ng/ml

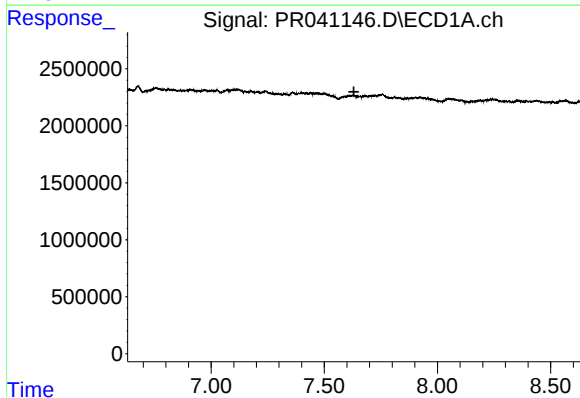


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.631 min
Response: 0
Conc: N.D.

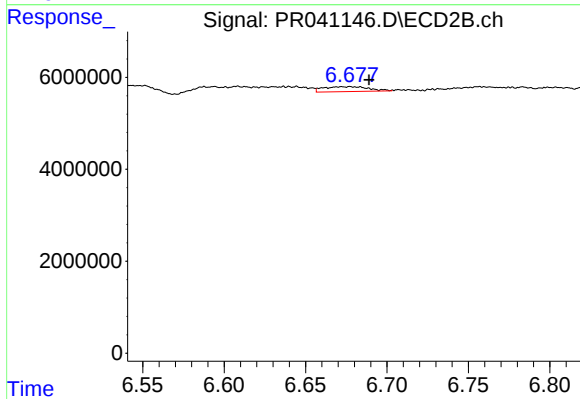

#29 AR-1254-4


R.T.: 6.677 min
Delta R.T.: -0.012 min
Response: 2056881
Conc: 3.93 ng/ml

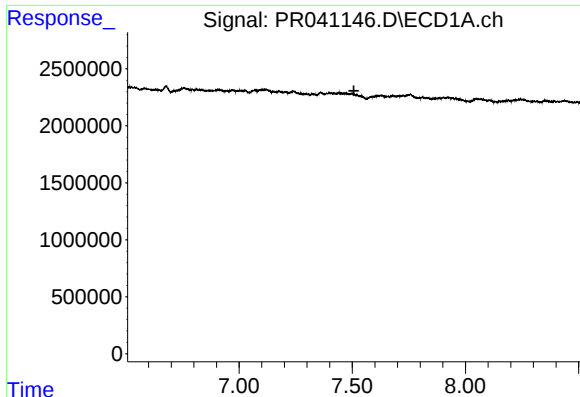

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AR5

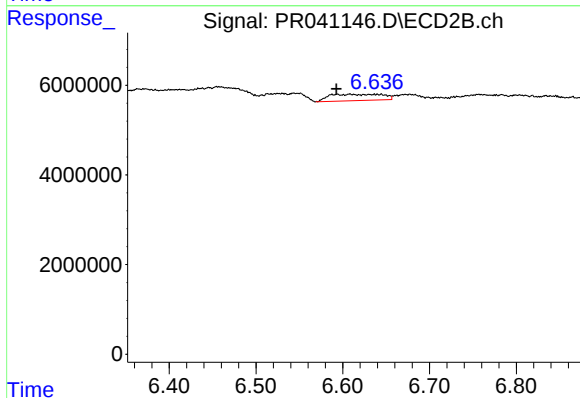


#31 AR-1260-1

R.T.: 6.609 min
Delta R.T.: 0.016 min
Response: 6058895
Conc: 11.89 ng/ml

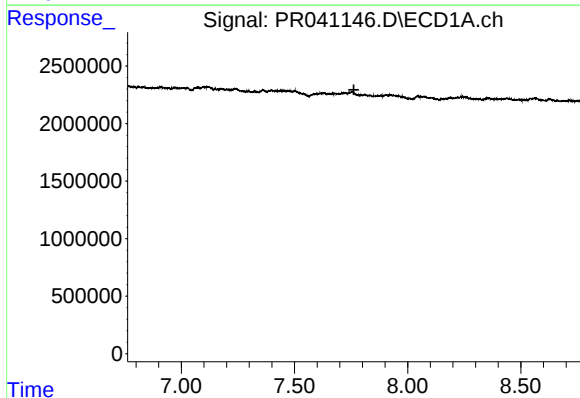


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.762 min
Response: 0
Conc: N.D.

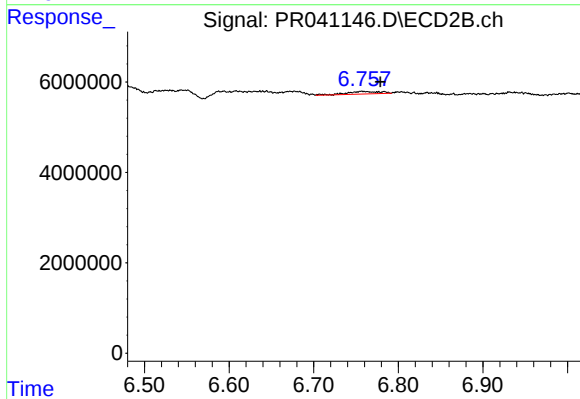

#32 AR-1260-2


R.T.: 6.758 min
Delta R.T.: -0.021 min
Response: 1548174
Conc: 2.44 ng/ml

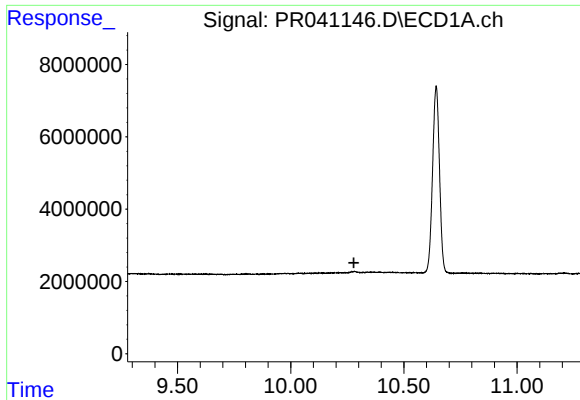

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
C0AR5

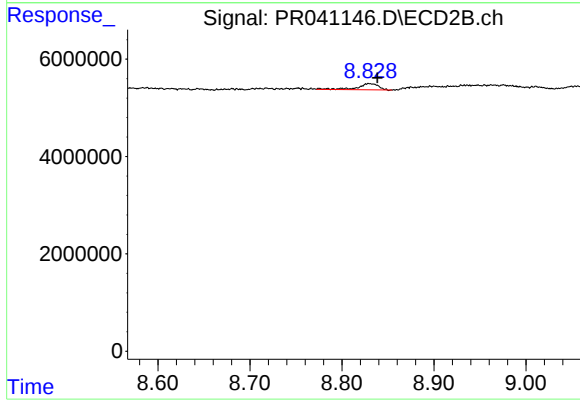

#45 AR-1268-5

R.T.: 8.830 min
Delta R.T.: -0.008 min
Response: 2000093
Conc: 0.54 ng/ml