

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091619\
 Data File : PR041203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2019 10:46
 Operator : SM\AJ
 Sample : AIBLK79
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 AIBLK79

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:38:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:01:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.723	3.991	72379407	289.3E6	23.551	21.726
2)	SA Decachlor...	10.645	9.115	98908446	305.0E6	35.539	31.208
Target Compounds							
7)	L1 AR-1016-5	0.000	5.554	0 11483427	N.D.	49.411	#
9)	L2 AR-1221-2	0.000	4.298	0 2468181	N.D.	32.141	#
15)	L3 AR-1232-5	0.000	5.554	0 11483427	N.D.	139.356	#
20)	L4 AR-1242-5	0.000	5.926	0 1978379	N.D.	8.626	#
24)	L5 AR-1248-4	0.000	5.554	0 11483427	N.D.	43.559	#
25)	L5 AR-1248-5	0.000	5.926	0 1978379	N.D.	6.260	#
26)	L6 AR-1254-1	0.000	5.926	0 1978379	N.D.	4.132	#
31)	L7 AR-1260-1	0.000	6.587	0 2913117	N.D.	5.718	#
45)	L9 AR-1268-5	0.000	8.831	0 2795931	N.D.	0.758	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091619\
Data File : PR041203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2019 10:46
Operator : SM\AJ
Sample : AIBLK79
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
AIBLK79

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:38:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:01:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

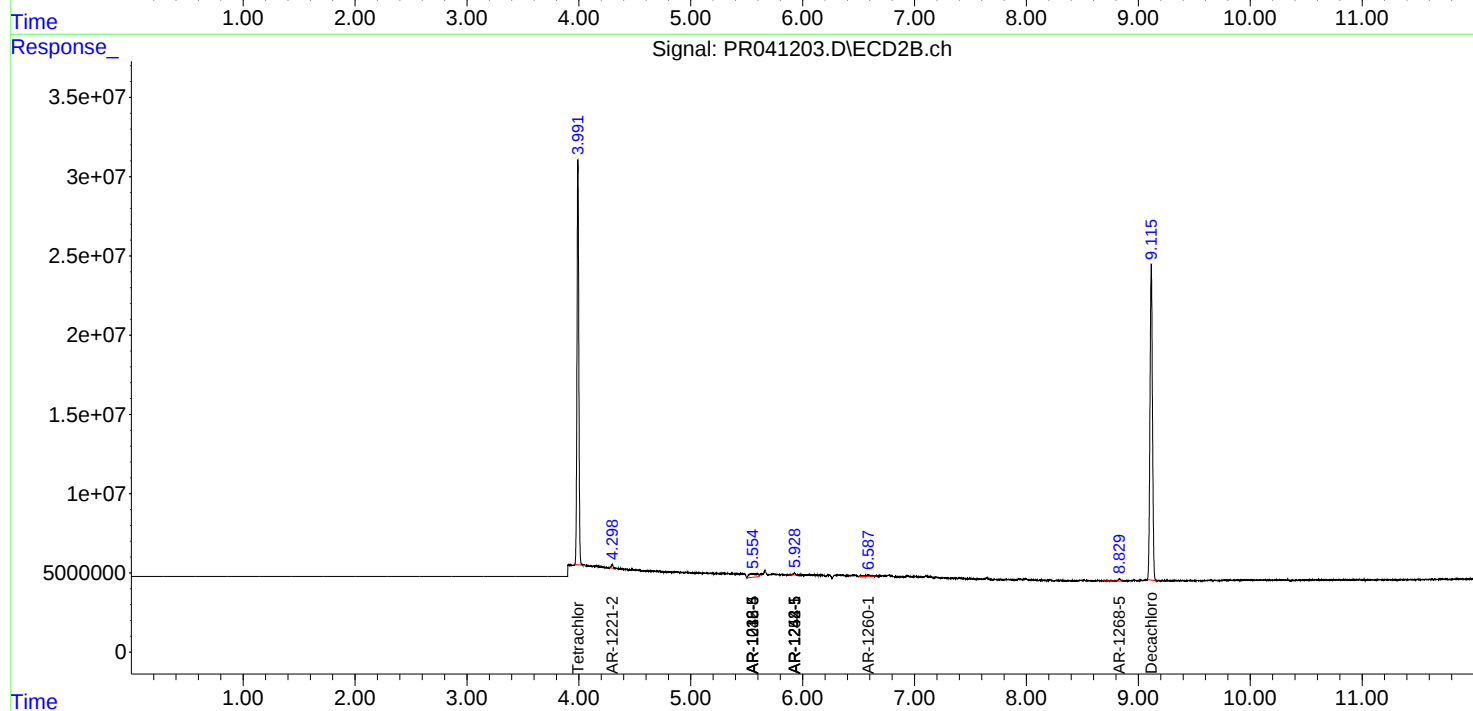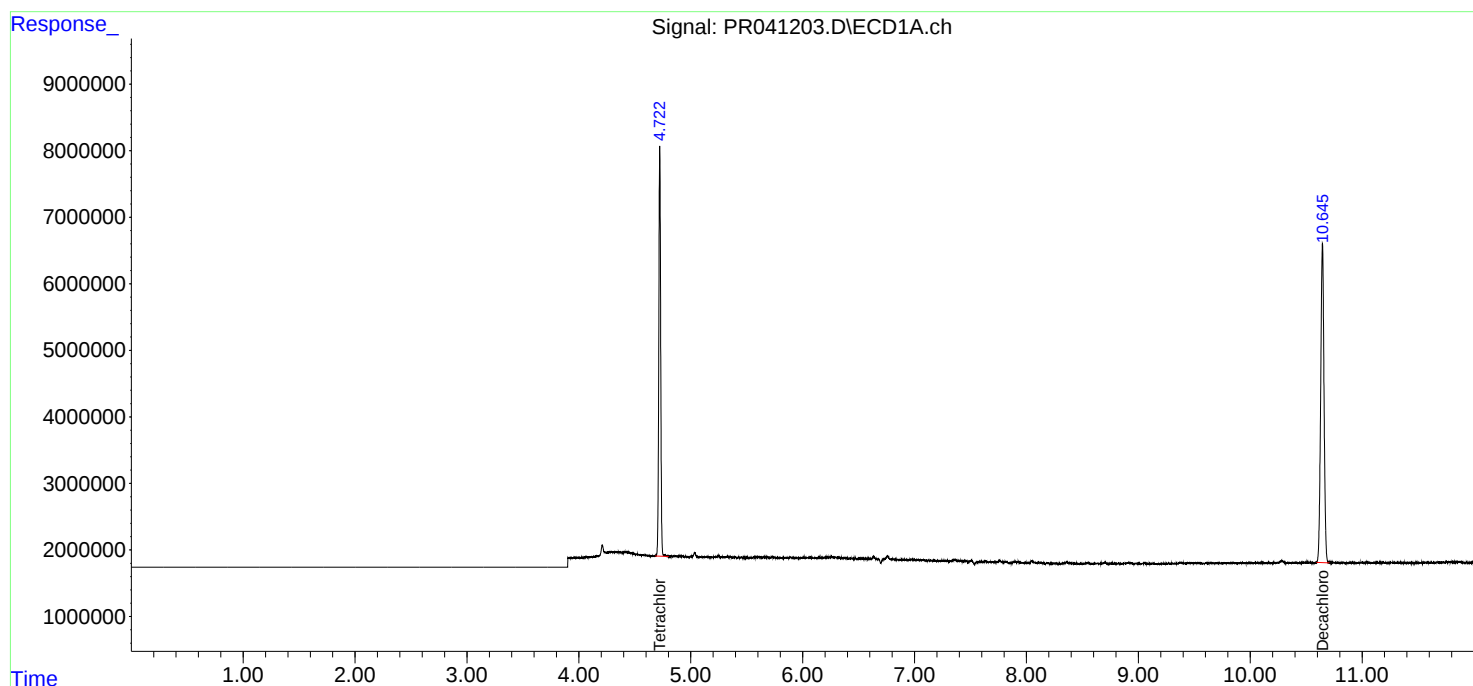


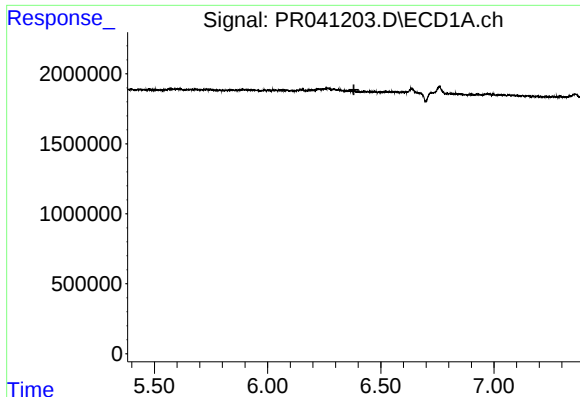

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.381 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK79

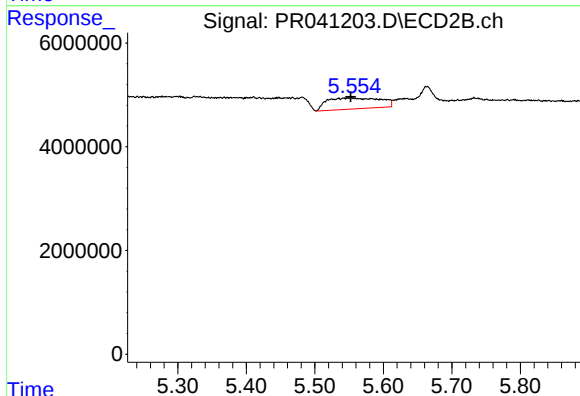


#7 AR-1016-5

R.T.: 5.554 min
Delta R.T.: 0.002 min
Response: 11483427
Conc: 49.41 ng/ml

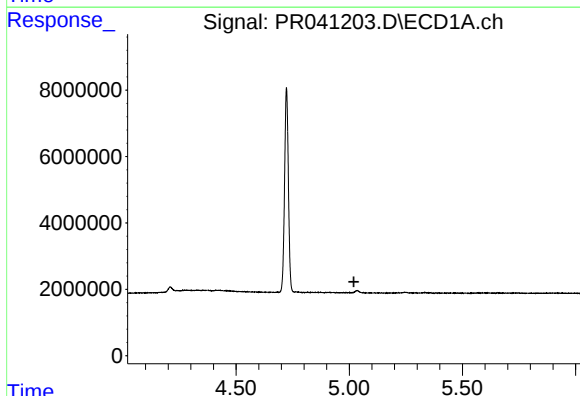


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.020 min
Response: 0
Conc: N.D.

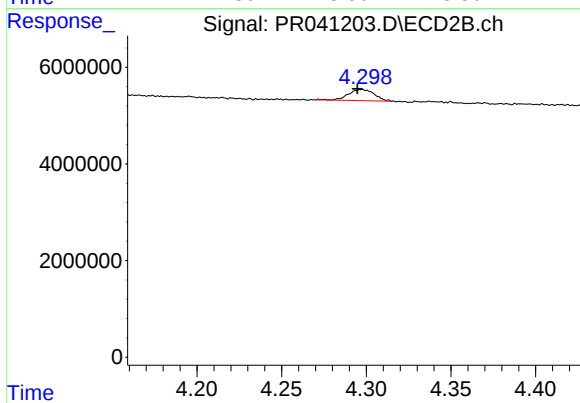

#9 AR-1221-2


R.T.: 4.298 min
Delta R.T.: 0.003 min
Response: 2468181
Conc: 32.14 ng/ml

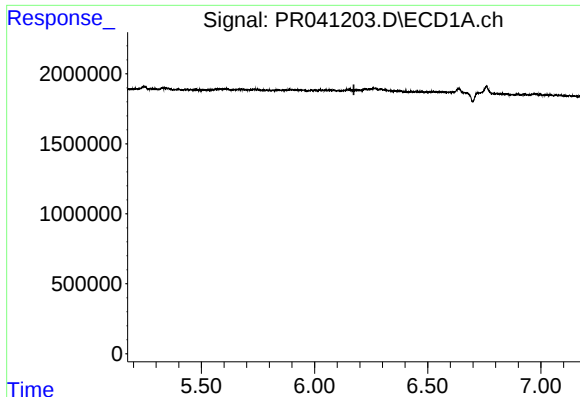

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 6.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK79

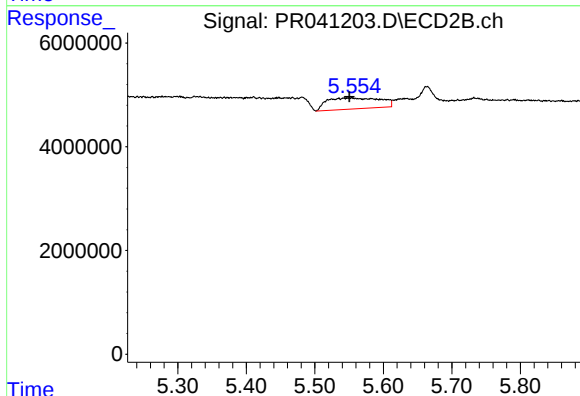


#15 AR-1232-5

R.T.: 5.554 min
Delta R.T.: 0.004 min
Response: 11483427
Conc: 139.36 ng/ml

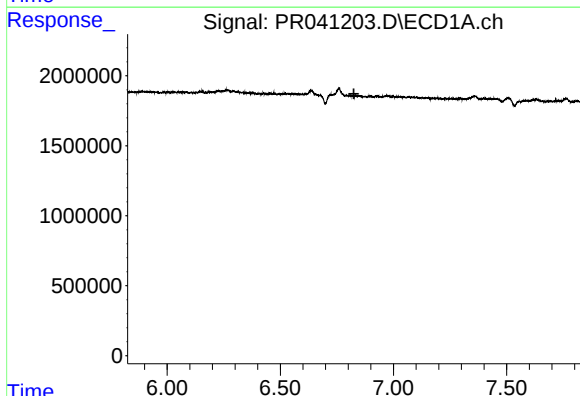


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

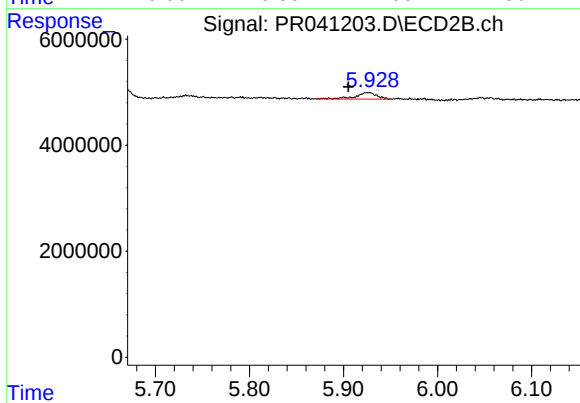

#20 AR-1242-5


R.T.: 5.926 min
Delta R.T.: 0.021 min
Response: 1978379
Conc: 8.63 ng/ml

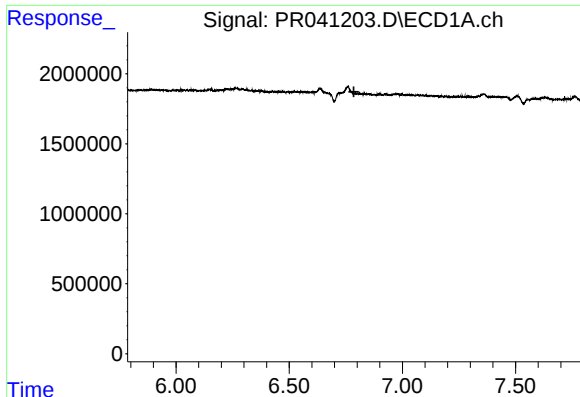

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.786 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK79

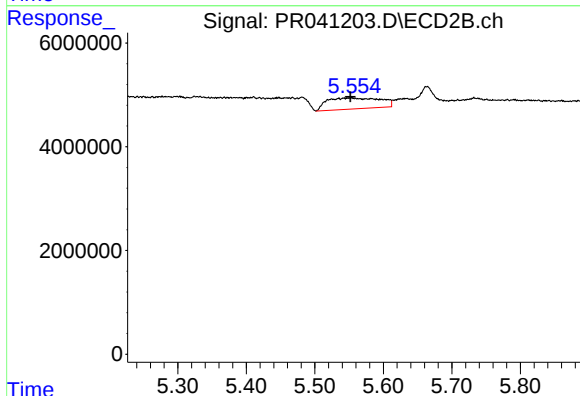


#24 AR-1248-4

R.T.: 5.554 min
Delta R.T.: 0.002 min
Response: 11483427
Conc: 43.56 ng/ml

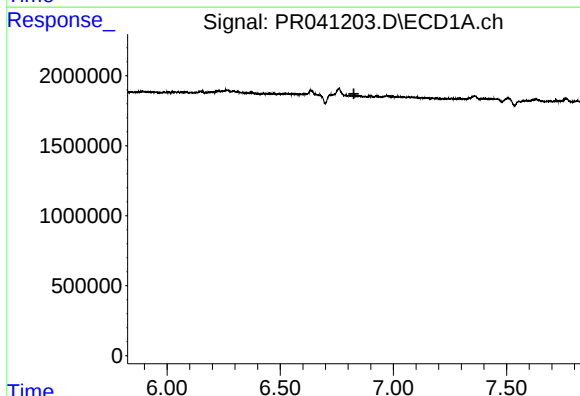


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.825 min
Response: 0
Conc: N.D.

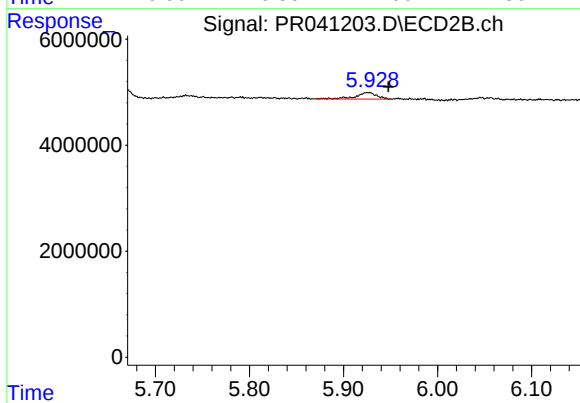

#25 AR-1248-5


R.T.: 5.926 min
Delta R.T.: -0.021 min
Response: 1978379
Conc: 6.26 ng/ml

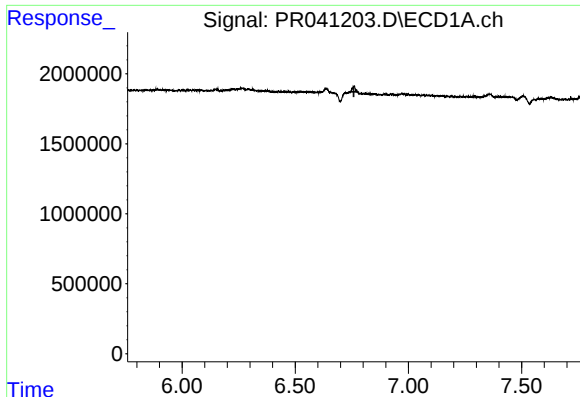

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.759 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK79

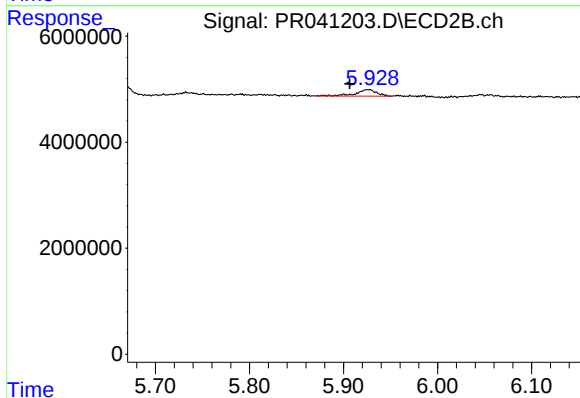


#26 AR-1254-1

R.T.: 5.926 min
Delta R.T.: 0.020 min
Response: 1978379
Conc: 4.13 ng/ml

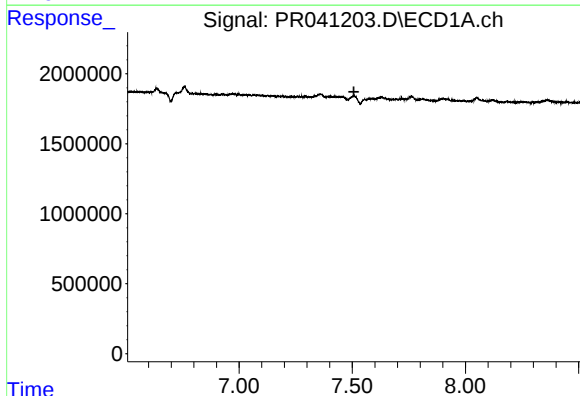


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 7.507 min
Response: 0
Conc: N.D.

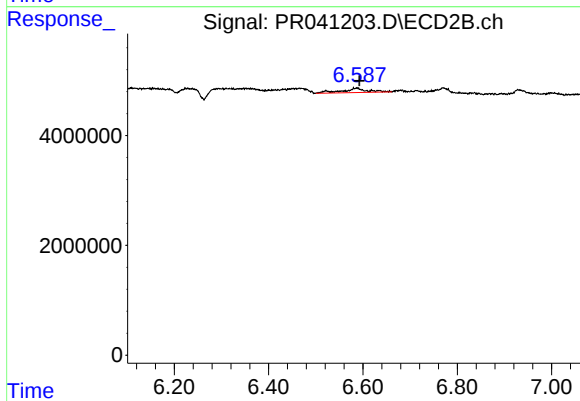

#31 AR-1260-1


R.T.: 6.587 min
Delta R.T.: -0.006 min
Response: 2913117
Conc: 5.72 ng/ml

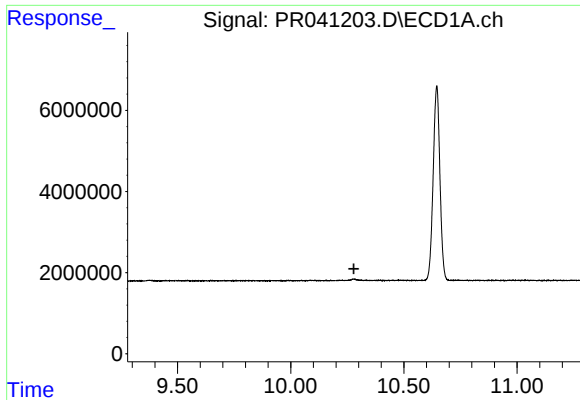

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK79

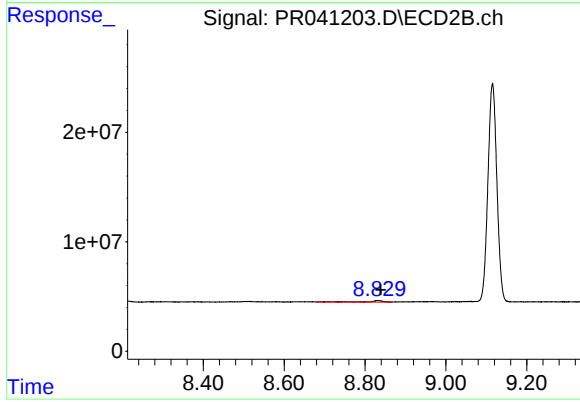

#45 AR-1268-5

R.T.: 8.831 min
Delta R.T.: -0.008 min
Response: 2795931
Conc: 0.76 ng/ml