

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092019\
 Data File : PR041280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2019 08:08
 Operator : SM\AJ
 Sample : AIBLK87
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 AIBLK87

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 11:07:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:01:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.726	3.992	72492802	313.6E6	23.588	23.551
2)	SA Decachlor...	10.649	9.115	101.0E6	330.5E6	36.299	33.815
Target Compounds							
9)	L2 AR-1221-2	0.000	4.297	0	2771924	N.D.	36.097 #
20)	L4 AR-1242-5	6.761f	0.000	461839	0	7.329	N.D. #
25)	L5 AR-1248-5	6.761f	0.000	461839	0	4.211	N.D. #
26)	L6 AR-1254-1	6.761	0.000	461839	0	3.768	N.D. #
28)	L6 AR-1254-3	0.000	6.458	0	13475101	N.D.	17.913 #
31)	L7 AR-1260-1	0.000	6.587	0	4233240	N.D.	8.309 #
35)	L7 AR-1260-5	0.000	7.643	0	2142818	N.D.	1.647 #
37)	L8 AR-1262-2	0.000	7.643	0	2142818	N.D.	1.373 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092019\
Data File : PR041280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2019 08:08
Operator : SM\AJ
Sample : AIBLK87
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
AIBLK87

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 11:07:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:01:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

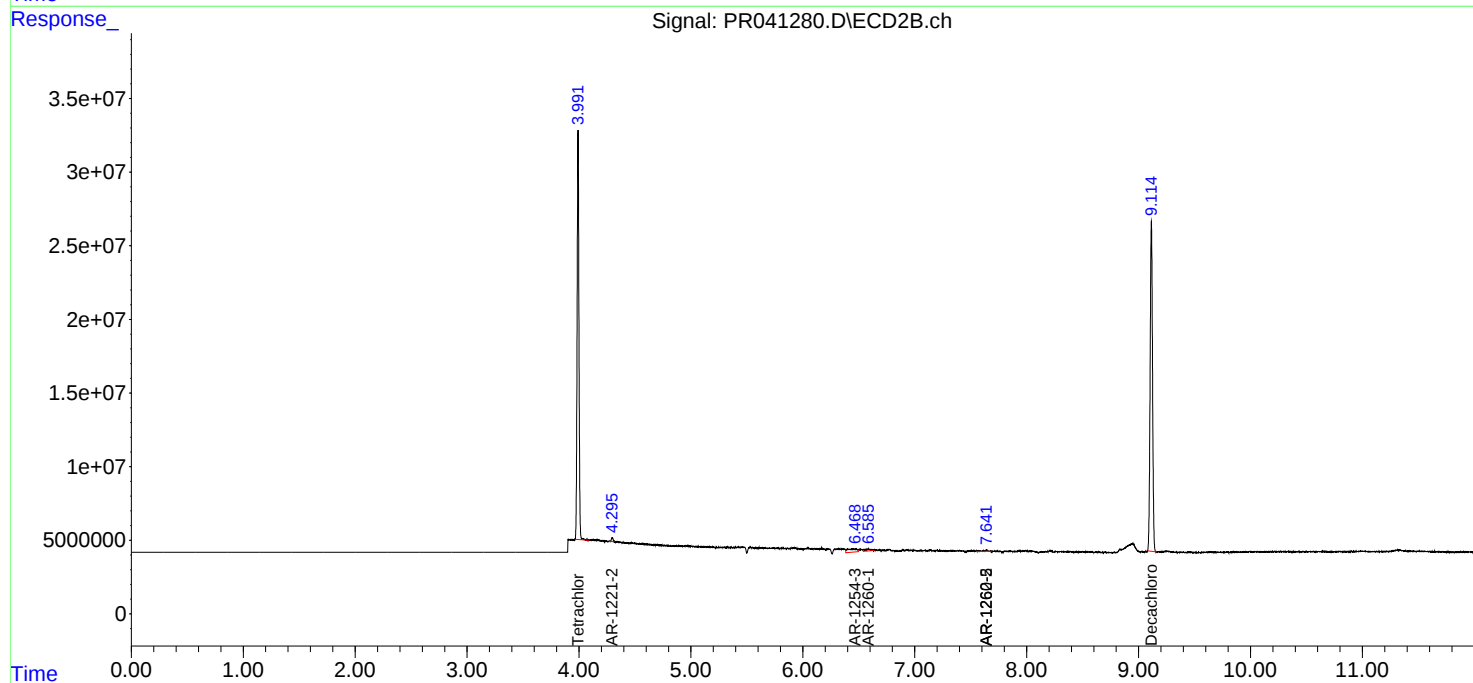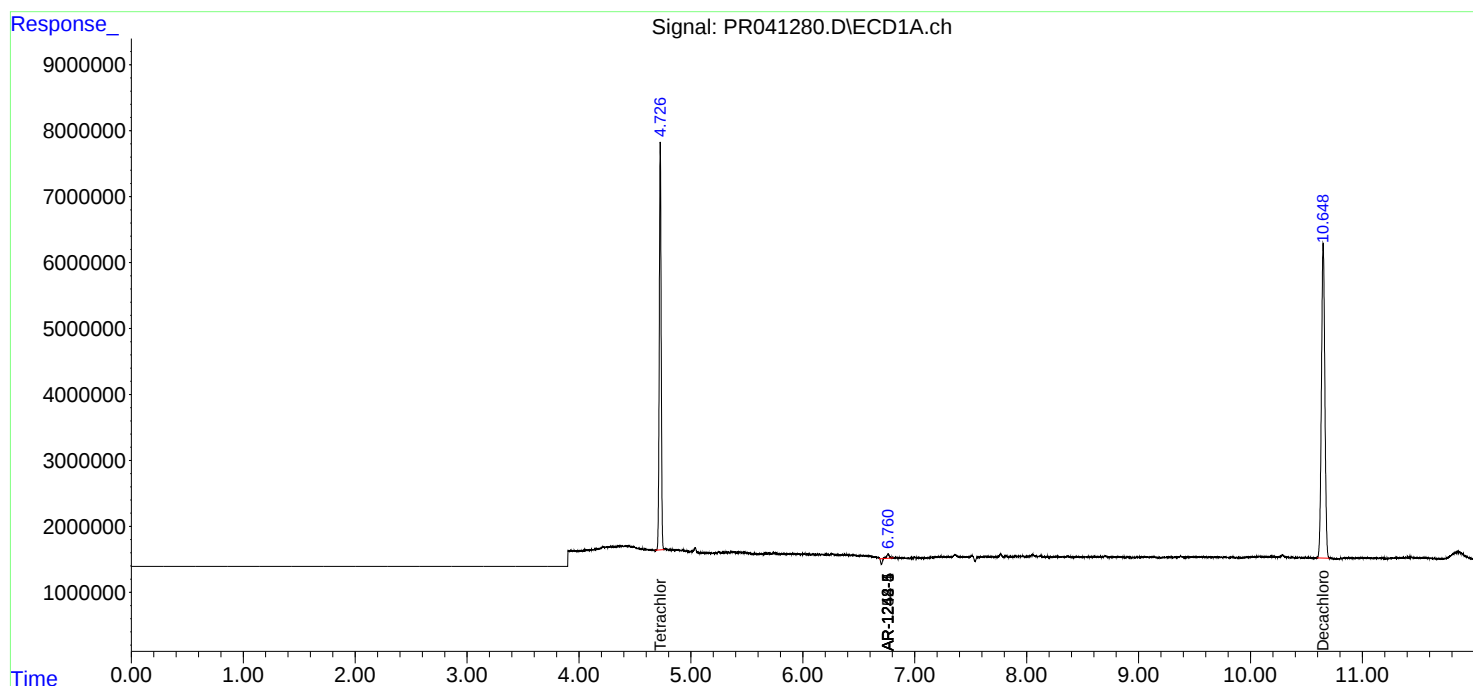


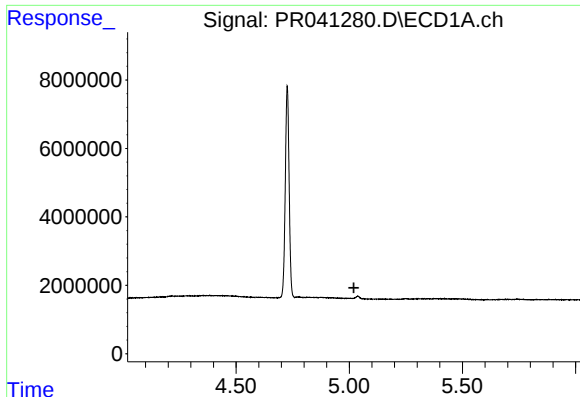

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK87

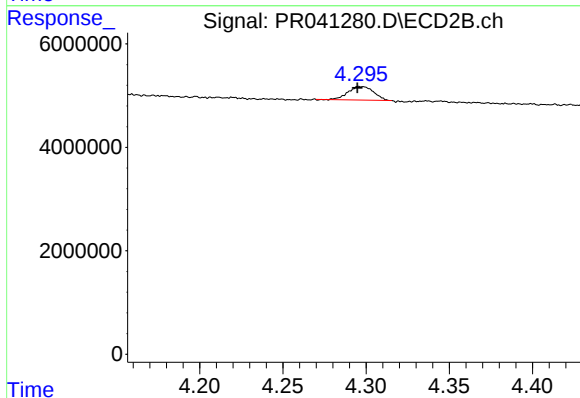


#9 AR-1221-2

R.T.: 4.297 min
Delta R.T.: 0.002 min
Response: 2771924
Conc: 36.10 ng/ml

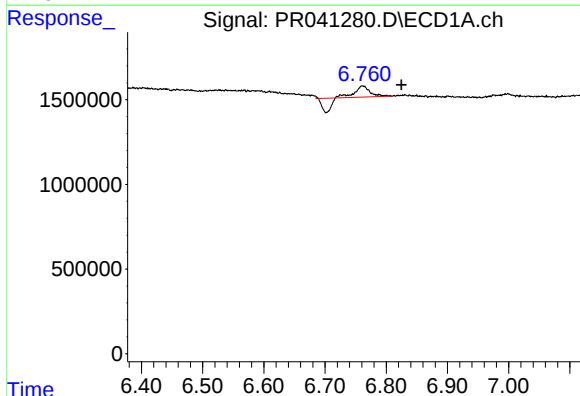


#20 AR-1242-5

R.T.: 6.761 min
Delta R.T.: -0.064 min
Response: 461839
Conc: 7.33 ng/ml

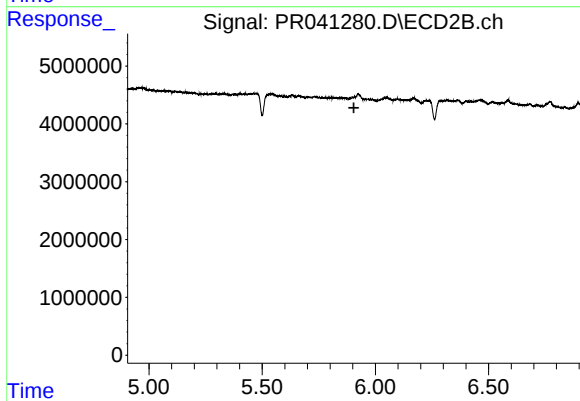

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 5.905 min
Response: 0
Conc: N.D.

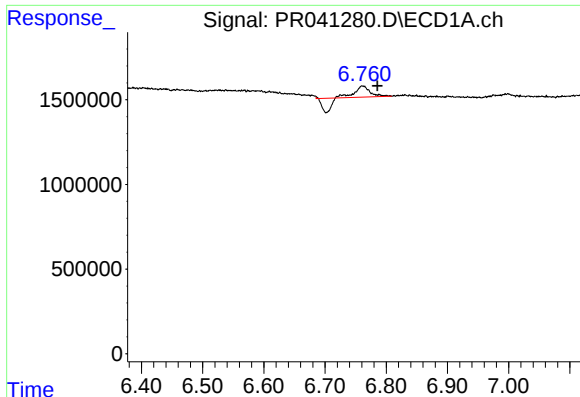

#24 AR-1248-4


R.T.: 6.761 min
Delta R.T.: -0.025 min
Response: 461839
Conc: 3.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK87

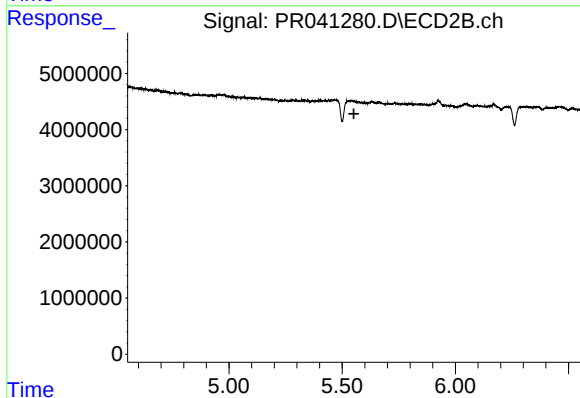


#24 AR-1248-4

R.T.: 5.540 min
Delta R.T.: -0.012 min
Response: -1055708
Conc: N.D.

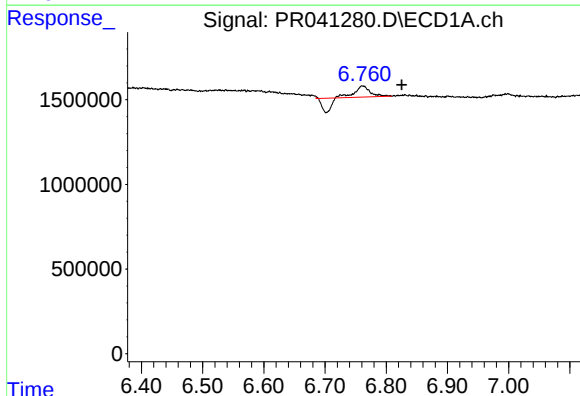


#25 AR-1248-5

R.T.: 6.761 min
Delta R.T.: -0.064 min
Response: 461839
Conc: 4.21 ng/ml

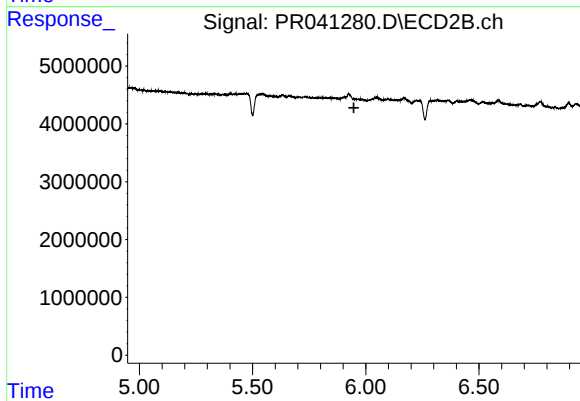

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.948 min
Response: 0
Conc: N.D.

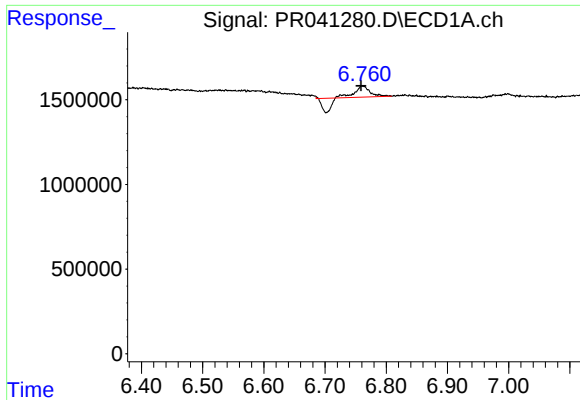

#26 AR-1254-1


R.T.: 6.761 min
Delta R.T.: 0.002 min
Response: 461839
Conc: 3.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK87

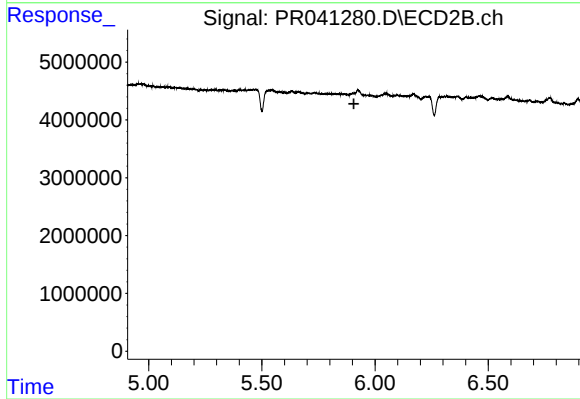


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.907 min
Response: 0
Conc: N.D.

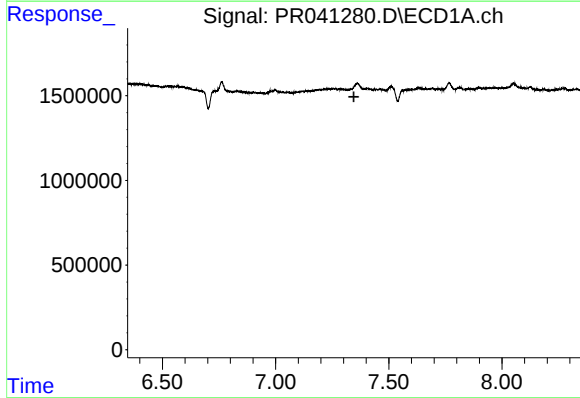


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 7.346 min
Response: 0
Conc: N.D.

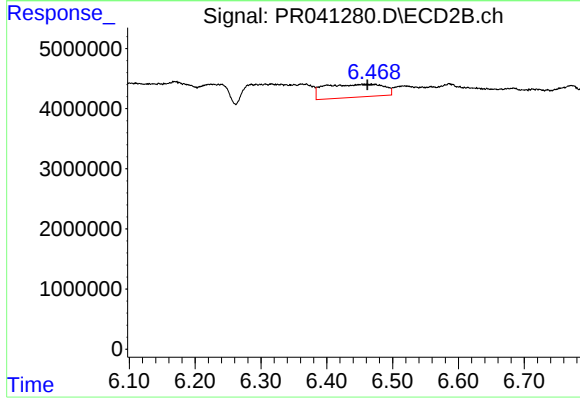

#28 AR-1254-3


R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 13475101
Conc: 17.91 ng/ml

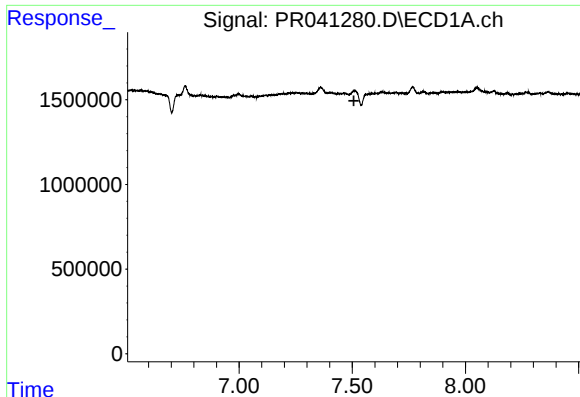

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK87

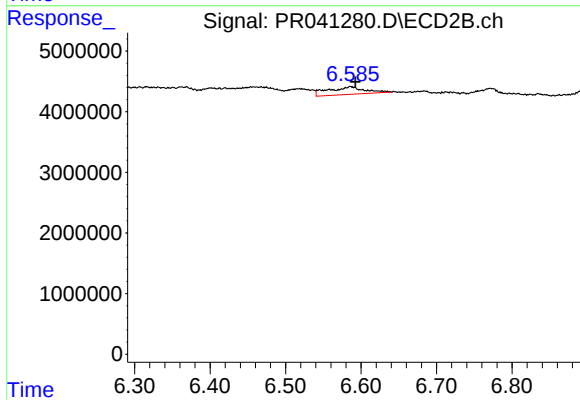


#31 AR-1260-1

R.T.: 6.587 min
Delta R.T.: -0.006 min
Response: 4233240
Conc: 8.31 ng/ml

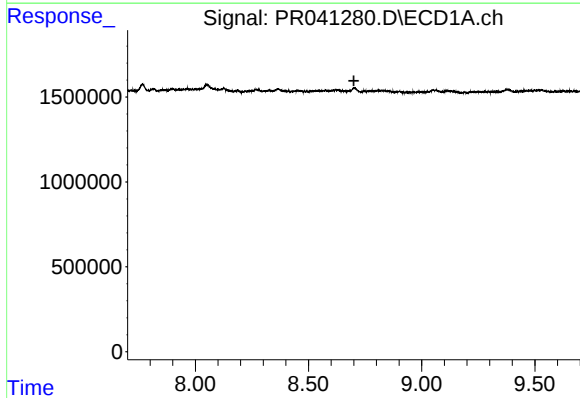


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.701 min
Response: 0
Conc: N.D.

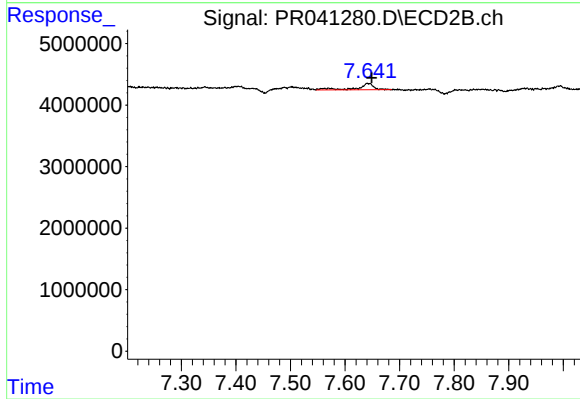

#35 AR-1260-5


R.T.: 7.643 min
Delta R.T.: -0.006 min
Response: 2142818
Conc: 1.65 ng/ml

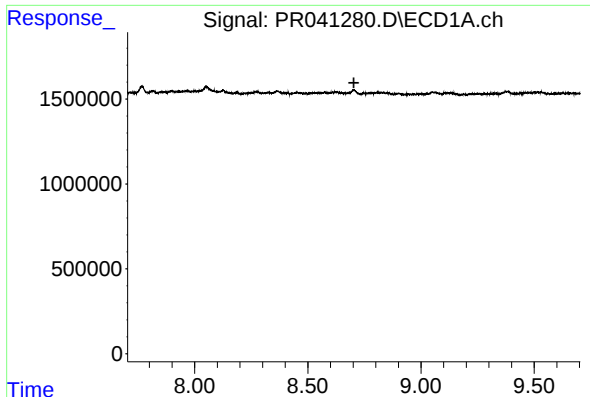

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK87

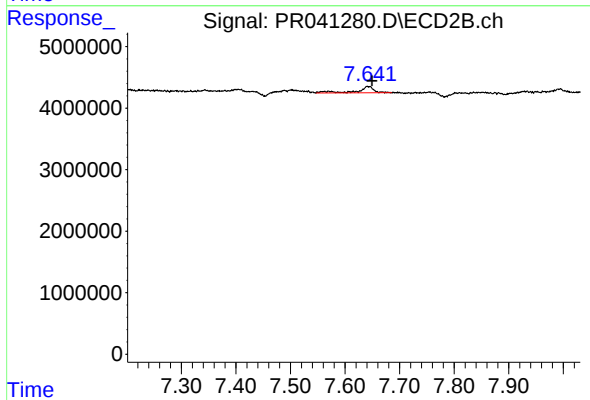

#37 AR-1262-2

R.T.: 7.643 min
Delta R.T.: -0.007 min
Response: 2142818
Conc: 1.37 ng/ml