

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092122\
 Data File : PR056915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2022 20:56
 Operator : AJ\MA
 Sample : N4720-02 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 ORA-0094

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2022
 Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 00:14:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.620	2.890	6450796	2848329	1.343	1.625
2) SA Decachlor...	9.503	8.092	2812626	2468841	1.417	1.484m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092122\
Data File : PR056915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2022 20:56
Operator : AJ\MA
Sample : N4720-02 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
ORA-0094


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 00:14:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

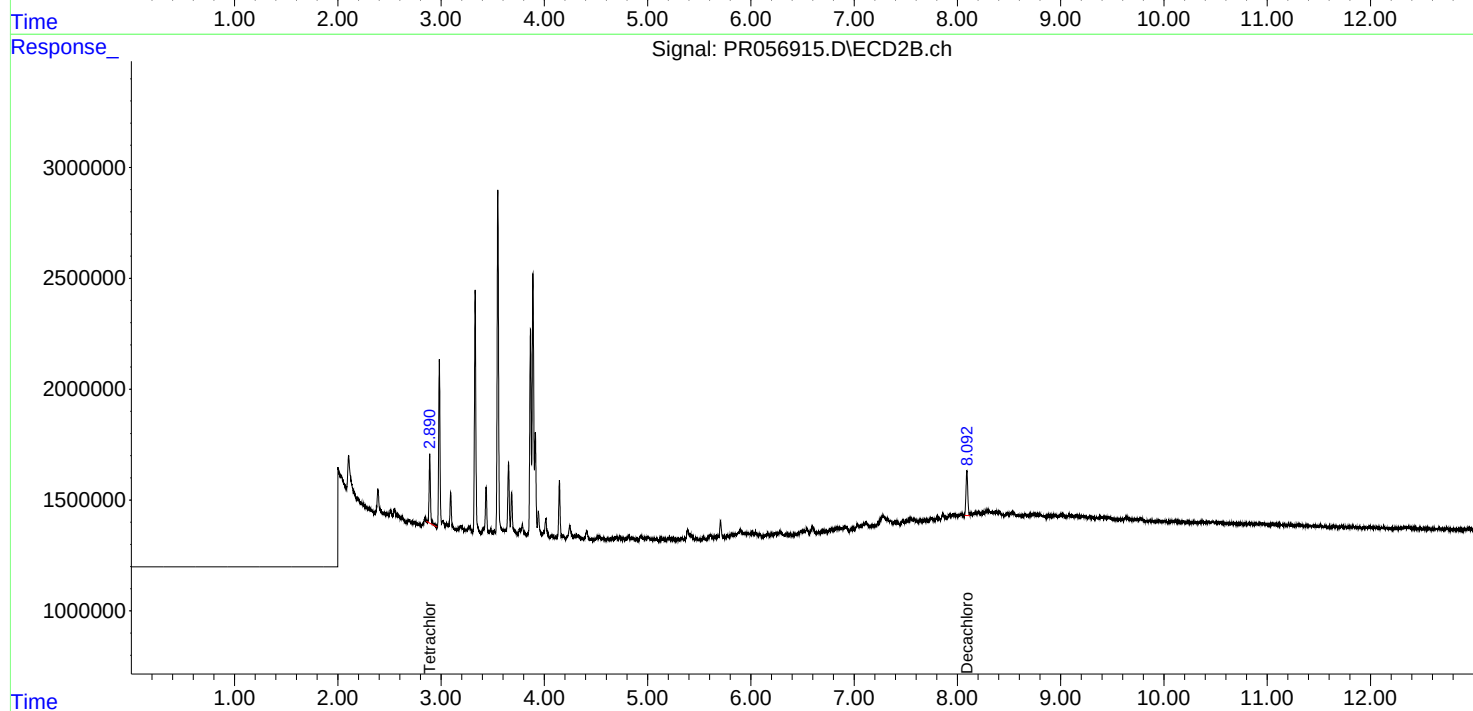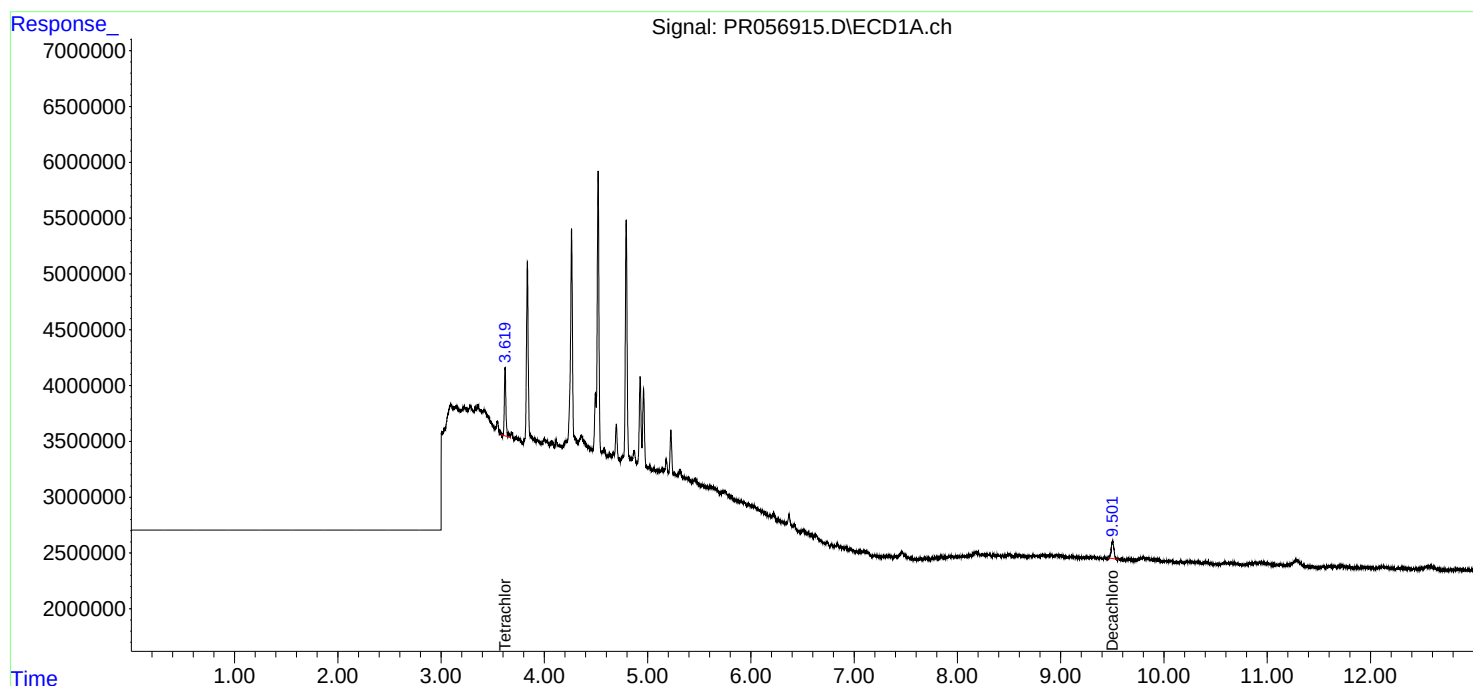

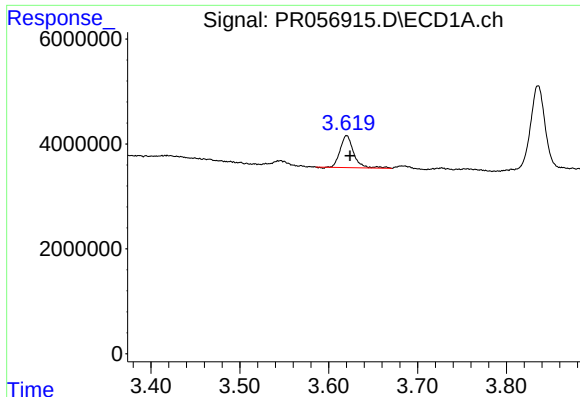


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.004 min
Response: 6450796
Conc: 1.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
ORA-0094


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

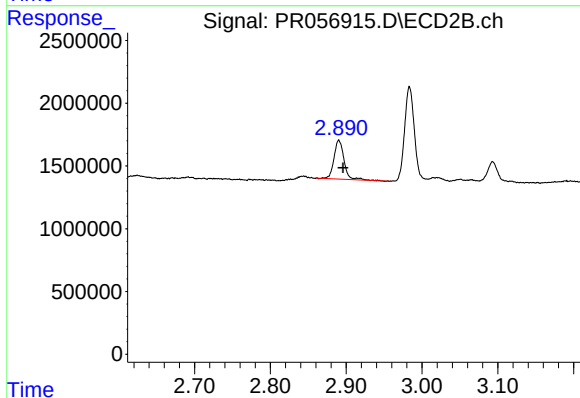


#1 Tetrachloro-m-xylene

R.T.: 2.890 min
Delta R.T.: -0.006 min
Response: 2848329
Conc: 1.63 ng/ml

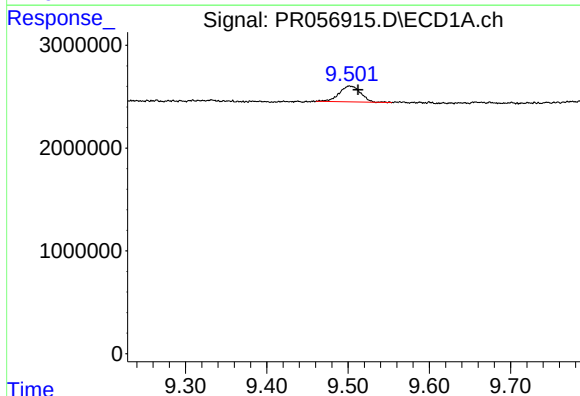

#2 Decachlorobiphenyl

R.T.: 9.503 min
Delta R.T.: -0.010 min
Response: 2812626
Conc: 1.42 ng/ml

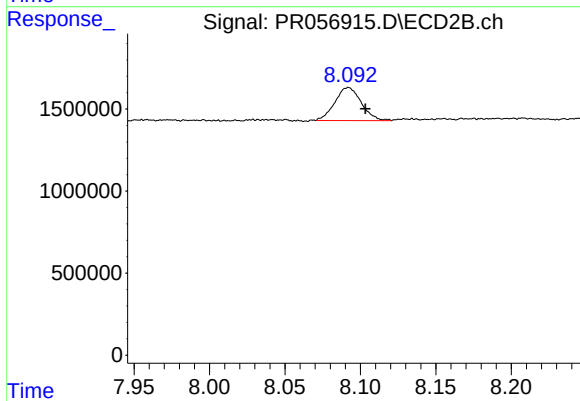

#2 Decachlorobiphenyl

R.T.: 8.092 min
Delta R.T.: -0.012 min
Response: 2468841
Conc: 1.48 ng/ml m