

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092122\
 Data File : PR056916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2022 21:12
 Operator : AJ\MA
 Sample : N4720-03 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 ORA-0135

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2022
 Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 00:14:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.614	2.888	8802899	5753337	1.832m	3.282m#
2) SA Decachlor...	9.508	8.094	3757487	2092084	1.894	1.257m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092122\
Data File : PR056916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2022 21:12
Operator : AJ\MA
Sample : N4720-03 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
ORA-0135


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 00:14:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

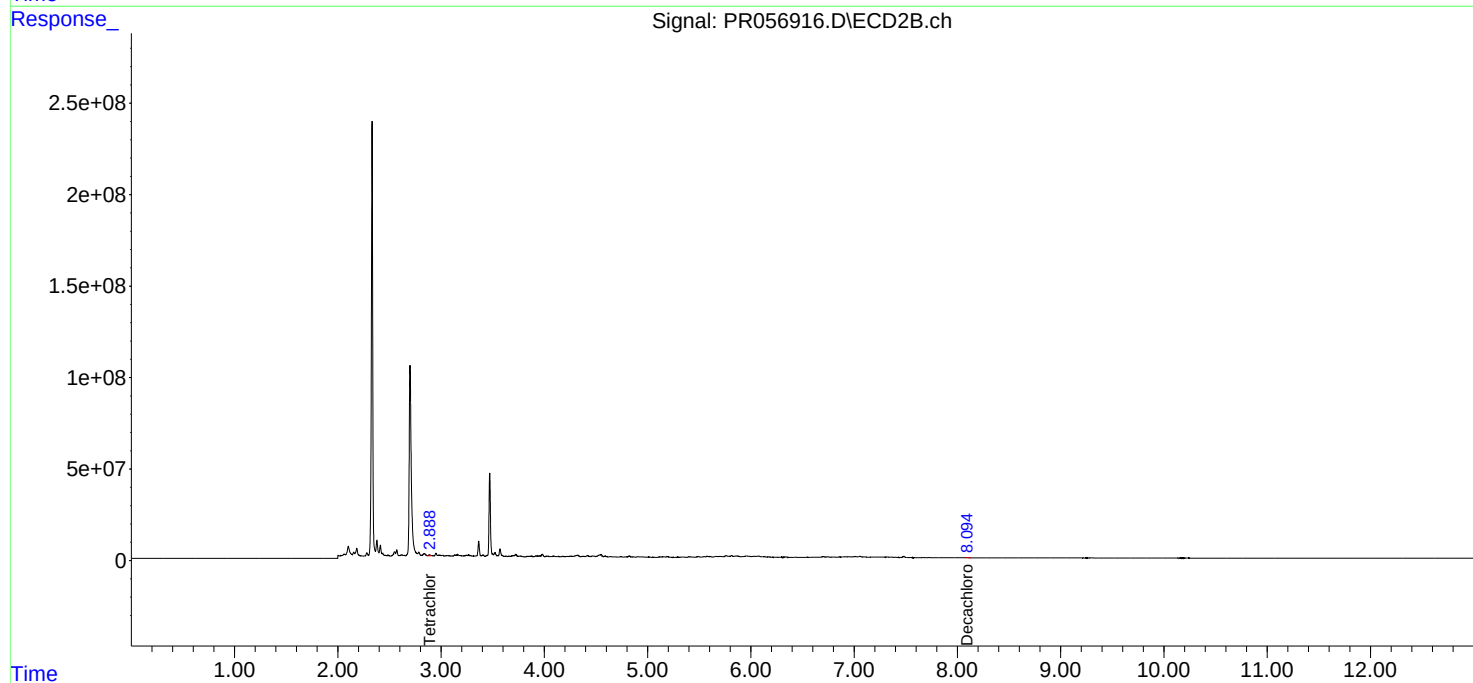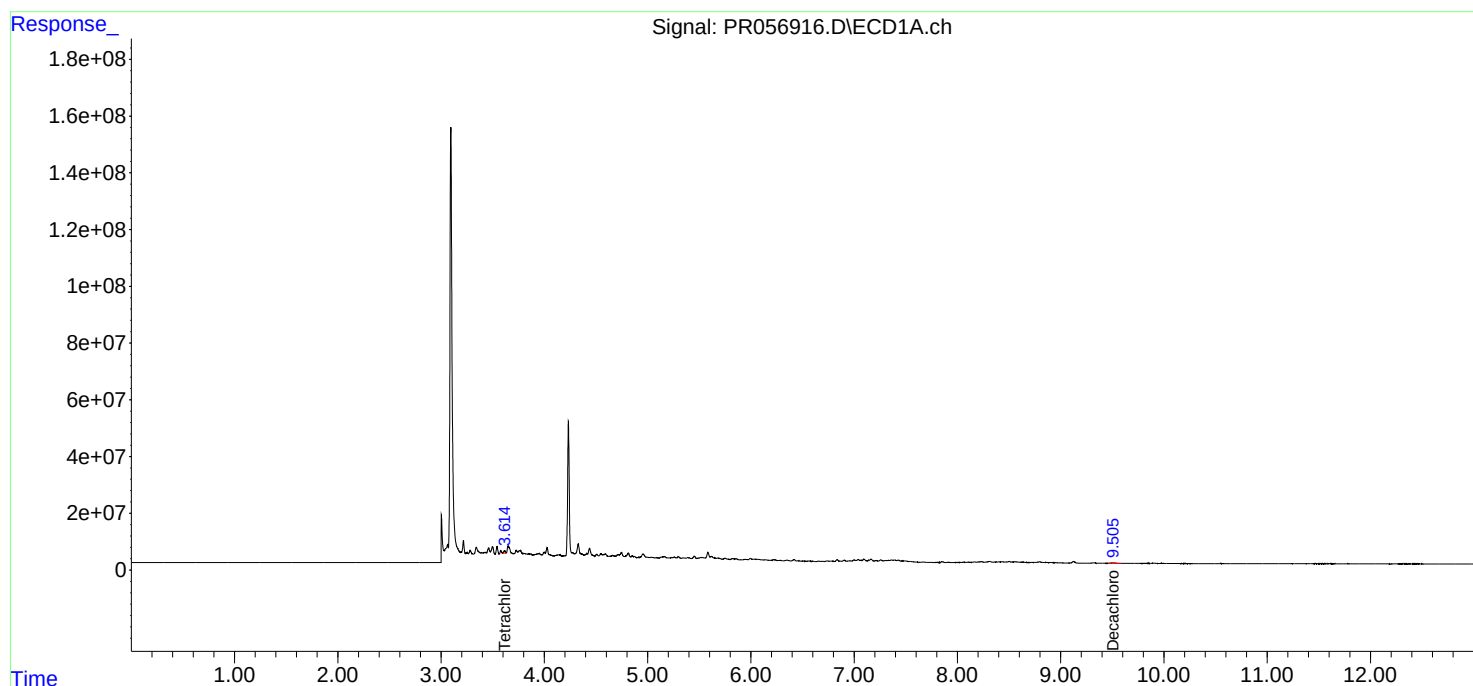

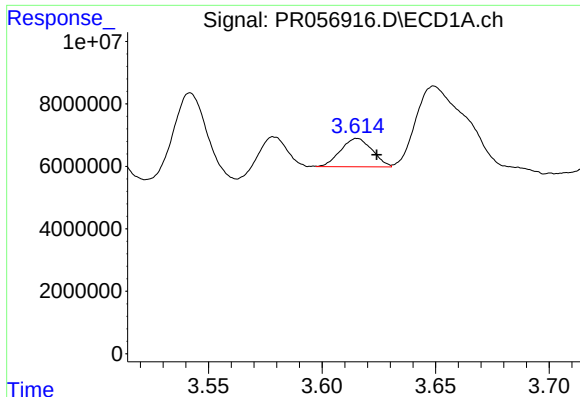


#1 Tetrachloro-m-xylene

R.T.: 3.614 min
Delta R.T.: -0.010 min
Response: 8802899
Conc: 1.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
ORA-0135


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

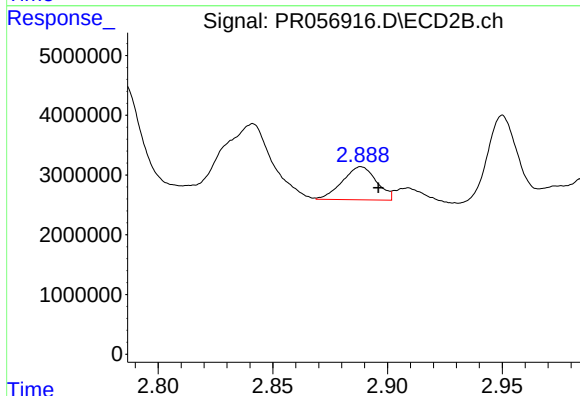


#1 Tetrachloro-m-xylene

R.T.: 2.888 min
Delta R.T.: -0.008 min
Response: 5753337
Conc: 3.28 ng/ml m

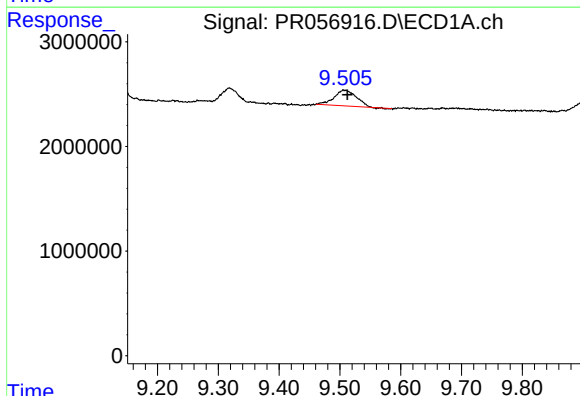

#2 Decachlorobiphenyl

R.T.: 9.508 min
Delta R.T.: -0.005 min
Response: 3757487
Conc: 1.89 ng/ml

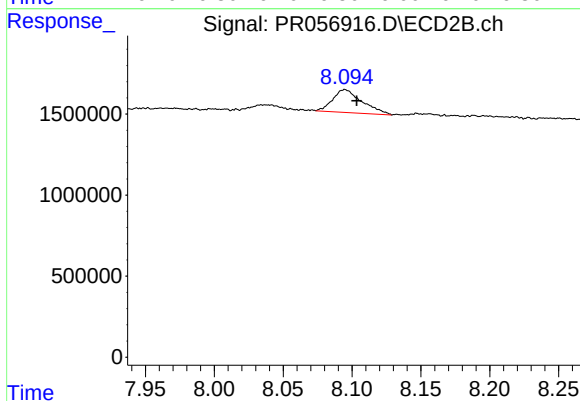

#2 Decachlorobiphenyl

R.T.: 8.094 min
Delta R.T.: -0.009 min
Response: 2092084
Conc: 1.26 ng/ml m