

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092122\
 Data File : PR056917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2022 21:28
 Operator : AJ\MA
 Sample : N4726-04 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 CLI-0621

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2022
 Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 00:15:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 07 09:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.618	2.891	13882087	1647222	2.889m	0.940m#
2) SA Decachlor...	9.502	8.094	1437678	1011301	0.725m	0.608

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092122\
Data File : PR056917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2022 21:28
Operator : AJ\MA
Sample : N4726-04 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
CLI-0621


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 00:15:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090722.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 07 09:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

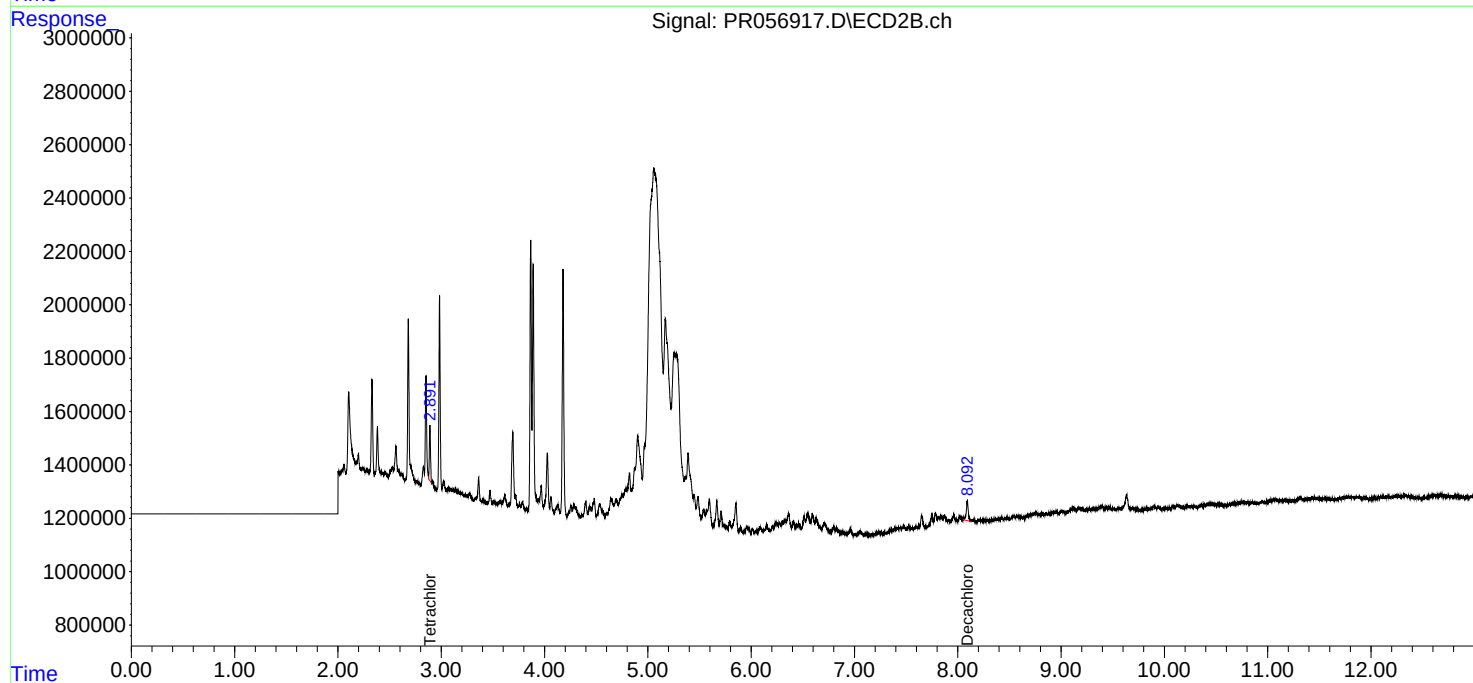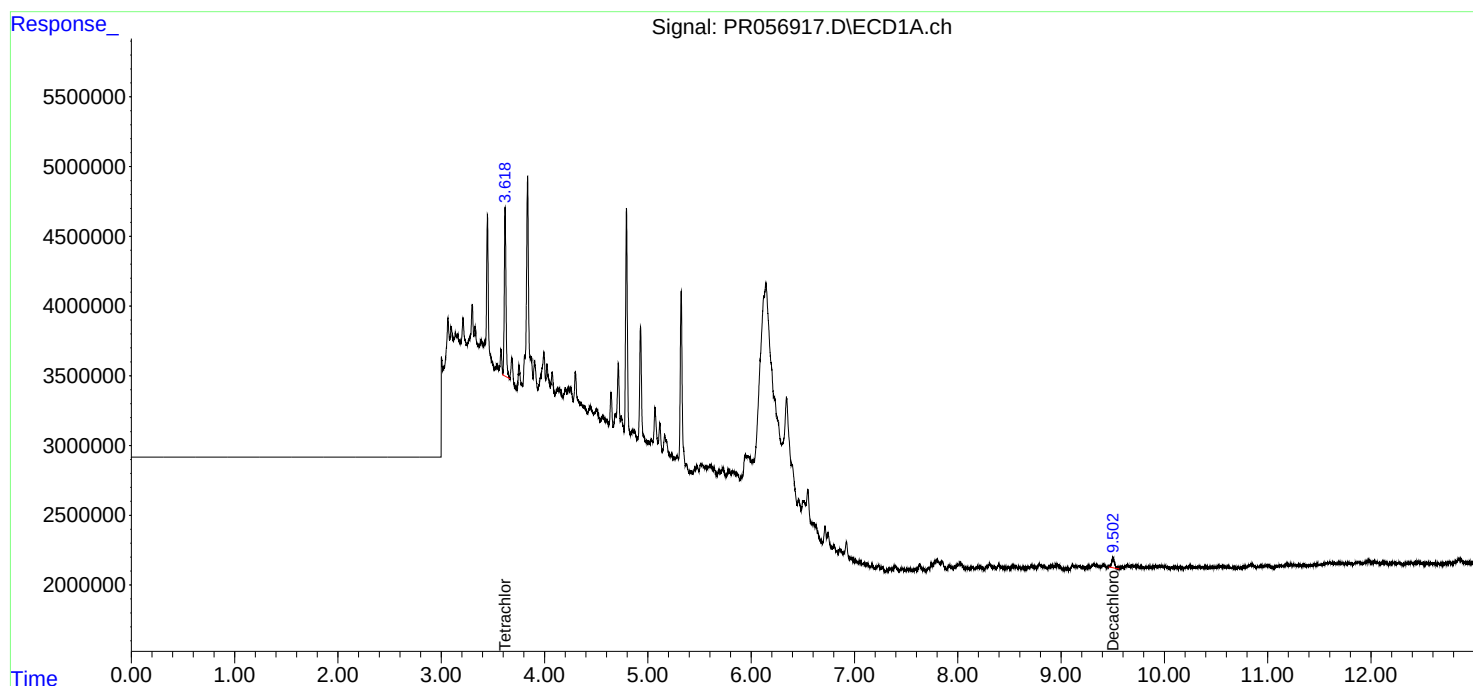

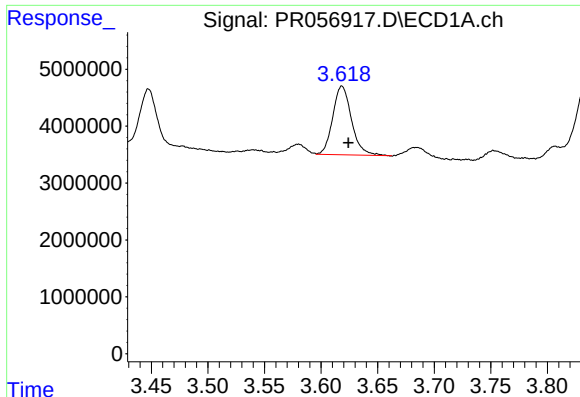


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.006 min
Response: 13882087
Conc: 2.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
CLI-0621


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

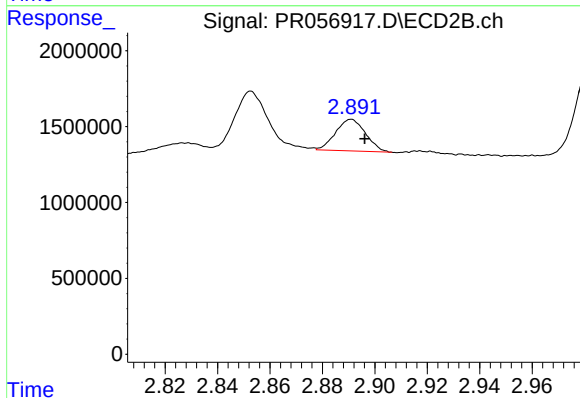


#1 Tetrachloro-m-xylene

R.T.: 2.891 min
Delta R.T.: -0.005 min
Response: 1647222
Conc: 0.94 ng/ml m

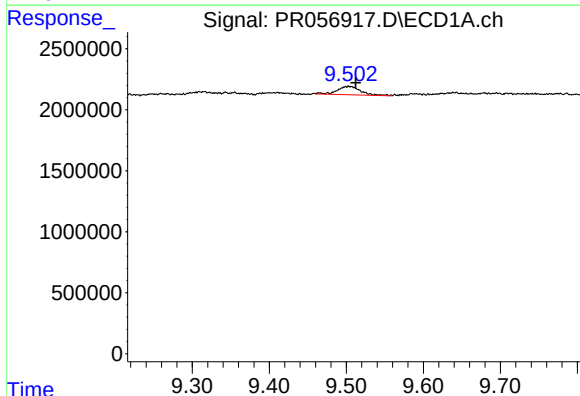

#2 Decachlorobiphenyl

R.T.: 9.502 min
Delta R.T.: -0.010 min
Response: 1437678
Conc: 0.72 ng/ml m

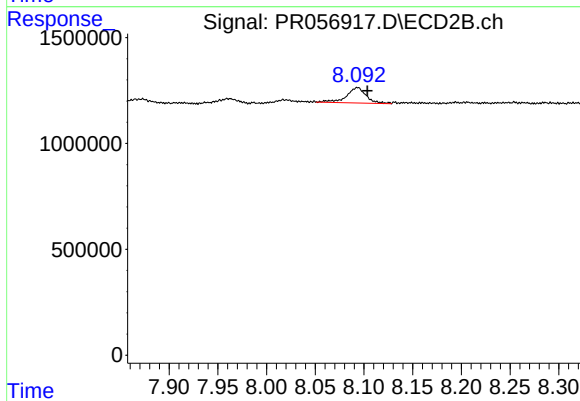

#2 Decachlorobiphenyl

R.T.: 8.094 min
Delta R.T.: -0.010 min
Response: 1011301
Conc: 0.61 ng/ml