

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092418\
 Data File : PR032271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 05:23
 Operator : SM\SJ
 Sample : J5056-01 (Sig #1); J5056-01RE (Sig #2)
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 RA-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 9/25/2018 12:01:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 07:36:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 19 03:49:43 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.515	3.646	364.3E6	631.3E6	18.324	15.086m
2) SA Decachlor...	10.254	8.502	320.1E6	184.6E6	10.929	8.207m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092418\
Data File : PR032271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 05:23
Operator : SM\SJ
Sample : J5056-01 (Sig #1); J5056-01RE (Sig #2)
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
RA-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
9/25/2018 12:01:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 07:36:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091818.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 19 03:49:43 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

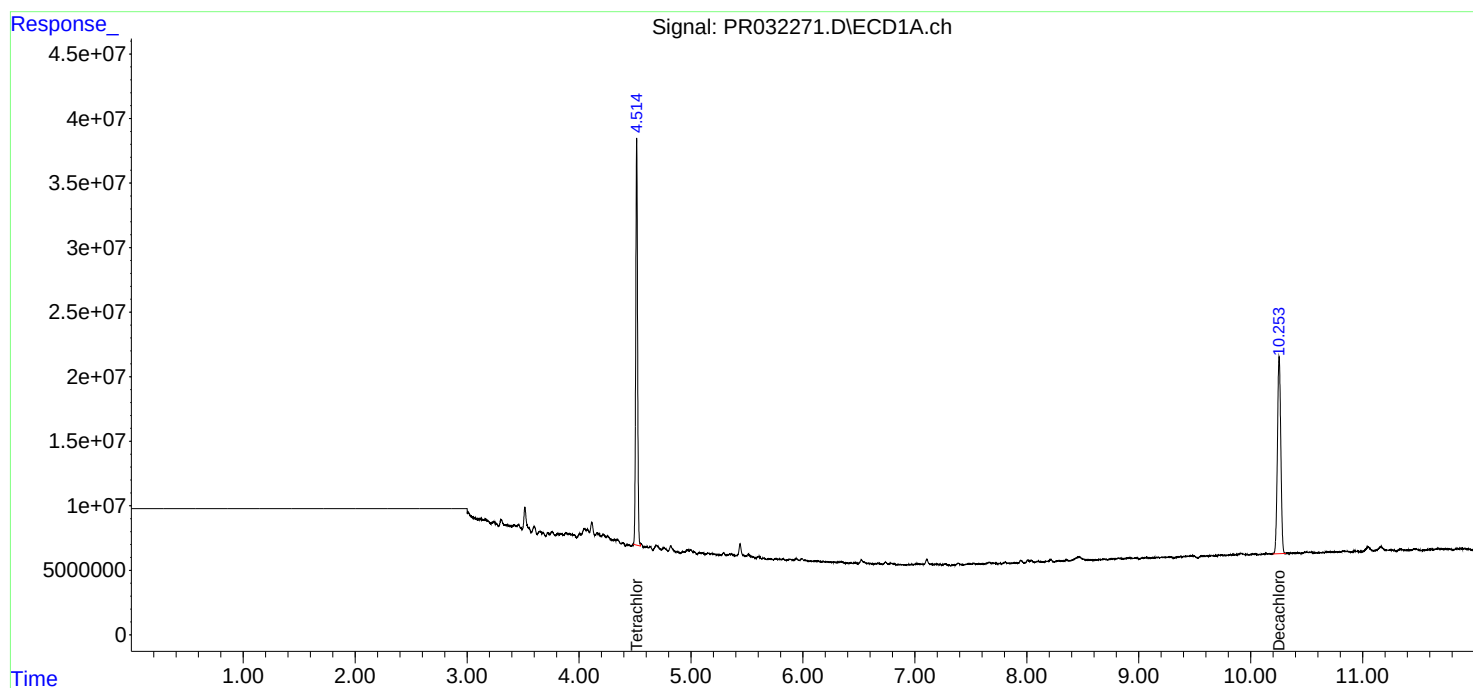

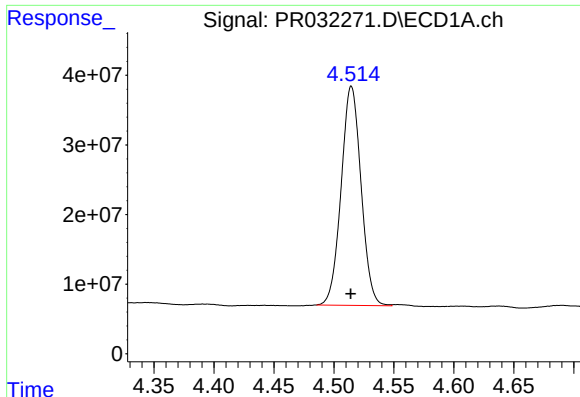


#1 Tetrachloro-m-xylene

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 364293317
Conc: 18.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
RA-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
9/25/2018 12:01:40 PM

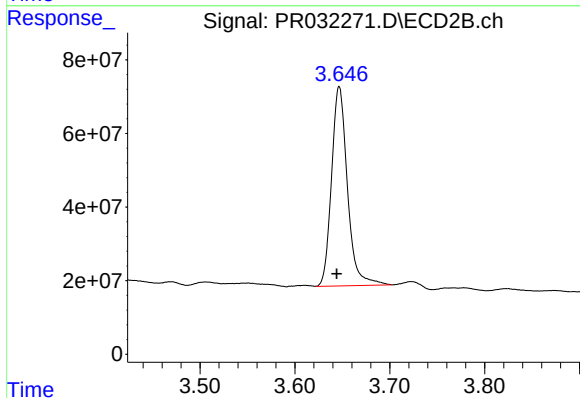


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.002 min
Response: 631300775
Conc: 15.09 ng/ml m

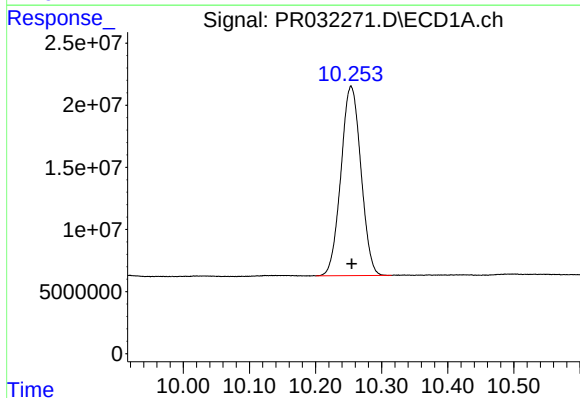

#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: 0.000 min
Response: 320138435
Conc: 10.93 ng/ml

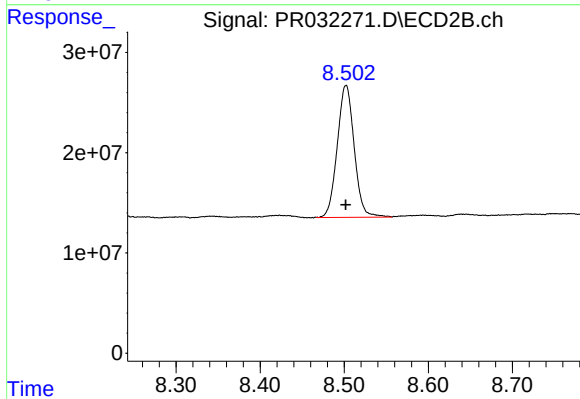

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: 0.000 min
Response: 184553103
Conc: 8.21 ng/ml m