

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092519\
 Data File : PR041498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2019 09:48
 Operator : SM\AJ
 Sample : MDL-AR1242-S-3
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-AR1242-S-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 10:34:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092319CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 24 04:36:18 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.739	4.006	17165355	76198669	12.931	12.597
2)	SA Decachlor...	10.661	9.121	119.4E6	362.6E6	37.418	33.612
Target Compounds							
3)	L1 AR-1016-1	5.913	0.000	1202907	0	18.811	N.D. #
4)	L1 AR-1016-2	5.937	0.000	1617604	0	17.764	N.D. #
5)	L1 AR-1016-3	6.000	0.000	996752	0	18.164	N.D. #
7)	L1 AR-1016-5	6.394	0.000	755614	0	15.274	N.D. #
13)	L3 AR-1232-3	5.937	0.000	1617604	0	42.667	N.D. #
15)	L3 AR-1232-5	6.187	0.000	675260	0	48.869	N.D. #
16)	L4 AR-1242-1	5.913	0.000	1202907	0	23.386	N.D. #
17)	L4 AR-1242-2	5.937	0.000	1617604	0	22.194	N.D. #
18)	L4 AR-1242-3	6.000	0.000	996752	0	22.542	N.D. #
20)	L4 AR-1242-5	6.836	0.000	1243130	0	24.252	N.D. #
21)	L5 AR-1248-1	5.913	0.000	1202907	0	32.772	N.D. #
22)	L5 AR-1248-2	6.187	0.000	675260	0	12.259	N.D. #
23)	L5 AR-1248-3	6.394	0.000	755614	0	11.768	N.D. #
24)	L5 AR-1248-4	6.796	0.000	1259204	0	14.755	N.D. #
25)	L5 AR-1248-5	6.836	0.000	1243130	0	15.256	N.D. #
26)	L6 AR-1254-1	6.769	0.000	868620	0	10.438	N.D. #
27)	L6 AR-1254-2	6.995	0.000	822441	0	5.853	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092519\
Data File : PR041498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2019 09:48
Operator : SM\AJ
Sample : MDL-AR1242-S-3
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 10:34:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 24 04:36:18 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

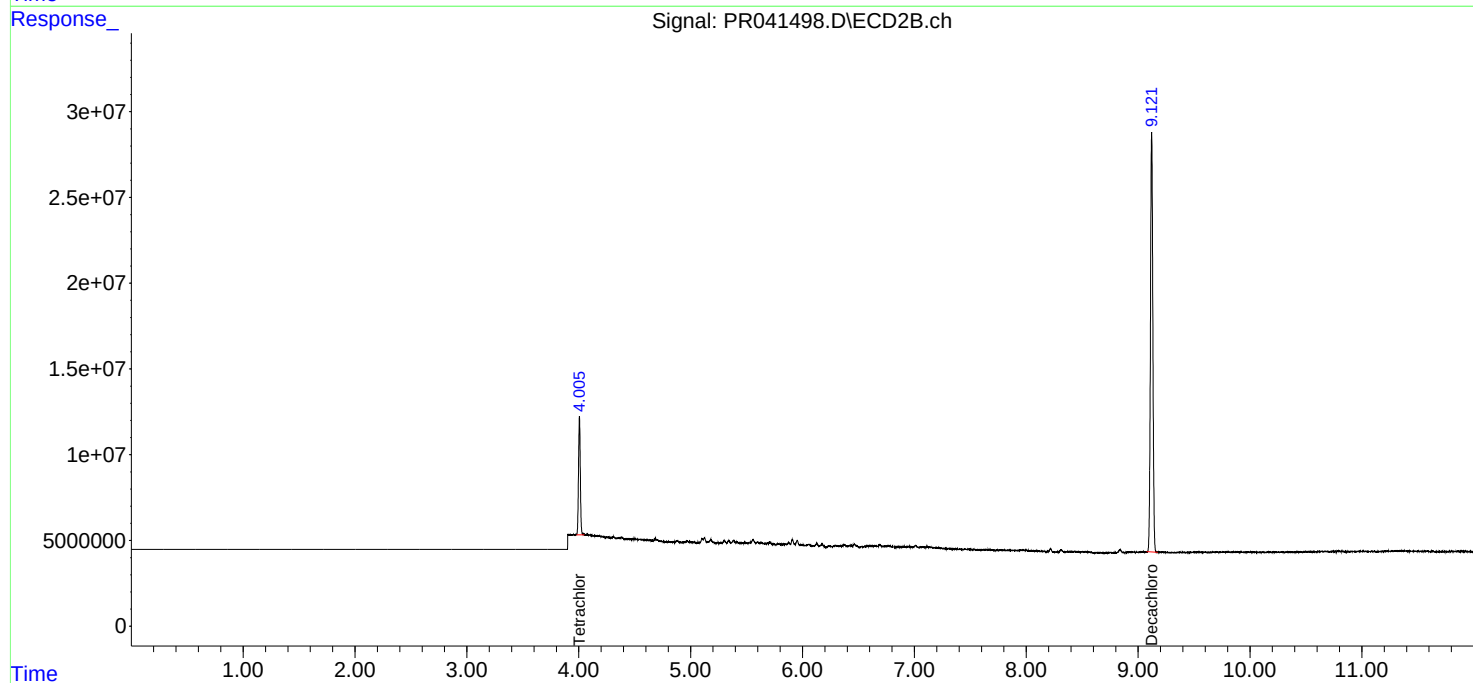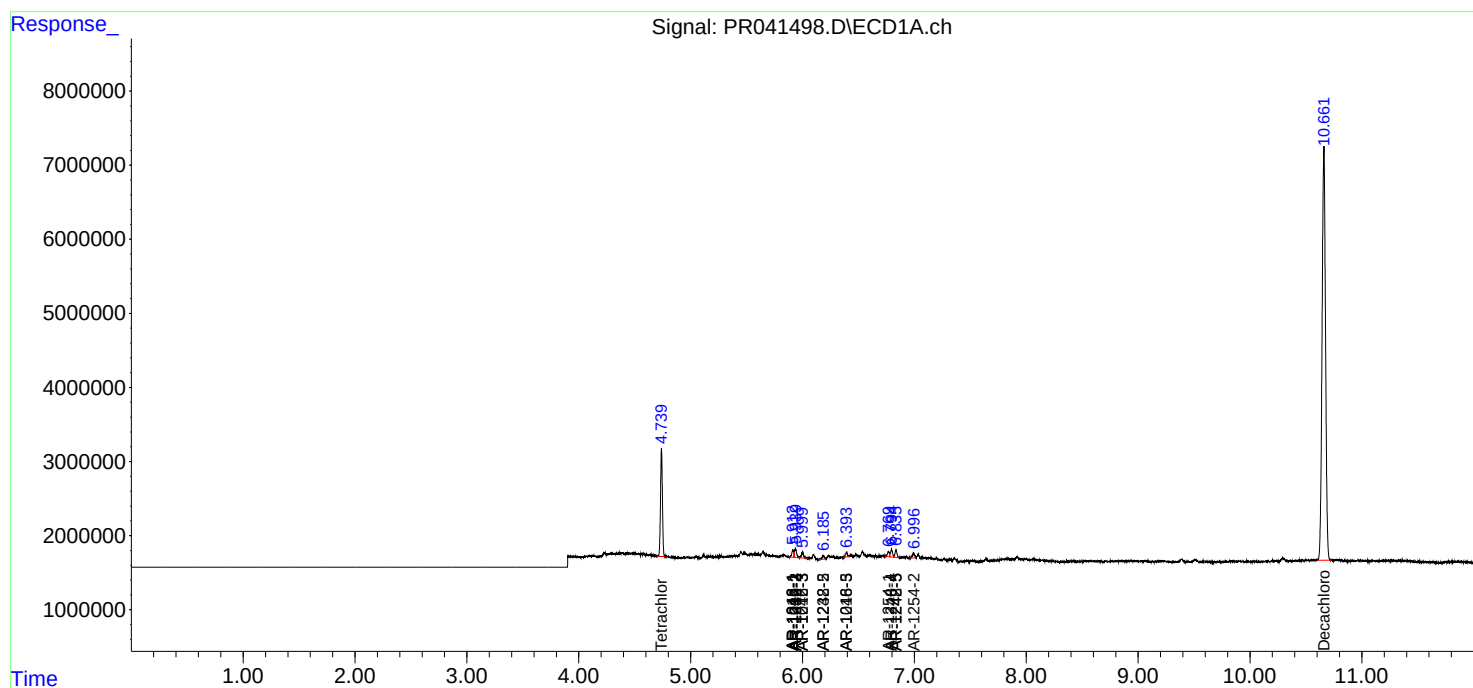


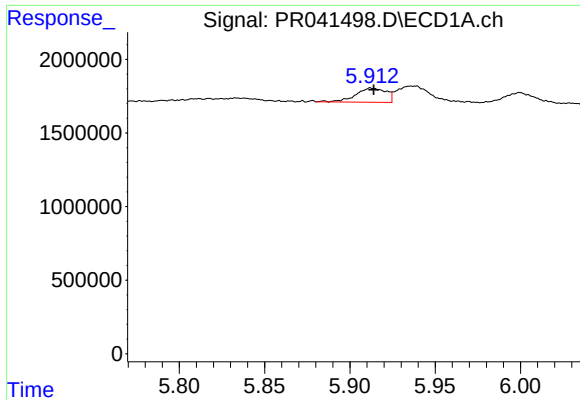

#3 AR-1016-1


R.T.: 5.913 min
Delta R.T.: -0.001 min
Response: 1202907
Conc: 18.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

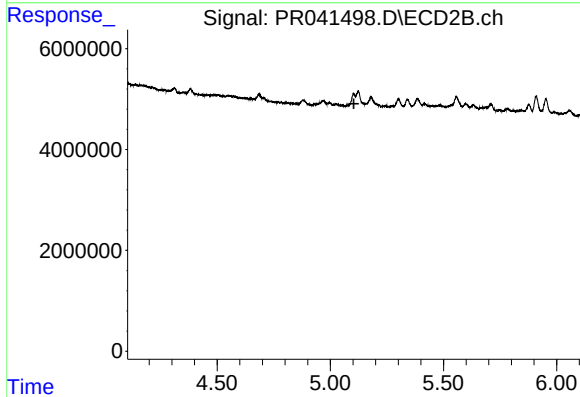


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 5.104 min
Response: 0
Conc: N.D.

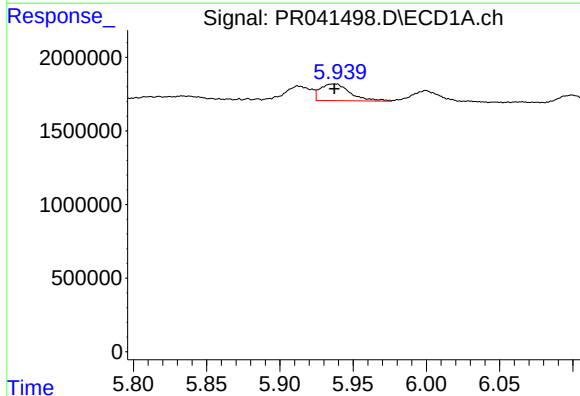


#4 AR-1016-2

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 1617604
Conc: 17.76 ng/ml

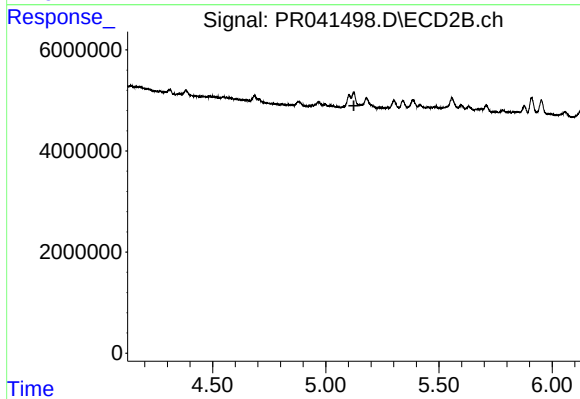

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 5.124 min
Response: 0
Conc: N.D.

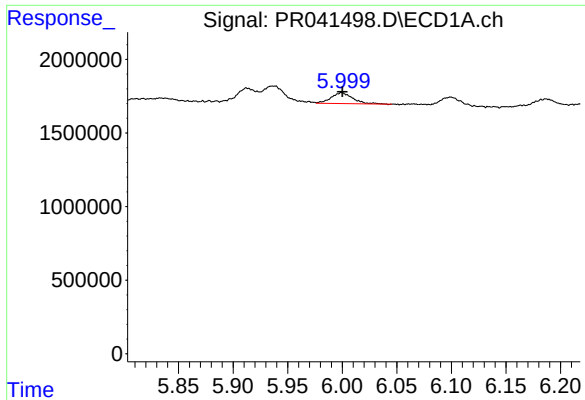

#5 AR-1016-3


R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 996752
Conc: 18.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

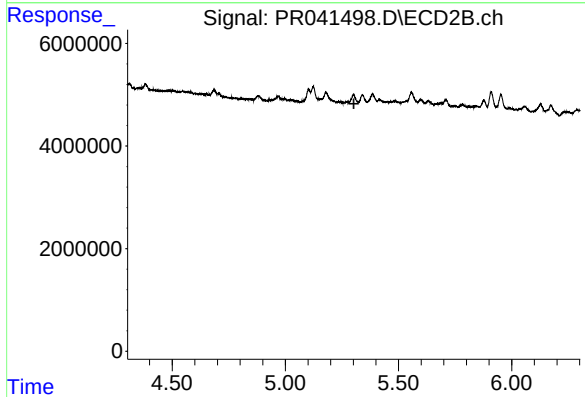


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.303 min
Response: 0
Conc: N.D.

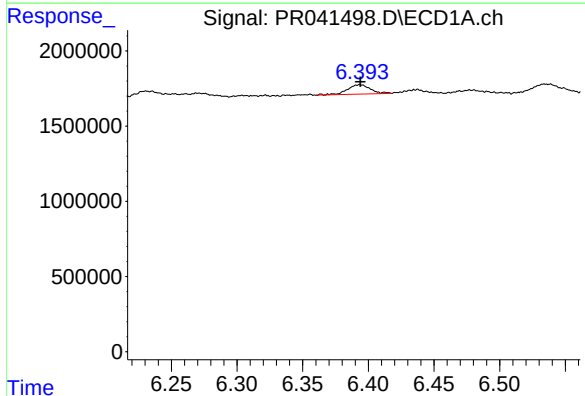


#7 AR-1016-5

R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 755614
Conc: 15.27 ng/ml

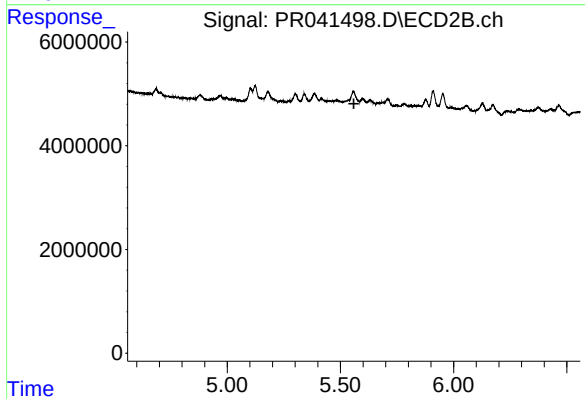

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.559 min
Response: 0
Conc: N.D.

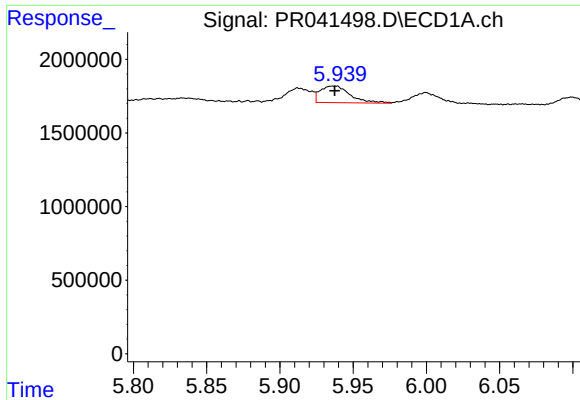

#13 AR-1232-3


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 1617604
Conc: 42.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

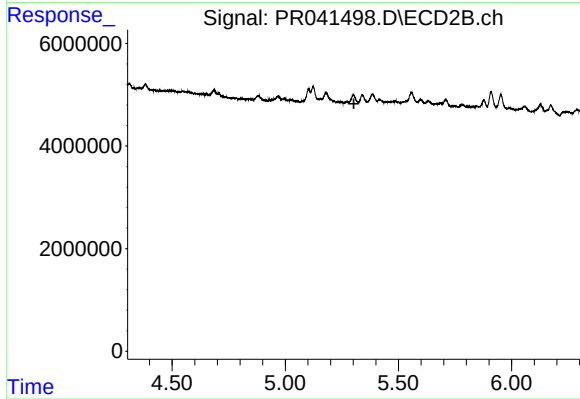


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.303 min
Response: 0
Conc: N.D.

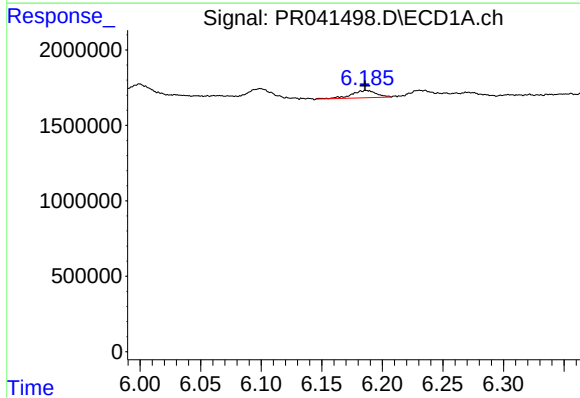


#15 AR-1232-5

R.T.: 6.187 min
Delta R.T.: 0.001 min
Response: 675260
Conc: 48.87 ng/ml

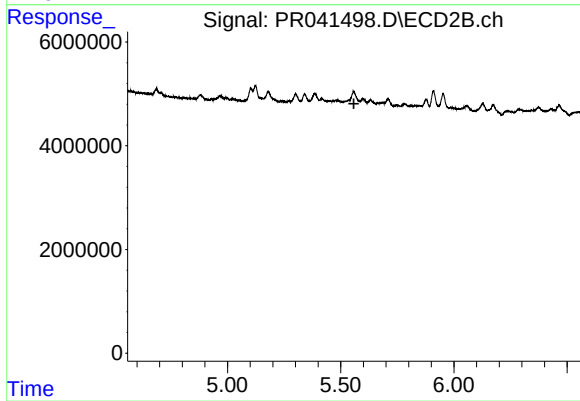

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.558 min
Response: 0
Conc: N.D.

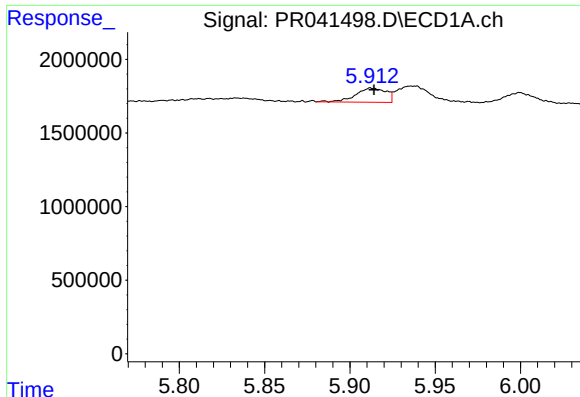

#16 AR-1242-1


R.T.: 5.913 min
Delta R.T.: -0.001 min
Response: 1202907
Conc: 23.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

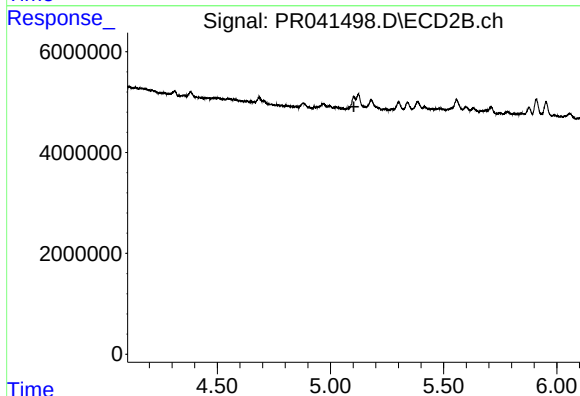


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.104 min
Response: 0
Conc: N.D.

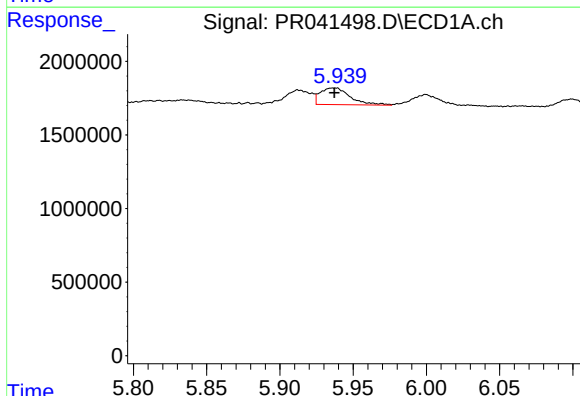


#17 AR-1242-2

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 1617604
Conc: 22.19 ng/ml

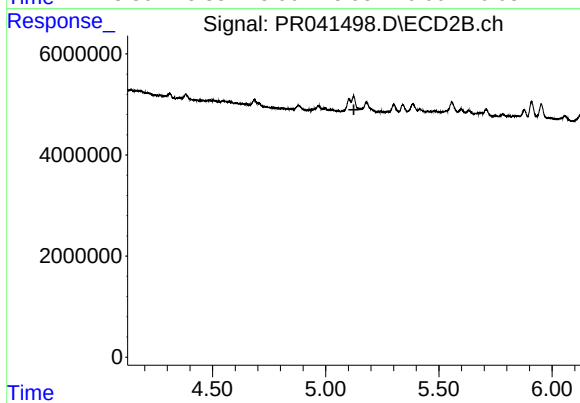

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 5.124 min
Response: 0
Conc: N.D.

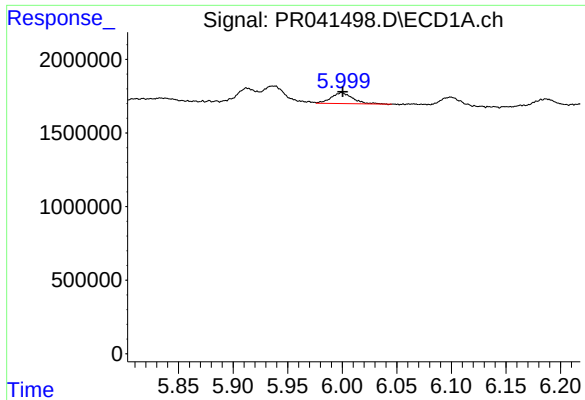

#18 AR-1242-3


R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 996752
Conc: 22.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

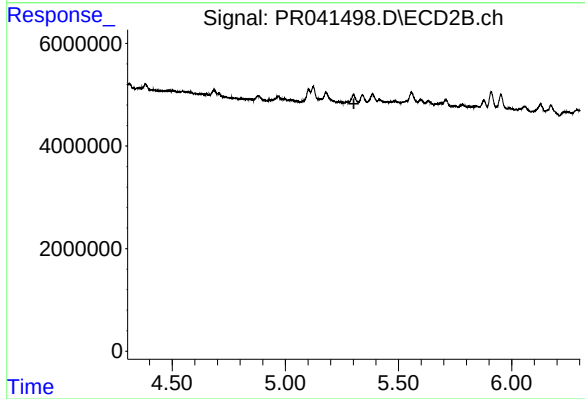


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 5.303 min
Response: 0
Conc: N.D.

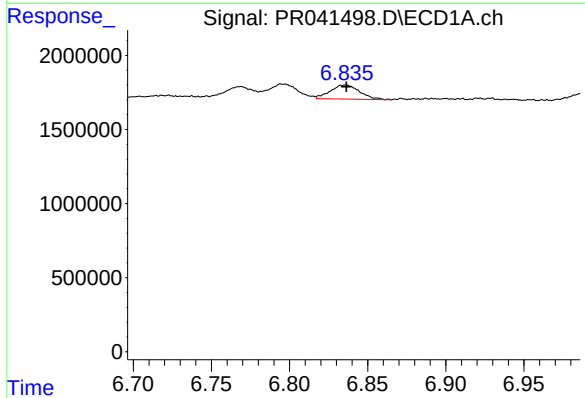


#20 AR-1242-5

R.T.: 6.836 min
Delta R.T.: 0.000 min
Response: 1243130
Conc: 24.25 ng/ml

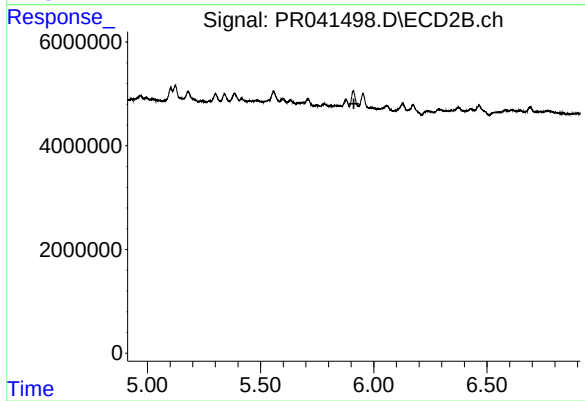

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.912 min
Response: 0
Conc: N.D.

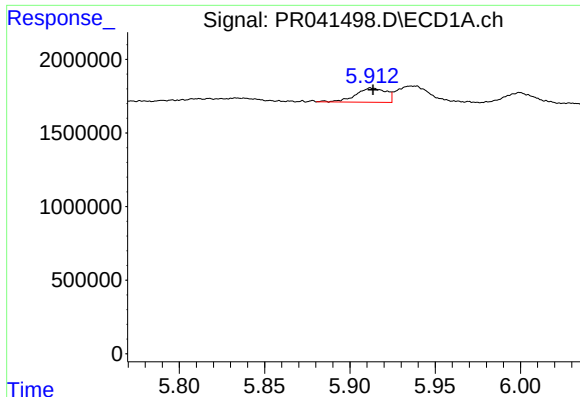

#21 AR-1248-1


R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 1202907
Conc: 32.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

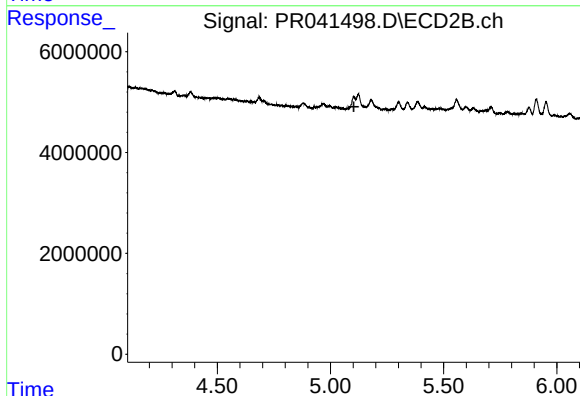


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

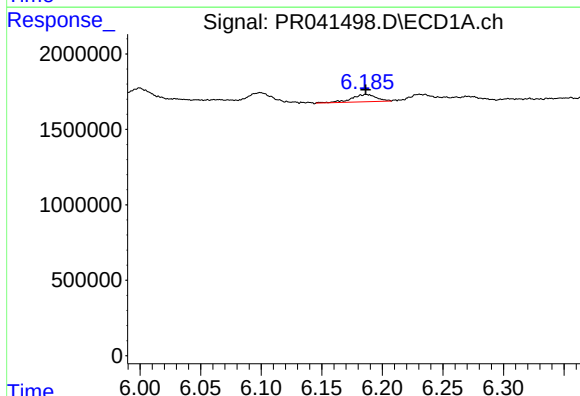


#22 AR-1248-2

R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 675260
Conc: 12.26 ng/ml

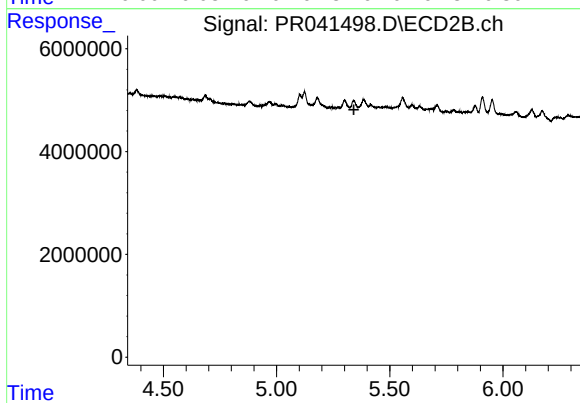

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.342 min
Response: 0
Conc: N.D.

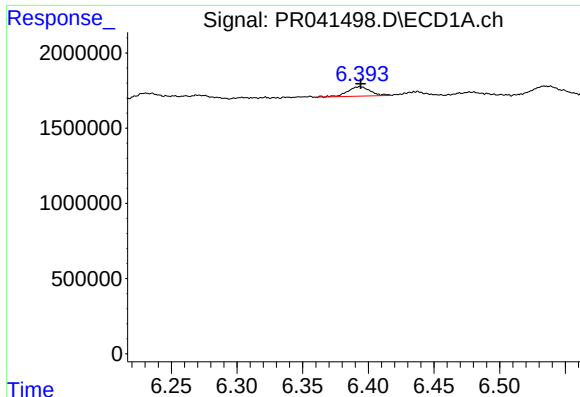

#23 AR-1248-3


R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 755614
Conc: 11.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

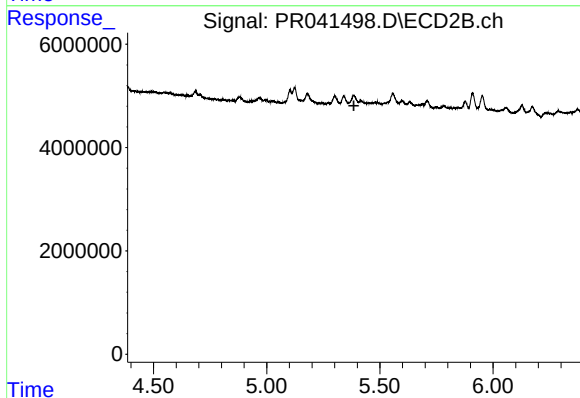


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.385 min
Response: 0
Conc: N.D.

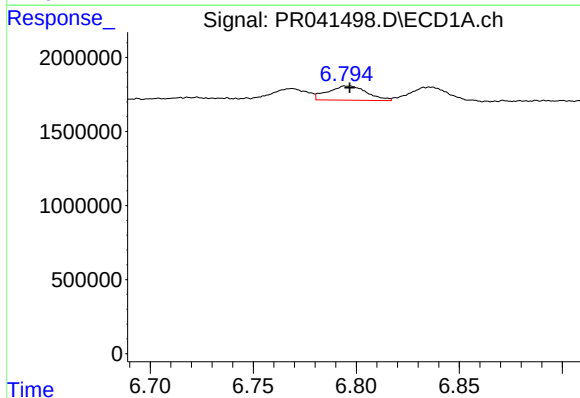


#24 AR-1248-4

R.T.: 6.796 min
Delta R.T.: -0.001 min
Response: 1259204
Conc: 14.75 ng/ml

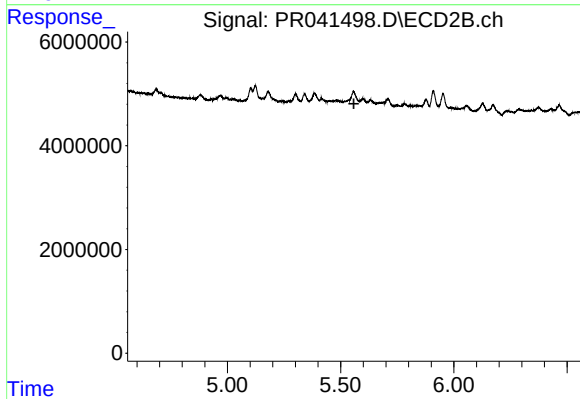

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.558 min
Response: 0
Conc: N.D.

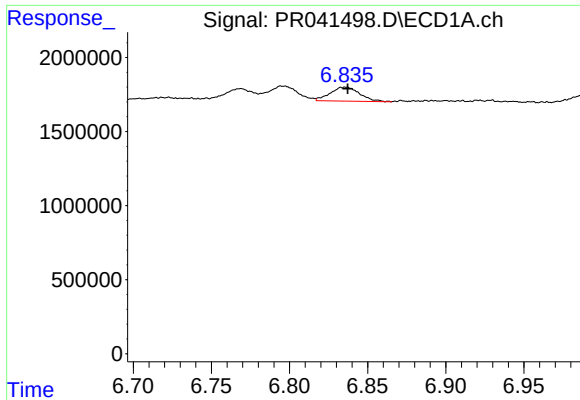

#25 AR-1248-5


R.T.: 6.836 min
Delta R.T.: -0.002 min
Response: 1243130
Conc: 15.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

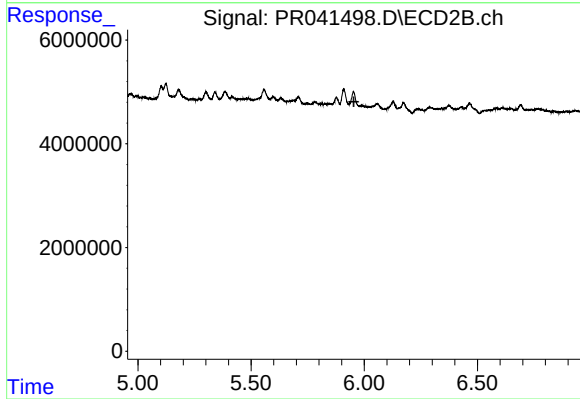


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

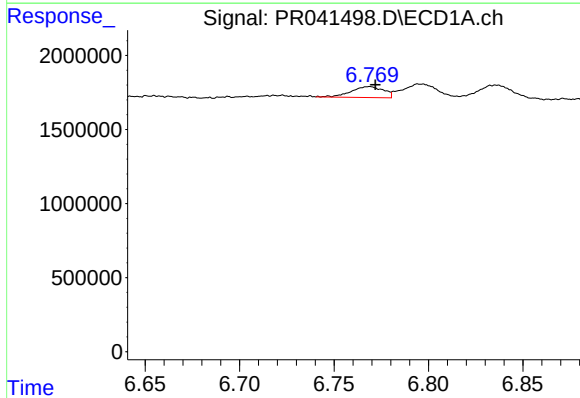


#26 AR-1254-1

R.T.: 6.769 min
Delta R.T.: -0.003 min
Response: 868620
Conc: 10.44 ng/ml

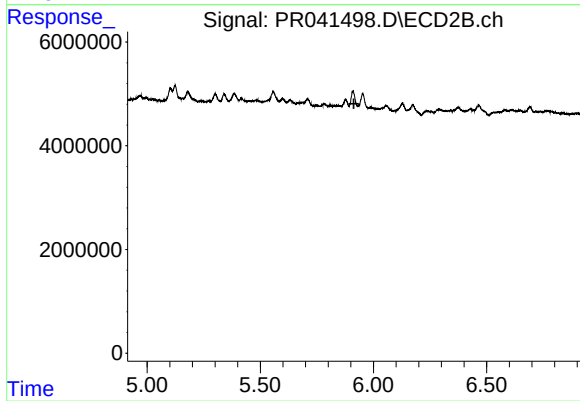

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.913 min
Response: 0
Conc: N.D.

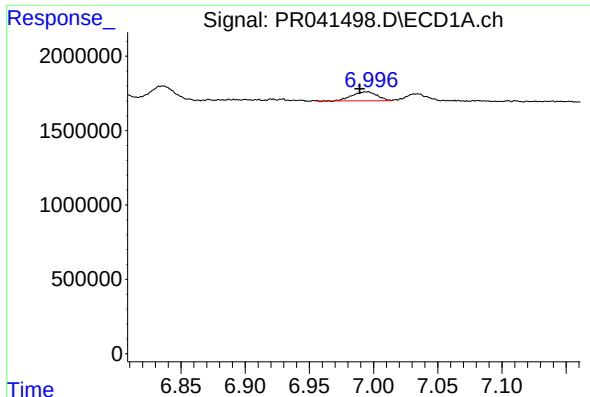

#27 AR-1254-2

R.T.: 6.995 min
Delta R.T.: 0.006 min
Response: 822441
Conc: 5.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-AR1242-S-3

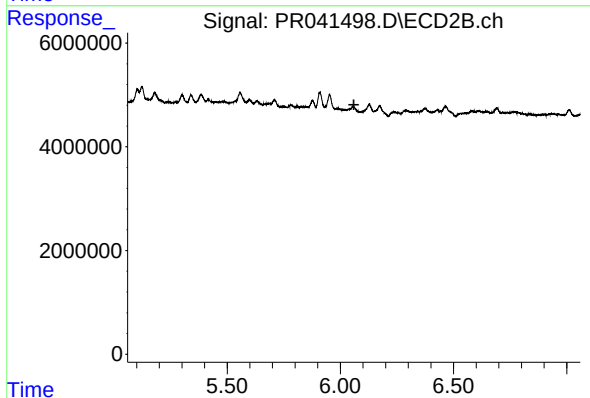

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.060 min
Response: 0
Conc: N.D.