

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092719\
 Data File : PR041601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2019 16:28
 Operator : SM\AJ
 Sample : PB123446BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 ABLK46

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 00:35:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092319CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 24 04:36:18 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.752	4.001	25696941	124.5E6	19.358	20.581
2)	SA Decachlor...	10.692	9.132	124.8E6	417.1E6	39.096	38.664
Target Compounds							
9)	L2 AR-1221-2	0.000	4.308	0	1211716	N.D.	34.745 #
31)	L7 AR-1260-1	0.000	6.542f	0	811455	N.D.	2.083 #
32)	L7 AR-1260-2	0.000	6.765	0	773127	N.D.	1.434 #
38)	L8 AR-1262-3	0.000	7.978f	0	291659	N.D.	0.510 #
39)	L8 AR-1262-4	0.000	7.978	0	291659	N.D.	0.288 #
41)	L9 AR-1268-1	0.000	7.978f	0	291659	N.D.	0.172 #
42)	L9 AR-1268-2	0.000	7.978	0	291659	N.D.	0.186 #
43)	L9 AR-1268-3	0.000	8.224	0	1709214	N.D.	1.292 #
45)	L9 AR-1268-5	0.000	8.848	0	2547474	N.D.	0.578 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092719\
Data File : PR041601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2019 16:28
Operator : SM\AJ
Sample : PB123446BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
ABLK46

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 00:35:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 24 04:36:18 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

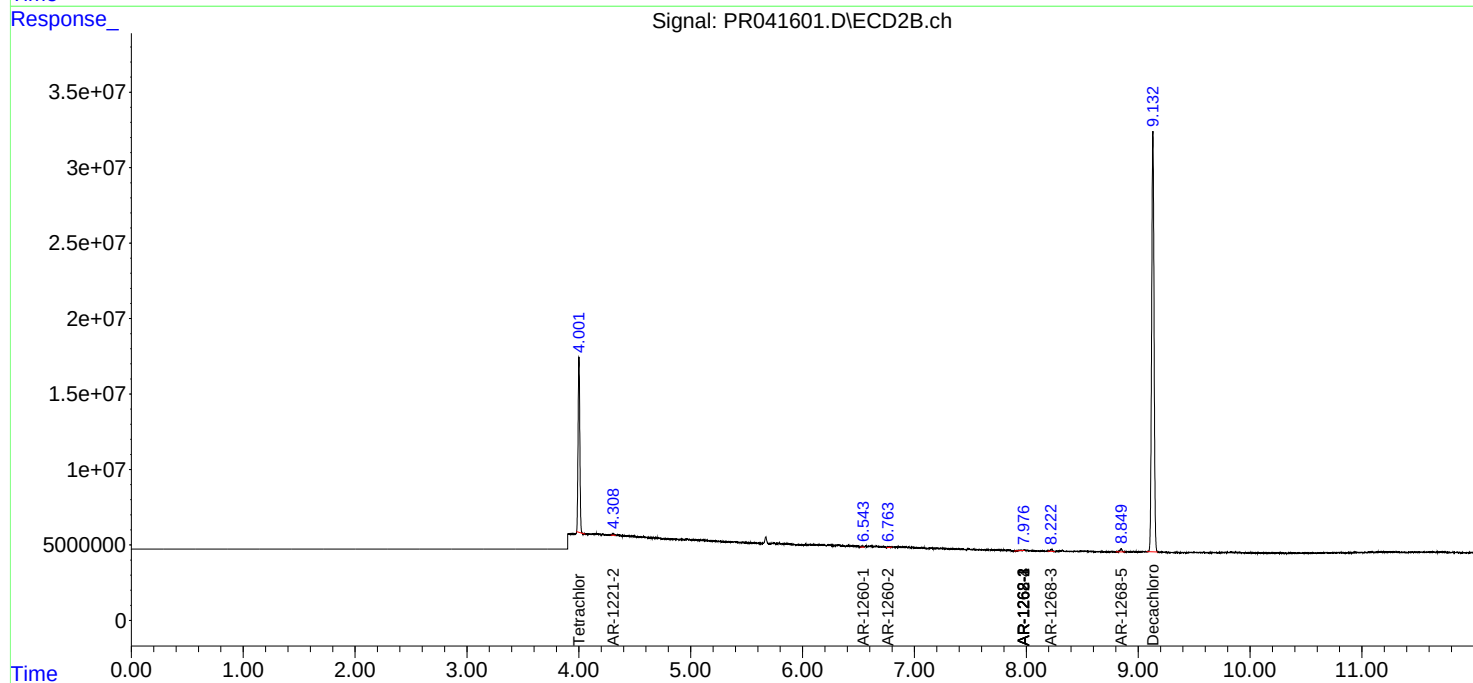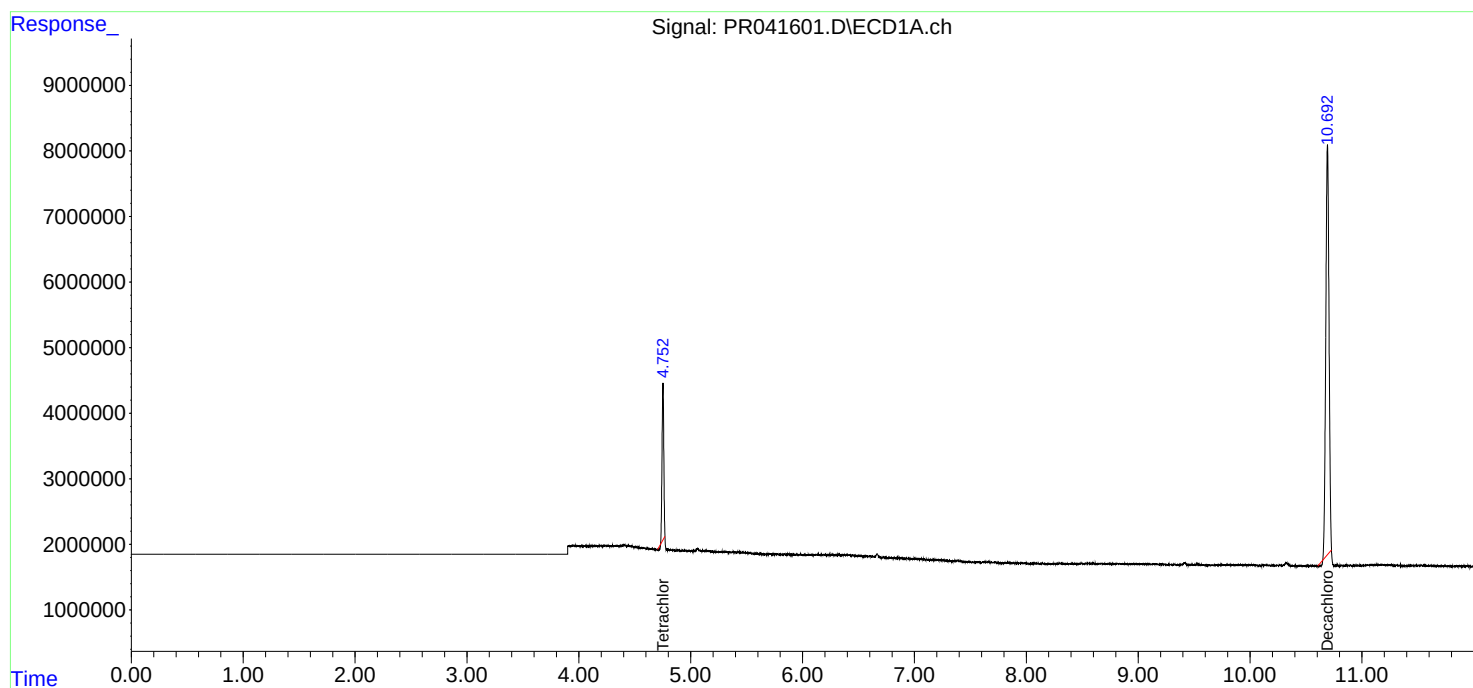


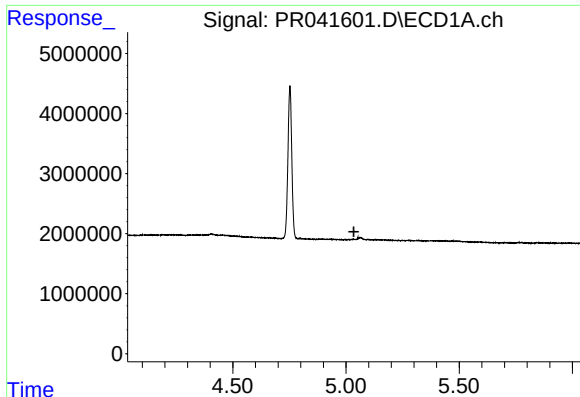

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK46

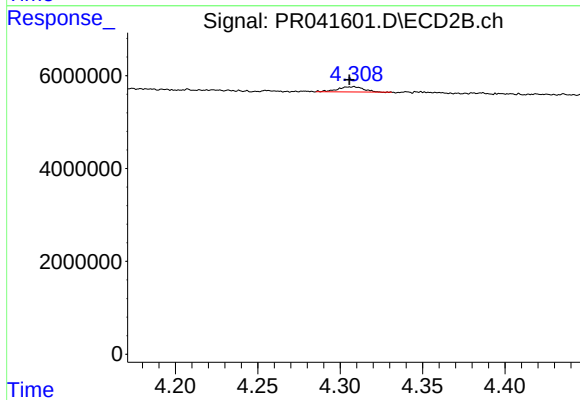


#9 AR-1221-2

R.T.: 4.308 min
Delta R.T.: 0.003 min
Response: 1211716
Conc: 34.75 ng/ml

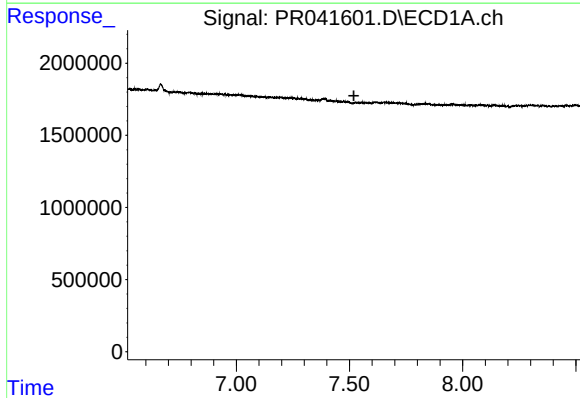


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 7.519 min
Response: 0
Conc: N.D.

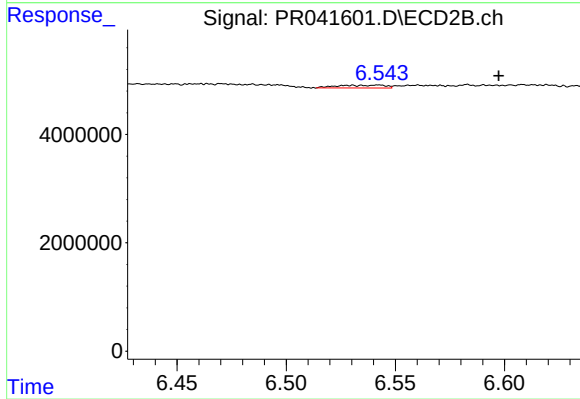

#31 AR-1260-1


R.T.: 6.542 min
Delta R.T.: -0.055 min
Response: 811455
Conc: 2.08 ng/ml

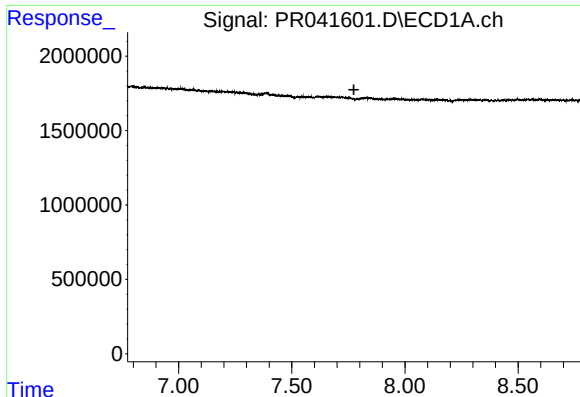

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK46

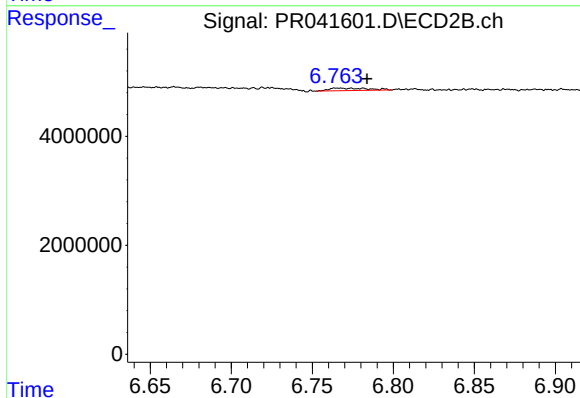


#32 AR-1260-2

R.T.: 6.765 min
Delta R.T.: -0.018 min
Response: 773127
Conc: 1.43 ng/ml

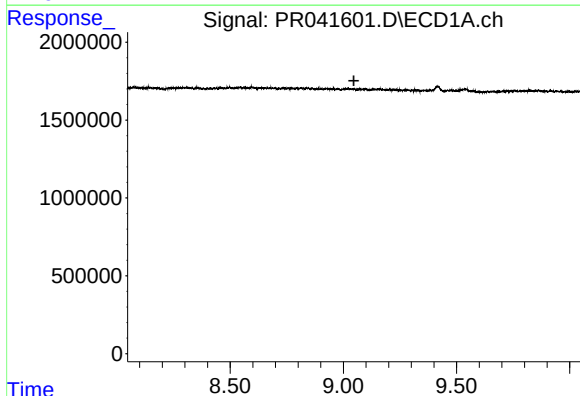


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.047 min
Response: 0
Conc: N.D.

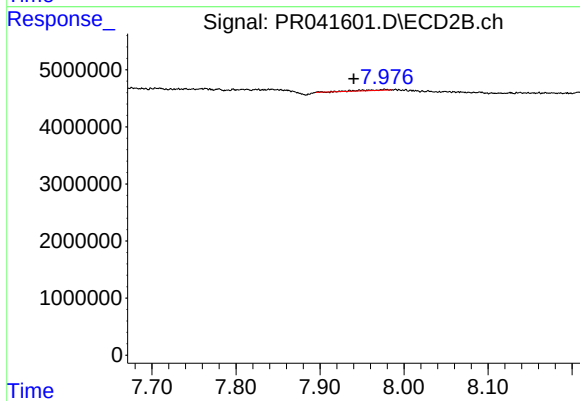

#38 AR-1262-3


R.T.: 7.978 min
Delta R.T.: 0.037 min
Response: 291659
Conc: 0.51 ng/ml

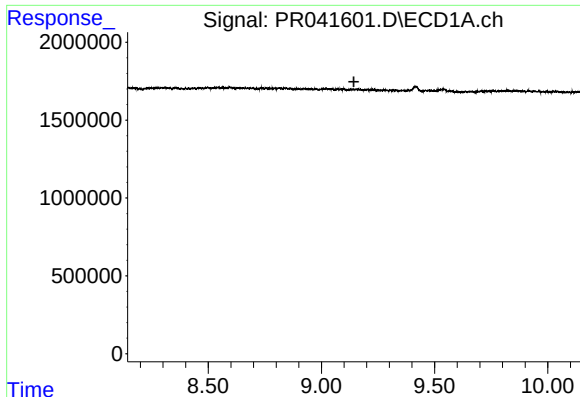

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.144 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK46

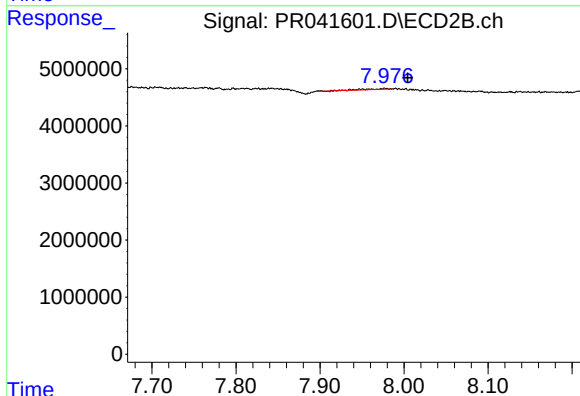


#39 AR-1262-4

R.T.: 7.978 min
Delta R.T.: -0.027 min
Response: 291659
Conc: 0.29 ng/ml

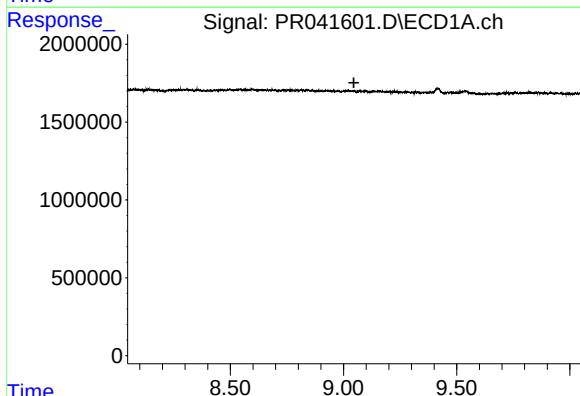


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.046 min
Response: 0
Conc: N.D.

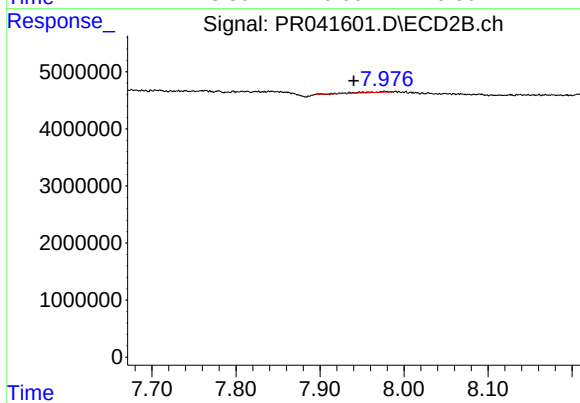

#41 AR-1268-1


R.T.: 7.978 min
Delta R.T.: 0.037 min
Response: 291659
Conc: 0.17 ng/ml

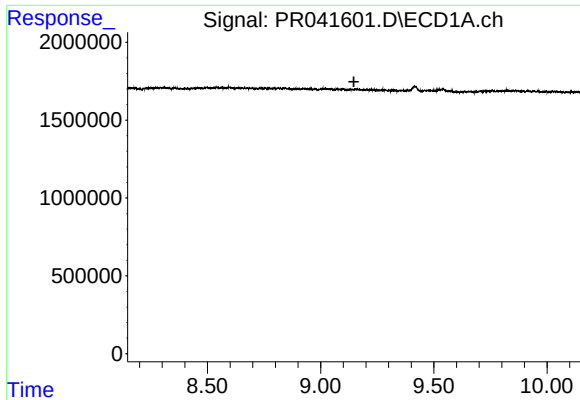

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK46

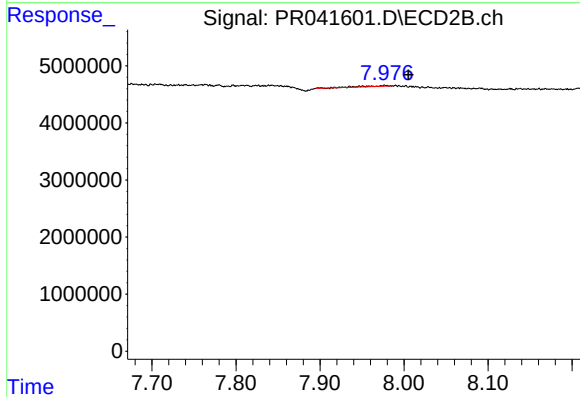


#42 AR-1268-2

R.T.: 7.978 min
Delta R.T.: -0.028 min
Response: 291659
Conc: 0.19 ng/ml

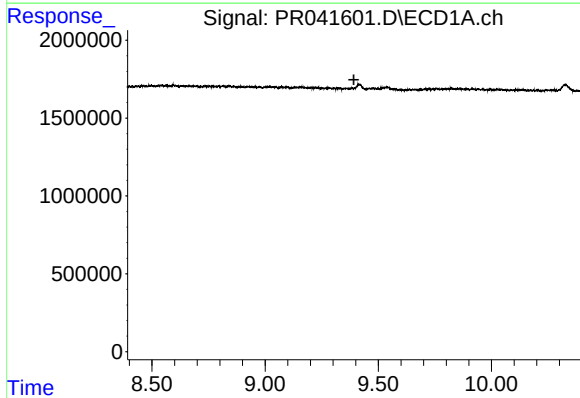


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.392 min
Response: 0
Conc: N.D.

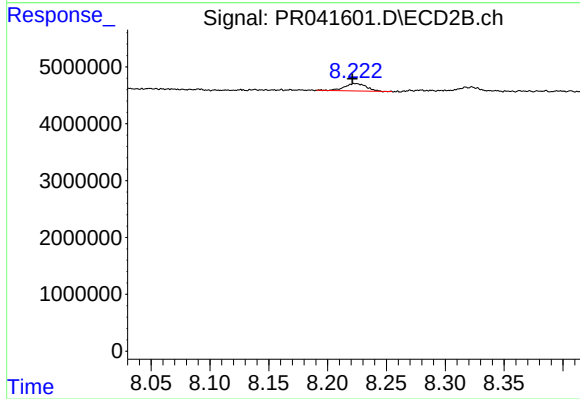

#43 AR-1268-3


R.T.: 8.224 min
Delta R.T.: 0.003 min
Response: 1709214
Conc: 1.29 ng/ml

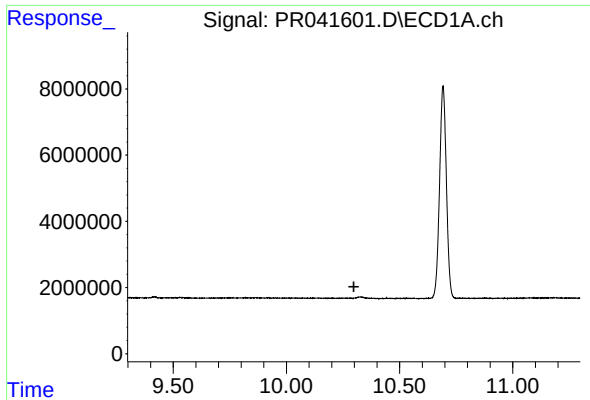

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
ABLK46

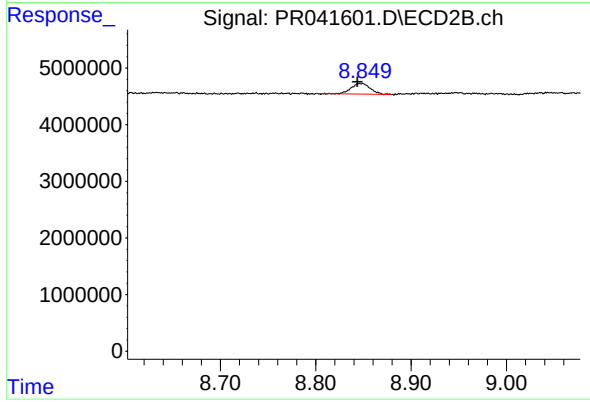

#45 AR-1268-5

R.T.: 8.848 min
Delta R.T.: 0.004 min
Response: 2547474
Conc: 0.58 ng/ml