

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092721\
 Data File : PR052116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2021 20:41
 Operator : AJ\MA
 Sample : PB139403BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 06:19:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091421CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 08:14:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.705	3.860	131.6E6	78842206	20.479	18.034
2)	SA Decachlor...	10.656	8.910	221.3E6	161.5E6	46.604	39.223
Target Compounds							
8)	L2 AR-1221-1	4.939	0.000	1846442	0	24.650	N.D. #
9)	L2 AR-1221-2	5.007	0.000	5787217	0	112.278	N.D. #
29)	L6 AR-1254-4	7.583f	0.000	3739	0	0.013	N.D. #
38)	L8 AR-1262-3	9.064	0.000	1018974	0	3.560	N.D. #
39)	L8 AR-1262-4	9.064f	0.000	1018974	0	5.911	N.D. #
40)	L8 AR-1262-5	9.874	0.000	1190552	0	4.775	N.D. #
41)	L9 AR-1268-1	9.064	0.000	1018974	0	1.305	N.D. #
42)	L9 AR-1268-2	9.064f	0.000	1018974	0	1.438	N.D. #
44)	L9 AR-1268-4	9.874	0.000	1190552	0	4.367	N.D. #
45)	L9 AR-1268-5	10.292	0.000	1598097	0	0.786	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092721\
Data File : PR052116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2021 20:41
Operator : AJ\MA
Sample : PB139403BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 06:19:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091421CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 08:14:53 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

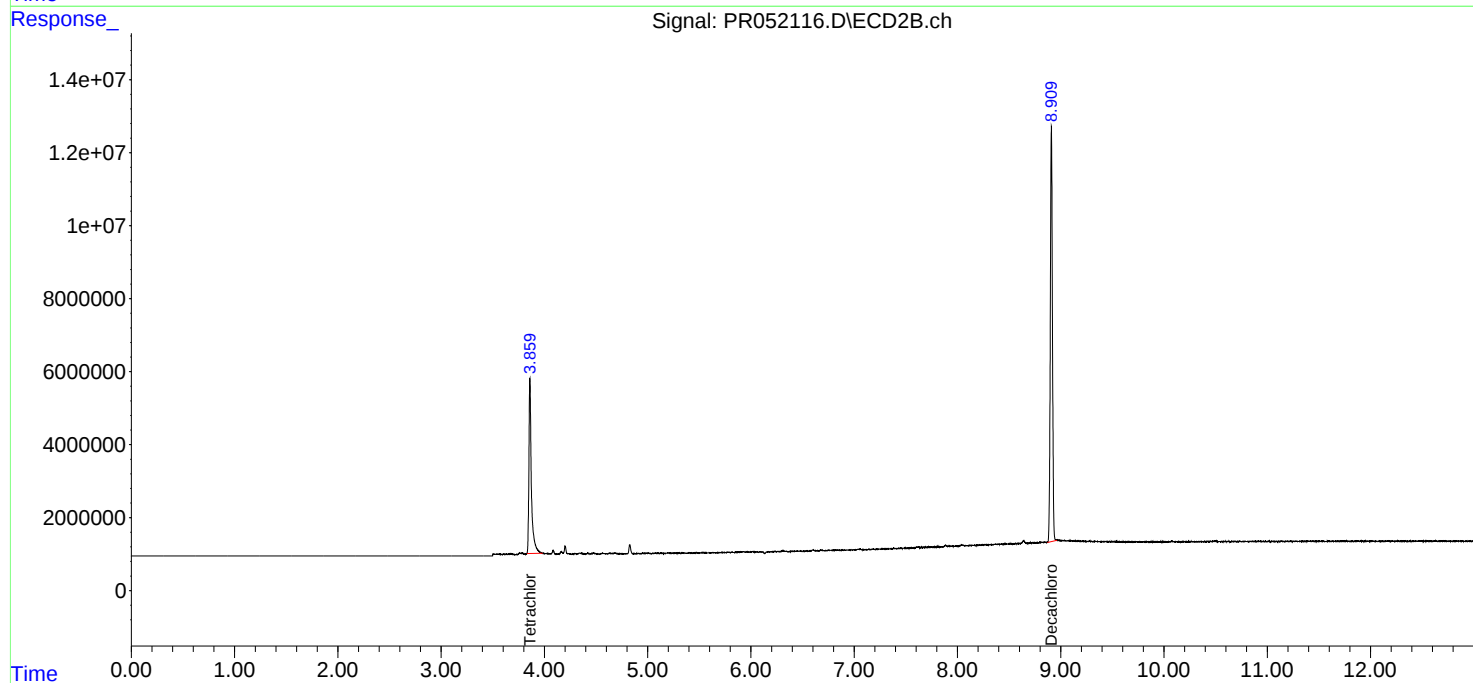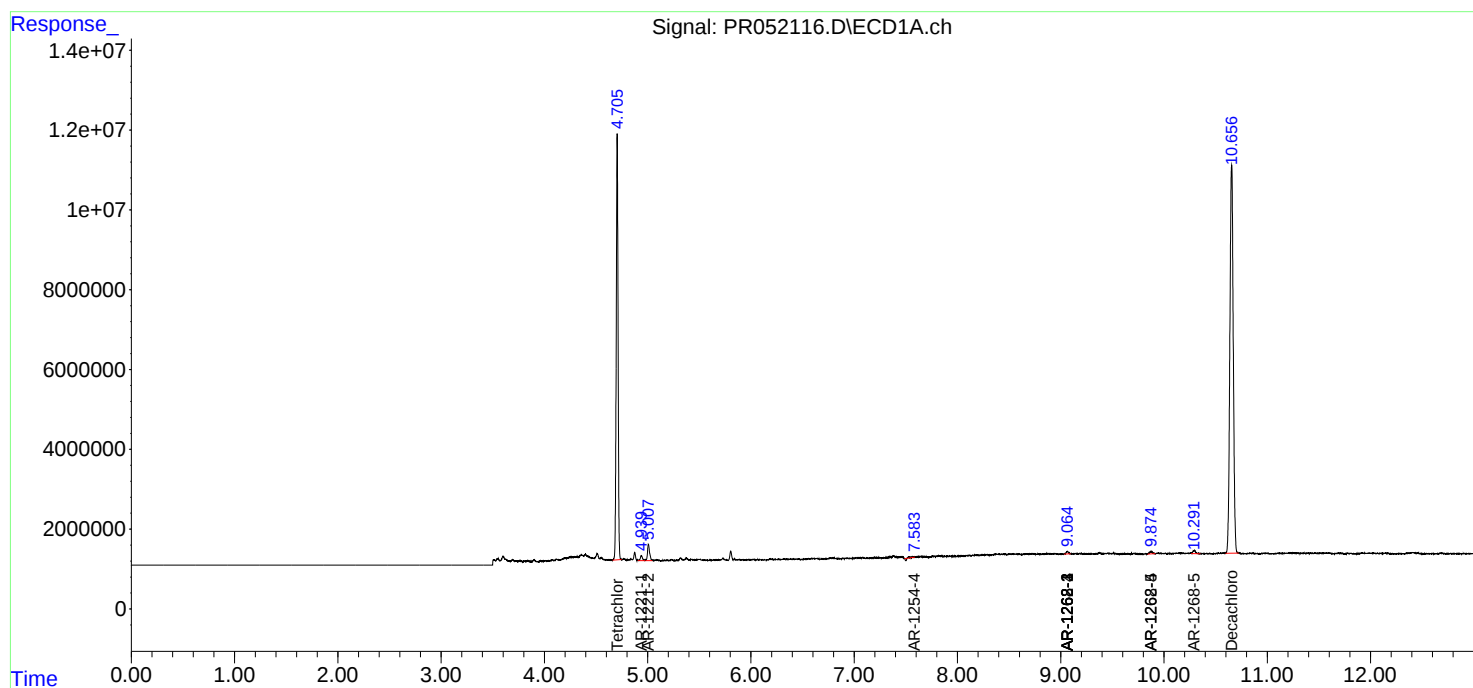

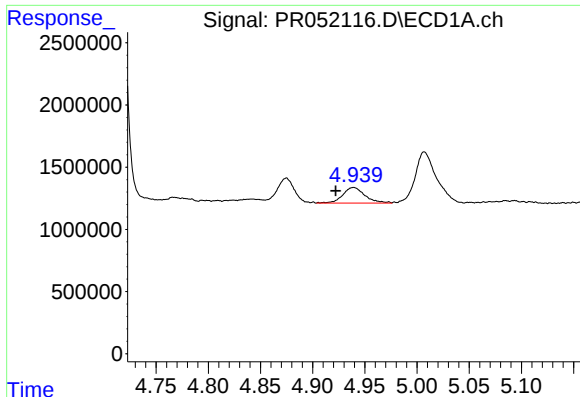


#8 AR-1221-1

R.T.: 4.939 min
Delta R.T.: 0.017 min
Response: 1846442
Conc: 24.65 ng/ml

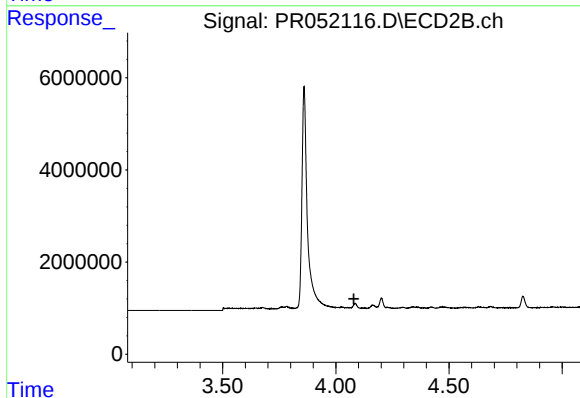


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.080 min
Response: 0
Conc: N.D.

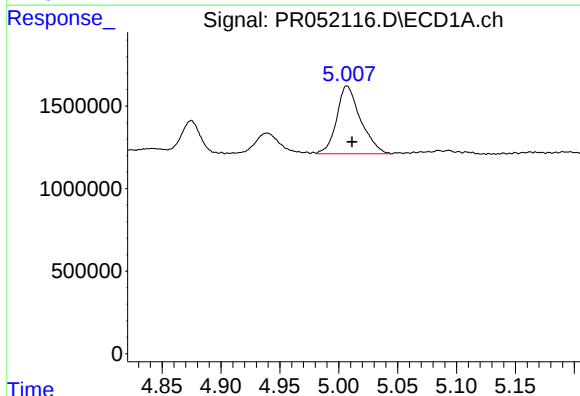


#9 AR-1221-2

R.T.: 5.007 min
Delta R.T.: -0.004 min
Response: 5787217
Conc: 112.28 ng/ml

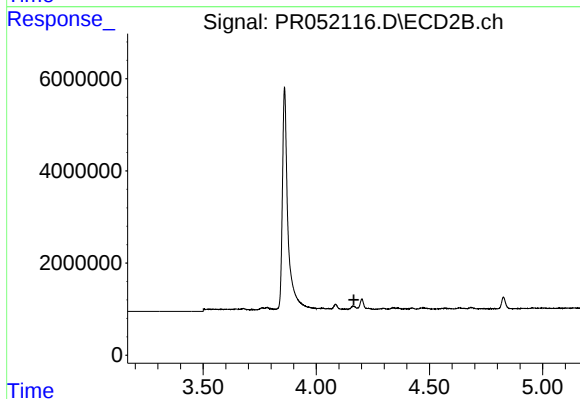


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.166 min
Response: 0
Conc: N.D.

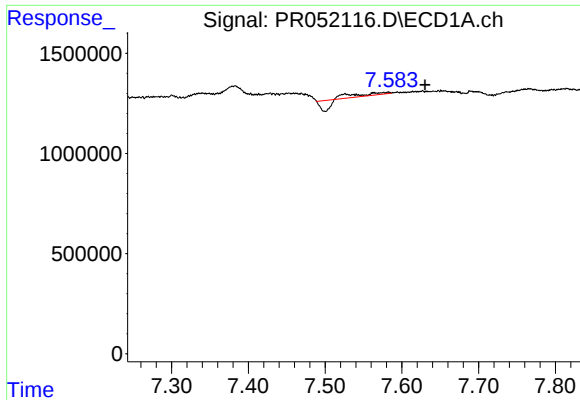


#29 AR-1254-4

R.T.: 7.583 min
Delta R.T.: -0.047 min
Response: 3739
Conc: 0.01 ng/ml

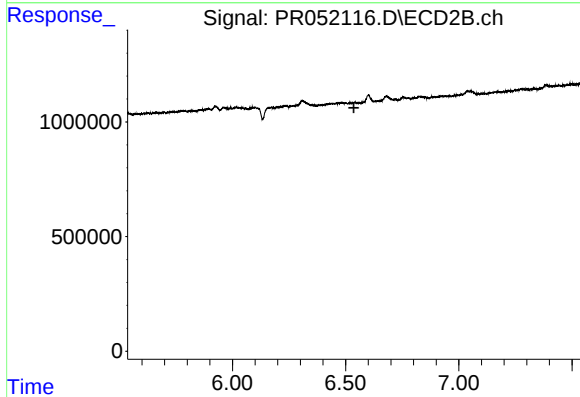


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 6.537 min
Response: 0
Conc: N.D.

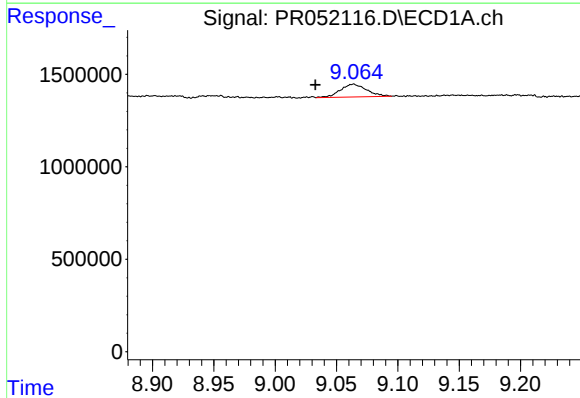


#38 AR-1262-3

R.T.: 9.064 min
Delta R.T.: 0.031 min
Response: 1018974
Conc: 3.56 ng/ml

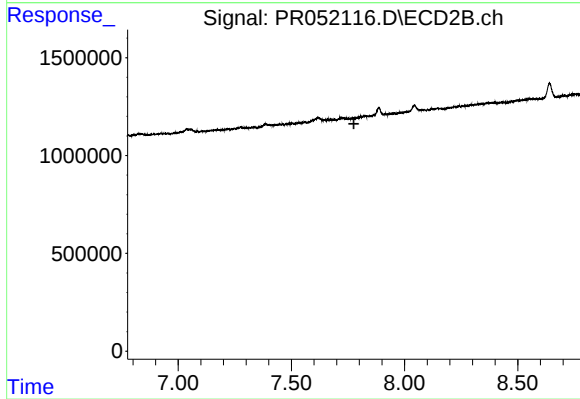


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 7.776 min
Response: 0
Conc: N.D.

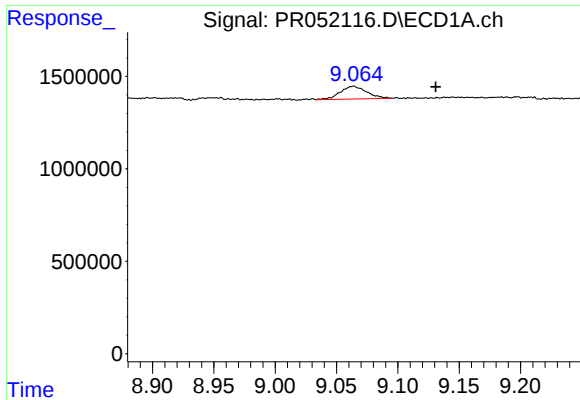


#39 AR-1262-4

R.T.: 9.064 min
Delta R.T.: -0.067 min
Response: 1018974
Conc: 5.91 ng/ml

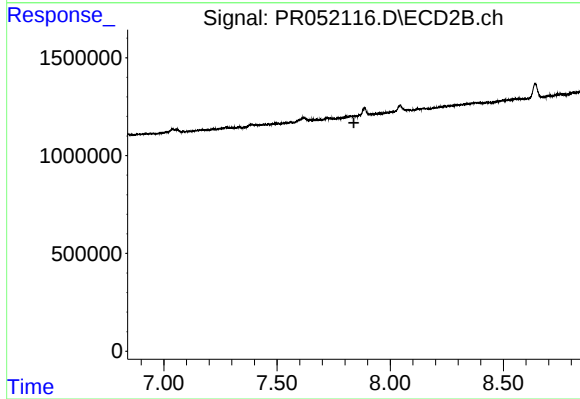


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 7.840 min
Response: 0
Conc: N.D.

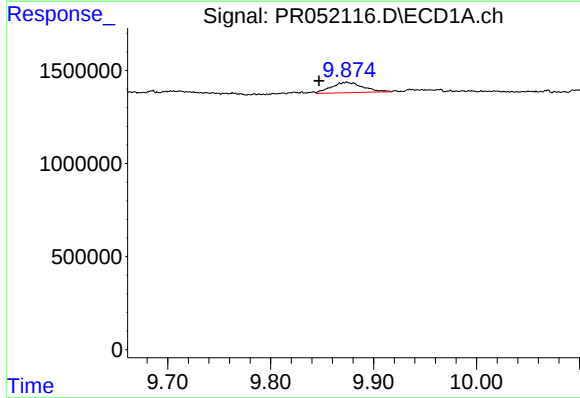


#40 AR-1262-5

R.T.: 9.874 min
Delta R.T.: 0.027 min
Response: 1190552
Conc: 4.77 ng/ml

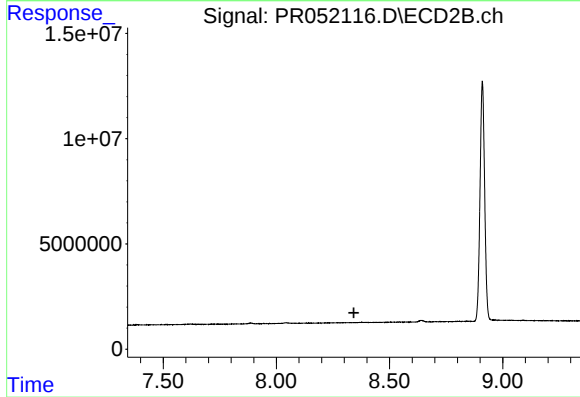


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 8.343 min
Response: 0
Conc: N.D.

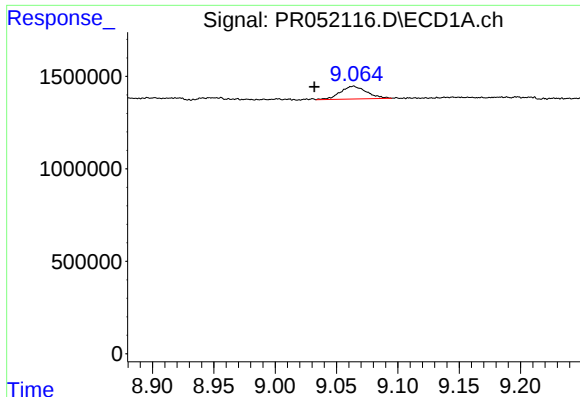


#41 AR-1268-1

R.T.: 9.064 min
Delta R.T.: 0.032 min
Response: 1018974
Conc: 1.31 ng/ml

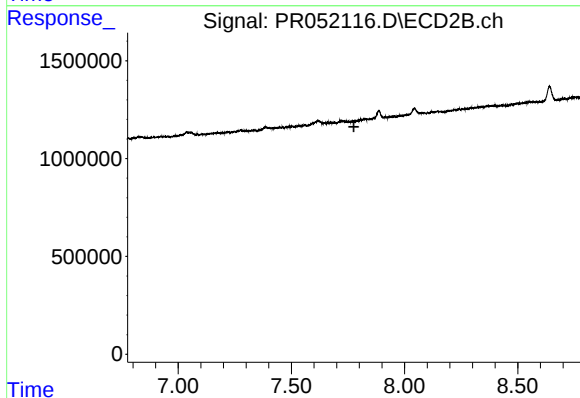


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.776 min
Response: 0
Conc: N.D.

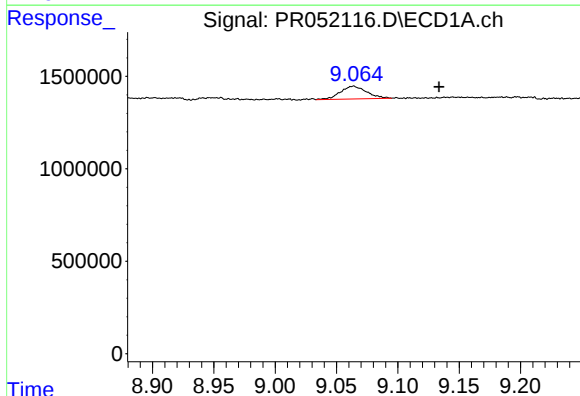


#42 AR-1268-2

R.T.: 9.064 min
Delta R.T.: -0.069 min
Response: 1018974
Conc: 1.44 ng/ml

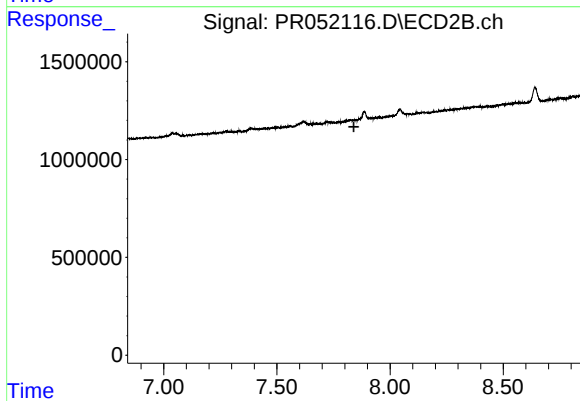


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.840 min
Response: 0
Conc: N.D.

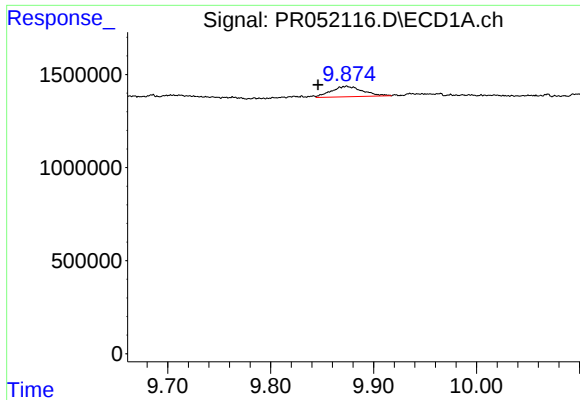


#44 AR-1268-4

R.T.: 9.874 min
Delta R.T.: 0.028 min
Response: 1190552
Conc: 4.37 ng/ml

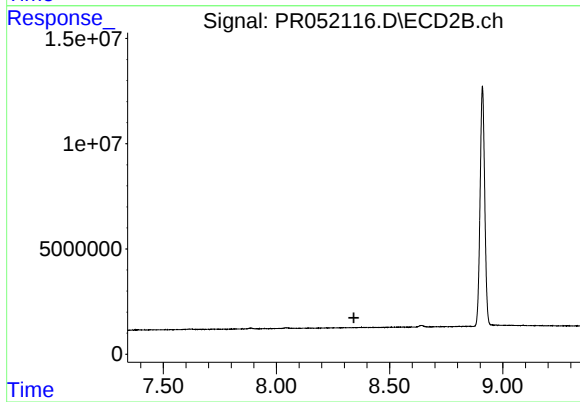


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

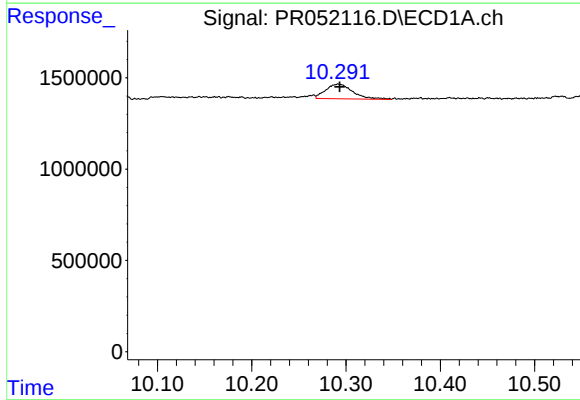

#45 AR-1268-5

R.T.: 10.292 min
Delta R.T.: -0.002 min
Response: 1598097
Conc: 0.79 ng/ml

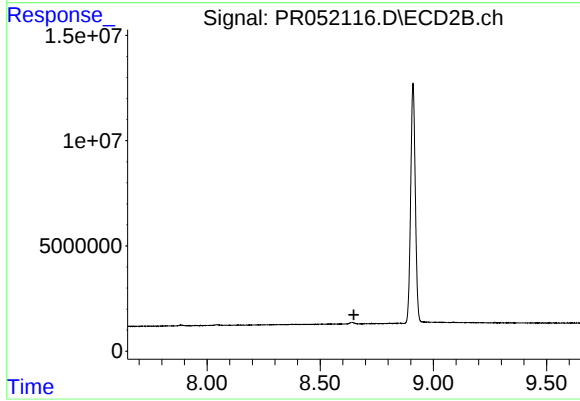

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.649 min
Response: 0
Conc: N.D.