

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092821\
 Data File : PR052181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2021 22:11
 Operator : AJ\MA
 Sample : M3876-11
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 02:33:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091421CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 08:14:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.705	3.858	122.8E6	73727663	19.104	16.865
2)	SA Decachlor...	10.654	8.907	153.8E6	127.0E6	32.385	30.837
Target Compounds							
8)	L2 AR-1221-1	4.937	0.000	3097651	0	41.353	N.D. #
9)	L2 AR-1221-2	5.020	4.162	1424641	1081928	27.640	31.843
28)	L6 AR-1254-3	0.000	6.302	0	931048	N.D.	2.792 #
29)	L6 AR-1254-4	0.000	6.529	0	825701	N.D.	4.408 #
30)	L6 AR-1254-5	8.047	6.945	1172286	1668741	3.839	5.883 #
32)	L7 AR-1260-2	0.000	6.618	0	1209819	N.D.	5.296 #
33)	L7 AR-1260-3	0.000	6.771	0	676595	N.D.	3.026 #
36)	L8 AR-1262-1	0.000	6.771	0	676595	N.D.	3.181 #
45)	L9 AR-1268-5	0.000	8.640	0	762649	N.D.	0.472 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092821\
Data File : PR052181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2021 22:11
Operator : AJ\MA
Sample : M3876-11
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 02:33:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091421CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 08:14:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

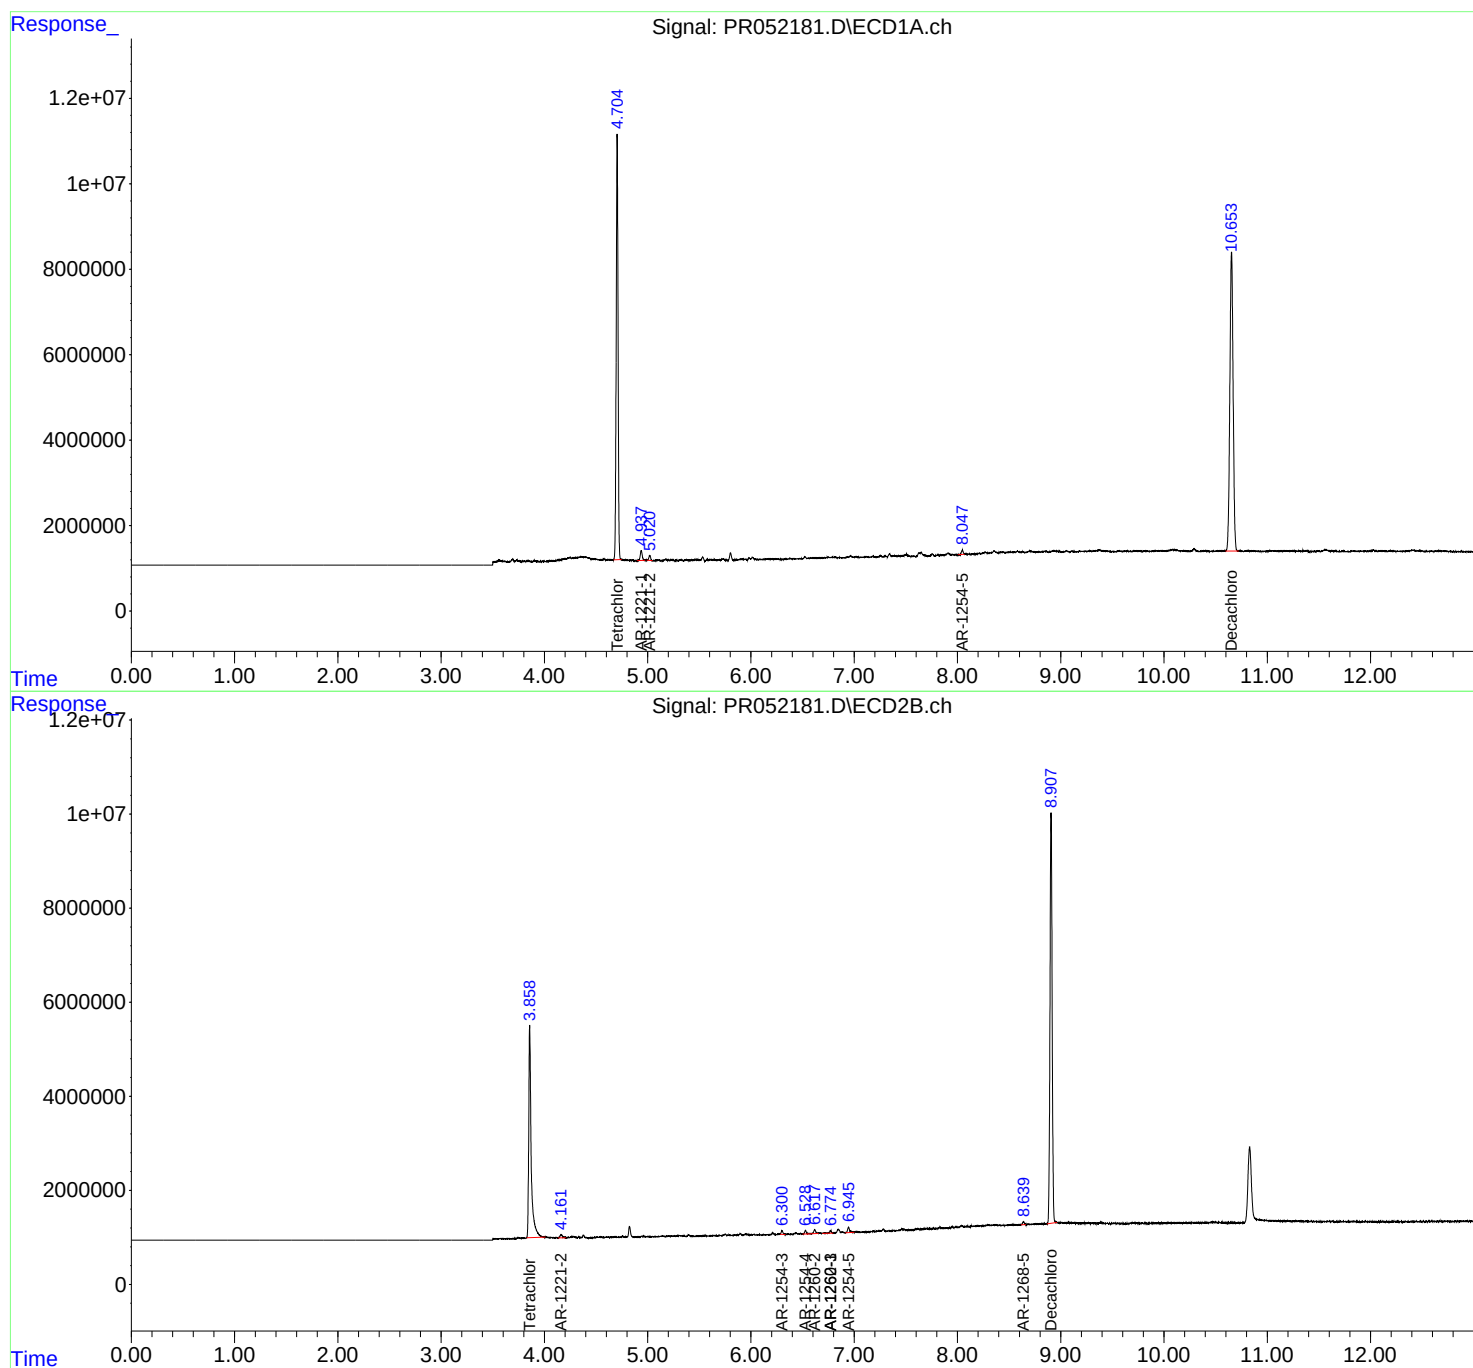


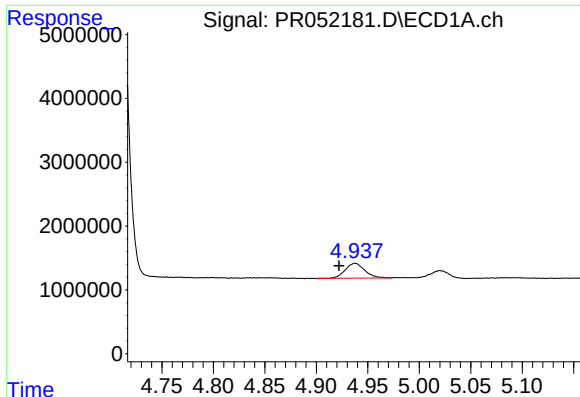

#8 AR-1221-1


R.T.: 4.937 min
Delta R.T.: 0.015 min
Response: 3097651
Conc: 41.35 ng/ml

Instrument :
ECD_R
ClientSampleId :

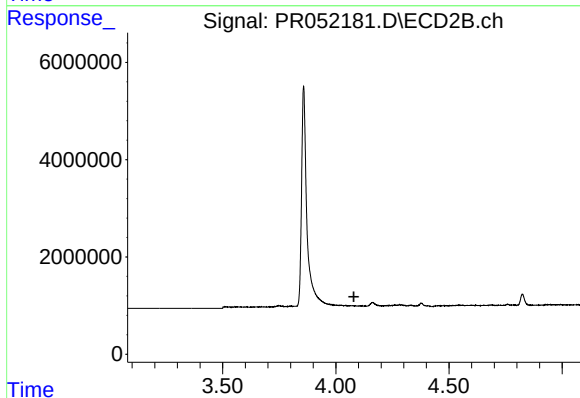


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.080 min
Response: 0
Conc: N.D.

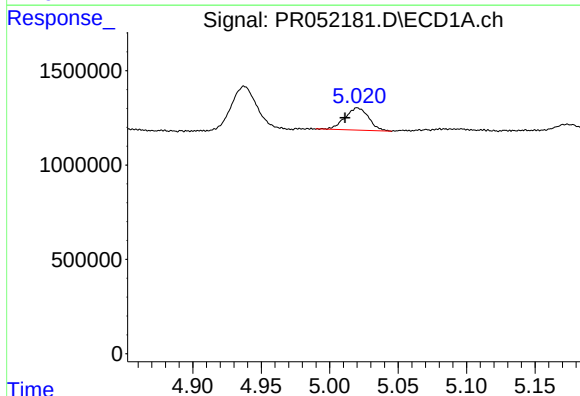


#9 AR-1221-2

R.T.: 5.020 min
Delta R.T.: 0.009 min
Response: 1424641
Conc: 27.64 ng/ml

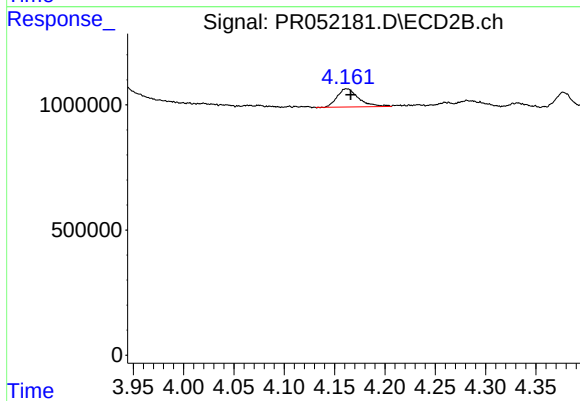

#9 AR-1221-2


R.T.: 4.162 min
Delta R.T.: -0.004 min
Response: 1081928
Conc: 31.84 ng/ml

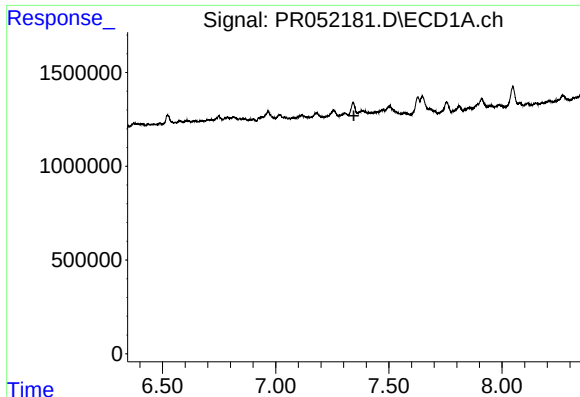

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

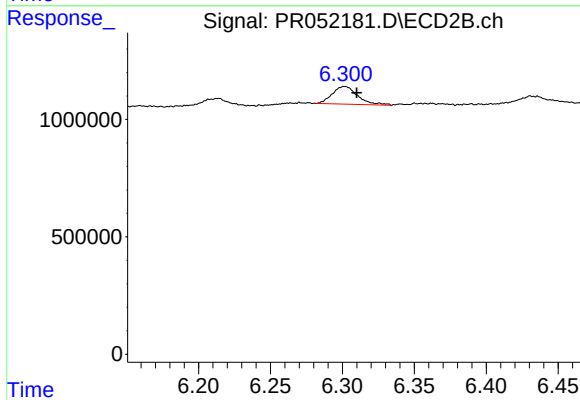


#28 AR-1254-3

R.T.: 6.302 min
Delta R.T.: -0.008 min
Response: 931048
Conc: 2.79 ng/ml

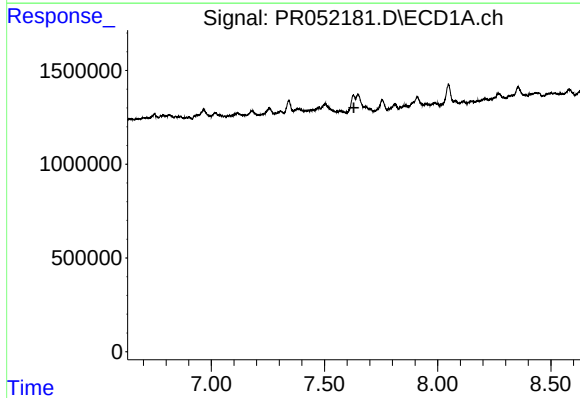


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.630 min
Response: 0
Conc: N.D.

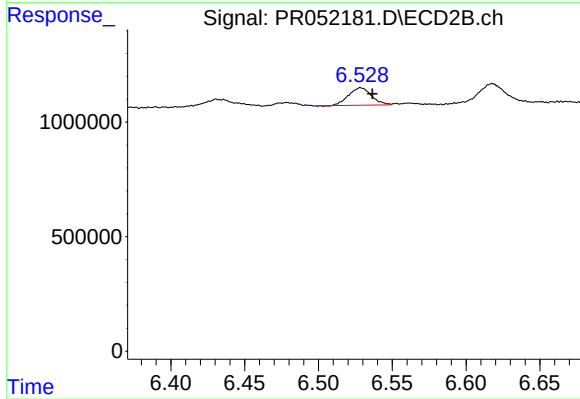

#29 AR-1254-4


R.T.: 6.529 min
Delta R.T.: -0.008 min
Response: 825701
Conc: 4.41 ng/ml

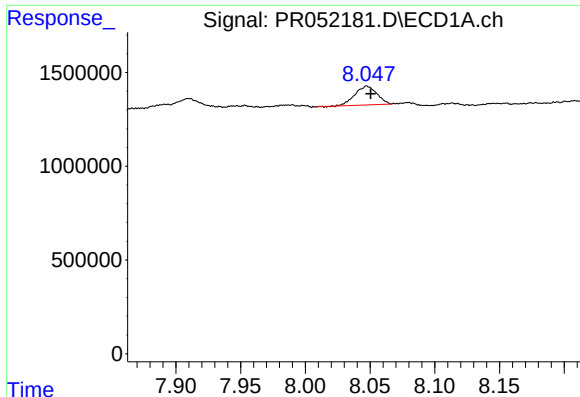

#30 AR-1254-5


R.T.: 8.047 min
Delta R.T.: -0.003 min
Response: 1172286
Conc: 3.84 ng/ml

Instrument :
ECD_R
ClientSampleId :

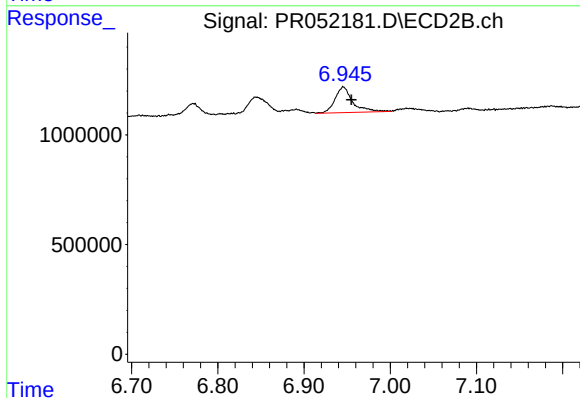


#30 AR-1254-5

R.T.: 6.945 min
Delta R.T.: -0.010 min
Response: 1668741
Conc: 5.88 ng/ml

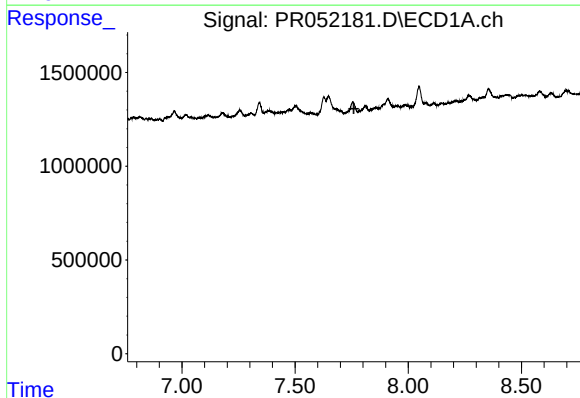


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.760 min
Response: 0
Conc: N.D.

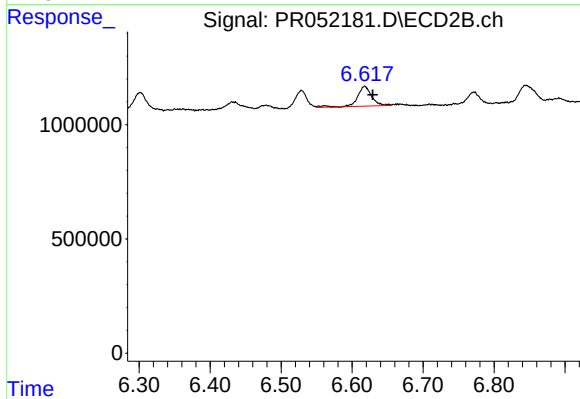

#32 AR-1260-2


R.T.: 6.618 min
Delta R.T.: -0.011 min
Response: 1209819
Conc: 5.30 ng/ml

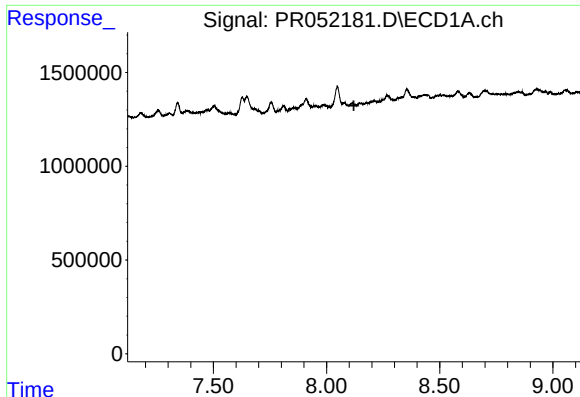

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

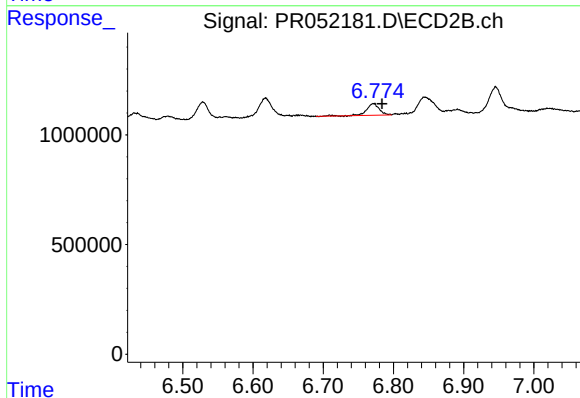


#33 AR-1260-3

R.T.: 6.771 min
Delta R.T.: -0.013 min
Response: 676595
Conc: 3.03 ng/ml

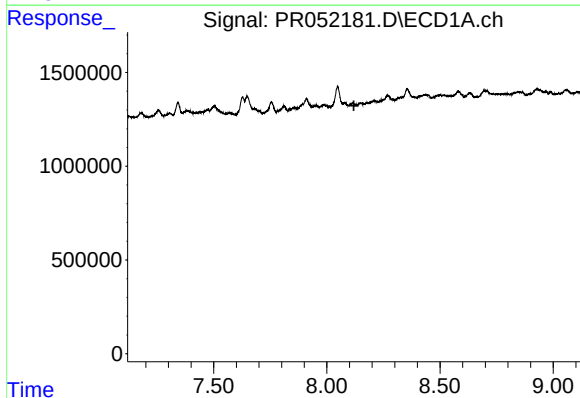


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.119 min
Response: 0
Conc: N.D.

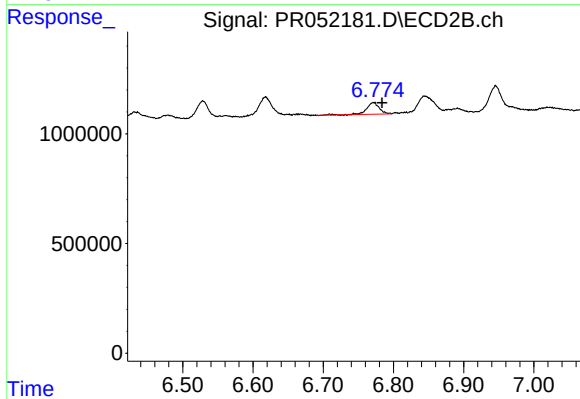

#36 AR-1262-1


R.T.: 6.771 min
Delta R.T.: -0.013 min
Response: 676595
Conc: 3.18 ng/ml

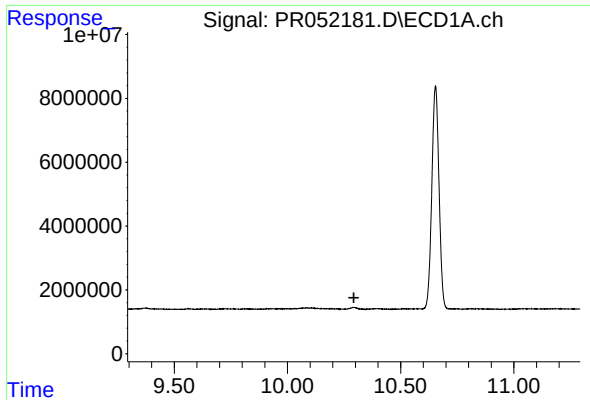

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

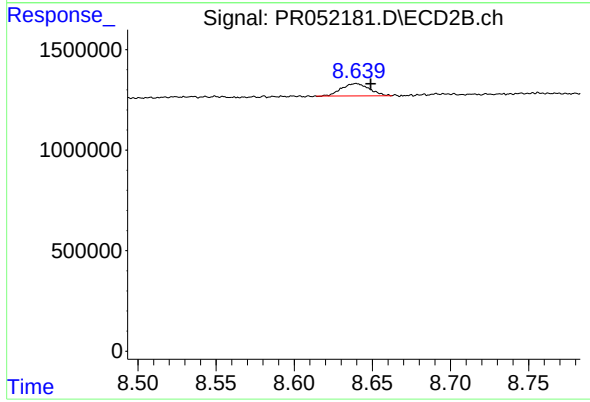

#45 AR-1268-5

R.T.: 8.640 min
Delta R.T.: -0.009 min
Response: 762649
Conc: 0.47 ng/ml