

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092822\
 Data File : PR057029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 15:36
 Operator : AJ\MA
 Sample : N4519-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-QT4-2022-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 17:17:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092622CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 27 09:08:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.616	2.887	81341561	40518565	21.465	22.585
2)	SA Decachlor...	9.501	8.089	86065749	65537918	51.729	45.413
Target Compounds							
3)	L1 AR-1016-1	4.837	3.991	2195992	1176778	21.322	22.887
4)	L1 AR-1016-2	4.858	4.007	3380980	1799228	22.521	22.902
5)	L1 AR-1016-3	4.922	4.184	2206953	872753	25.553	21.161
6)	L1 AR-1016-4	5.025	4.234	1928319	700134	27.704	24.278
7)	L1 AR-1016-5	5.340	4.449	2196137	807511	32.048	20.851 #
8)	L2 AR-1221-1	3.857	3.107	1189391	214046	26.574	10.345 #
9)	L2 AR-1221-2	3.927	3.188	1812100	587217	59.811	40.785 #
10)	L2 AR-1221-3	4.005	3.270	1460280	711427	15.022	14.317
11)	L3 AR-1232-1	4.005	3.270	1460280	711427	17.485	16.531
12)	L3 AR-1232-2	4.552	4.007	2307604	1799228	61.700	46.345
13)	L3 AR-1232-3	4.858	4.184	3380980	872753	46.860	44.271
14)	L3 AR-1232-4	5.025	4.275	1928319	895129	56.902	55.374
15)	L3 AR-1232-5	5.128	4.449	1594375	807511	64.043	44.140 #
16)	L4 AR-1242-1	4.837	3.991	2195992	1176778	24.547	26.854
17)	L4 AR-1242-2	4.858	4.007	3380980	1799228	25.689	26.388
18)	L4 AR-1242-3	4.922	4.184	2206953	872753	29.205	24.161
19)	L4 AR-1242-4	5.025	4.275	1928319	895129	30.632	28.079
20)	L4 AR-1242-5	5.810	4.815	518454	922896	8.254	22.506 #
21)	L5 AR-1248-1	4.837	3.991	2195992	1176778	31.919	34.648
22)	L5 AR-1248-2	5.128	4.234	1594375	700134	17.791	15.067
23)	L5 AR-1248-3	5.340	4.275	2196137	895129	20.921	18.501
24)	L5 AR-1248-4	5.774	4.449	440562	807511	3.909	13.796 #
25)	L5 AR-1248-5	5.810	4.855	518454	352698	4.746	5.924
26)	L6 AR-1254-1	5.742	4.815	1599869	922896	13.005	10.353
27)	L6 AR-1254-2	5.981	4.973	1569047	761964	8.622	9.912
28)	L6 AR-1254-3	6.374	5.408	943469	1409574	5.076	11.207 #
29)	L6 AR-1254-4	6.685	5.633	516804	181652	3.785	2.358 #
30)	L6 AR-1254-5	7.138	6.075	3840222	2425726	29.365	21.416 #
31)	L7 AR-1260-1	6.551	5.528	3033366	1902941	27.057	25.264
32)	L7 AR-1260-2	6.835	5.733	3824451	2440798	26.819	26.530
33)	L7 AR-1260-3	7.225	5.889	2983648	2089342	27.903	23.968
34)	L7 AR-1260-4	7.468	6.390	2825644	1898260	26.234	26.348
35)	L7 AR-1260-5	7.807	6.655	5800880	4779431	25.258	26.801
36)	L8 AR-1262-1	7.225	6.119	2983648	2094786	16.561	18.510
37)	L8 AR-1262-2	7.807	6.655	5800880	4779431	19.949	22.518
38)	L8 AR-1262-3	8.119	6.957	3099257	1147300	16.126	13.160
39)	L8 AR-1262-4	8.197	7.024	1034077	2901684	11.306	17.827 #
40)	L8 AR-1262-5	8.817	7.562	1957575	1125791	19.224	14.305 #
41)	L9 AR-1268-1	8.119	6.957	3099257	1147300	8.461	4.518 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092822\
 Data File : PR057029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2022 15:36
 Operator : AJ\MA
 Sample : N4519-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-QT4-2022-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 17:17:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092622CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 27 09:08:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.197	7.024	1034077	2901684	3.089	11.833 #
43) L9	AR-1268-3	8.412	7.245	212079	116580	0.745	0.558 #
44) L9	AR-1268-4	8.817	7.562	1957575	1125791	16.960	12.718 #
45) L9	AR-1268-5	9.198	7.855	1668690	1331004	1.974	1.967



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR092822\
Data File : PR057029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2022 15:36
Operator : AJ\MA
Sample : N4519-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 17:17:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092622CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 27 09:08:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

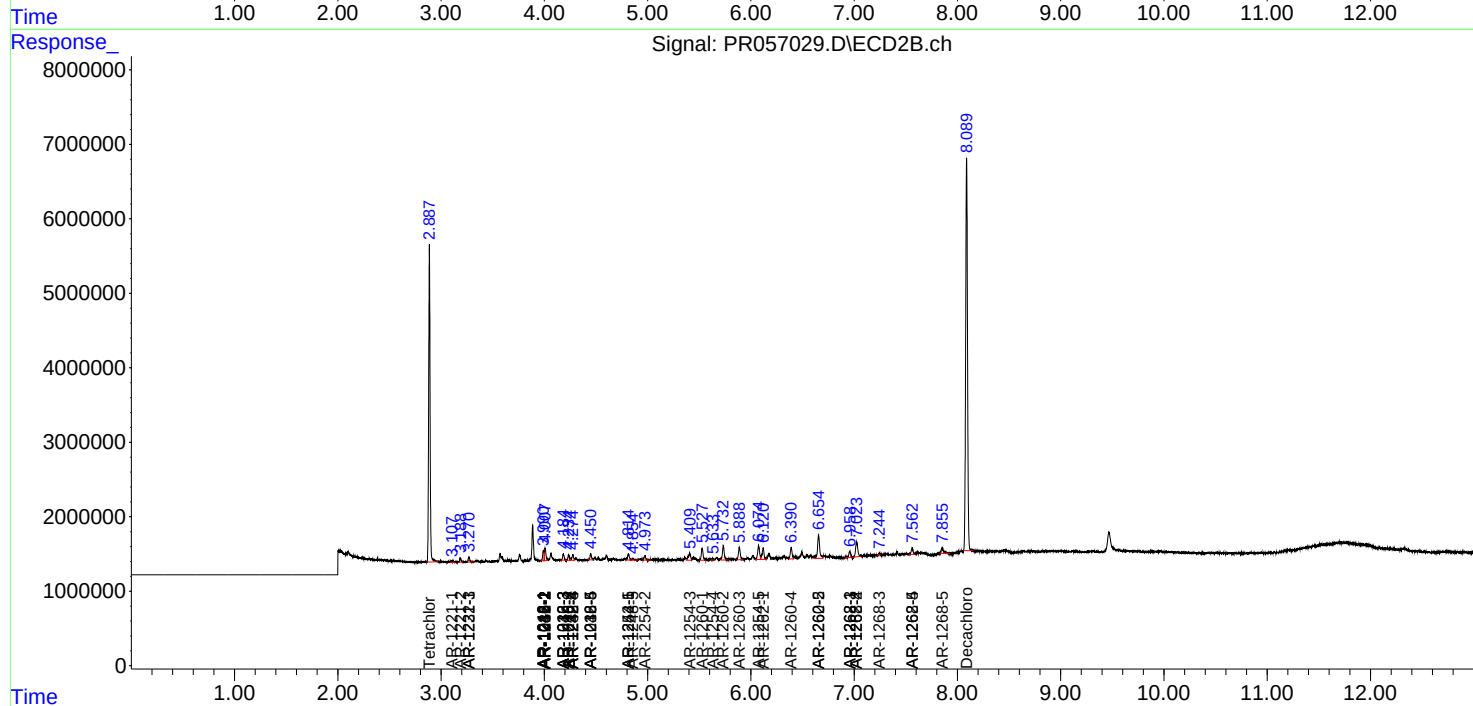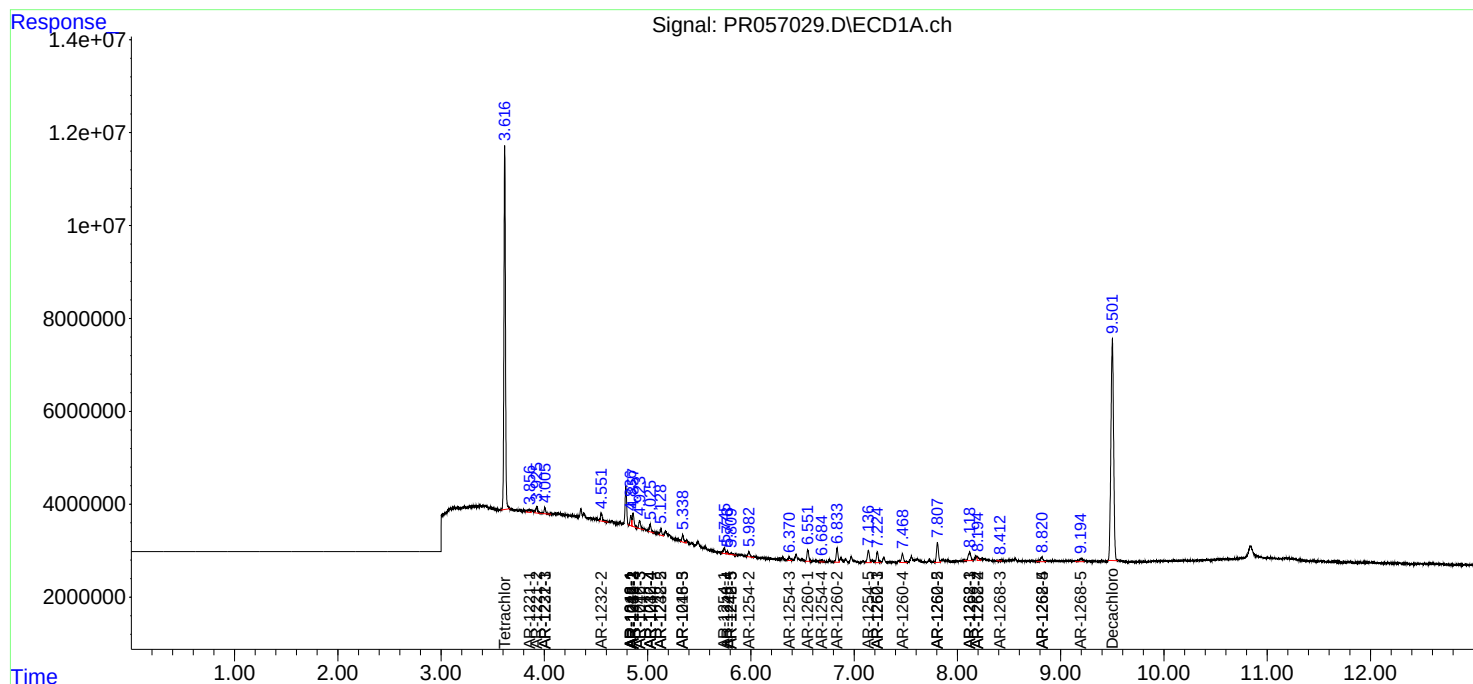


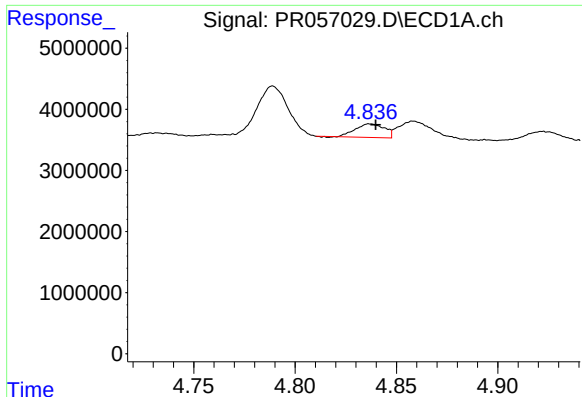

#3 AR-1016-1


R.T.: 4.837 min
Delta R.T.: -0.003 min
Response: 2195992
Conc: 21.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

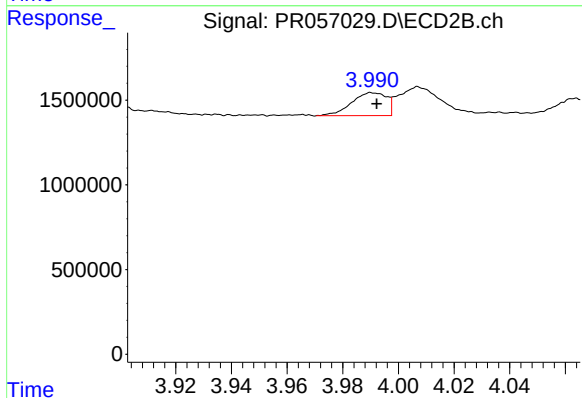


#3 AR-1016-1

R.T.: 3.991 min
Delta R.T.: -0.001 min
Response: 1176778
Conc: 22.89 ng/ml

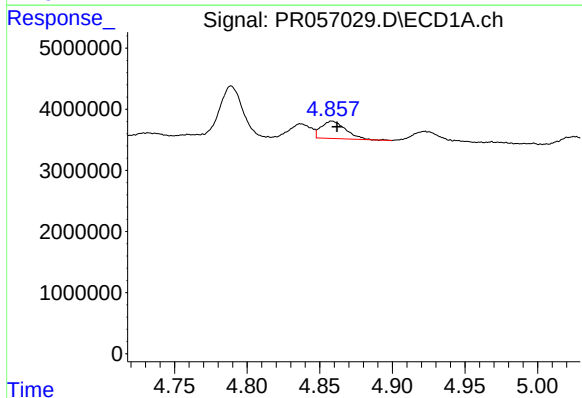


#4 AR-1016-2

R.T.: 4.858 min
Delta R.T.: -0.003 min
Response: 3380980
Conc: 22.52 ng/ml

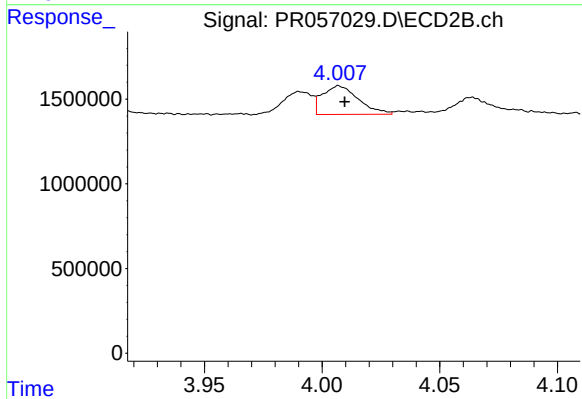

#4 AR-1016-2


R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 1799228
Conc: 22.90 ng/ml

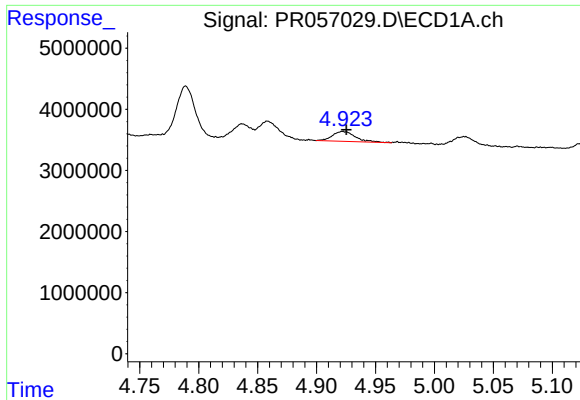

#5 AR-1016-3


R.T.: 4.922 min
Delta R.T.: -0.003 min
Response: 2206953
Conc: 25.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

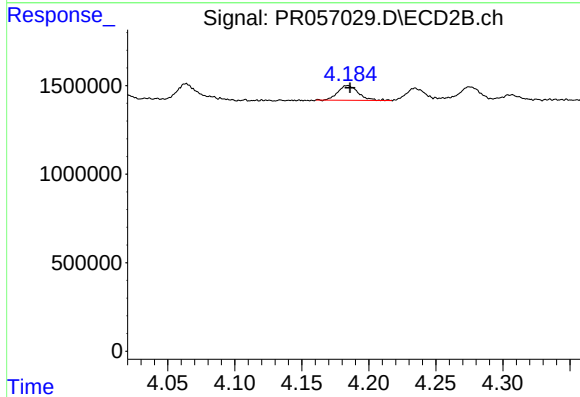


#5 AR-1016-3

R.T.: 4.184 min
Delta R.T.: -0.002 min
Response: 872753
Conc: 21.16 ng/ml

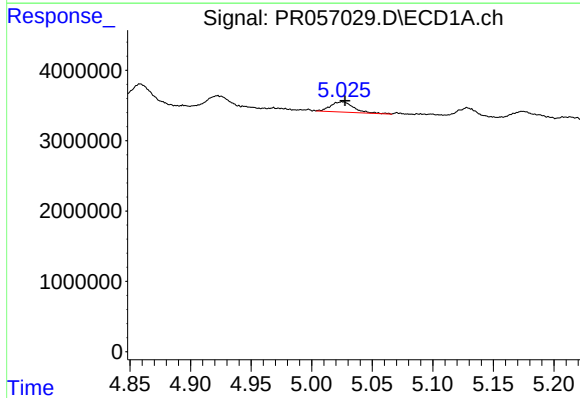


#6 AR-1016-4

R.T.: 5.025 min
Delta R.T.: -0.002 min
Response: 1928319
Conc: 27.70 ng/ml

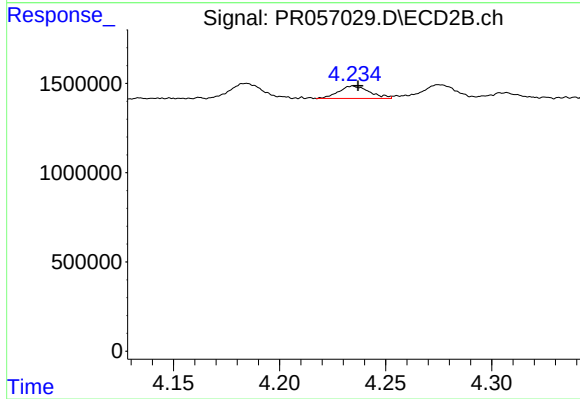

#6 AR-1016-4


R.T.: 4.234 min
Delta R.T.: -0.003 min
Response: 700134
Conc: 24.28 ng/ml

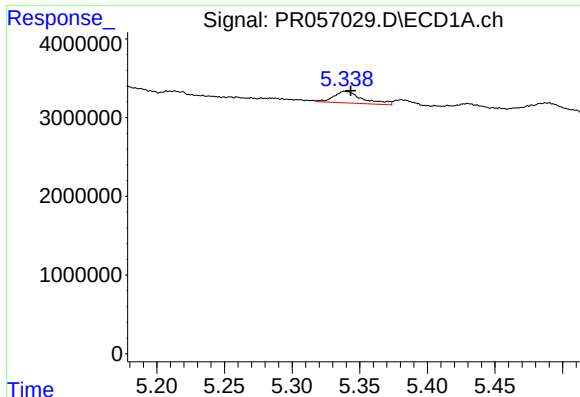

#7 AR-1016-5


R.T.: 5.340 min
Delta R.T.: -0.004 min
Response: 2196137
Conc: 32.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

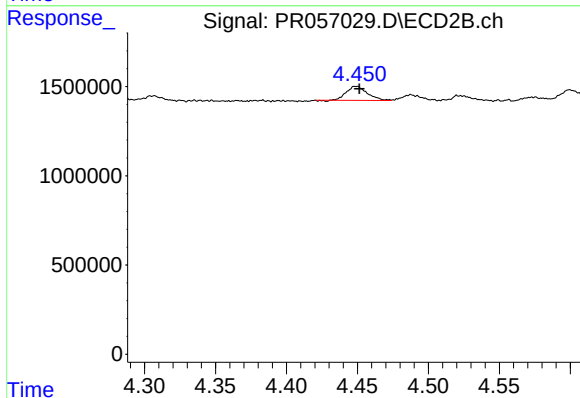


#7 AR-1016-5

R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 807511
Conc: 20.85 ng/ml

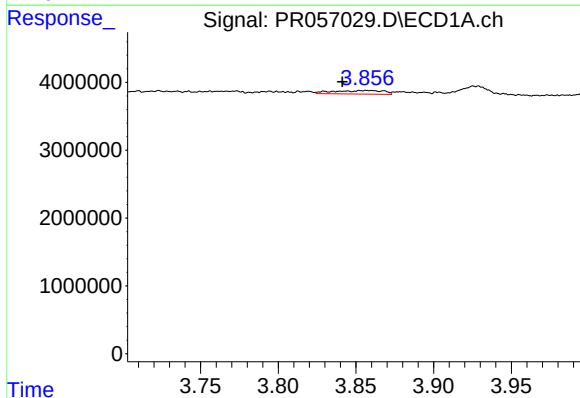


#8 AR-1221-1

R.T.: 3.857 min
Delta R.T.: 0.015 min
Response: 1189391
Conc: 26.57 ng/ml

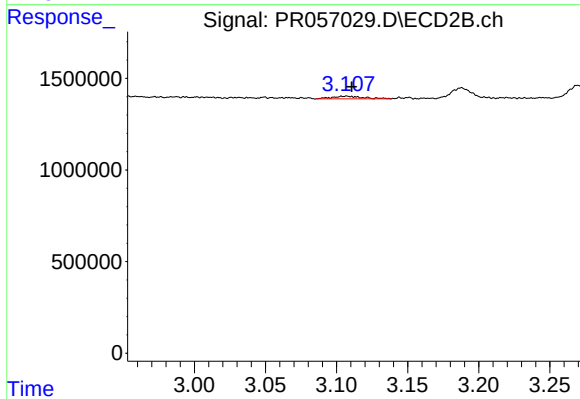

#8 AR-1221-1


R.T.: 3.107 min
Delta R.T.: -0.004 min
Response: 214046
Conc: 10.34 ng/ml

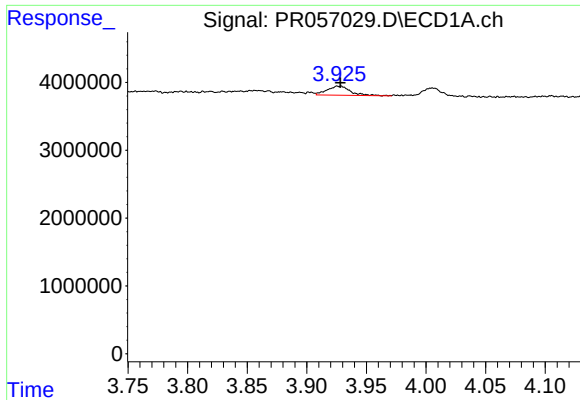

#9 AR-1221-2


R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 1812100
Conc: 59.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

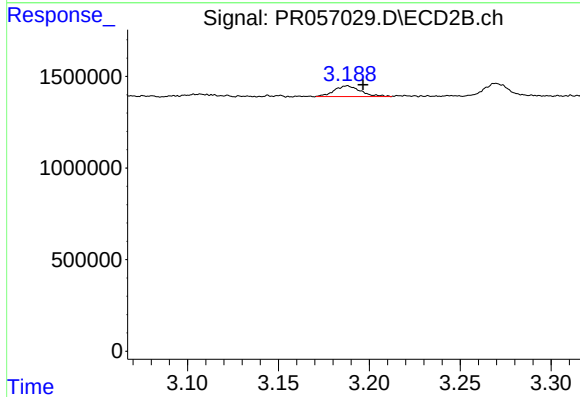


#9 AR-1221-2

R.T.: 3.188 min
Delta R.T.: -0.009 min
Response: 587217
Conc: 40.79 ng/ml

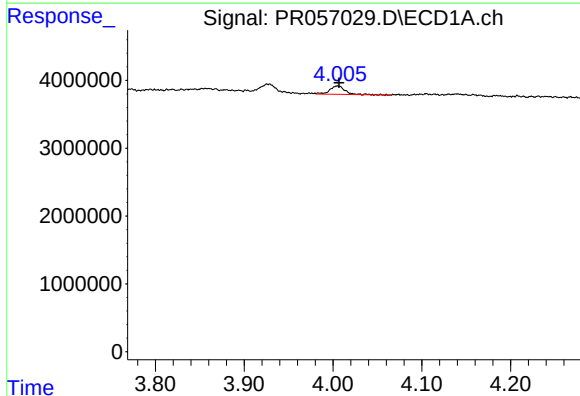


#10 AR-1221-3

R.T.: 4.005 min
Delta R.T.: -0.002 min
Response: 1460280
Conc: 15.02 ng/ml

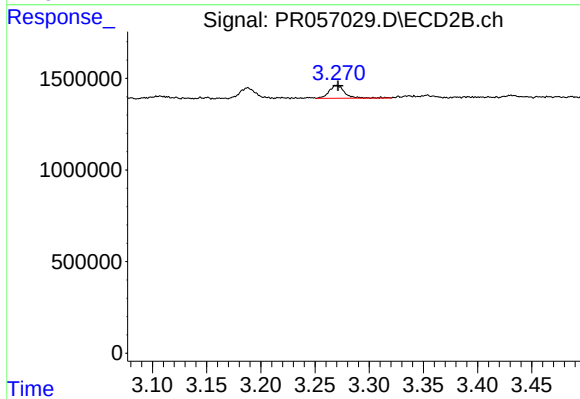

#10 AR-1221-3


R.T.: 3.270 min
Delta R.T.: -0.001 min
Response: 711427
Conc: 14.32 ng/ml

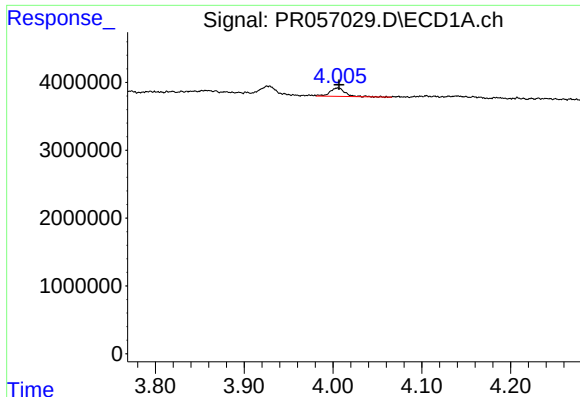

#11 AR-1232-1


R.T.: 4.005 min
Delta R.T.: -0.001 min
Response: 1460280
Conc: 17.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

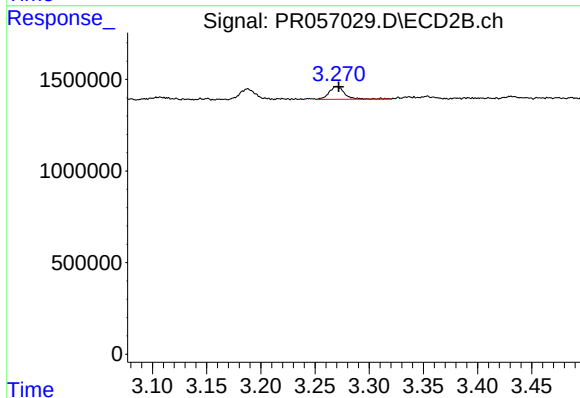


#11 AR-1232-1

R.T.: 3.270 min
Delta R.T.: -0.002 min
Response: 711427
Conc: 16.53 ng/ml

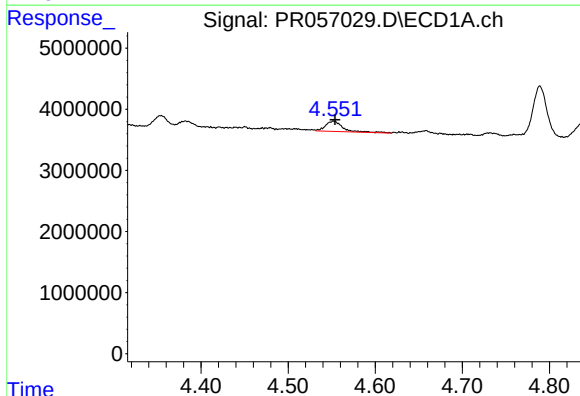


#12 AR-1232-2

R.T.: 4.552 min
Delta R.T.: -0.001 min
Response: 2307604
Conc: 61.70 ng/ml

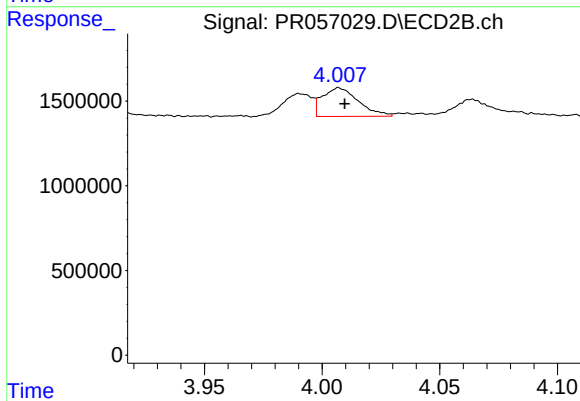

#12 AR-1232-2


R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 1799228
Conc: 46.35 ng/ml

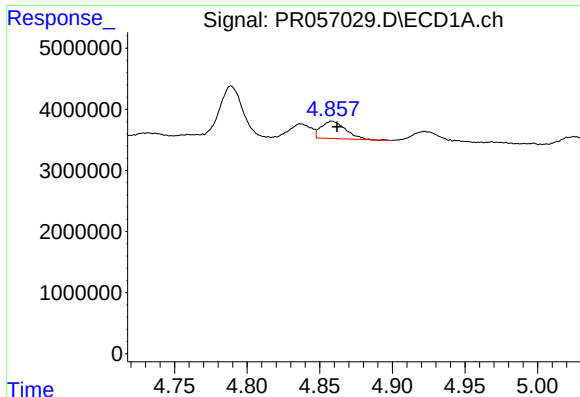

#13 AR-1232-3


R.T.: 4.858 min
Delta R.T.: -0.003 min
Response: 3380980
Conc: 46.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

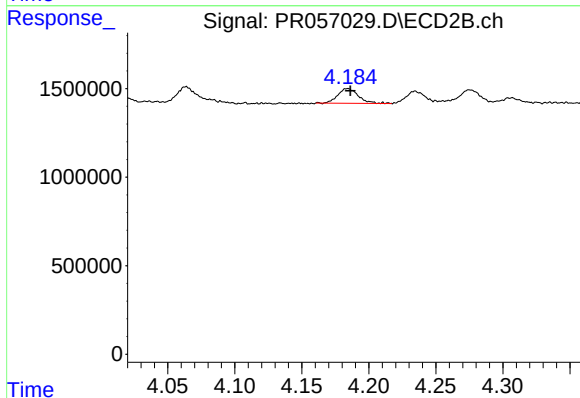


#13 AR-1232-3

R.T.: 4.184 min
Delta R.T.: -0.002 min
Response: 872753
Conc: 44.27 ng/ml

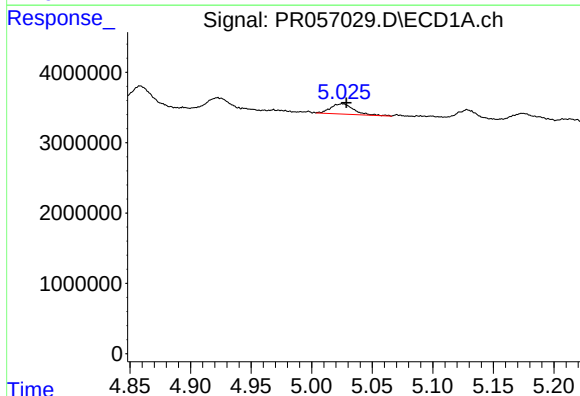


#14 AR-1232-4

R.T.: 5.025 min
Delta R.T.: -0.003 min
Response: 1928319
Conc: 56.90 ng/ml

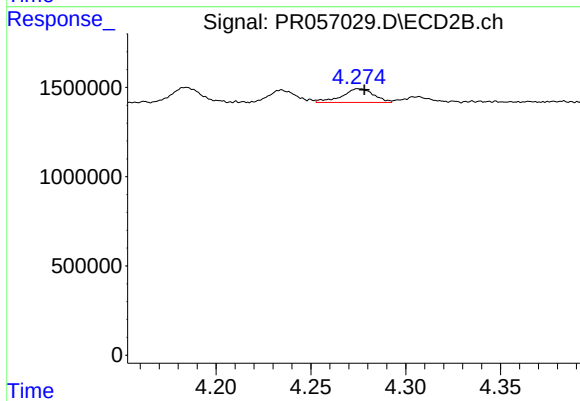

#14 AR-1232-4


R.T.: 4.275 min
Delta R.T.: -0.003 min
Response: 895129
Conc: 55.37 ng/ml

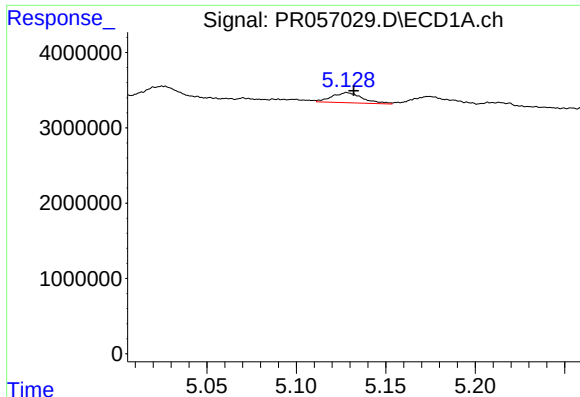

#15 AR-1232-5


R.T.: 5.128 min
Delta R.T.: -0.004 min
Response: 1594375
Conc: 64.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

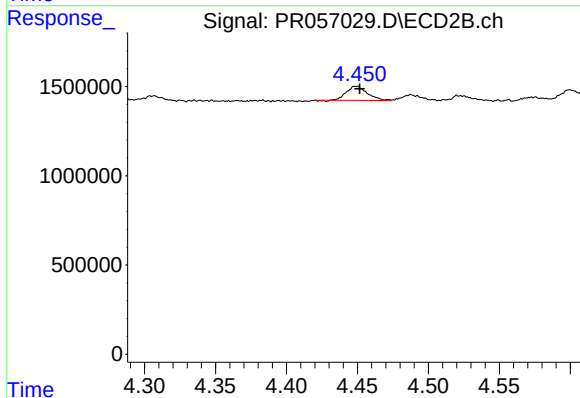


#15 AR-1232-5

R.T.: 4.449 min
Delta R.T.: -0.003 min
Response: 807511
Conc: 44.14 ng/ml

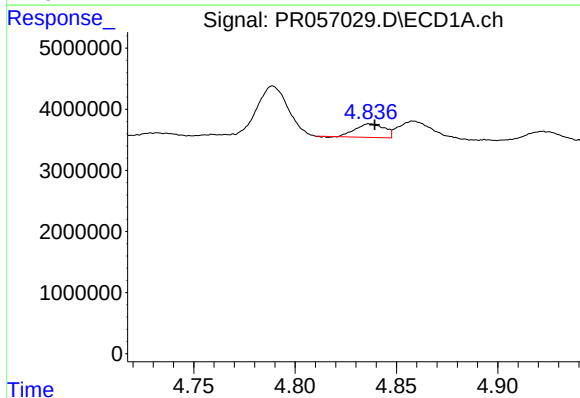


#16 AR-1242-1

R.T.: 4.837 min
Delta R.T.: -0.002 min
Response: 2195992
Conc: 24.55 ng/ml

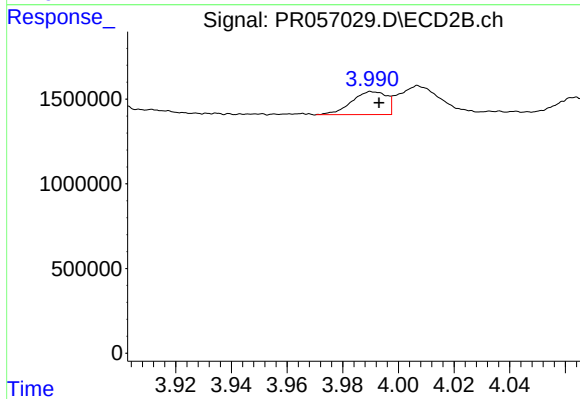

#16 AR-1242-1


R.T.: 3.991 min
Delta R.T.: -0.002 min
Response: 1176778
Conc: 26.85 ng/ml

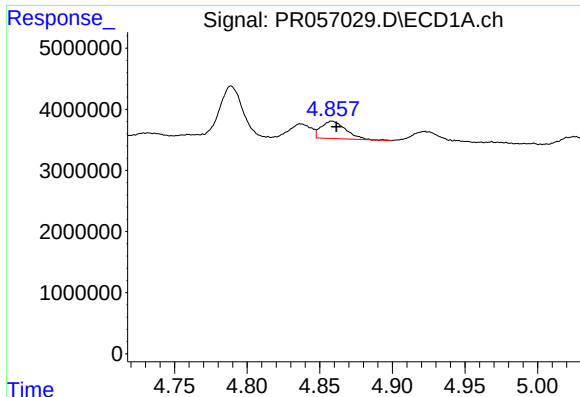

#17 AR-1242-2


R.T.: 4.858 min
Delta R.T.: -0.003 min
Response: 3380980
Conc: 25.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

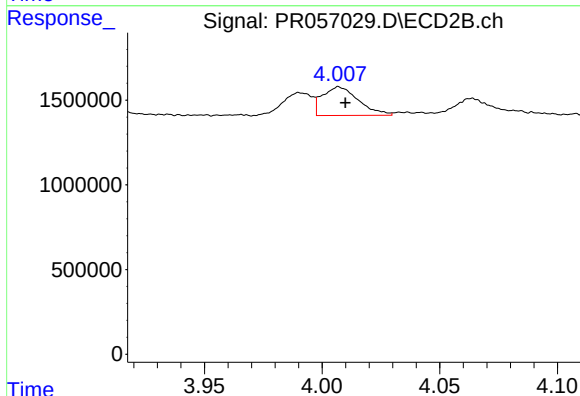


#17 AR-1242-2

R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 1799228
Conc: 26.39 ng/ml

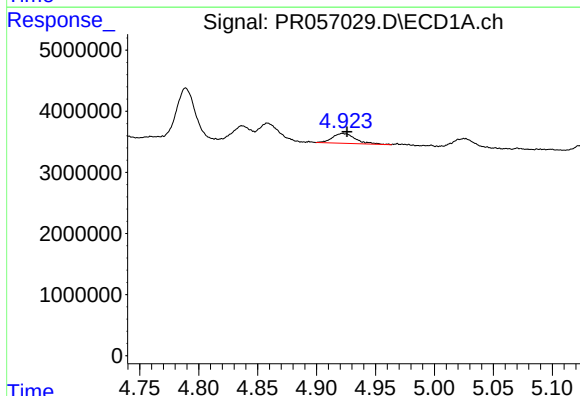


#18 AR-1242-3

R.T.: 4.922 min
Delta R.T.: -0.003 min
Response: 2206953
Conc: 29.21 ng/ml

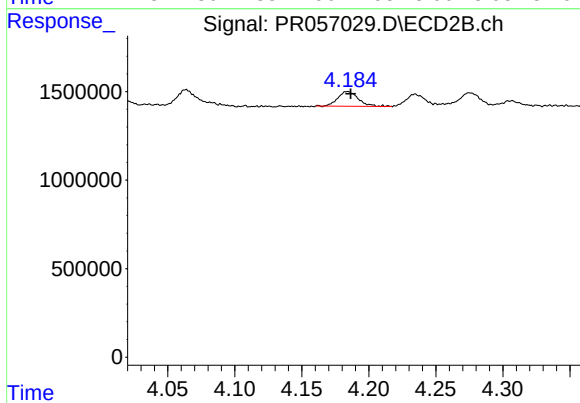

#18 AR-1242-3


R.T.: 4.184 min
Delta R.T.: -0.002 min
Response: 872753
Conc: 24.16 ng/ml

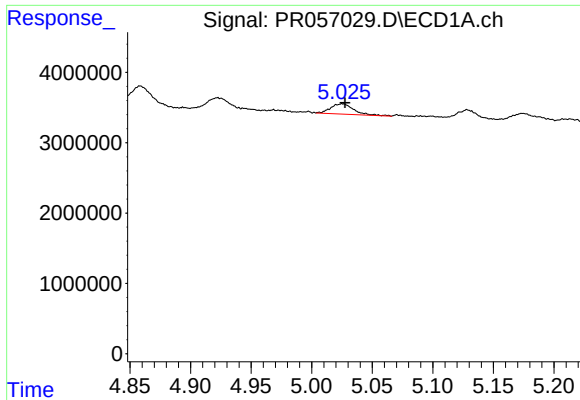

#19 AR-1242-4


R.T.: 5.025 min
Delta R.T.: -0.002 min
Response: 1928319
Conc: 30.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

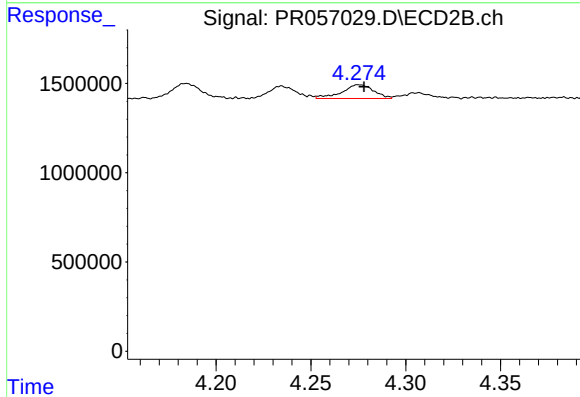


#19 AR-1242-4

R.T.: 4.275 min
Delta R.T.: -0.003 min
Response: 895129
Conc: 28.08 ng/ml

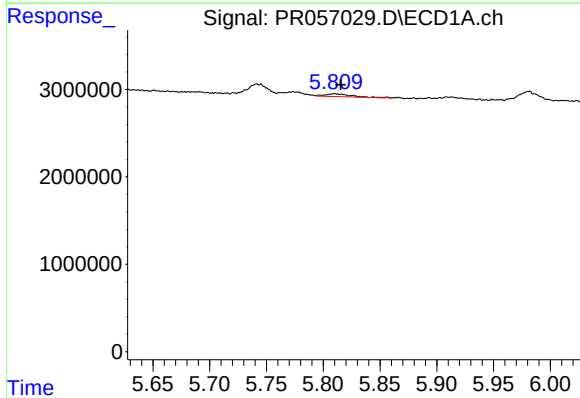


#20 AR-1242-5

R.T.: 5.810 min
Delta R.T.: -0.006 min
Response: 518454
Conc: 8.25 ng/ml

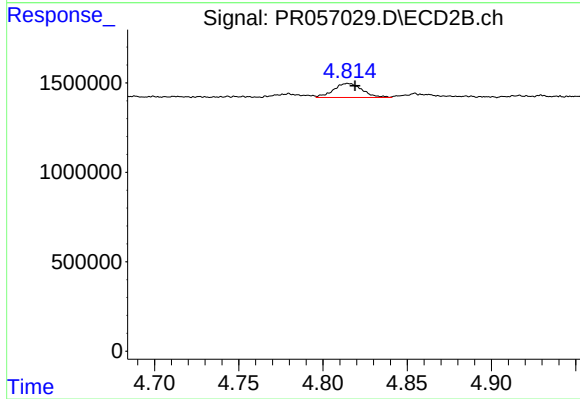

#20 AR-1242-5


R.T.: 4.815 min
Delta R.T.: -0.004 min
Response: 922896
Conc: 22.51 ng/ml

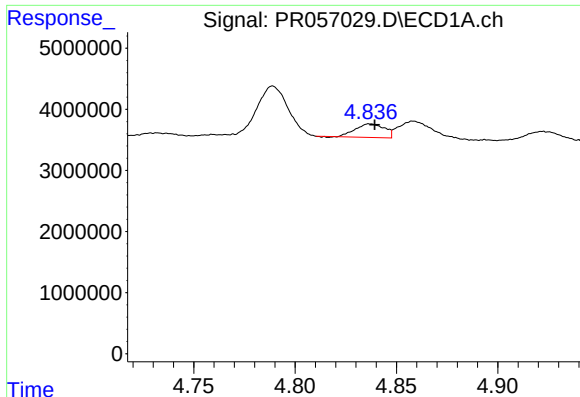

#21 AR-1248-1


R.T.: 4.837 min
Delta R.T.: -0.002 min
Response: 2195992
Conc: 31.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

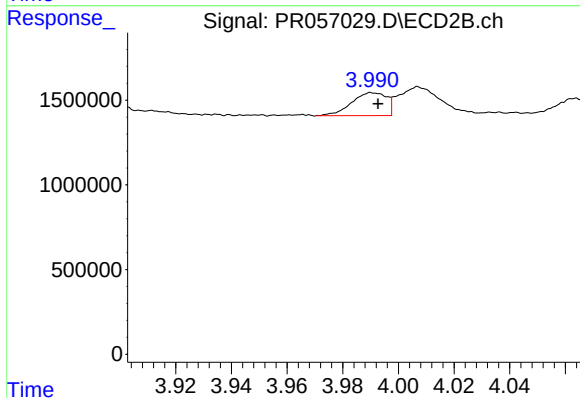


#21 AR-1248-1

R.T.: 3.991 min
Delta R.T.: -0.002 min
Response: 1176778
Conc: 34.65 ng/ml

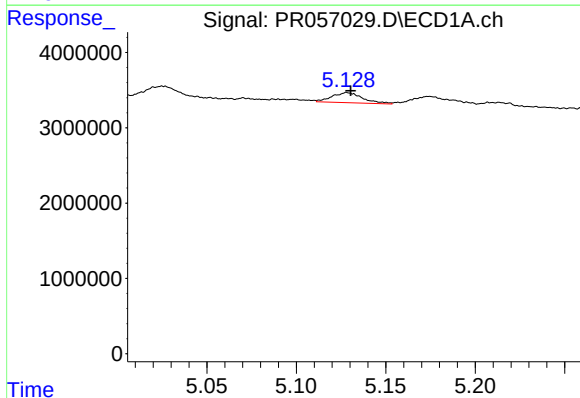


#22 AR-1248-2

R.T.: 5.128 min
Delta R.T.: -0.002 min
Response: 1594375
Conc: 17.79 ng/ml

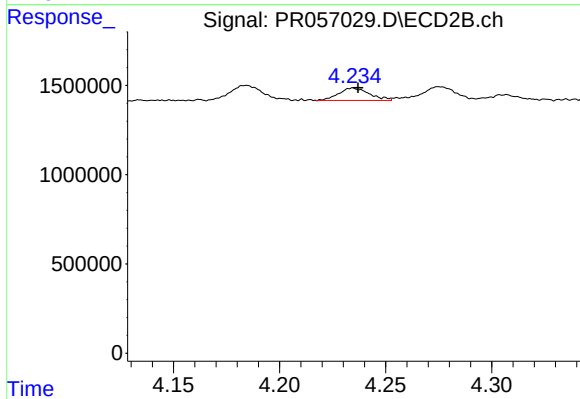

#22 AR-1248-2


R.T.: 4.234 min
Delta R.T.: -0.003 min
Response: 700134
Conc: 15.07 ng/ml

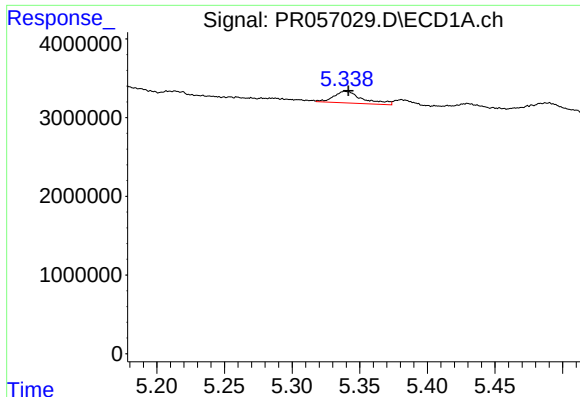

#23 AR-1248-3


R.T.: 5.340 min
Delta R.T.: -0.002 min
Response: 2196137
Conc: 20.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

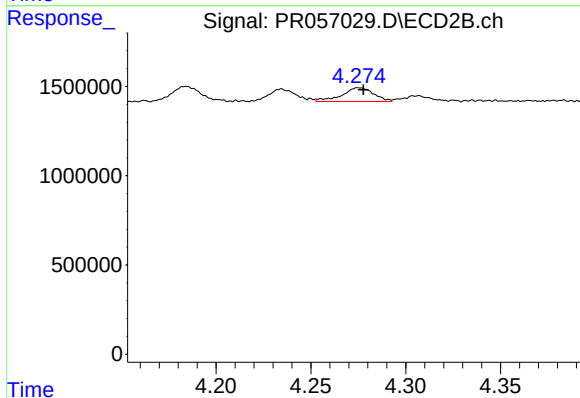


#23 AR-1248-3

R.T.: 4.275 min
Delta R.T.: -0.002 min
Response: 895129
Conc: 18.50 ng/ml

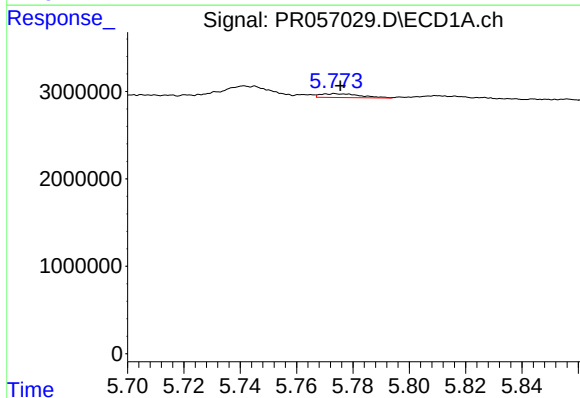


#24 AR-1248-4

R.T.: 5.774 min
Delta R.T.: -0.002 min
Response: 440562
Conc: 3.91 ng/ml

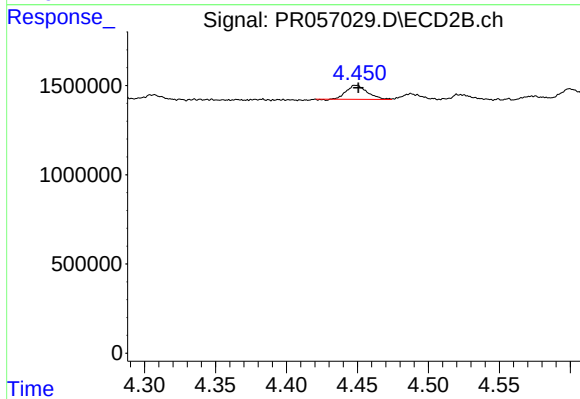

#24 AR-1248-4


R.T.: 4.449 min
Delta R.T.: -0.001 min
Response: 807511
Conc: 13.80 ng/ml

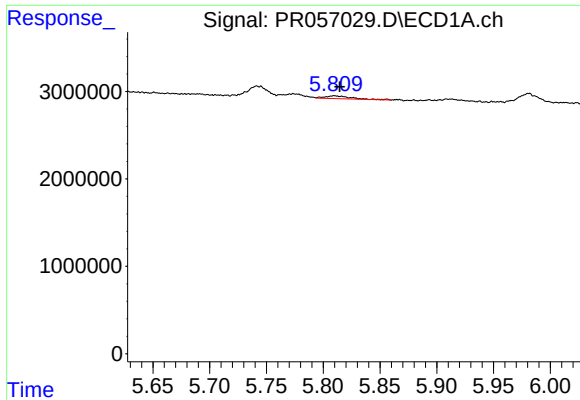

#25 AR-1248-5


R.T.: 5.810 min
Delta R.T.: -0.005 min
Response: 518454
Conc: 4.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

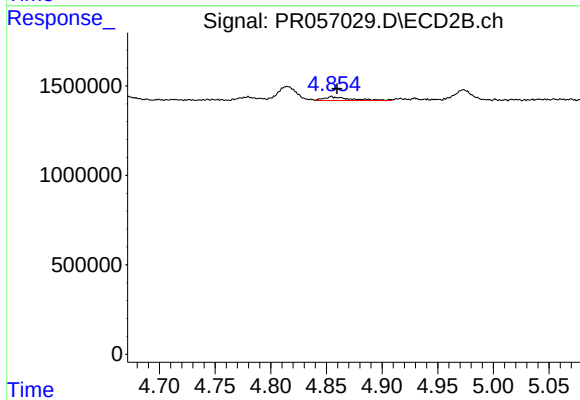


#25 AR-1248-5

R.T.: 4.855 min
Delta R.T.: -0.005 min
Response: 352698
Conc: 5.92 ng/ml

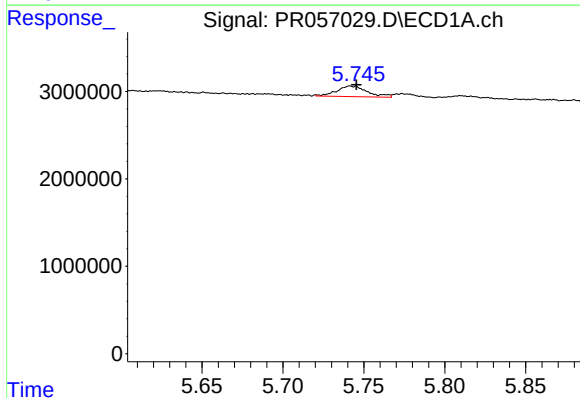


#26 AR-1254-1

R.T.: 5.742 min
Delta R.T.: -0.004 min
Response: 1599869
Conc: 13.01 ng/ml

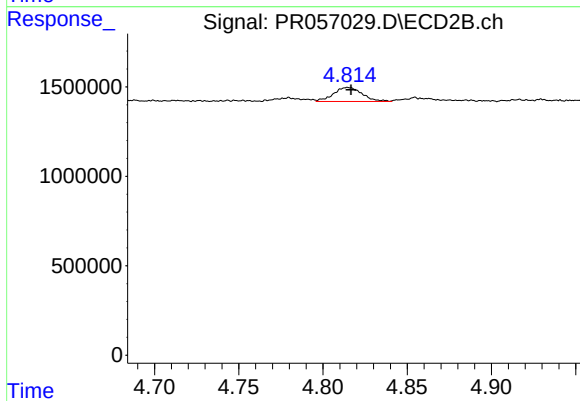

#26 AR-1254-1


R.T.: 4.815 min
Delta R.T.: -0.002 min
Response: 922896
Conc: 10.35 ng/ml

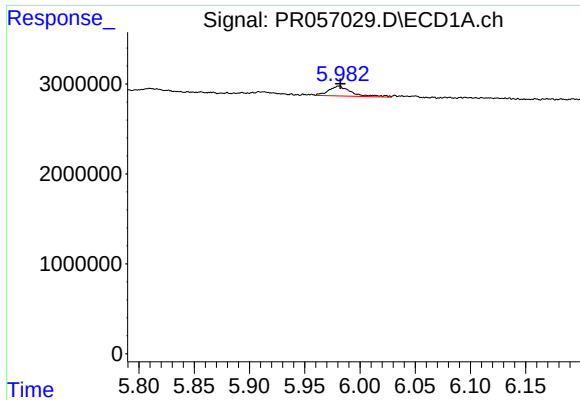

#27 AR-1254-2


R.T.: 5.981 min
Delta R.T.: -0.001 min
Response: 1569047
Conc: 8.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

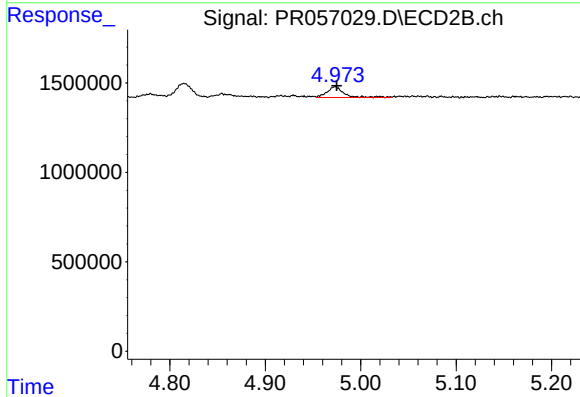


#27 AR-1254-2

R.T.: 4.973 min
Delta R.T.: -0.002 min
Response: 761964
Conc: 9.91 ng/ml

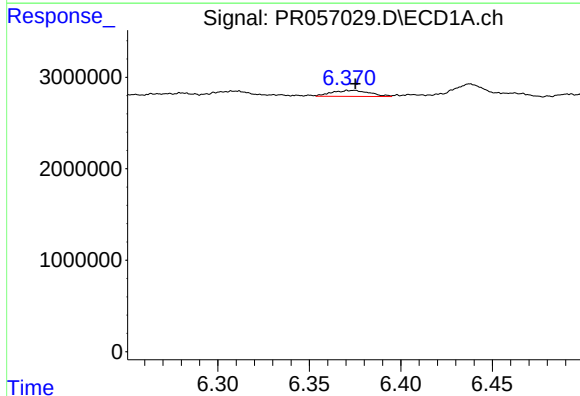


#28 AR-1254-3

R.T.: 6.374 min
Delta R.T.: -0.001 min
Response: 943469
Conc: 5.08 ng/ml

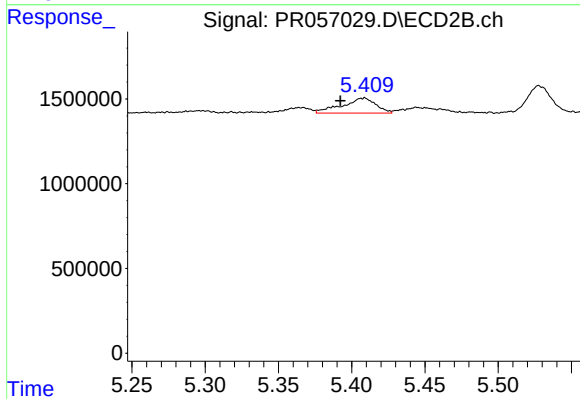

#28 AR-1254-3


R.T.: 5.408 min
Delta R.T.: 0.016 min
Response: 1409574
Conc: 11.21 ng/ml

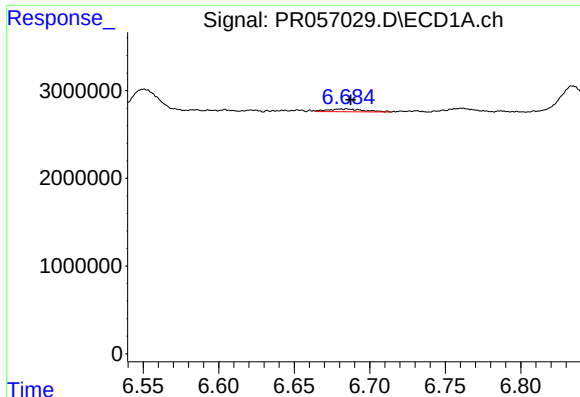

#29 AR-1254-4


R.T.: 6.685 min
Delta R.T.: -0.003 min
Response: 516804
Conc: 3.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

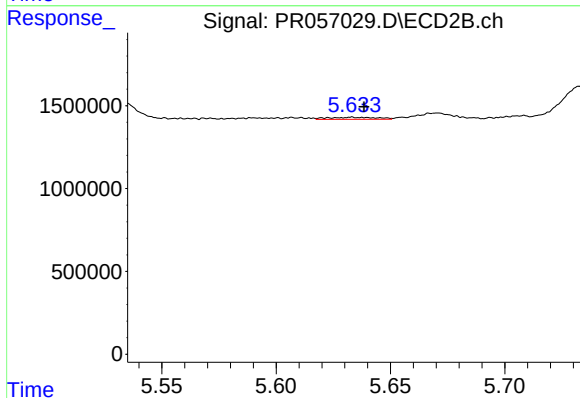


#29 AR-1254-4

R.T.: 5.633 min
Delta R.T.: -0.005 min
Response: 181652
Conc: 2.36 ng/ml

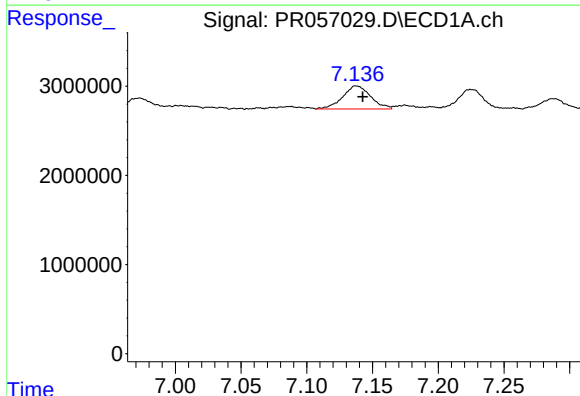


#30 AR-1254-5

R.T.: 7.138 min
Delta R.T.: -0.005 min
Response: 3840222
Conc: 29.37 ng/ml

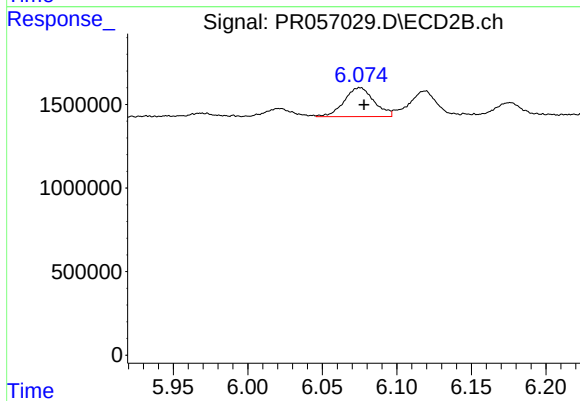

#30 AR-1254-5


R.T.: 6.075 min
Delta R.T.: -0.003 min
Response: 2425726
Conc: 21.42 ng/ml

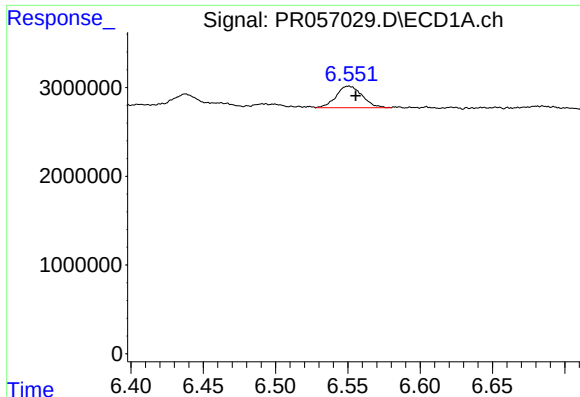

#31 AR-1260-1


R.T.: 6.551 min
Delta R.T.: -0.005 min
Response: 3033366
Conc: 27.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

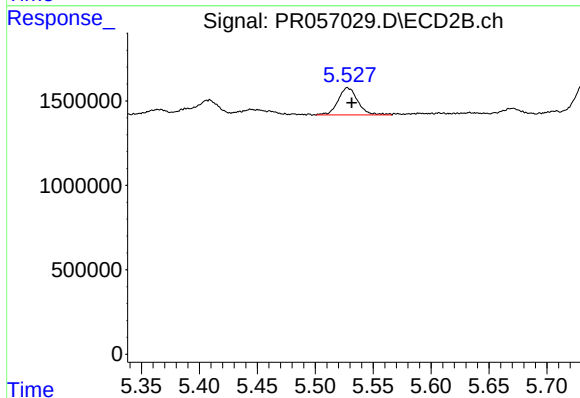


#31 AR-1260-1

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 1902941
Conc: 25.26 ng/ml

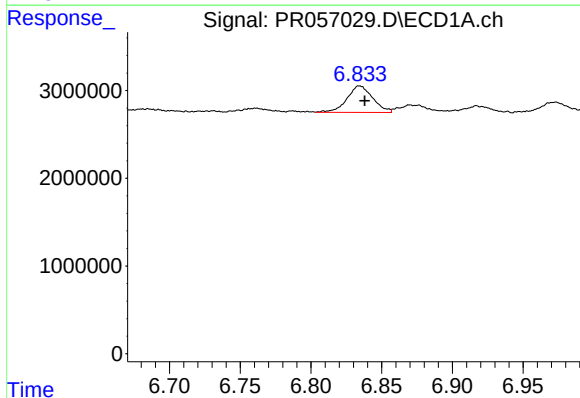


#32 AR-1260-2

R.T.: 6.835 min
Delta R.T.: -0.004 min
Response: 3824451
Conc: 26.82 ng/ml

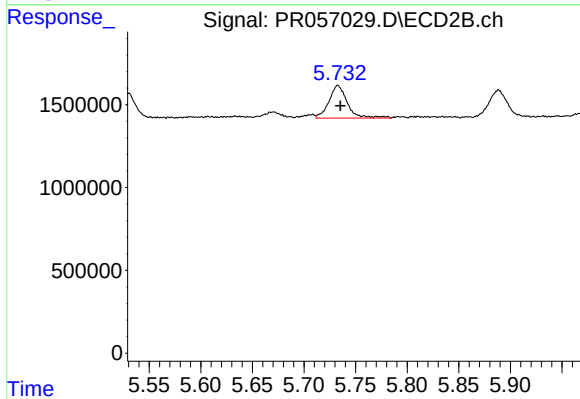

#32 AR-1260-2


R.T.: 5.733 min
Delta R.T.: -0.003 min
Response: 2440798
Conc: 26.53 ng/ml

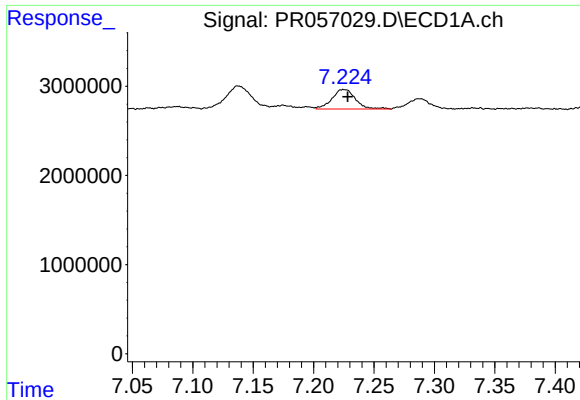

#33 AR-1260-3


R.T.: 7.225 min
Delta R.T.: -0.003 min
Response: 2983648
Conc: 27.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

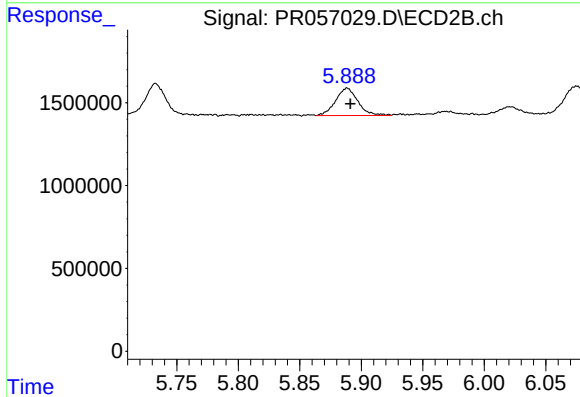


#33 AR-1260-3

R.T.: 5.889 min
Delta R.T.: -0.003 min
Response: 2089342
Conc: 23.97 ng/ml

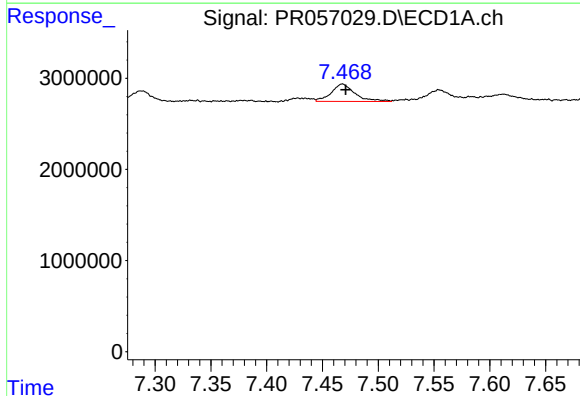


#34 AR-1260-4

R.T.: 7.468 min
Delta R.T.: -0.003 min
Response: 2825644
Conc: 26.23 ng/ml

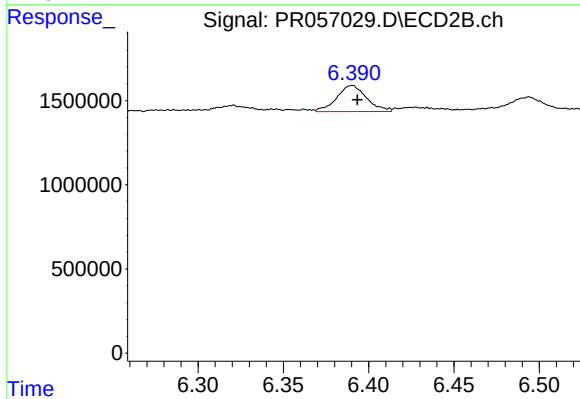

#34 AR-1260-4


R.T.: 6.390 min
Delta R.T.: -0.003 min
Response: 1898260
Conc: 26.35 ng/ml

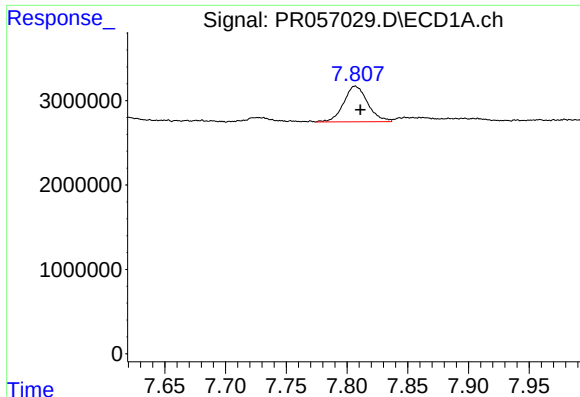

#35 AR-1260-5


R.T.: 7.807 min
Delta R.T.: -0.004 min
Response: 5800880
Conc: 25.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

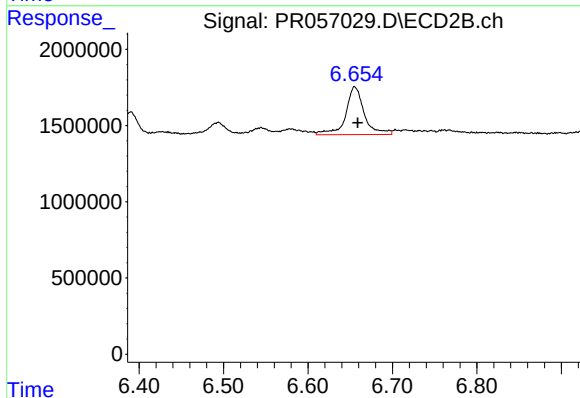


#35 AR-1260-5

R.T.: 6.655 min
Delta R.T.: -0.004 min
Response: 4779431
Conc: 26.80 ng/ml

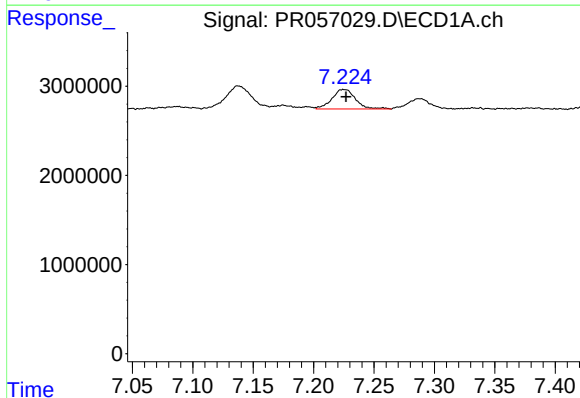


#36 AR-1262-1

R.T.: 7.225 min
Delta R.T.: -0.002 min
Response: 2983648
Conc: 16.56 ng/ml

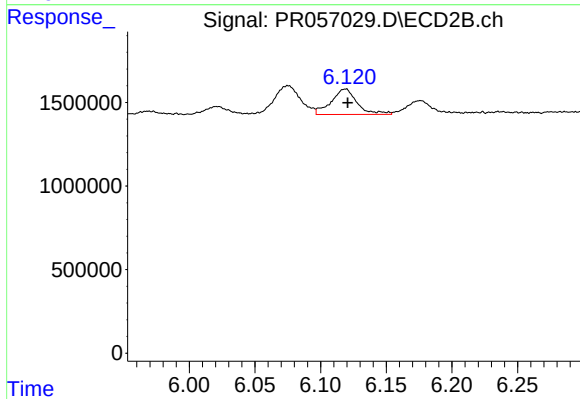

#36 AR-1262-1


R.T.: 6.119 min
Delta R.T.: -0.002 min
Response: 2094786
Conc: 18.51 ng/ml

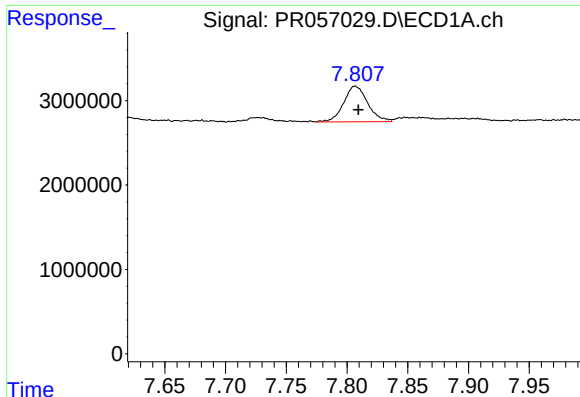

#37 AR-1262-2


R.T.: 7.807 min
Delta R.T.: -0.003 min
Response: 5800880
Conc: 19.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

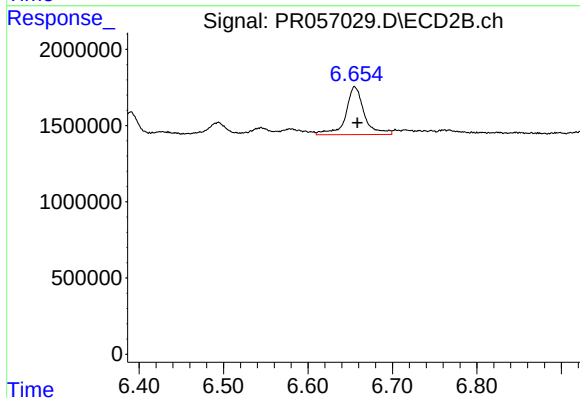


#37 AR-1262-2

R.T.: 6.655 min
Delta R.T.: -0.003 min
Response: 4779431
Conc: 22.52 ng/ml

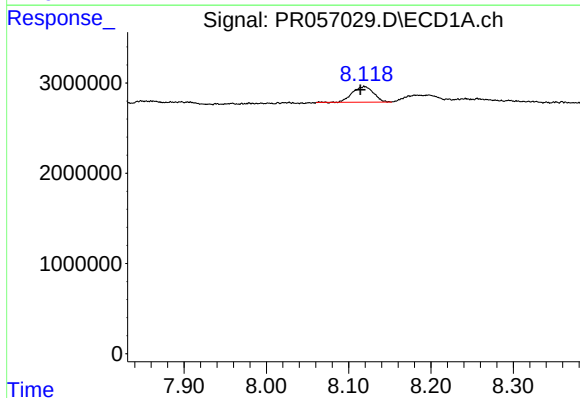


#38 AR-1262-3

R.T.: 8.119 min
Delta R.T.: 0.005 min
Response: 3099257
Conc: 16.13 ng/ml

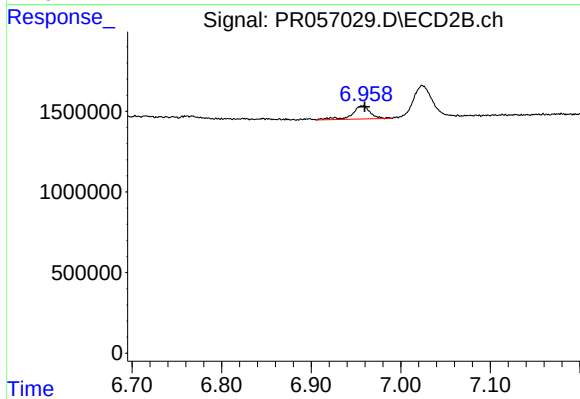

#38 AR-1262-3


R.T.: 6.957 min
Delta R.T.: -0.002 min
Response: 1147300
Conc: 13.16 ng/ml

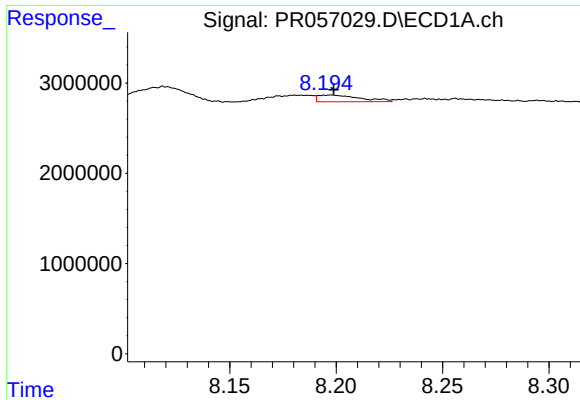

#39 AR-1262-4


R.T.: 8.197 min
Delta R.T.: -0.001 min
Response: 1034077
Conc: 11.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

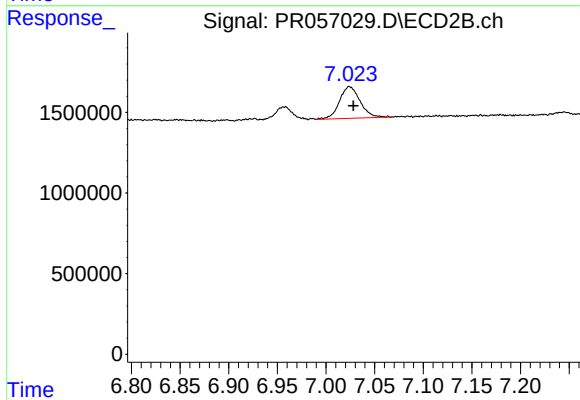


#39 AR-1262-4

R.T.: 7.024 min
Delta R.T.: -0.004 min
Response: 2901684
Conc: 17.83 ng/ml

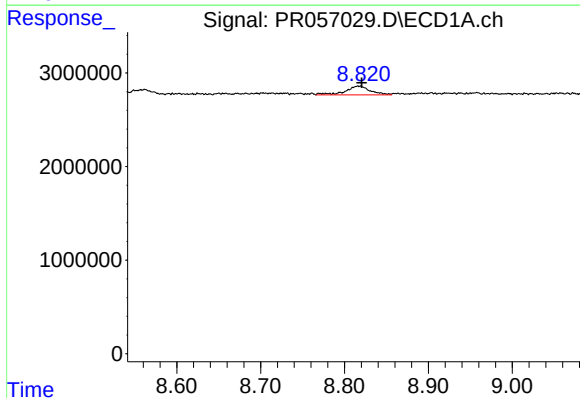


#40 AR-1262-5

R.T.: 8.817 min
Delta R.T.: -0.004 min
Response: 1957575
Conc: 19.22 ng/ml

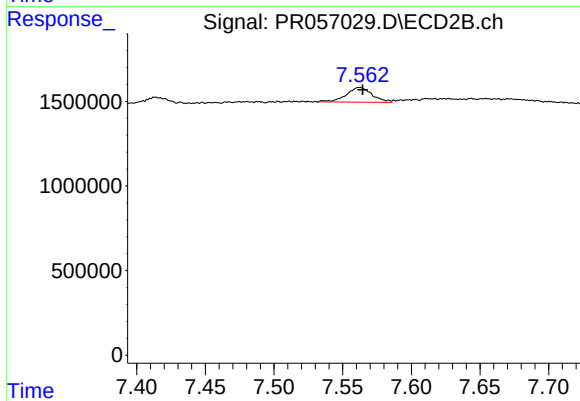

#40 AR-1262-5


R.T.: 7.562 min
Delta R.T.: -0.002 min
Response: 1125791
Conc: 14.30 ng/ml

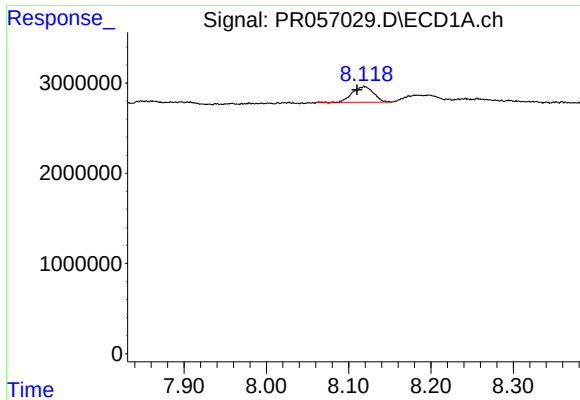

#41 AR-1268-1


R.T.: 8.119 min
Delta R.T.: 0.009 min
Response: 3099257
Conc: 8.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

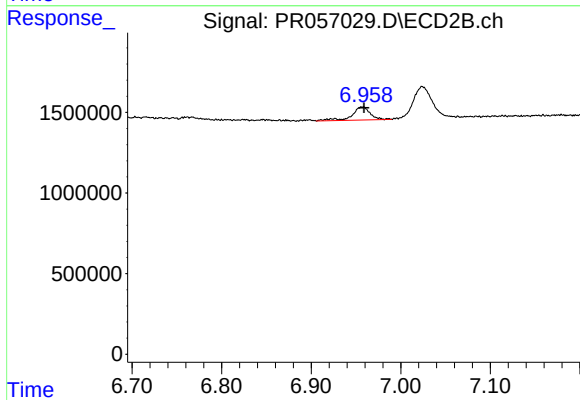


#41 AR-1268-1

R.T.: 6.957 min
Delta R.T.: -0.001 min
Response: 1147300
Conc: 4.52 ng/ml

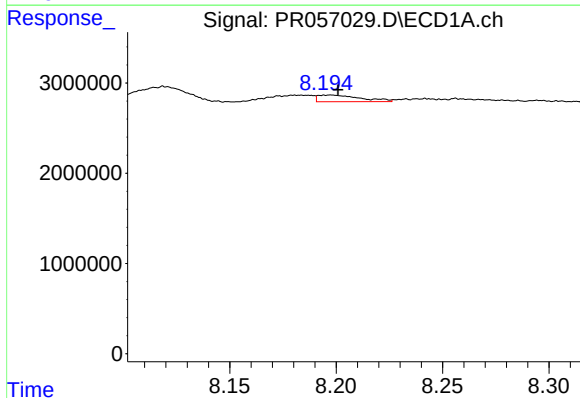


#42 AR-1268-2

R.T.: 8.197 min
Delta R.T.: -0.004 min
Response: 1034077
Conc: 3.09 ng/ml

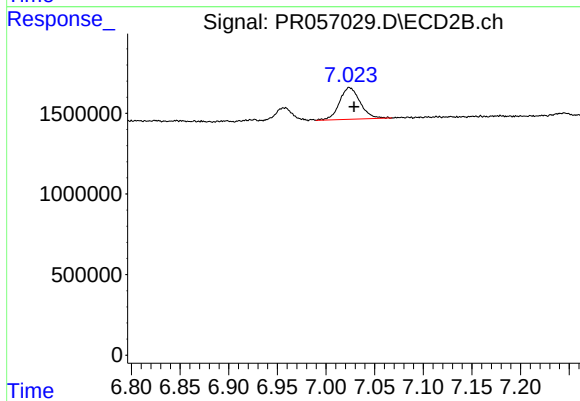

#42 AR-1268-2


R.T.: 7.024 min
Delta R.T.: -0.005 min
Response: 2901684
Conc: 11.83 ng/ml

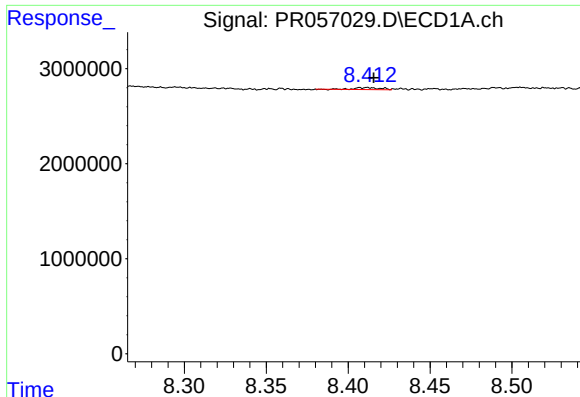

#43 AR-1268-3


R.T.: 8.412 min
Delta R.T.: -0.004 min
Response: 212079
Conc: 0.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

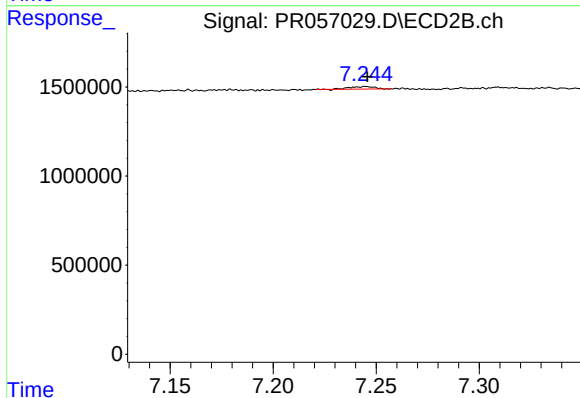


#43 AR-1268-3

R.T.: 7.245 min
Delta R.T.: 0.000 min
Response: 116580
Conc: 0.56 ng/ml

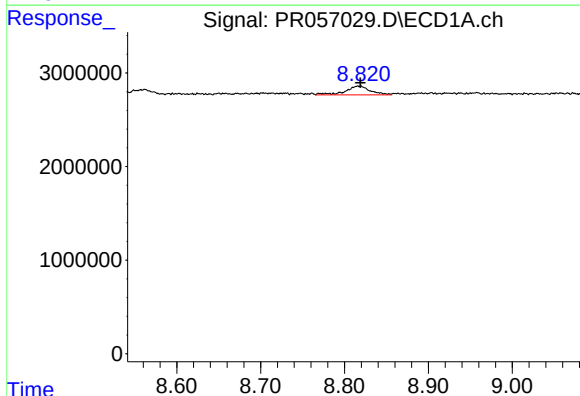


#44 AR-1268-4

R.T.: 8.817 min
Delta R.T.: -0.002 min
Response: 1957575
Conc: 16.96 ng/ml

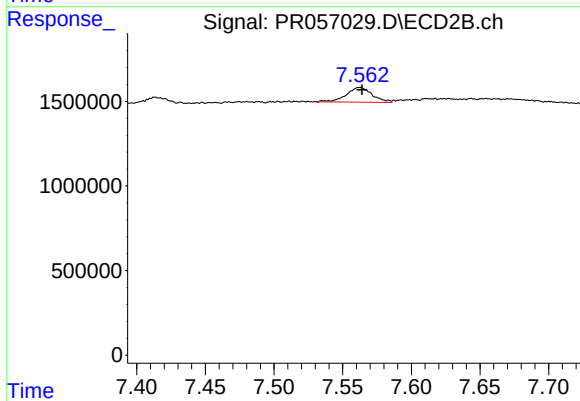

#44 AR-1268-4


R.T.: 7.562 min
Delta R.T.: -0.002 min
Response: 1125791
Conc: 12.72 ng/ml

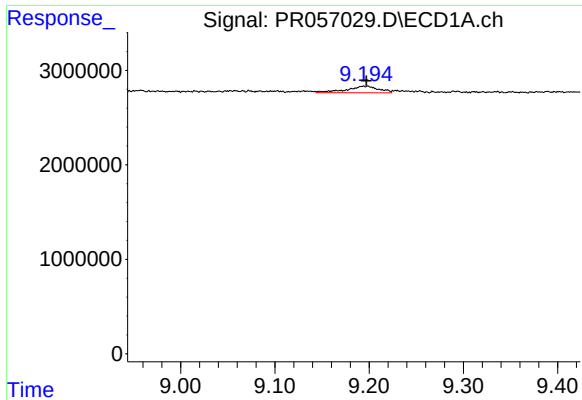

#45 AR-1268-5

R.T.: 9.198 min
Delta R.T.: 0.001 min
Response: 1668690
Conc: 1.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT4-2022-08

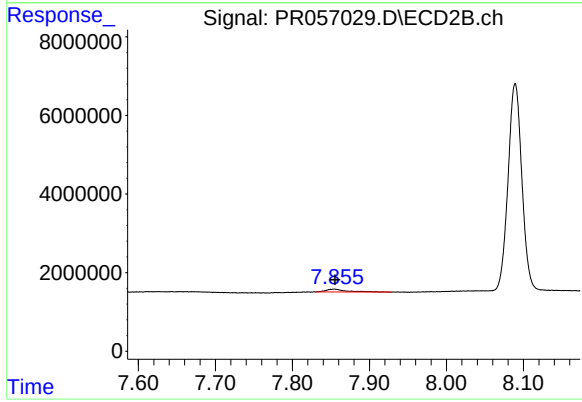

#45 AR-1268-5

R.T.: 7.855 min
Delta R.T.: 0.000 min
Response: 1331004
Conc: 1.97 ng/ml