

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100522\
 Data File : PR057171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 12:43
 Operator : AJ\MA
 Sample : N4958-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 33527

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2022
 Supervised By :Ankita Jodhani 10/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:09:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 29 10:58:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.615	2.885	67301260	31768102	20.937	18.270
2) SA Decachlor...	9.496	8.085	53662062	41481678	26.269	25.705

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100522\
Data File : PR057171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 12:43
Operator : AJ\MA
Sample : N4958-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
33527


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2022
Supervised By :Ankita Jodhani 10/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:09:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR092922.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 29 10:58:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

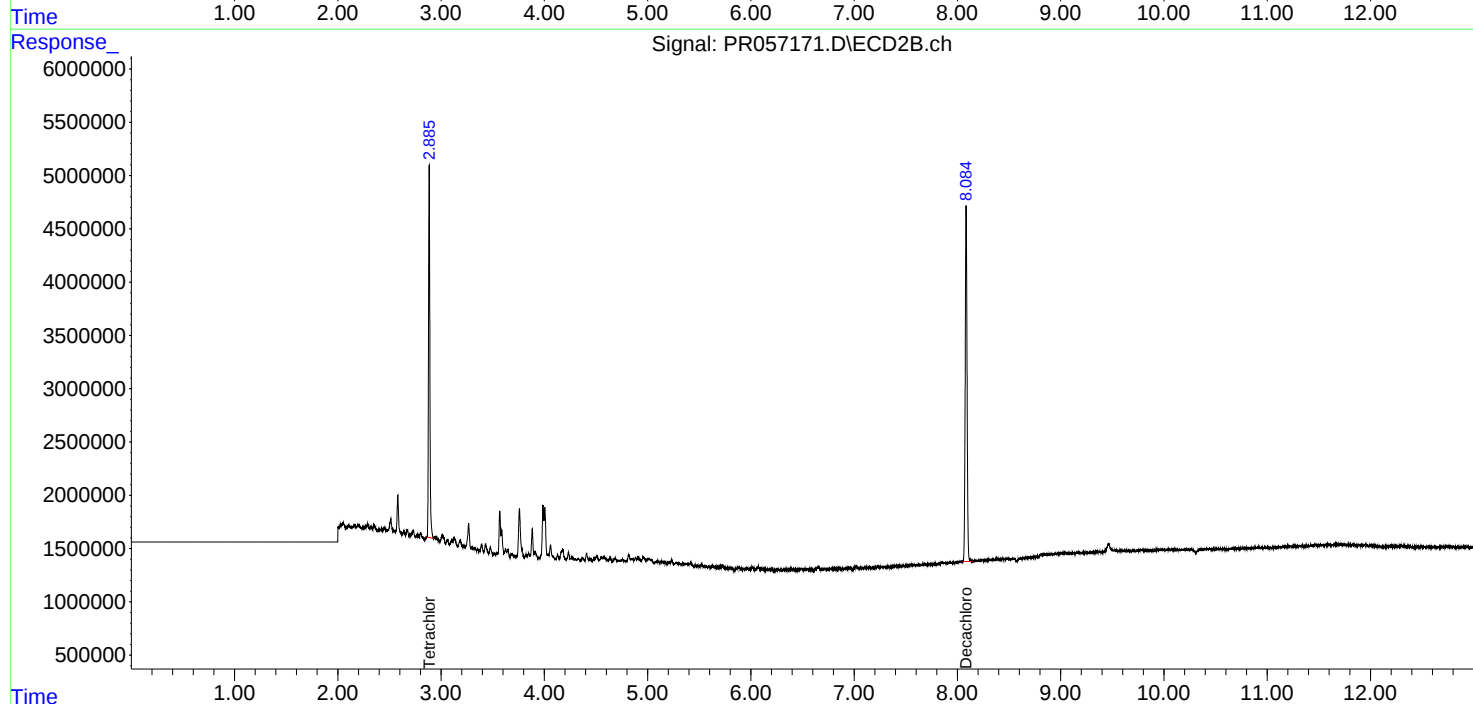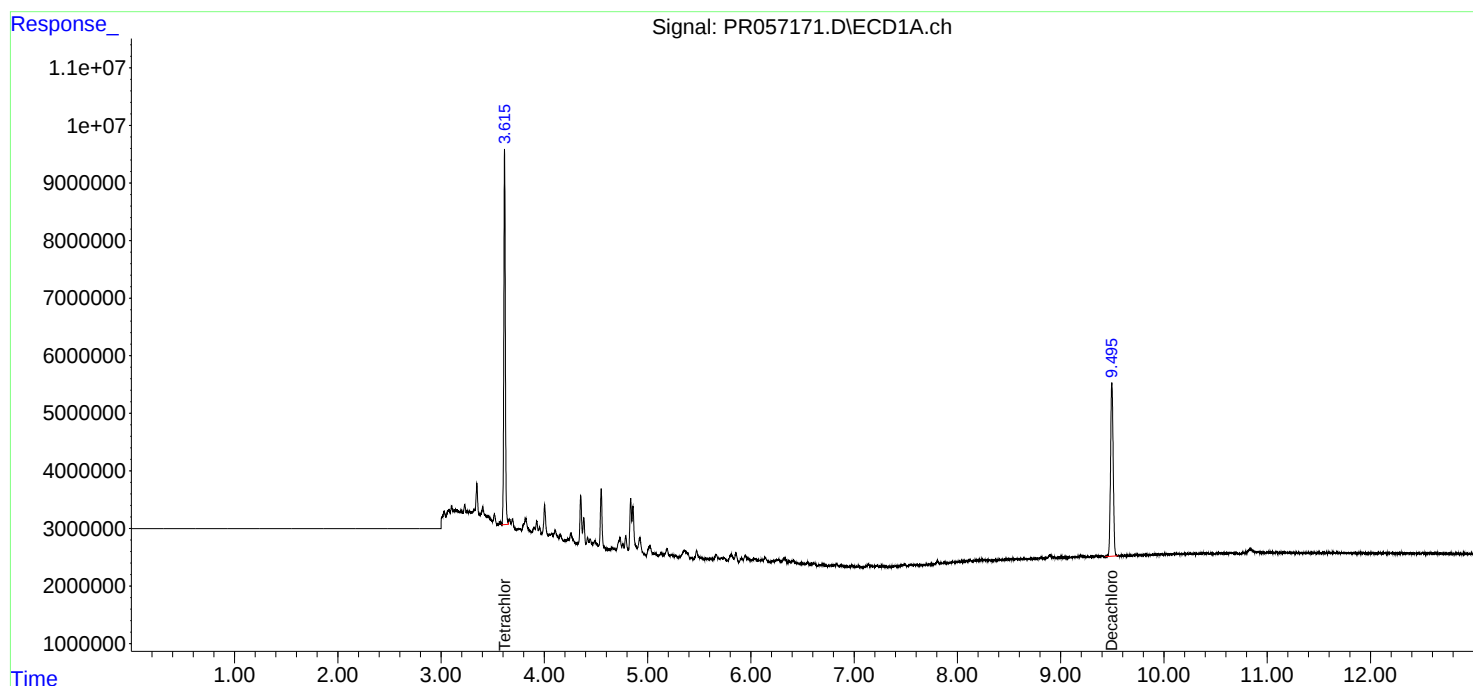

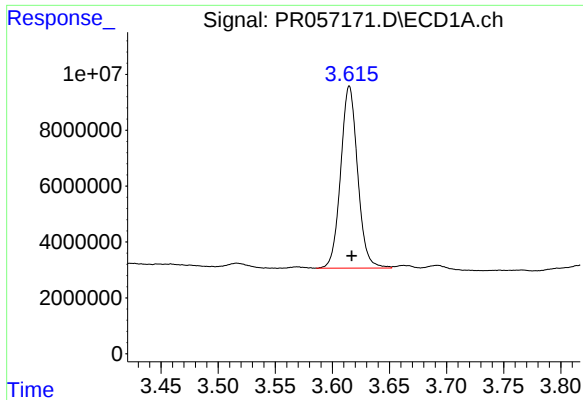


#1 Tetrachloro-m-xylene

R.T.: 3.615 min
Delta R.T.: -0.002 min
Response: 67301260
Conc: 20.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
33527


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2022
Supervised By :Ankita Jodhani 10/10/2022

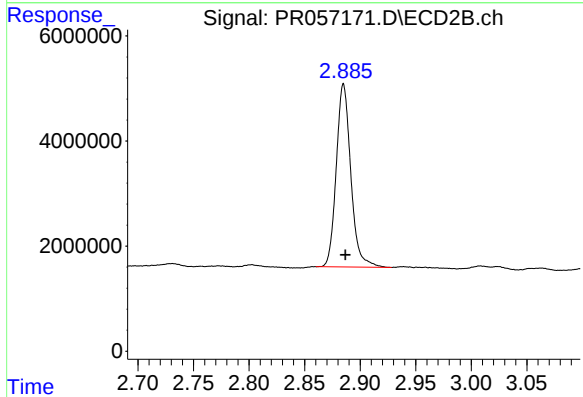


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: -0.002 min
Response: 31768102
Conc: 18.27 ng/ml

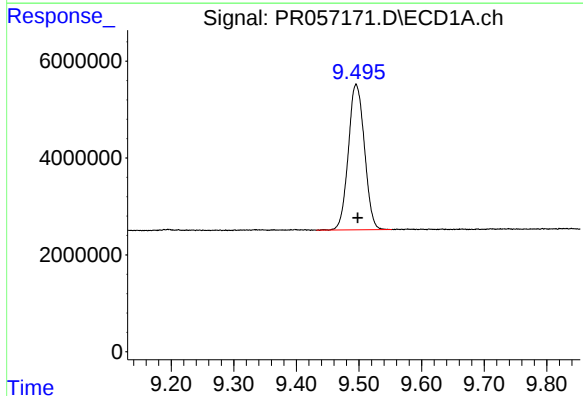

#2 Decachlorobiphenyl

R.T.: 9.496 min
Delta R.T.: -0.002 min
Response: 53662062
Conc: 26.27 ng/ml

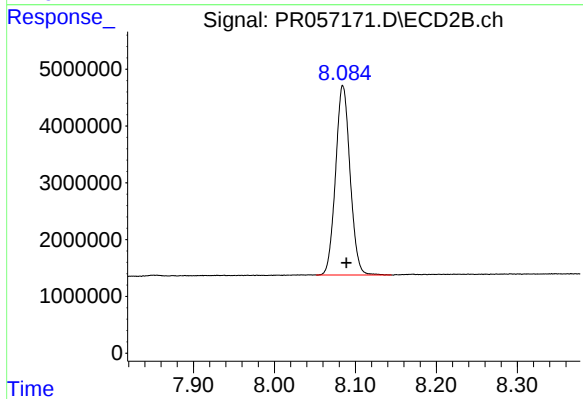

#2 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.004 min
Response: 41481678
Conc: 25.70 ng/ml