

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100719\
 Data File : PR042017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 08:39
 Operator : SM\AJ
 Sample : AIBLK77
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 AIBLK77

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 02:30:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 04 06:59:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.721	3.983	81958027	348.7E6	20.147	22.804
2) SA Decachlor...	10.643	9.097	110.5E6	406.3E6	32.150	40.978 #
Target Compounds						
9) L2 AR-1221-2	5.032	4.289	1181584	4630012	40.725	37.674
10) L2 AR-1221-3	5.032f	0.000	1181584	0	12.145	N.D. #
11) L3 AR-1232-1	5.032f	0.000	1181584	0	14.121	N.D. #
27) L6 AR-1254-2	0.000	6.050	0	4641464	N.D.	9.258 #
28) L6 AR-1254-3	7.358	0.000	1428407	0	5.293	N.D. #
32) L7 AR-1260-2	0.000	6.752	0	4124575	N.D.	5.059 #
43) L9 AR-1268-3	9.377	8.197	1088388	1552074	2.668	0.926 #
45) L9 AR-1268-5	10.280	8.816	1282286	76979099	0.984	16.775 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100719\
Data File : PR042017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 08:39
Operator : SM\AJ
Sample : AIBLK77
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
AIBLK77

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:30:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

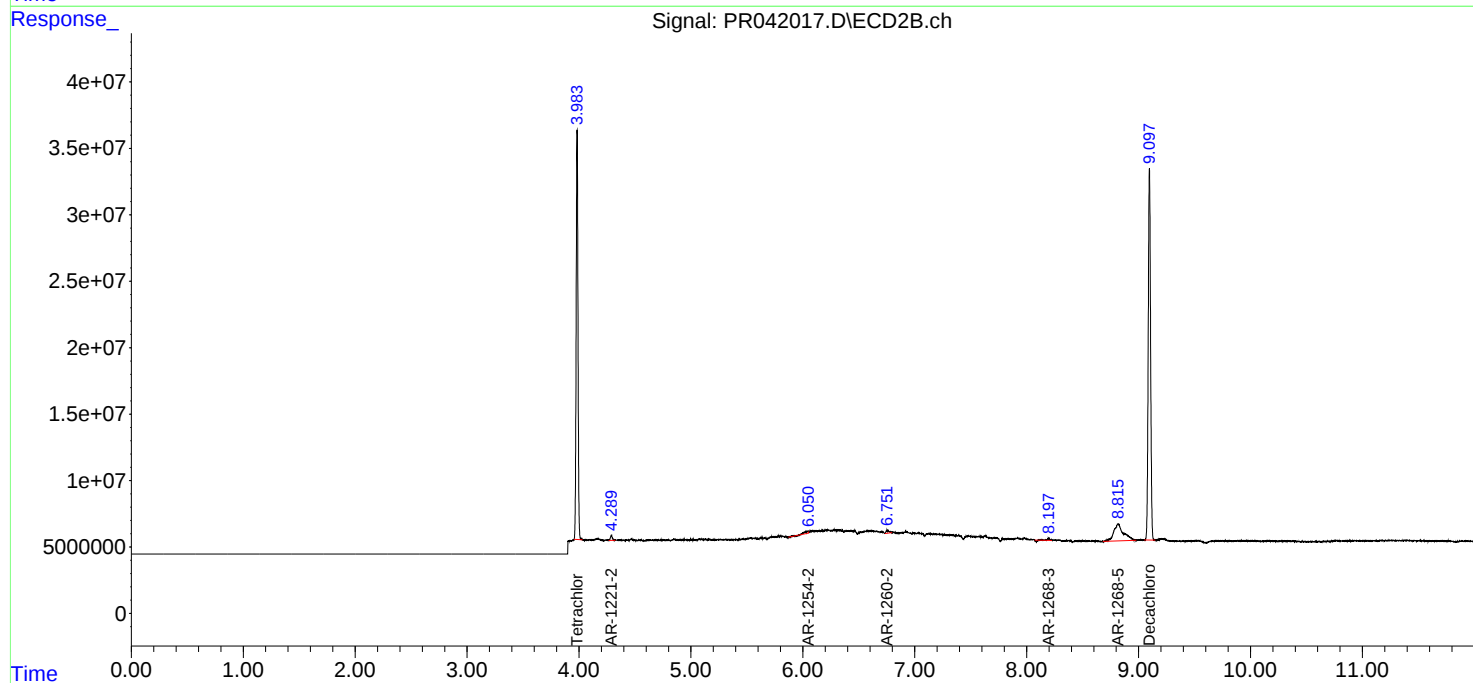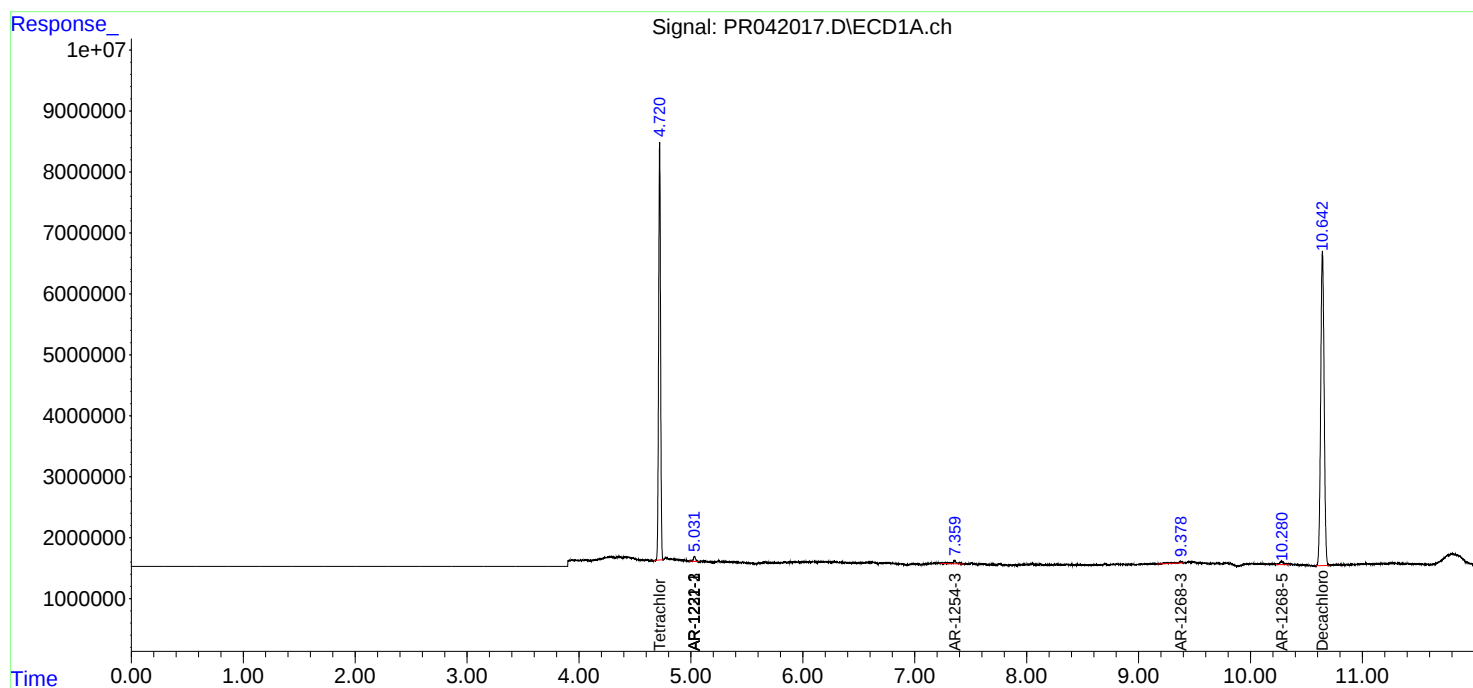


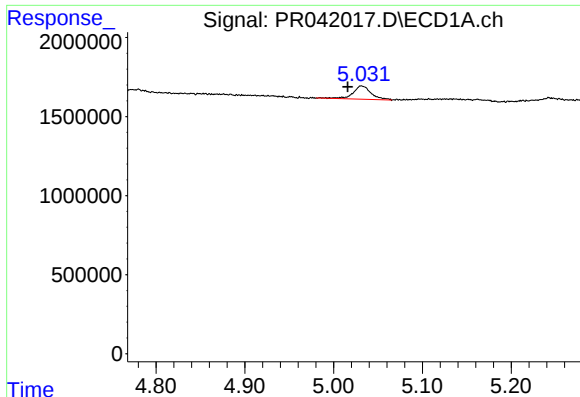

#9 AR-1221-2


R.T.: 5.032 min
Delta R.T.: 0.016 min
Response: 1181584
Conc: 40.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK77

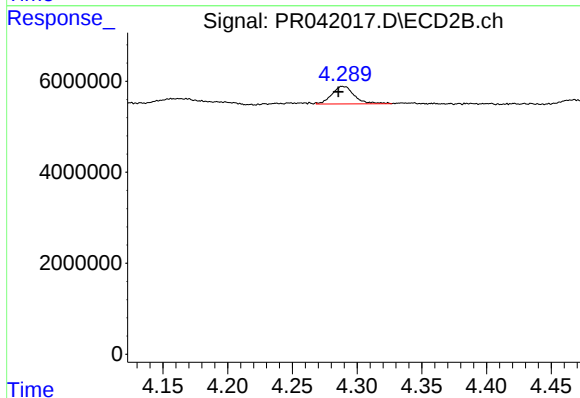


#9 AR-1221-2

R.T.: 4.289 min
Delta R.T.: 0.003 min
Response: 4630012
Conc: 37.67 ng/ml

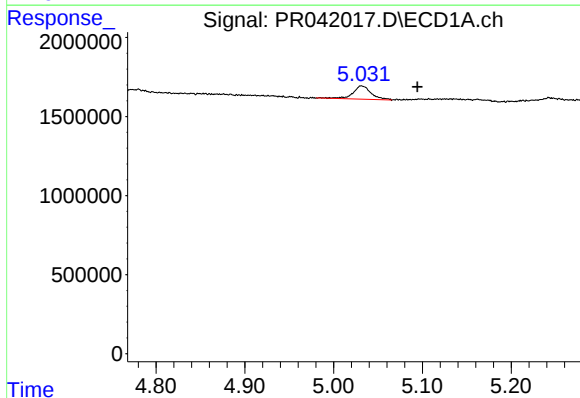


#10 AR-1221-3

R.T.: 5.032 min
Delta R.T.: -0.062 min
Response: 1181584
Conc: 12.14 ng/ml

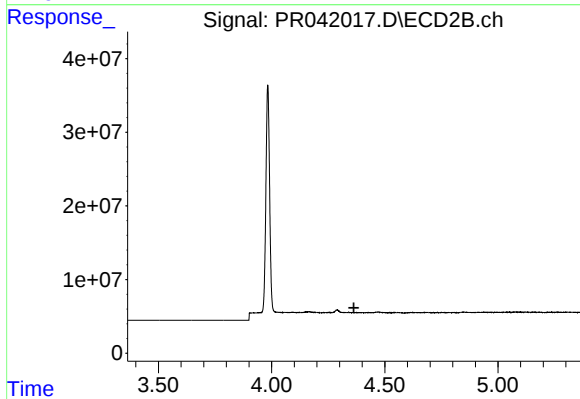

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.363 min
Response: 0
Conc: N.D.

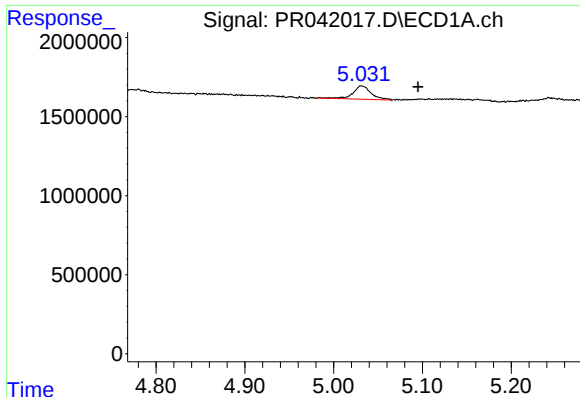

#11 AR-1232-1


R.T.: 5.032 min
Delta R.T.: -0.063 min
Response: 1181584
Conc: 14.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK77

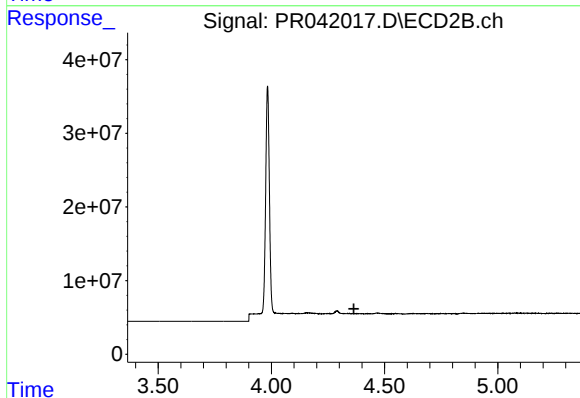


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.364 min
Response: 0
Conc: N.D.

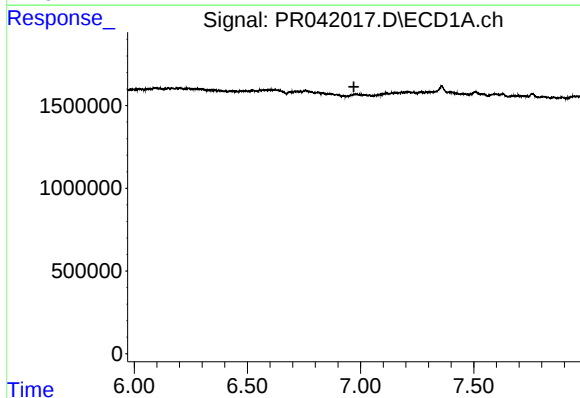


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.970 min
Response: 0
Conc: N.D.

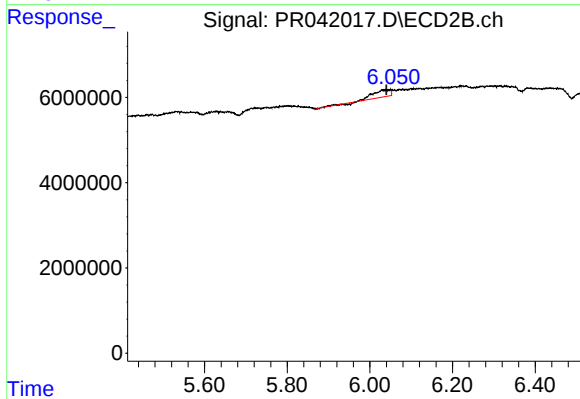

#27 AR-1254-2


R.T.: 6.050 min
Delta R.T.: 0.010 min
Response: 4641464
Conc: 9.26 ng/ml

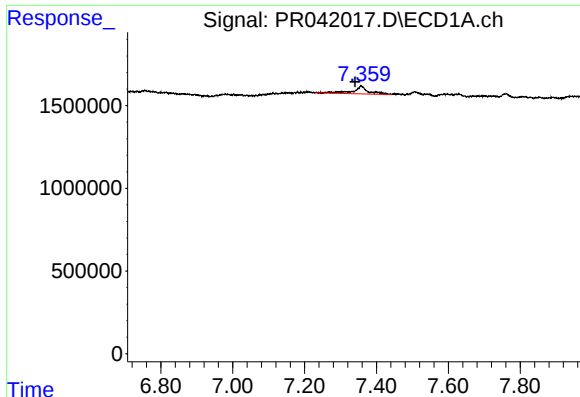

#28 AR-1254-3


R.T.: 7.358 min
Delta R.T.: 0.018 min
Response: 1428407
Conc: 5.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK77

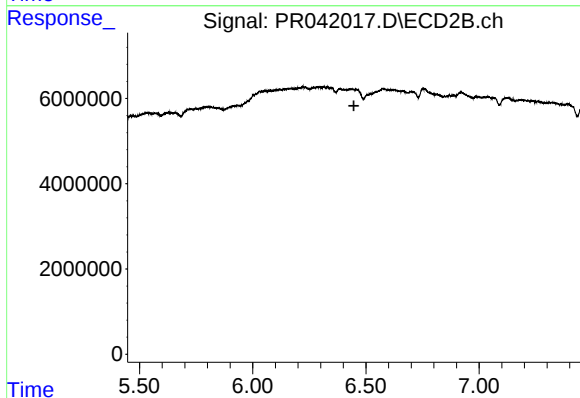


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.447 min
Response: 0
Conc: N.D.

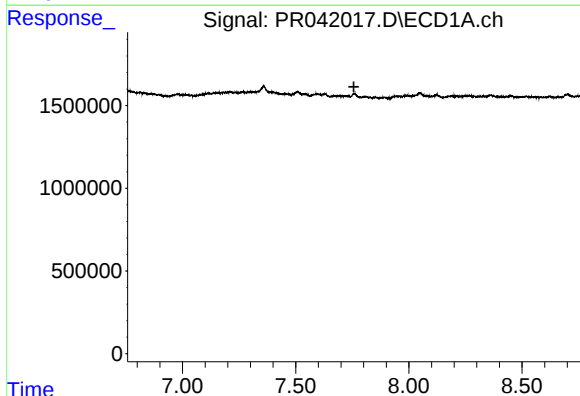


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.757 min
Response: 0
Conc: N.D.

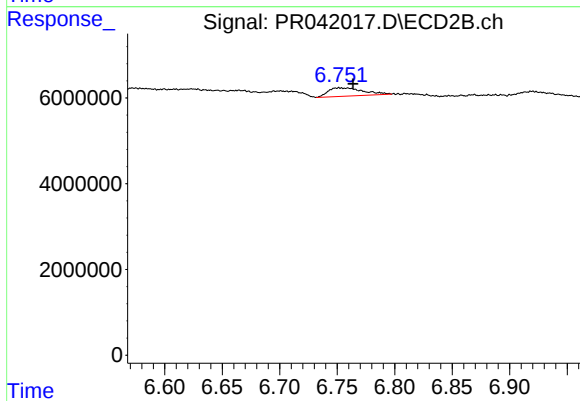

#32 AR-1260-2


R.T.: 6.752 min
Delta R.T.: -0.012 min
Response: 4124575
Conc: 5.06 ng/ml

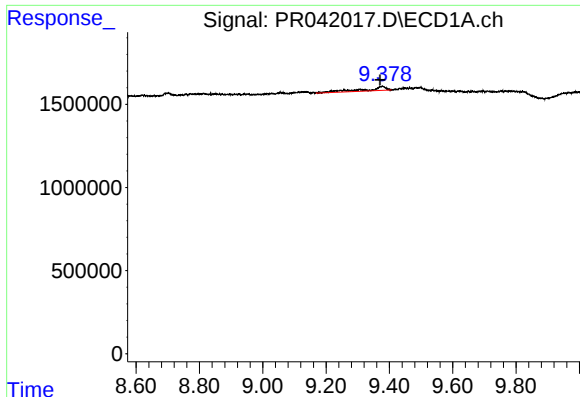

#43 AR-1268-3


R.T.: 9.377 min
Delta R.T.: 0.006 min
Response: 1088388
Conc: 2.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK77

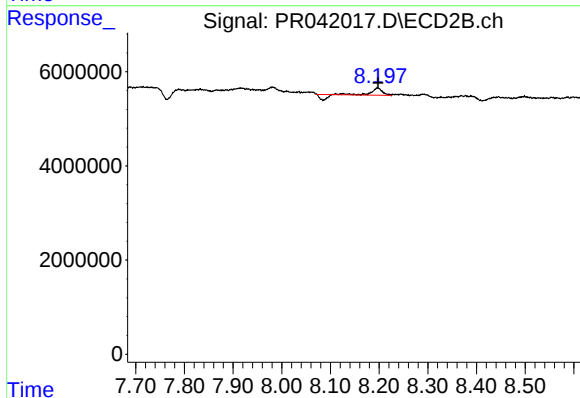


#43 AR-1268-3

R.T.: 8.197 min
Delta R.T.: -0.001 min
Response: 1552074
Conc: 0.93 ng/ml

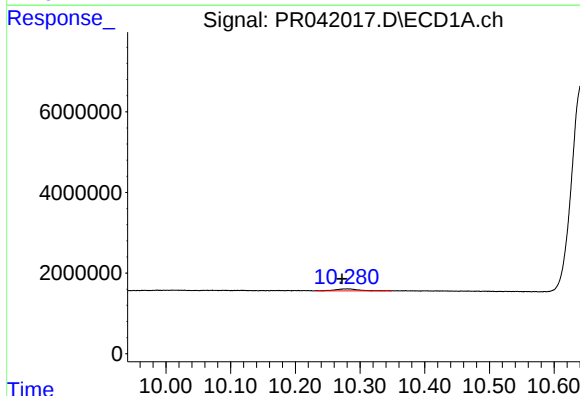

#45 AR-1268-5

R.T.: 10.280 min
Delta R.T.: 0.008 min
Response: 1282286
Conc: 0.98 ng/ml

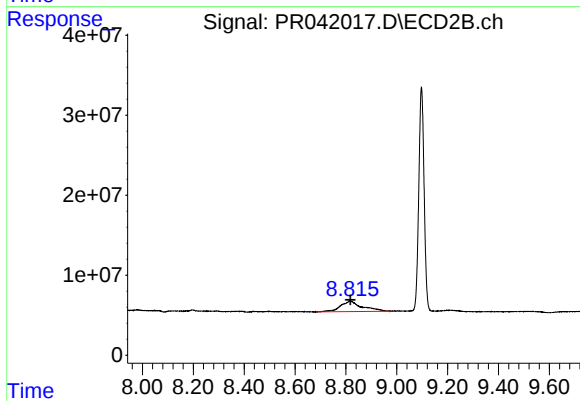

#45 AR-1268-5

R.T.: 8.816 min
Delta R.T.: -0.002 min
Response: 76979099
Conc: 16.77 ng/ml