

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100719\
 Data File : PR042024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 10:53
 Operator : SM\AJ
 Sample : K5084-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 C0B10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 02:32:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 04 06:59:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.718	3.983	79146880	321.2E6	19.456	21.008
2) SA Decachlor...	10.634	9.093	96521523	330.6E6	28.090	33.343
Target Compounds						
9) L2 AR-1221-2	5.028	4.288	897778	3860600	30.944	31.413
10) L2 AR-1221-3	5.108	4.357	702649	3154903	7.222	8.100
11) L3 AR-1232-1	5.108	4.357	702649	3154903	8.397	9.259
27) L6 AR-1254-2	7.040f	0.000	920464	0	3.710	N.D. #
32) L7 AR-1260-2	7.756	0.000	542815	0	2.297	N.D. #
34) L7 AR-1260-4	8.289f	0.000	2351317	0	11.700	N.D. #
40) L8 AR-1262-5	9.769f	0.000	953804	0	6.612	N.D. #
44) L9 AR-1268-4	9.769f	0.000	953804	0	5.436	N.D. #
45) L9 AR-1268-5	10.266	0.000	1275987	0	0.979	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100719\
Data File : PR042024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 10:53
Operator : SM\AJ
Sample : K5084-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
C0B10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 02:32:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

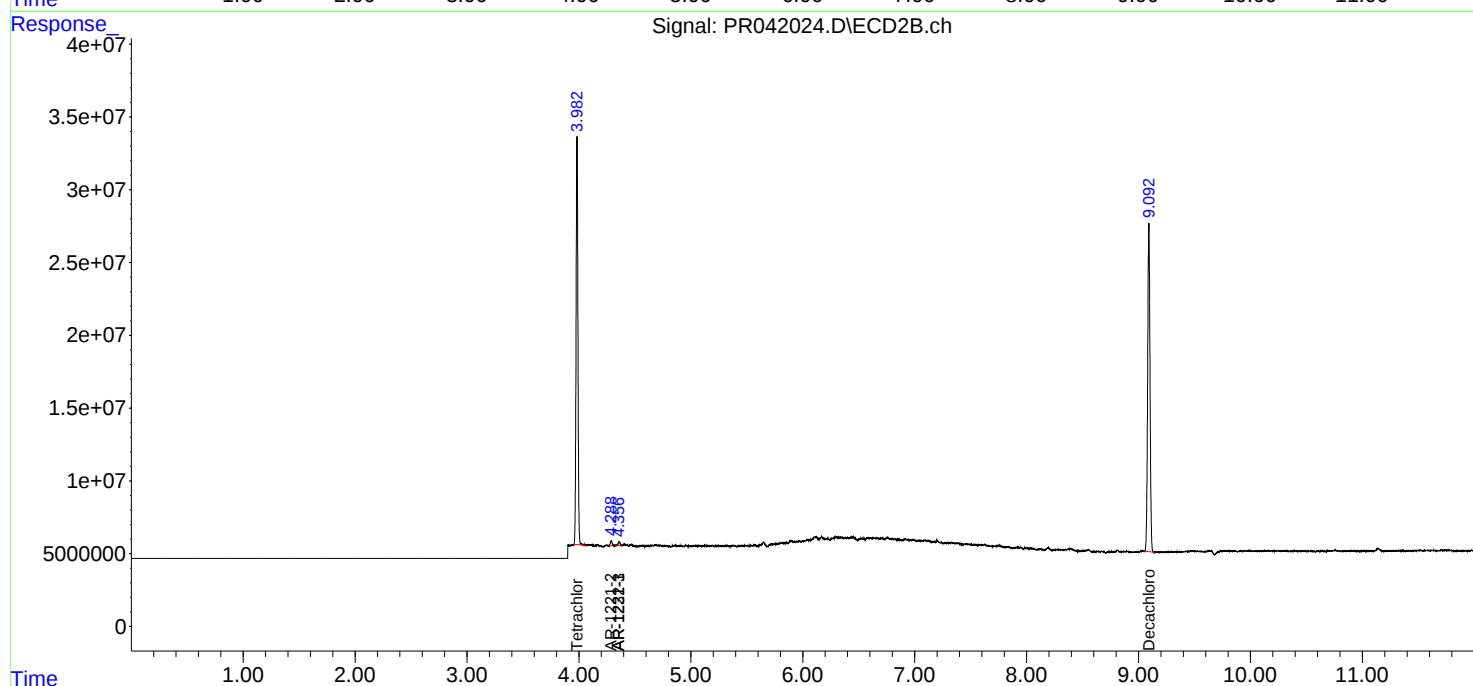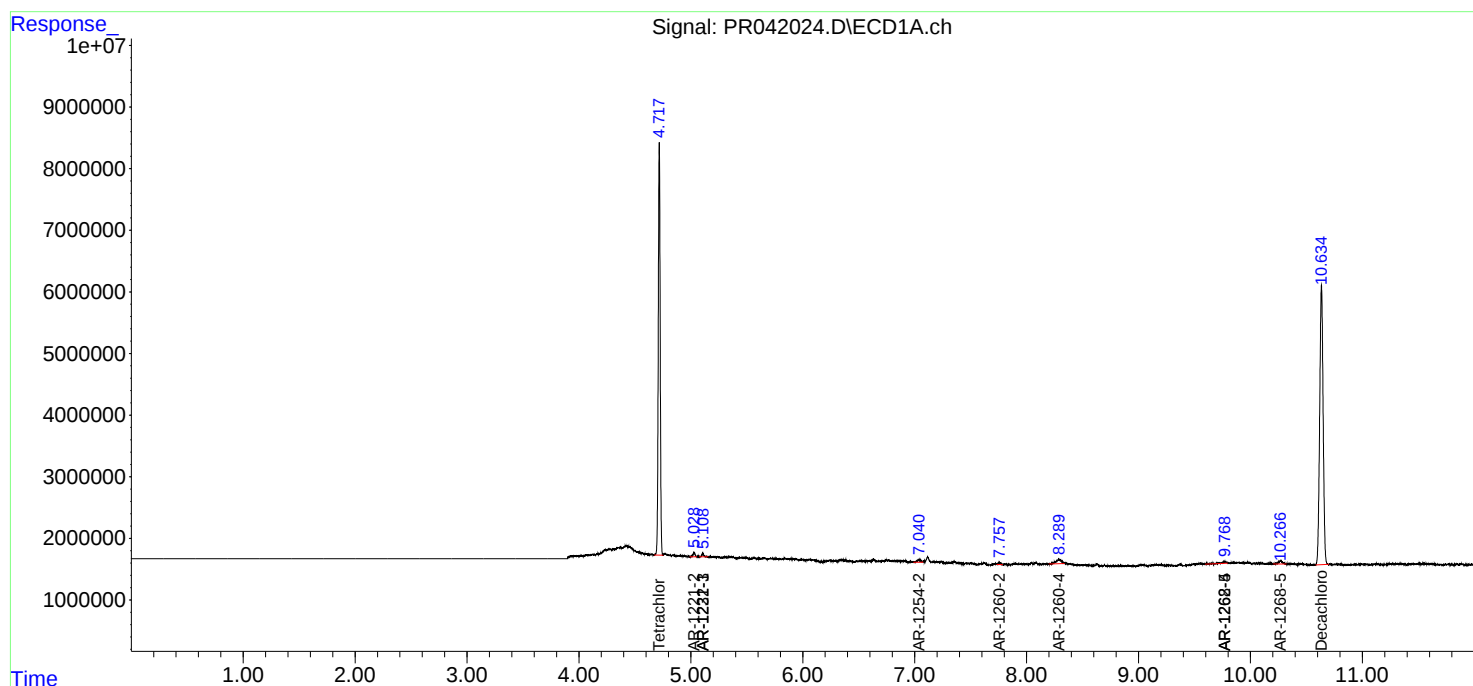


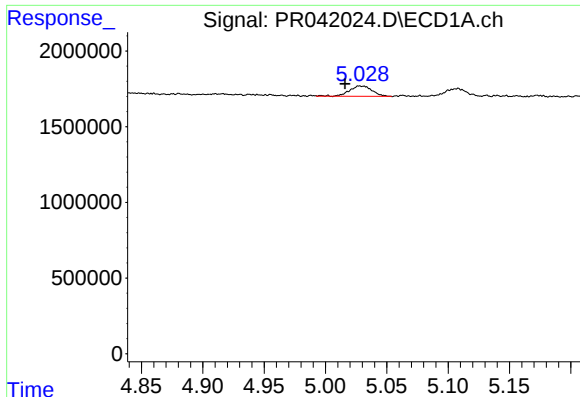

#9 AR-1221-2


R.T.: 5.028 min
Delta R.T.: 0.012 min
Response: 897778
Conc: 30.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
C0B10

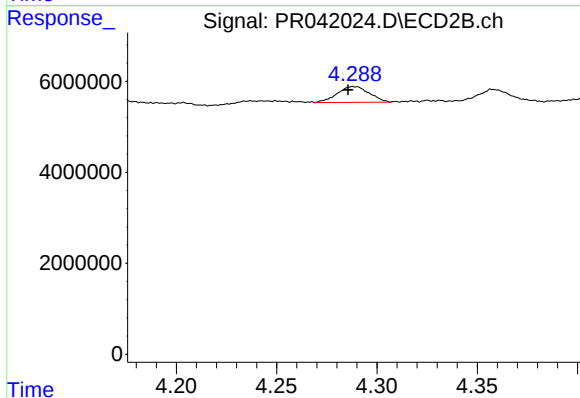


#9 AR-1221-2

R.T.: 4.288 min
Delta R.T.: 0.003 min
Response: 3860600
Conc: 31.41 ng/ml

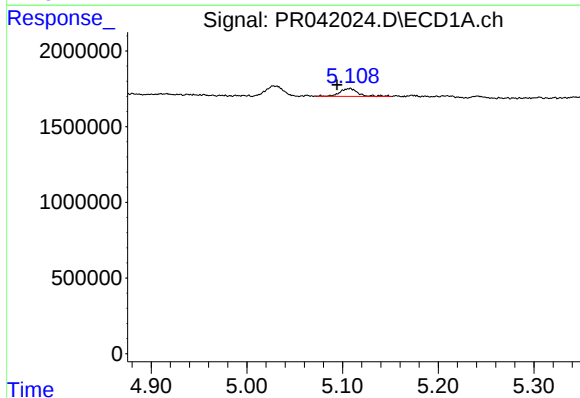


#10 AR-1221-3

R.T.: 5.108 min
Delta R.T.: 0.013 min
Response: 702649
Conc: 7.22 ng/ml

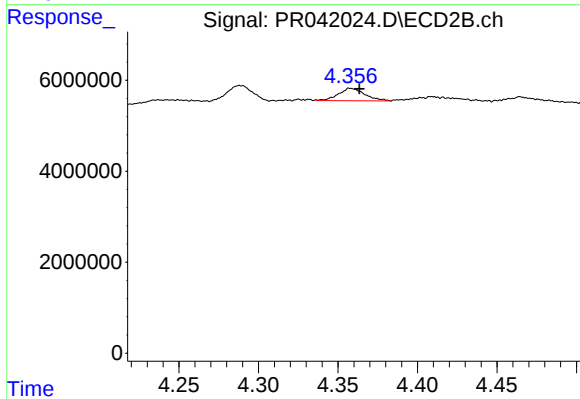

#10 AR-1221-3


R.T.: 4.357 min
Delta R.T.: -0.006 min
Response: 3154903
Conc: 8.10 ng/ml

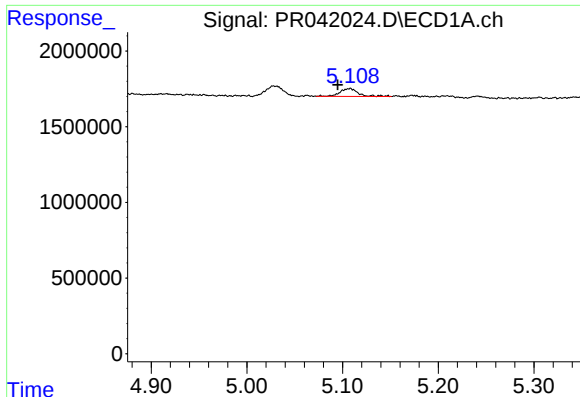

#11 AR-1232-1


R.T.: 5.108 min
Delta R.T.: 0.013 min
Response: 702649
Conc: 8.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
C0B10

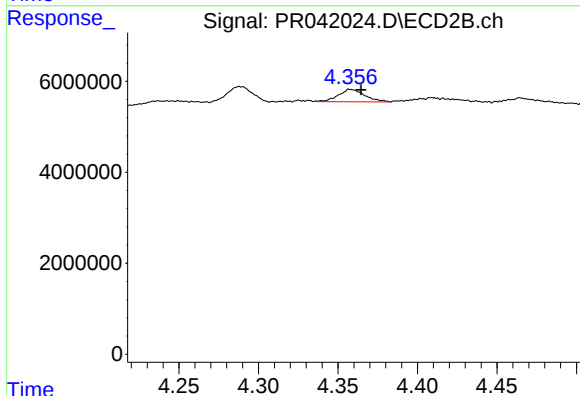


#11 AR-1232-1

R.T.: 4.357 min
Delta R.T.: -0.007 min
Response: 3154903
Conc: 9.26 ng/ml

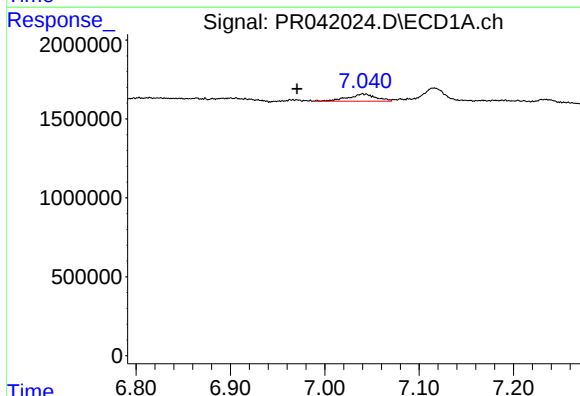


#27 AR-1254-2

R.T.: 7.040 min
Delta R.T.: 0.070 min
Response: 920464
Conc: 3.71 ng/ml

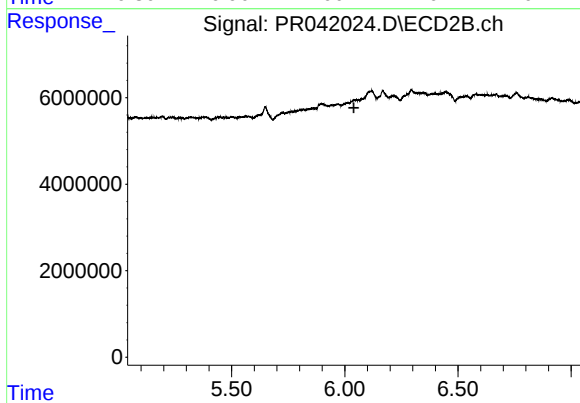

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.040 min
Response: 0
Conc: N.D.

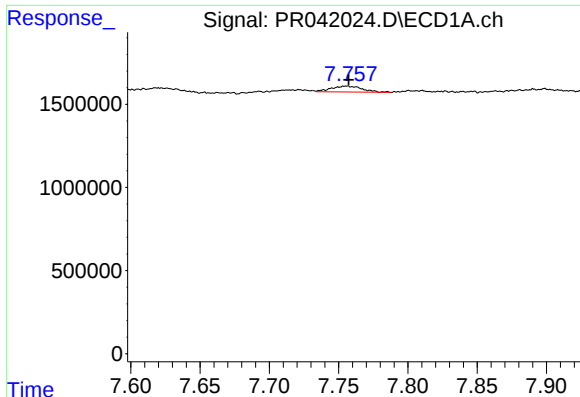

#32 AR-1260-2


R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 542815
Conc: 2.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
C0B10

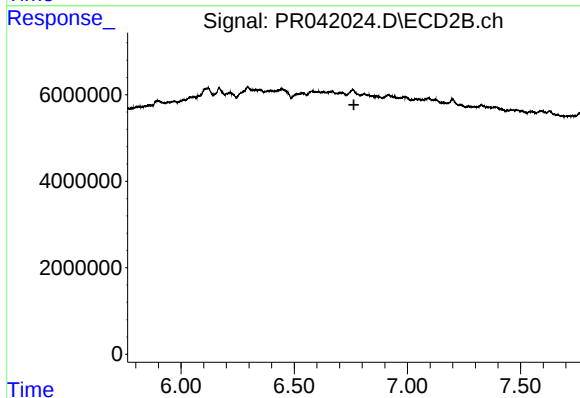


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

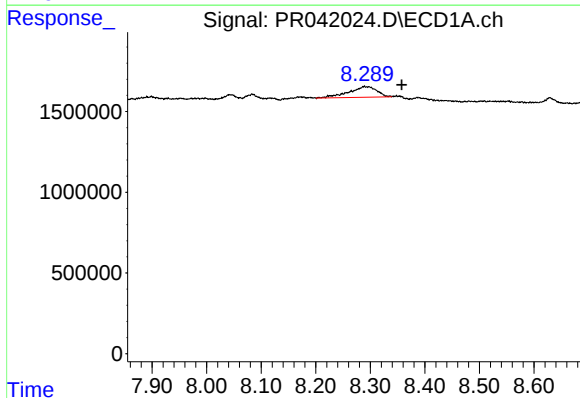


#34 AR-1260-4

R.T.: 8.289 min
Delta R.T.: -0.069 min
Response: 2351317
Conc: 11.70 ng/ml

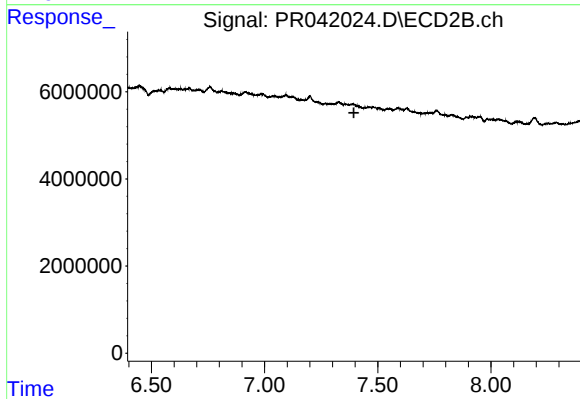

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.394 min
Response: 0
Conc: N.D.

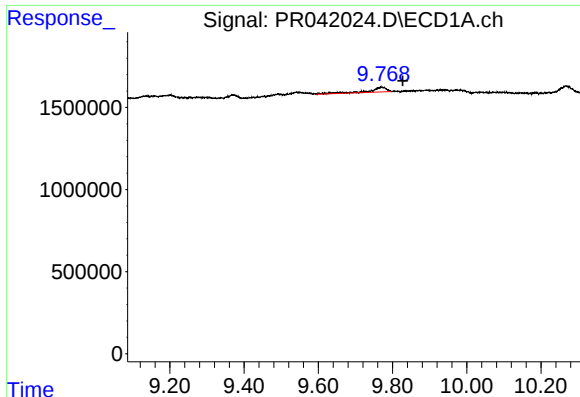

#40 AR-1262-5


R.T.: 9.769 min
Delta R.T.: -0.058 min
Response: 953804
Conc: 6.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
C0B10

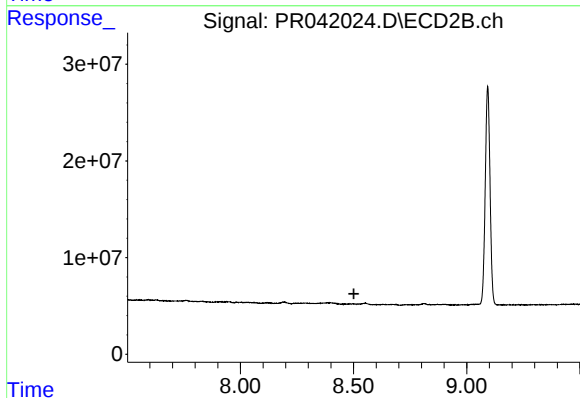


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.502 min
Response: 0
Conc: N.D.

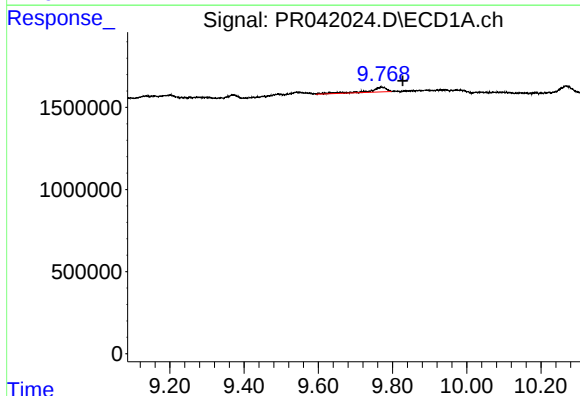


#44 AR-1268-4

R.T.: 9.769 min
Delta R.T.: -0.058 min
Response: 953804
Conc: 5.44 ng/ml

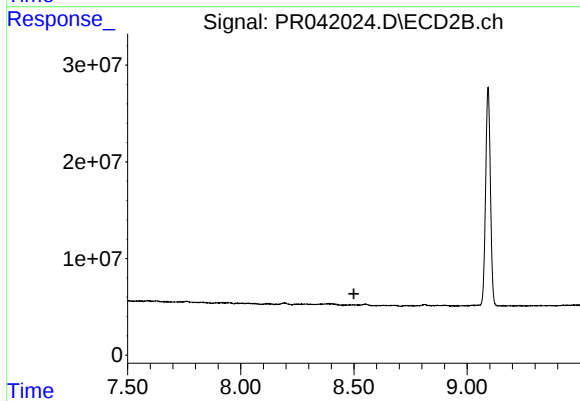

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.500 min
Response: 0
Conc: N.D.

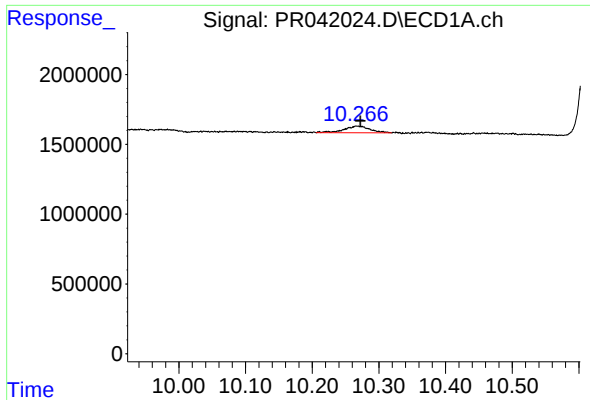

#45 AR-1268-5

R.T.: 10.266 min
Delta R.T.: -0.006 min
Response: 1275987
Conc: 0.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
C0B10

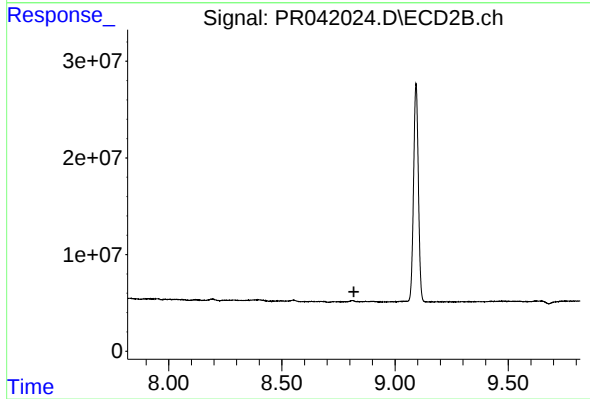

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.818 min
Response: 0
Conc: N.D.