

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
 Data File : PR042057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2019 08:21
 Operator : SM\AJ
 Sample : K5177-07
 Misc :
 ALS Vial : 33 Sample Multiplier: 1


Instrument :
 ECD_R
 ClientSampleId :
 BEP96

Manual Integrations
 APPROVED

Ankita
 10/21/2019 11:40:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 07:00:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 04 06:59:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

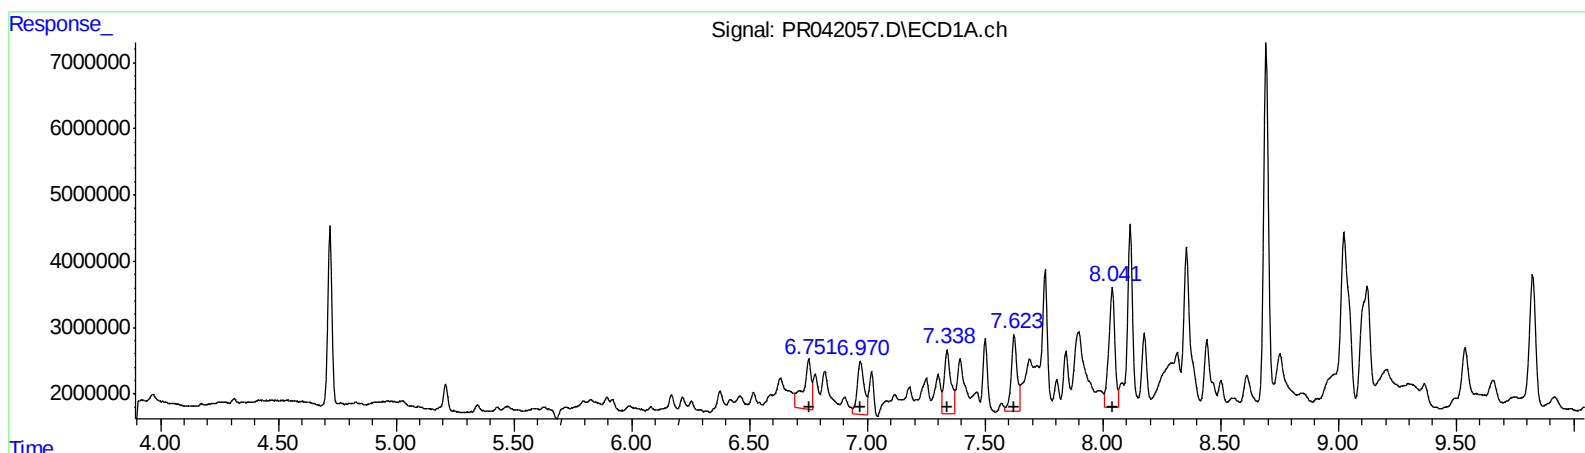

(26) AR-1254-1 (L6)
 R.T. Response Conc
 6.75 17601851 107.78
 6.97 16448790 66.30
 7.34 19409680 71.92
 7.62 19844295 97.78
 8.04 32391007 152.32

(26) AR-1254-1 #2 (L6)
 R.T. Response Conc
 5.89 21785776 41.13
 6.04 18504732 36.91
 6.44 77710363 82.37
 6.67 52631393 79.49
 7.09 89815614 104.60

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
Data File : PR042057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 08:21
Operator : SM\AJ
Sample : K5177-07
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
BEP96

Manual Integrations
APPROVED

Ankita
10/21/2019 11:40:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 07:00:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

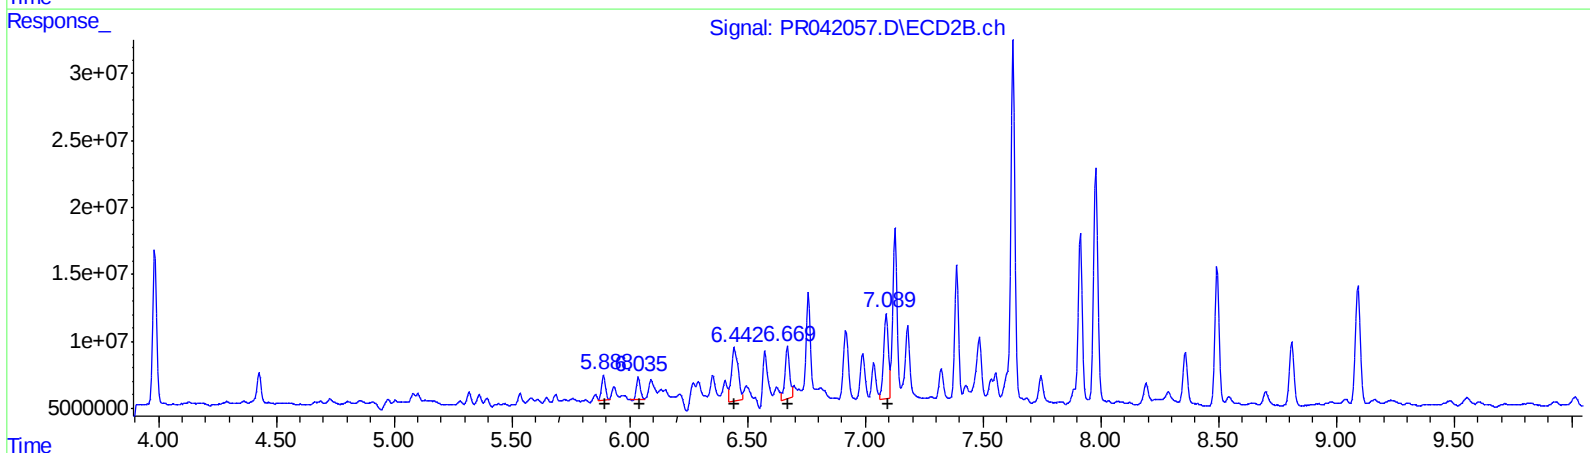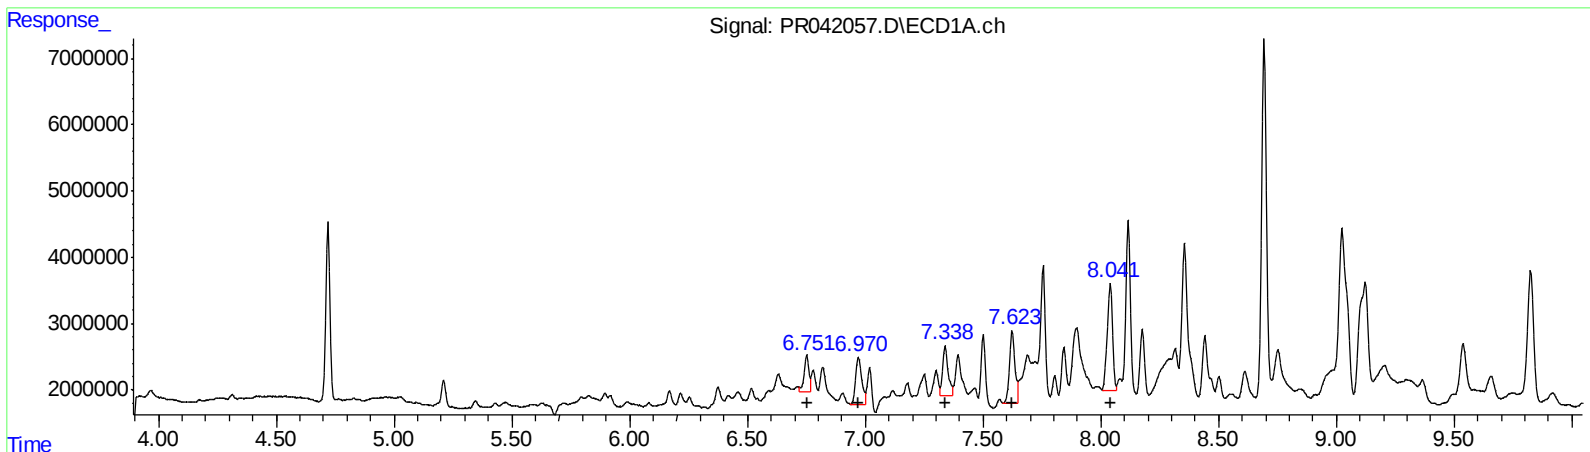

QEdit

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
6.75 7572198 46.37
6.97 12778999 51.51
7.34 12141302 44.99
7.62 18050953 88.94
8.04 25527897 120.04

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
5.89 21785776 41.13
6.04 18504732 36.91
6.44 77710363 82.37
6.67 52631393 79.49
7.09 89815614 104.60

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
Data File : PR042057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 08:21
Operator : SM\AJ
Sample : K5177-07
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
BEP96

Manual Integrations
APPROVED

Ankita
10/21/2019 11:40:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 07:00:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

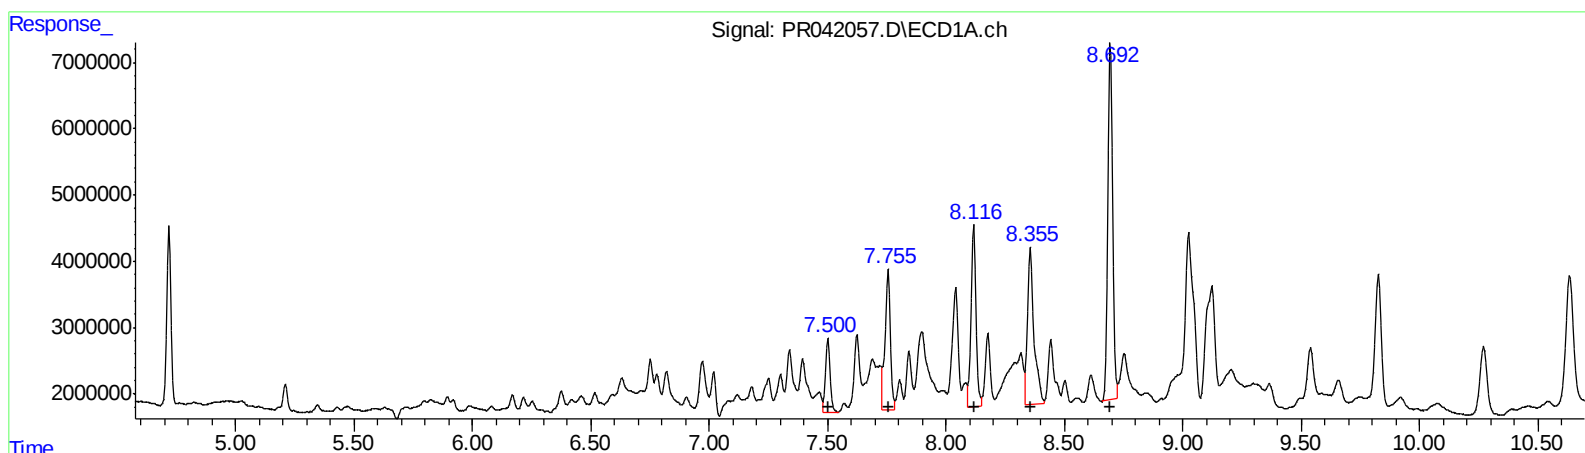

(31) AR-1260-1 (L7)

R.T.	Response	Conc
7.50	15032154	79.34
7.76	33042373	139.80
8.12	39907520	212.58
8.36	45920187	228.50
8.69	76526805	176.78

(31) AR-1260-1 #2 (L7)

R.T.	Response	Conc
6.57	61956409	104.52
6.76	87841269	107.74
6.92	75266922	108.88
7.39	115236365	198.58
7.63	349625750	215.04

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
Data File : PR042057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 08:21
Operator : SM\AJ
Sample : K5177-07
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
BEP96

Manual Integrations
APPROVED

Ankita
10/21/2019 11:40:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 07:00:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

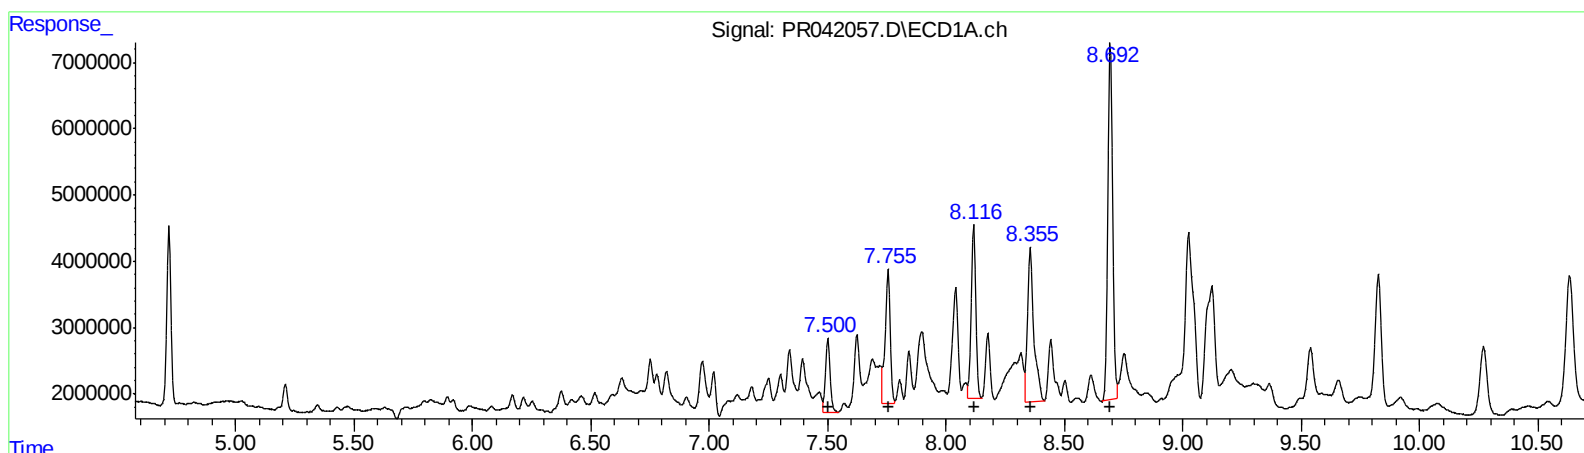

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
7.50 15032154 79.34
7.75 29738297 125.82
8.12 35498341 189.09
8.36 43886425 218.38
8.69 76526805 176.78
(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.57 61956409 104.52
6.76 87841269 107.74
6.92 75266922 108.88
7.39 115236365 198.58
7.63 349625750 215.04

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
 Data File : PR042057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2019 08:21
 Operator : SM\AJ
 Sample : K5177-07
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 BEP96

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 07:00:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 04 06:59:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

Ankita
 10/21/2019 11:40:09 AM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.719	3.983	32445046	132.2E6	7.976	8.645
2) SA Decachlor...	10.633	9.091	43682619	128.3E6	12.713	12.941
Target Compounds						
26) L6 AR-1254-1	6.751	5.889	7572198	21785776	46.366m	41.126
27) L6 AR-1254-2	6.970	6.036	12778999	18504732	51.507m	36.909 #
28) L6 AR-1254-3	7.338	6.443	12141302	77710363	44.991m	82.369 #
29) L6 AR-1254-4	7.623	6.669	18050953	52631393	88.940m	79.494
30) L6 AR-1254-5	8.041	7.089	25527897	89815614	120.045m	104.602
31) L7 AR-1260-1	7.501	6.574	15032154	61956409	79.340	104.520 #
32) L7 AR-1260-2	7.755	6.758	29738297	87841269	125.817m	107.744
33) L7 AR-1260-3	8.116	6.918	35498341	75266922	189.094m	108.876 #
34) L7 AR-1260-4	8.355	7.388	43886425	115.2E6	218.377m	198.583
35) L7 AR-1260-5	8.693	7.627	76526805	349.6E6	176.783	215.041

A.J
 10/11/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.