

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
Data File : PR042133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2019 04:20
Operator : SM\AJ
Sample : K5202-07
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
C0AB1

Manual Integrations
APPROVED

Ankita
10/10/2019 1:38:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:29:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

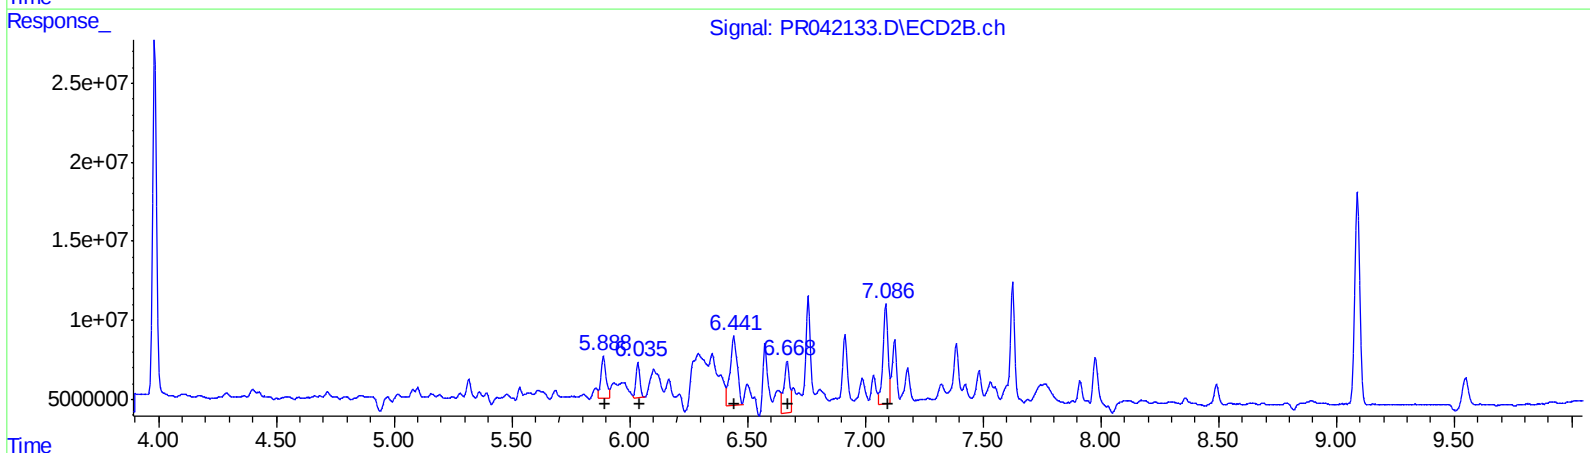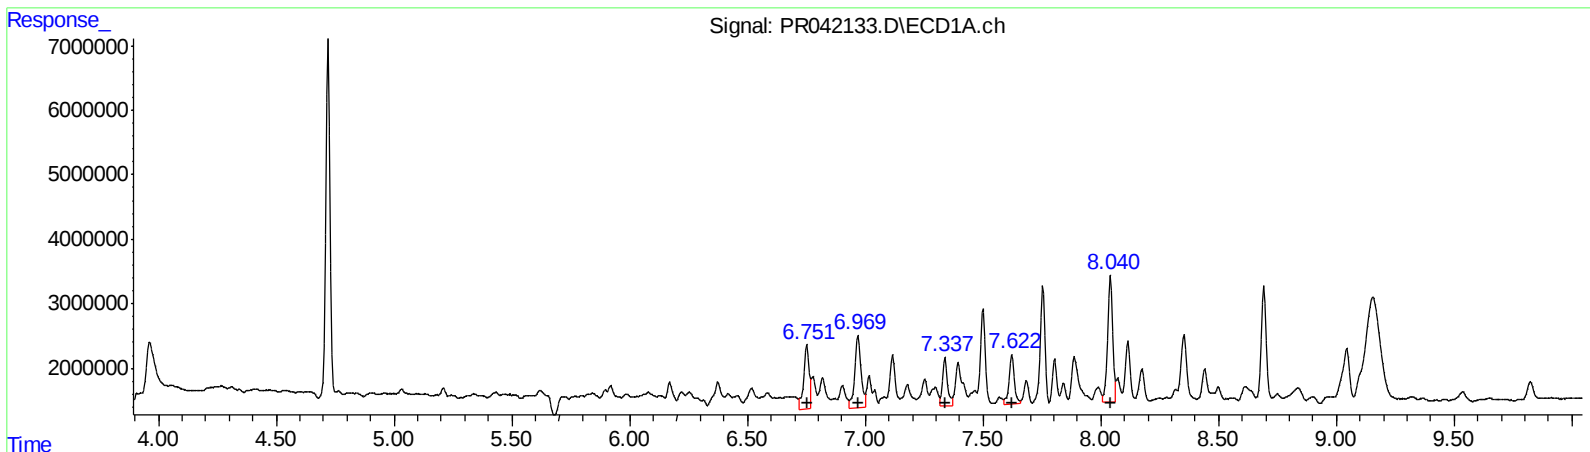

QEdit

(26) AR-1254-1 (L6)

R.T.	Response	Conc
6.75	16235255	99.41
6.97	20681036	83.36
7.34	10759417	39.87
7.62	12120017	59.72
8.04	29500154	138.72

(26) AR-1254-1 #2 (L6)

R.T.	Response	Conc
5.89	40731236	76.89
6.03	25682546	51.23
6.44	91546342	97.03
6.67	53366338	80.60
7.09	95257226	110.94

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
Data File : PR042133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2019 04:20
Operator : SM\AJ
Sample : K5202-07
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
C0AB1

Manual Integrations
APPROVED

Ankita
10/10/2019 1:38:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:29:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

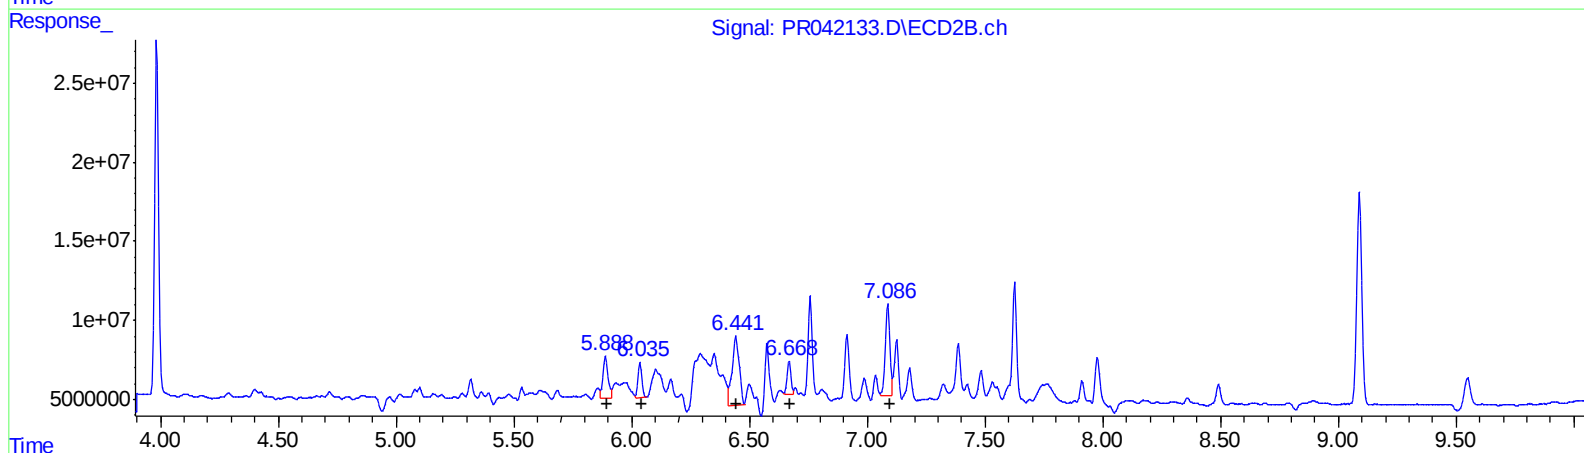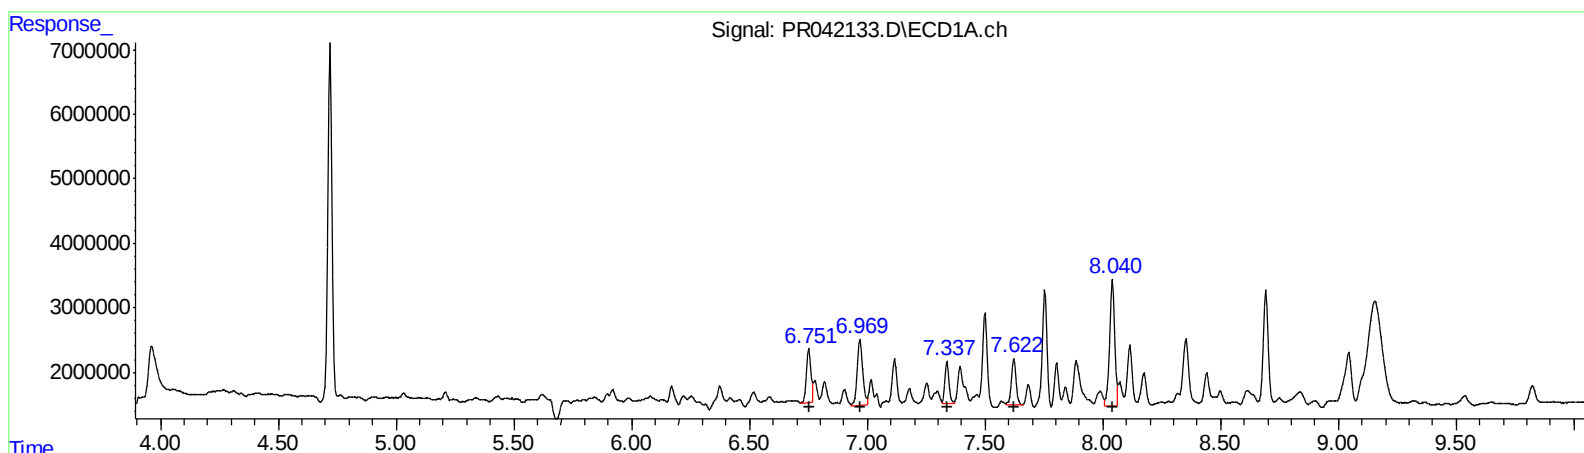

QEdit

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
6.75 11307674 69.24
6.97 16571692 66.79
7.34 7596949 28.15
7.62 9863834 48.60
8.04 29500154 138.72

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
5.89 40731236 76.89
6.03 25682546 51.23
6.44 91546342 97.03
6.67 23548629 35.57
7.09 78921103 91.91

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
Data File : PR042133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2019 04:20
Operator : SM\AJ
Sample : K5202-07
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
C0AB1

Manual Integrations
APPROVED

Ankita
10/10/2019 1:38:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:29:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

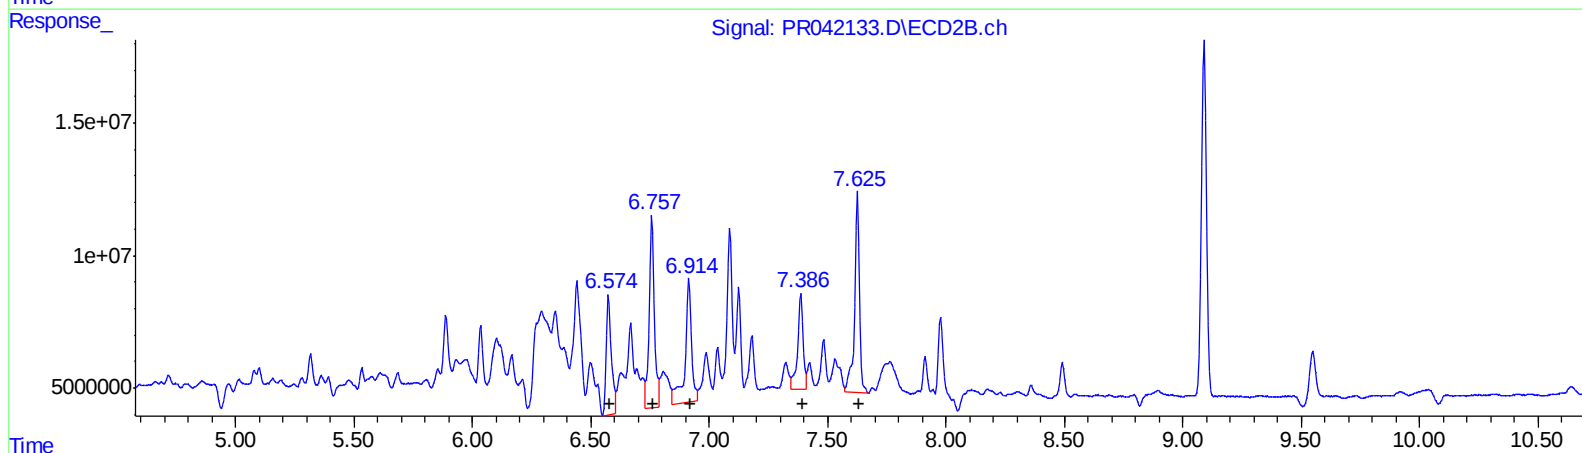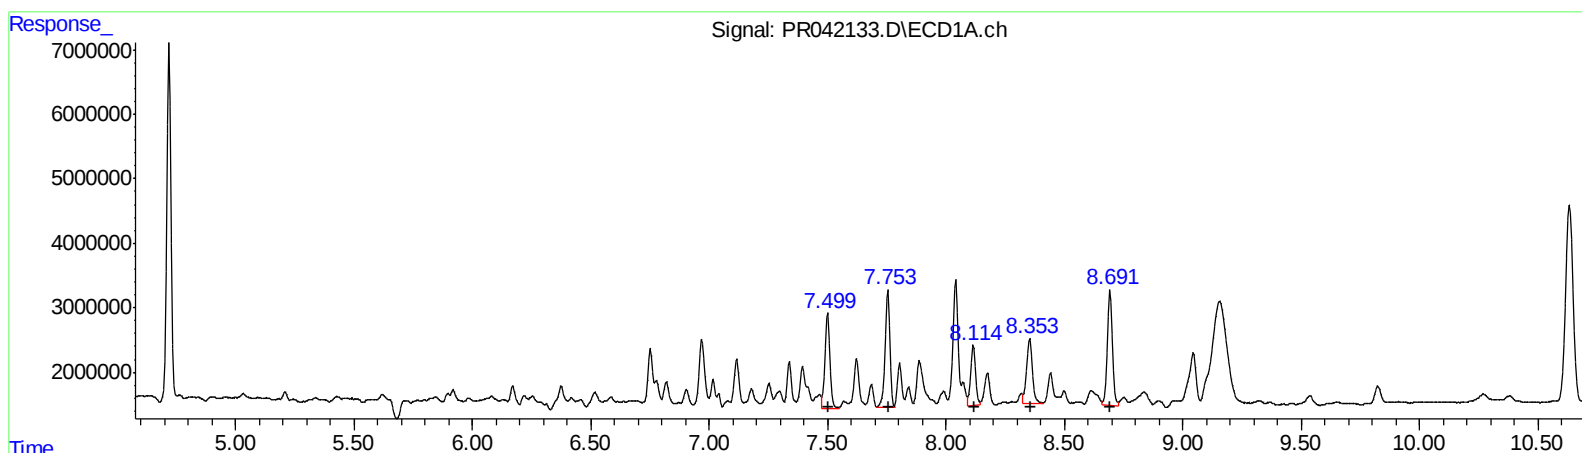

QEdit

(31) AR-1260-1 (L7)

R.T.	Response	Conc
7.50	21537973	113.68
7.75	25522457	107.98
8.11	13443017	71.61
8.35	17345759	86.31
8.69	26362993	60.90

(31) AR-1260-1 #2 (L7)

R.T.	Response	Conc
6.57	67893923	114.54
6.76	107635662	132.02
6.91	86739544	125.47
7.39	57874449	99.73
7.63	108726917	66.87

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
Data File : PR042133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2019 04:20
Operator : SM\AJ
Sample : K5202-07
Misc :
ALS Vial : 50 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
C0AB1

Manual Integrations
APPROVED

Ankita
10/10/2019 1:38:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:29:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 04 06:59:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

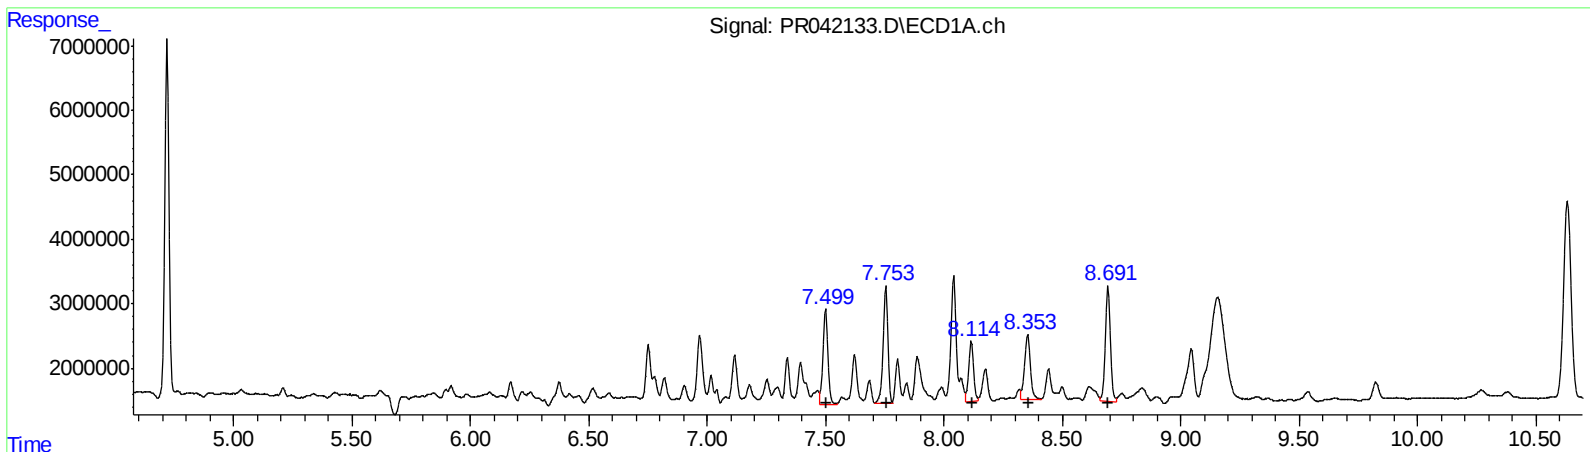

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
7.50 21537973 113.68
7.75 25522457 107.98
8.11 13443017 71.61
8.35 17345759 86.31
8.69 26362993 60.90
(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.57 45907589 77.45
6.76 75661411 92.80
6.91 54544303 78.90
7.39 57874449 99.73
7.63 108726917 66.87

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR100819\
 Data File : PR042133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2019 04:20
 Operator : SM\AJ
 Sample : K5202-07
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 C0AB1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:29:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100319CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 04 06:59:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

Ankita
 10/10/2019 1:38:07 PM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.719	3.983	66494462	256.0E6	16.346	16.742
2) SA Decachlor...	10.631	9.089	66677127	198.4E6	19.405	20.007
Target Compounds						
26) L6 AR-1254-1	6.751	5.888	11307674	40731236	69.240m	76.890
27) L6 AR-1254-2	6.969	6.035	16571692	25682546	66.794m	51.226
28) L6 AR-1254-3	7.337	6.441	7596949	91546342	28.151m	97.034 #
29) L6 AR-1254-4	7.622	6.668	9863834	23548629	48.601m	35.568m#
30) L6 AR-1254-5	8.041	7.086	29500154	78921103	138.724	91.914m#
31) L7 AR-1260-1	7.499	6.574	21537973	45907589	113.677	77.446m#
32) L7 AR-1260-2	7.754	6.757	25522457	75661411	107.981	92.805m
33) L7 AR-1260-3	8.115	6.914	13443017	54544303	71.609	78.900m
34) L7 AR-1260-4	8.353	7.386	17345759	57874449	86.312	99.733
35) L7 AR-1260-5	8.692	7.625	26362993	108.7E6	60.900	66.873

A.J
 10/11/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.