

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101023\
 Data File : PR063939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 05:15
 Operator : AJ\MA
 Sample : PB156077BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PB156077BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/11/2023
 Supervised By :Ankita Jodhani 10/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 07:03:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 10 14:16:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.736	3.025	131.8E6	84482644	20.884	21.613
2) SA Decachlor...	9.758	8.425	103.9E6	67405068	22.025	22.110m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101023\
Data File : PR063939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 05:15
Operator : AJ\MA
Sample : PB156077BL
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PB156077BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/11/2023
Supervised By :Ankita Jodhani 10/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 07:03:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101023.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 10 14:16:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

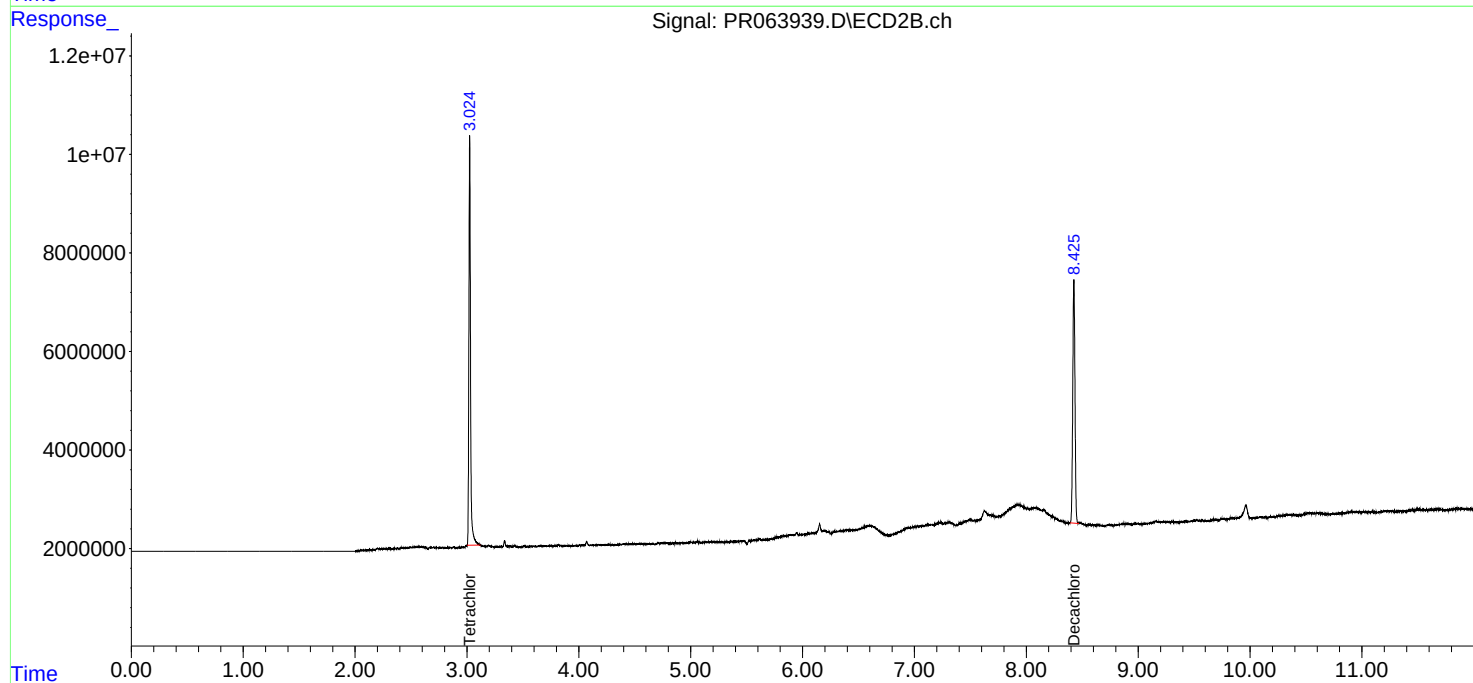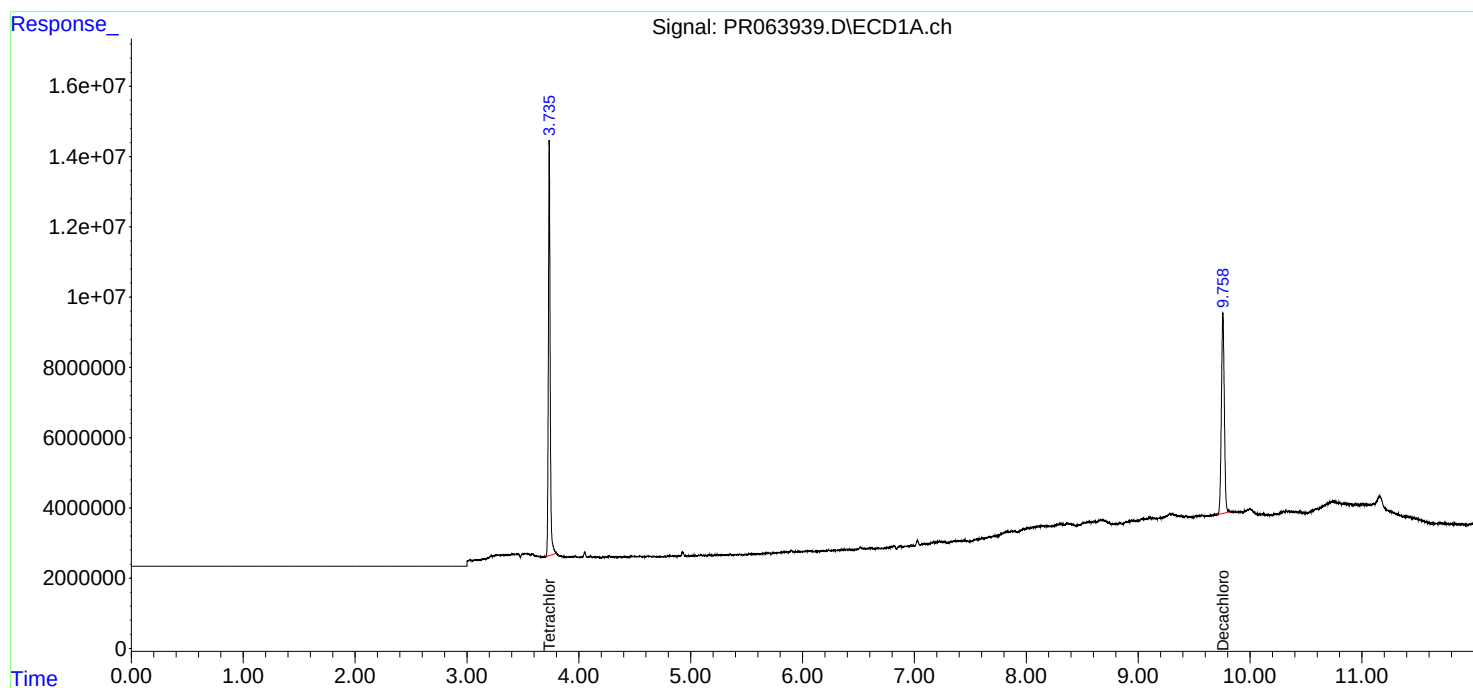

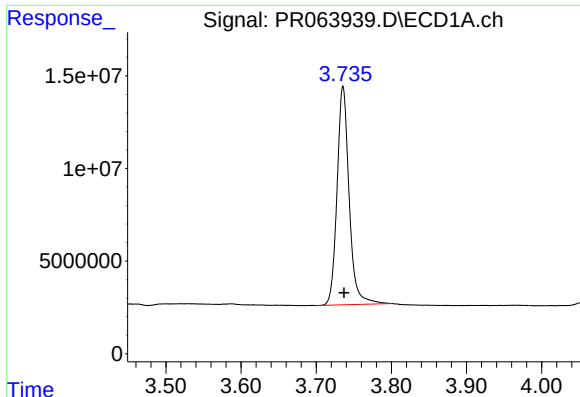

#1 Tetrachloro-m-xylene

R.T.: 3.736 min
Delta R.T.: -0.001 min
Response: 131793111
Conc: 20.88 ng/ml

Instrument :

ECD_R


ClientSampleId :

PB156077BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/11/2023
Supervised By :Ankita Jodhani 10/11/2023

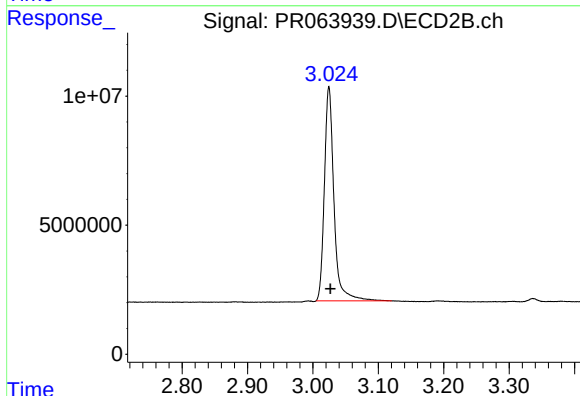


#1 Tetrachloro-m-xylene

R.T.: 3.025 min
Delta R.T.: -0.002 min
Response: 84482644
Conc: 21.61 ng/ml

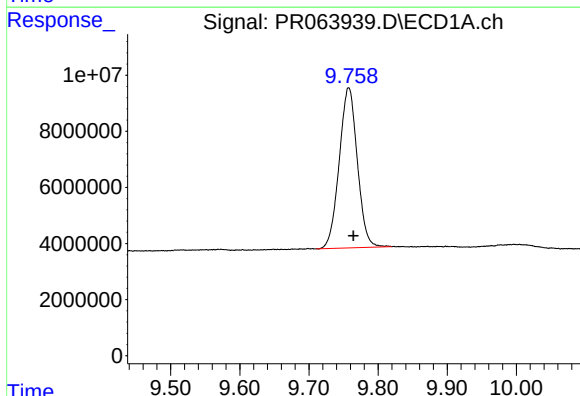

#2 Decachlorobiphenyl

R.T.: 9.758 min
Delta R.T.: -0.007 min
Response: 103934902
Conc: 22.03 ng/ml

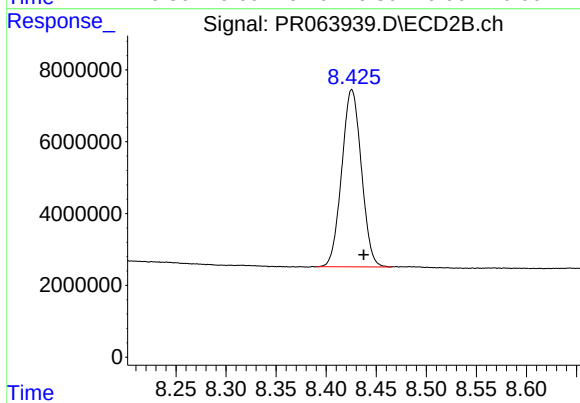

#2 Decachlorobiphenyl

R.T.: 8.425 min
Delta R.T.: -0.012 min
Response: 67405068
Conc: 22.11 ng/ml m