

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101123\
 Data File : PR063970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 13:23
 Operator : AJ\MA
 Sample : 04699-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 22:24:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 10 14:16:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.736	3.025	113.5E6	71119542	17.985	18.194
2)	SA Decachlor...	9.757	8.428	92900617	58008102	19.687	19.028
Target Compounds							
8)	L2 AR-1221-1	3.964	3.257	1933433	1156462	26.111	23.962
9)	L2 AR-1221-2	4.053	3.340	2332201	1677683	44.302	45.303
10)	L2 AR-1221-3	4.133	3.426	4473451	3009263	26.594	27.128



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101123\
Data File : PR063970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 13:23
Operator : AJ\MA
Sample : 04699-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 83 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 22:24:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101023.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 10 14:16:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

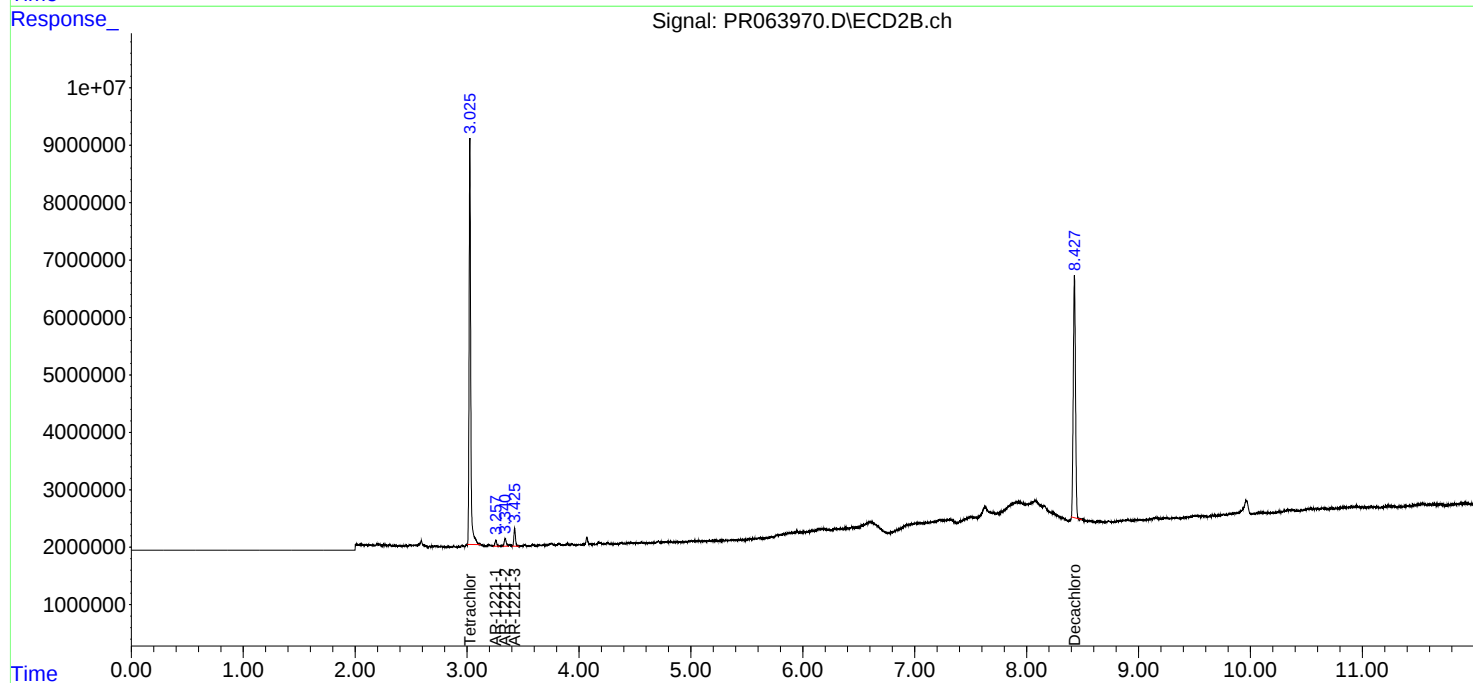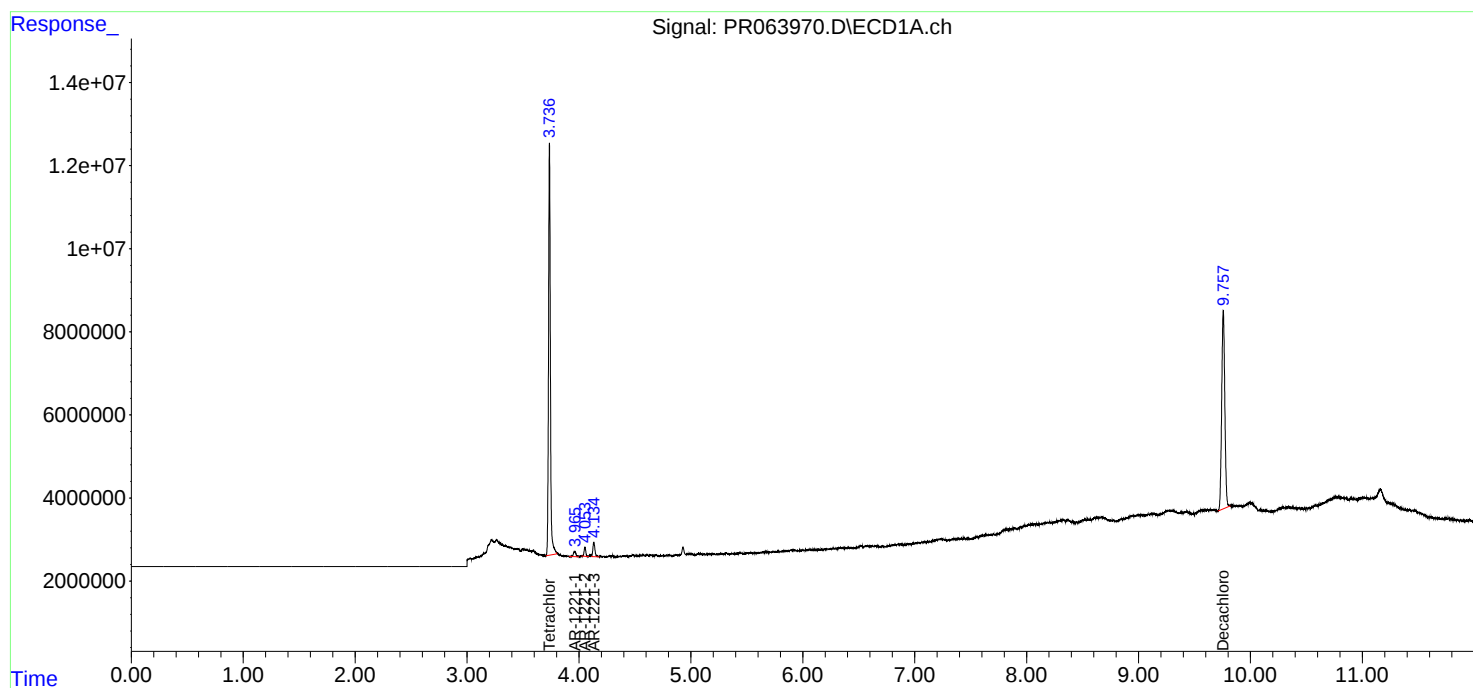


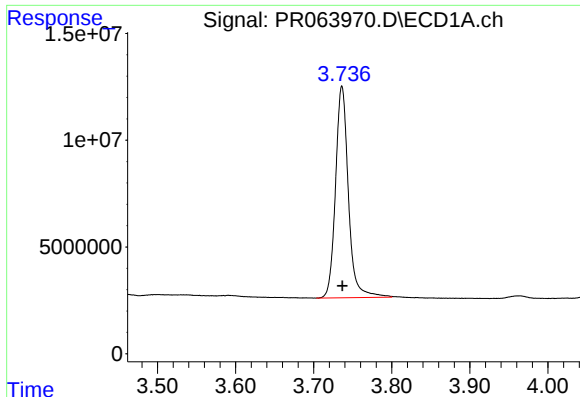

#1 Tetrachloro-m-xylene


R.T.: 3.736 min
Delta R.T.: 0.000 min
Response: 113495216
Conc: 17.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2023

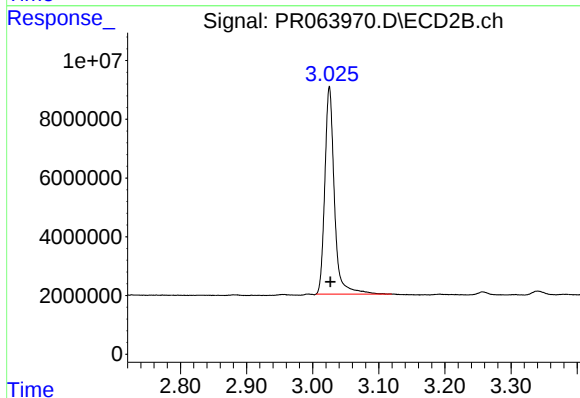


#1 Tetrachloro-m-xylene

R.T.: 3.025 min
Delta R.T.: -0.002 min
Response: 71119542
Conc: 18.19 ng/ml

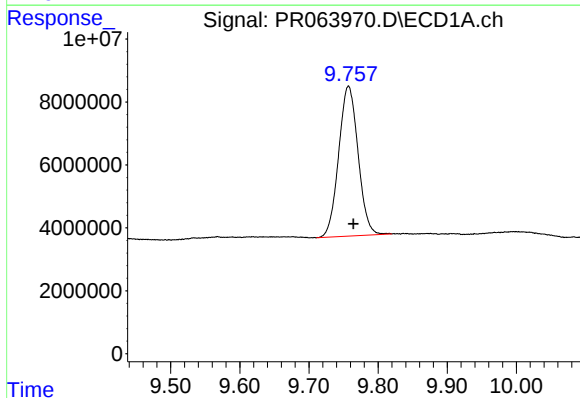


#2 Decachlorobiphenyl

R.T.: 9.757 min
Delta R.T.: -0.007 min
Response: 92900617
Conc: 19.69 ng/ml

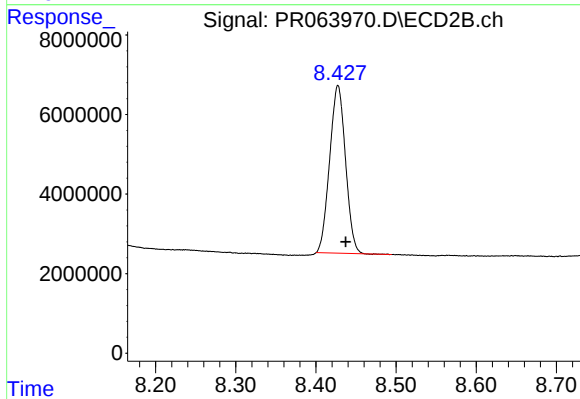

#2 Decachlorobiphenyl


R.T.: 8.428 min
Delta R.T.: -0.010 min
Response: 58008102
Conc: 19.03 ng/ml

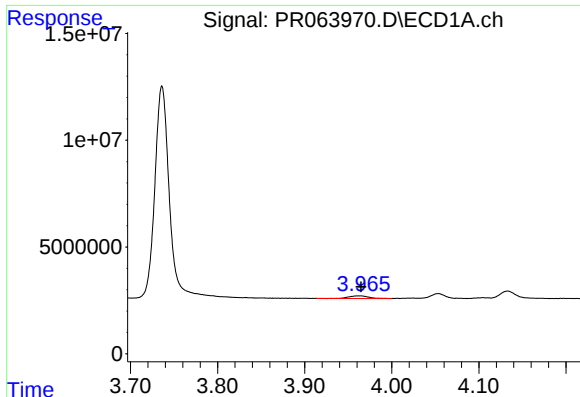

#8 AR-1221-1


R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 1933433
Conc: 26.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2023

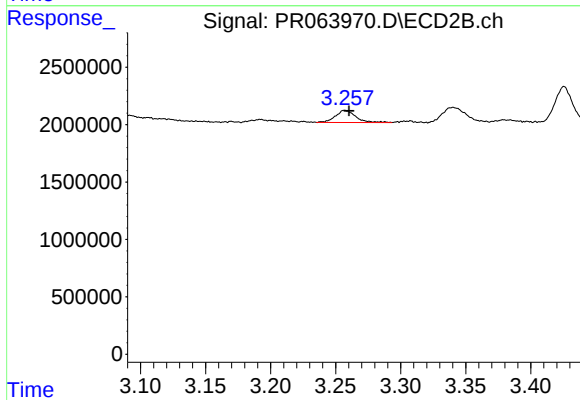


#8 AR-1221-1

R.T.: 3.257 min
Delta R.T.: -0.003 min
Response: 1156462
Conc: 23.96 ng/ml

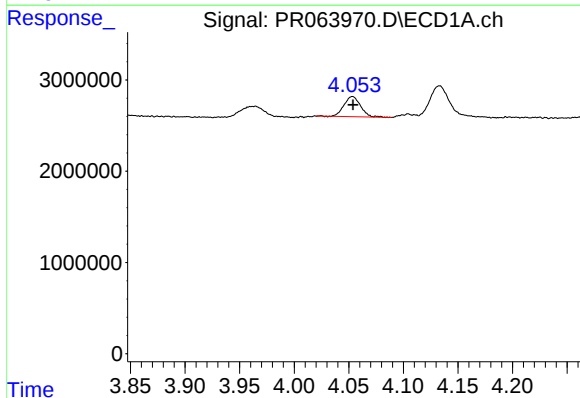


#9 AR-1221-2

R.T.: 4.053 min
Delta R.T.: 0.000 min
Response: 2332201
Conc: 44.30 ng/ml

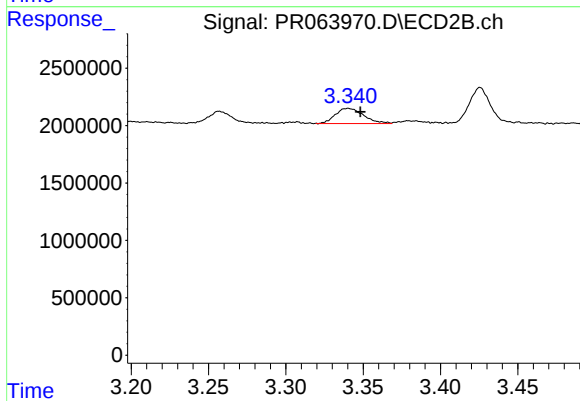

#9 AR-1221-2


R.T.: 3.340 min
Delta R.T.: -0.008 min
Response: 1677683
Conc: 45.30 ng/ml

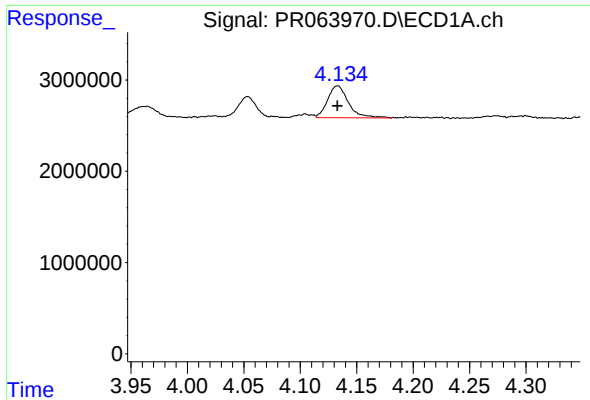

#10 AR-1221-3

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 4473451
Conc: 26.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2023

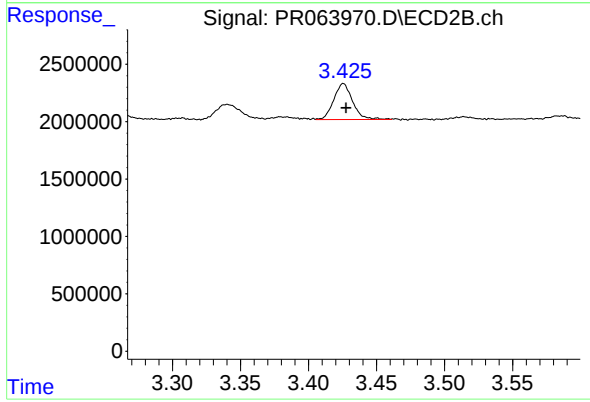

#10 AR-1221-3

R.T.: 3.426 min
Delta R.T.: -0.002 min
Response: 3009263
Conc: 27.13 ng/ml