

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101322\
 Data File : PR057358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 09:12
 Operator : AJ\MA
 Sample : N5116-03 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 SWRN-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/14/2022
 Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 11:12:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 13 04:58:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.882	0	9232545	N.D.	6.553 #
2) SA Decachlor...	9.492	8.092	3462067	22319742	1.315m	12.105m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101322\
Data File : PR057358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 09:12
Operator : AJ\MA
Sample : N5116-03 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
SWRN-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 11:12:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 13 04:58:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

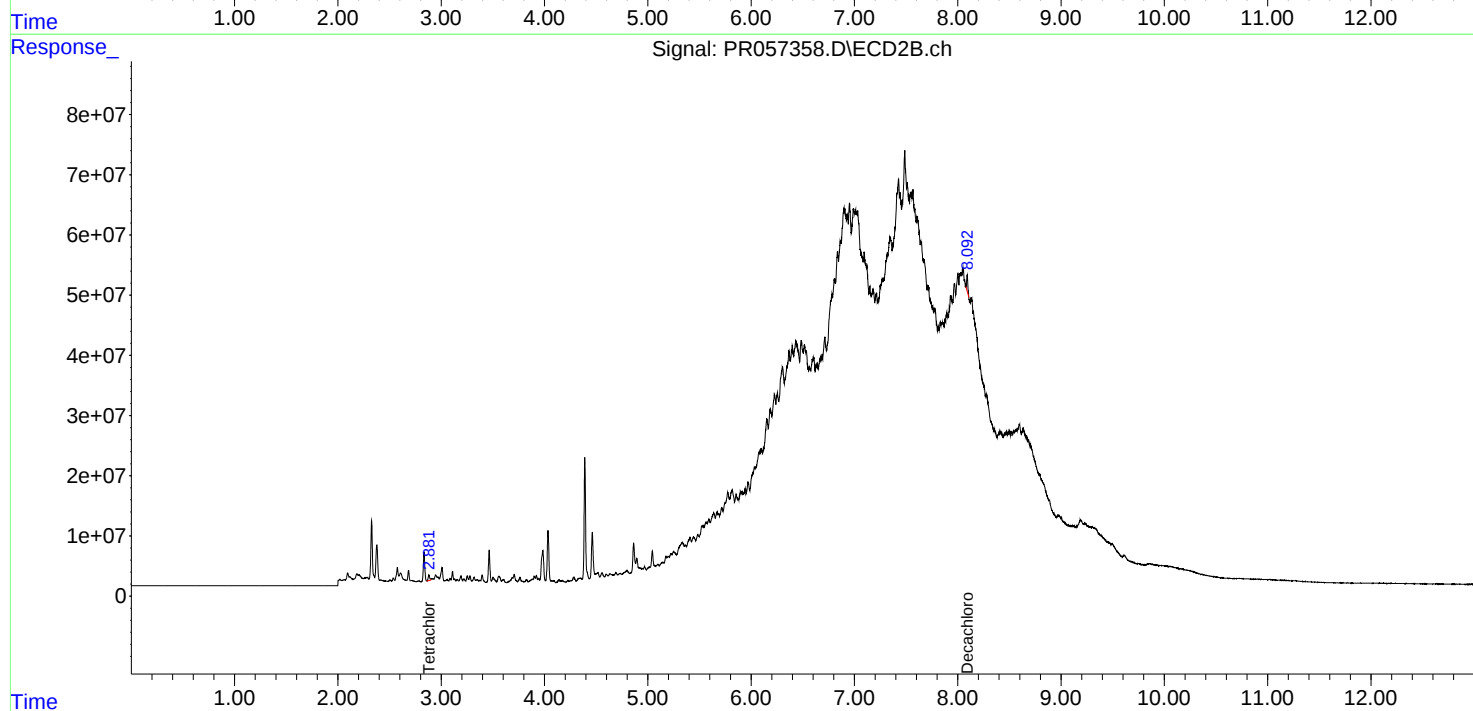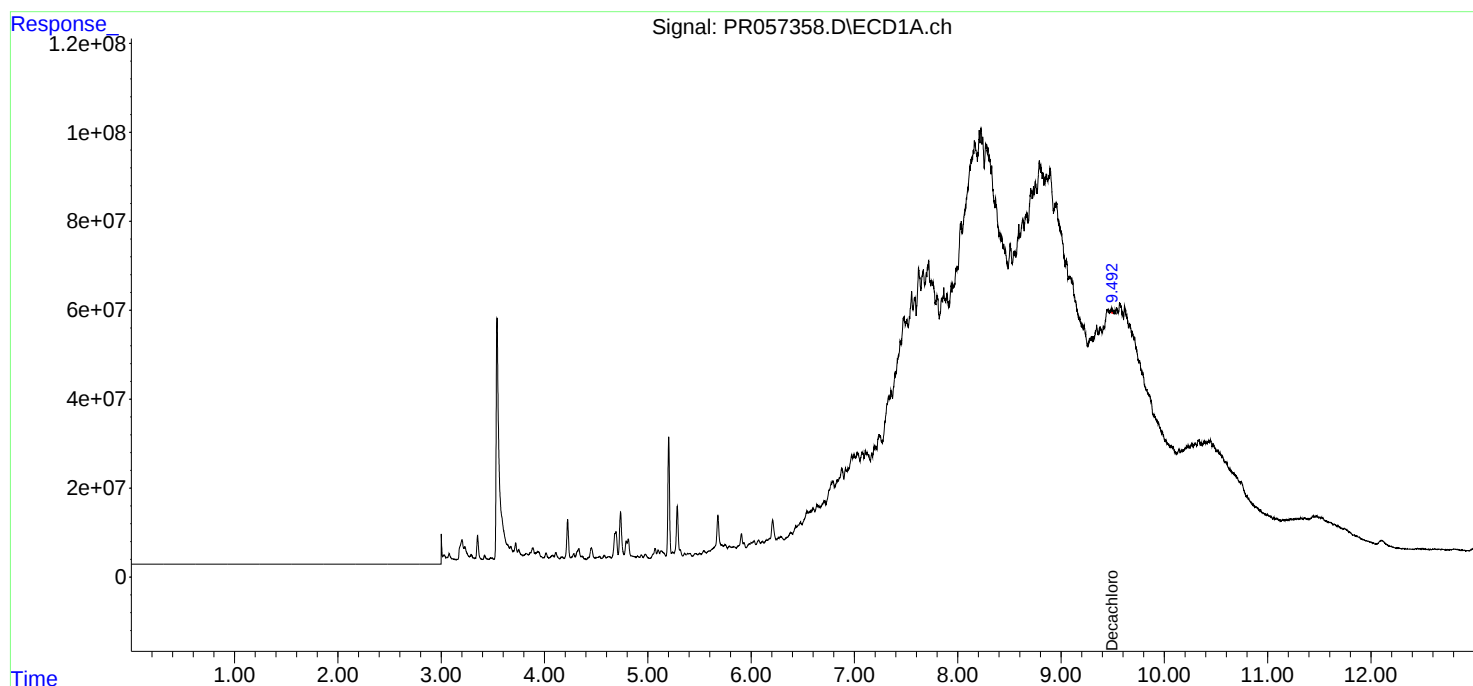

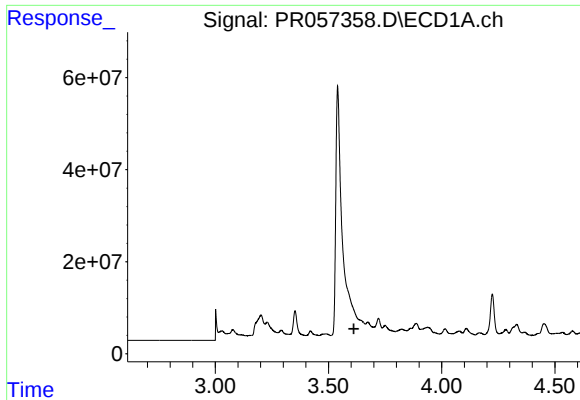


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
SWRN-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/14/2022
Supervised By :Ankita Jodhani 10/14/2022

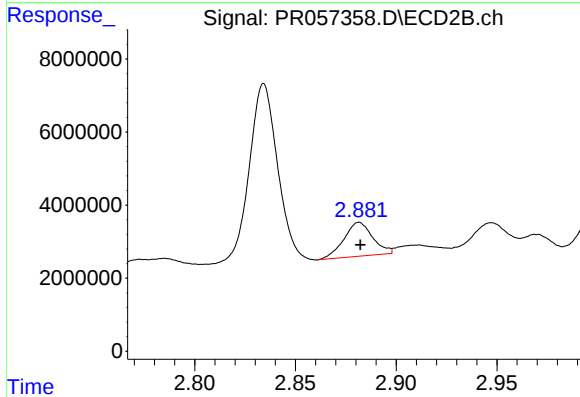


#1 Tetrachloro-m-xylene

R.T.: 2.882 min
Delta R.T.: 0.000 min
Response: 9232545
Conc: 6.55 ng/ml

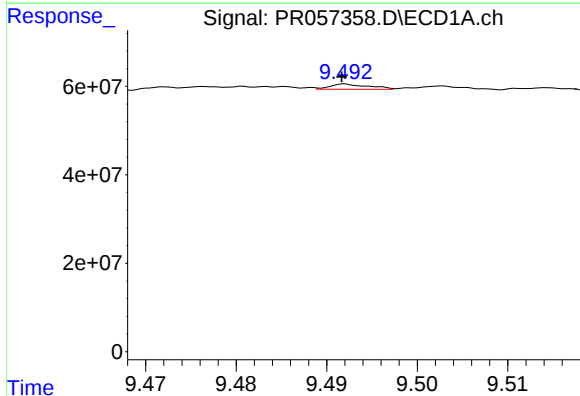

#2 Decachlorobiphenyl

R.T.: 9.492 min
Delta R.T.: 0.000 min
Response: 3462067
Conc: 1.32 ng/ml m

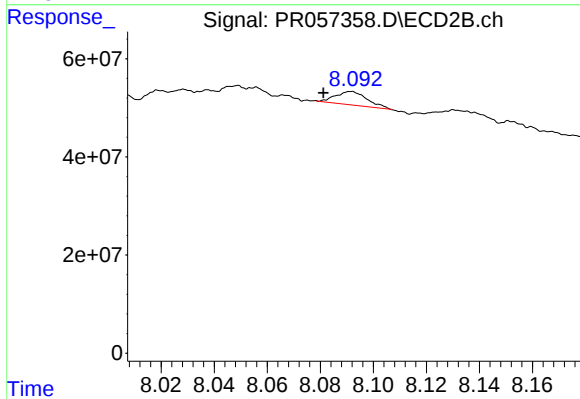

#2 Decachlorobiphenyl

R.T.: 8.092 min
Delta R.T.: 0.011 min
Response: 22319742
Conc: 12.10 ng/ml m