

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101520\
Data File : PR047689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 05:36
Operator : AJ\MA
Sample : L4285-13
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
BEQD9

Manual Integrations
APPROVED

Ankita
10/15/2020 11:23:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 08:26:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100920CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 10 06:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

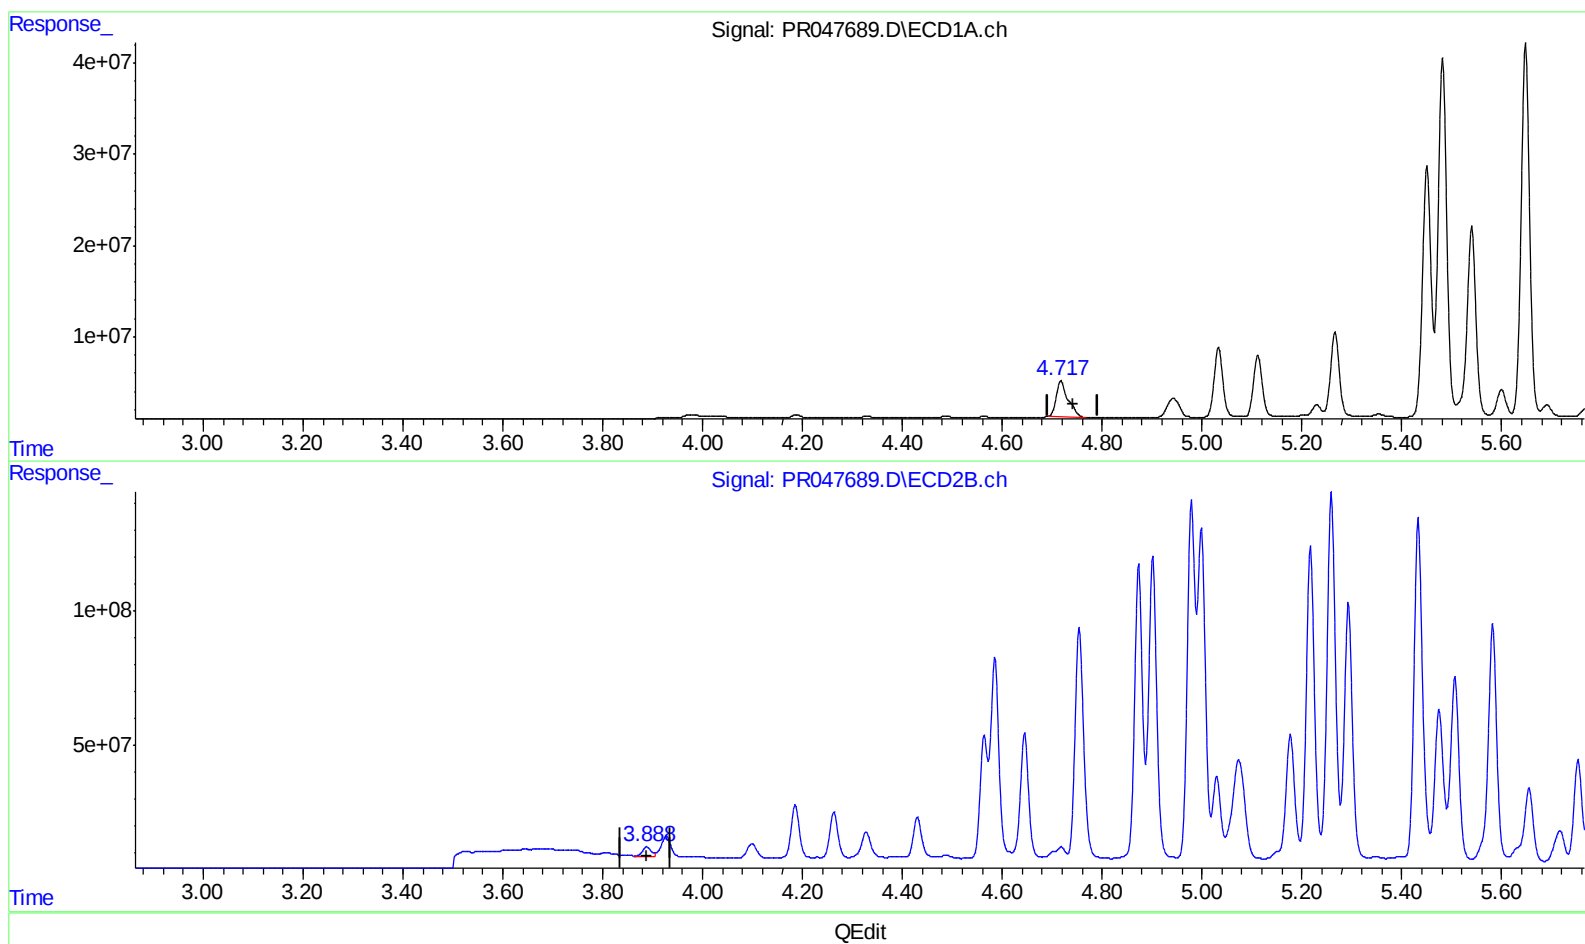

(1) Tetrachloro-m-xylene (SA)

4.717min 53.122 ng/ml

response 63796095

(1) Tetrachloro-m-xylene #2 (SA)

3.888min 11.793 ng/ml

response 41358751

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101520\
Data File : PR047689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 05:36
Operator : AJ\MA
Sample : L4285-13
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
BEQD9

Manual Integrations
APPROVED

Ankita
10/15/2020 11:23:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 08:26:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100920CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 10 06:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

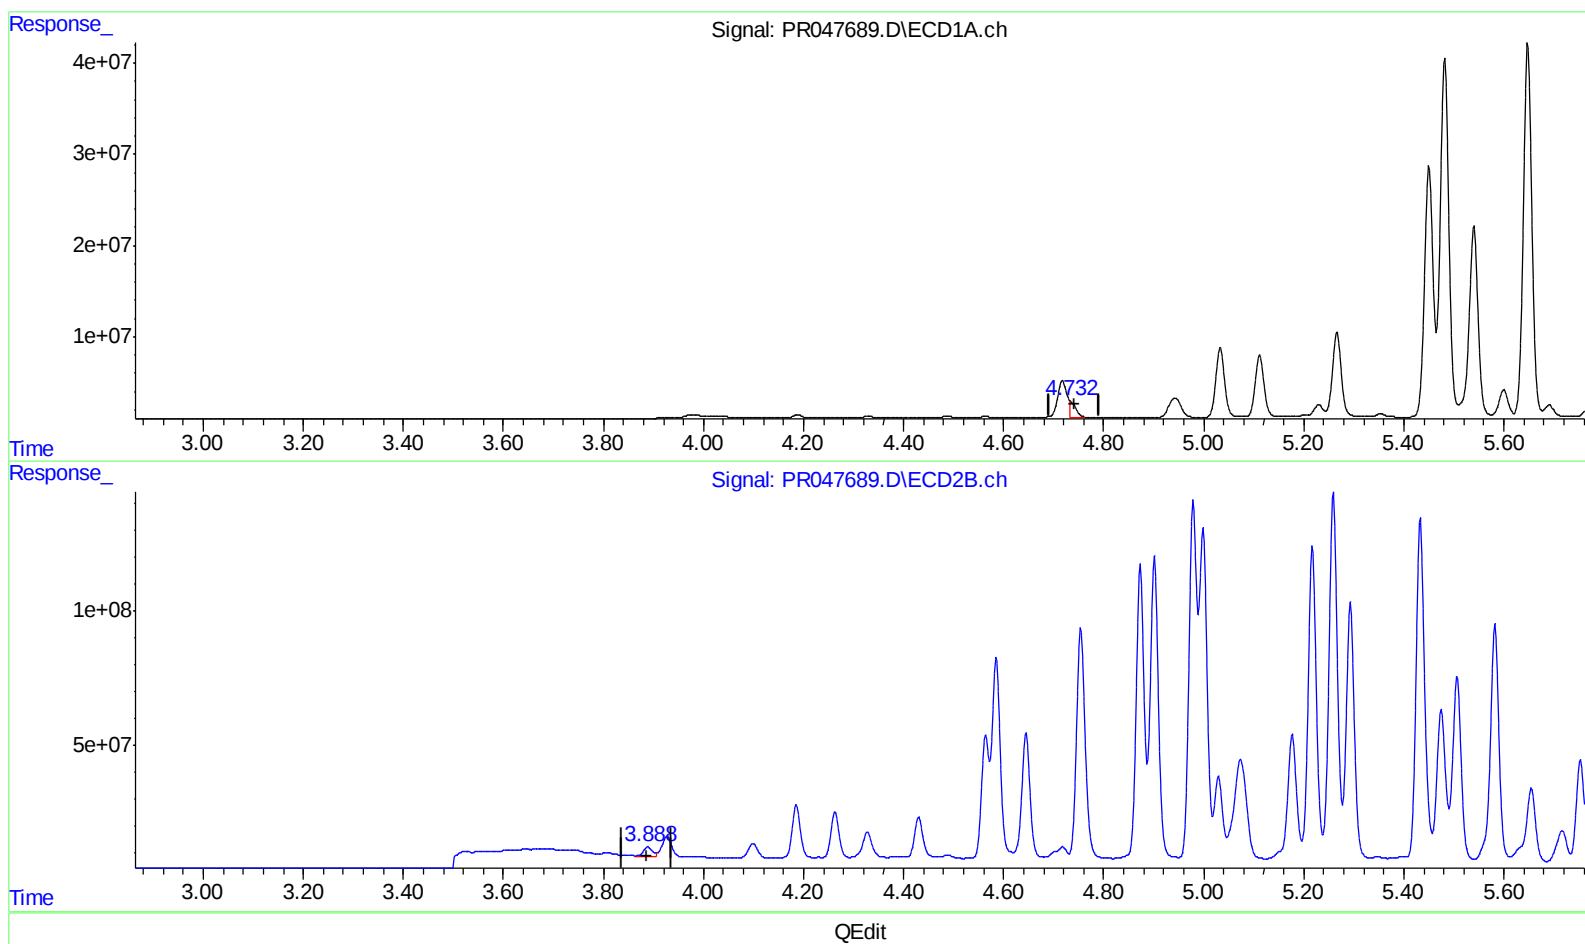

(1) Tetrachloro-m-xylene (SA)

4.732min 11.672 ng/ml m

response 14016989

(1) Tetrachloro-m-xylene #2 (SA)

3.888min 11.793 ng/ml

response 41358751

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101520\
 Data File : PR047689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 05:36
 Operator : AJ\MA
 Sample : L4285-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 BEQD9

Manual Integrations
 APPROVED

Ankita
 10/15/2020 11:23:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 08:26:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100920CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 10 06:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.732	3.888	14016989	41358751	11.672m	11.793
2) SA Decachlor...	10.674	8.968	65757459	304.0E6	36.903	25.205 #
Target Compounds						
21) L5 AR-1248-1	5.916	4.979	831.7E6	1420.6E6	24548.513	18077.256 #
22) L5 AR-1248-2	6.190	5.217	946.3E6	1303.4E6	19092.236	13774.179 #
23) L5 AR-1248-3	6.397	5.259	752.0E6	1565.7E6	13339.270	13472.528
24) L5 AR-1248-4	6.802	5.433	353.8E6	1479.6E6	5316.094	9635.664 #
25) L5 AR-1248-5	6.843	5.828	487.7E6	991.5E6	7584.159	4607.416 #
26) L6 AR-1254-1	6.776	5.787	538.3E6	1348.2E6	8188.959	5682.338 #
27) L6 AR-1254-2	6.997	5.936	783.4E6	768.6E6	7613.136	3371.638 #
28) L6 AR-1254-3	7.363	6.341	756.3E6	2205.1E6	7000.999	4922.346 #
29) L6 AR-1254-4	7.648	6.569	382.0E6	1491.9E6	4353.380	3373.004
30) L6 AR-1254-5	8.067	6.986	421.6E6	1594.7E6	4376.185	2681.795 #
31) L7 AR-1260-1	7.526	6.470	238.1E6	866.0E6	2800.128	3478.640
32) L7 AR-1260-2	7.779	6.658	333.6E6	1131.9E6	3203.272	1924.916 #
33) L7 AR-1260-3	8.141	6.813	182.2E6	664.7E6	2250.622	1647.020 #
34) L7 AR-1260-4	8.378	7.287	228.5E6	534.9E6	2331.059	1195.151 #
35) L7 AR-1260-5	8.720	7.528	321.8E6	3000.5E6	1641.513	1537.193

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 10/24/20