

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101620\
 Data File : PR047748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 08:49
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:04:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100920CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 10 06:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7)	L1	AR-1016-5	0.000	5.426	0	933948	N.D.	7.879 #
15)	L3	AR-1232-5	0.000	5.426	0	933948	N.D.	19.028 #
20)	L4	AR-1242-5	0.000	5.810	0	3084740	N.D.	21.737 #
24)	L5	AR-1248-4	0.000	5.426	0	933948	N.D.	6.082 #
25)	L5	AR-1248-5	0.000	5.810	0	3084740	N.D.	14.334 #
26)	L6	AR-1254-1	0.000	5.810	0	3084740	N.D.	13.002 #
30)	L6	AR-1254-5	0.000	7.032f	0	96515	N.D.	0.162 #
32)	L7	AR-1260-2	0.000	6.641	0	2181522	N.D.	3.710 #
36)	L8	AR-1262-1	0.000	7.032f	0	96515	N.D.	0.286 #
43)	L9	AR-1268-3	0.000	8.050f	0	114009	N.D.	0.050 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101620\
Data File : PR047748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 08:49
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:04:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR100920CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 10 06:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

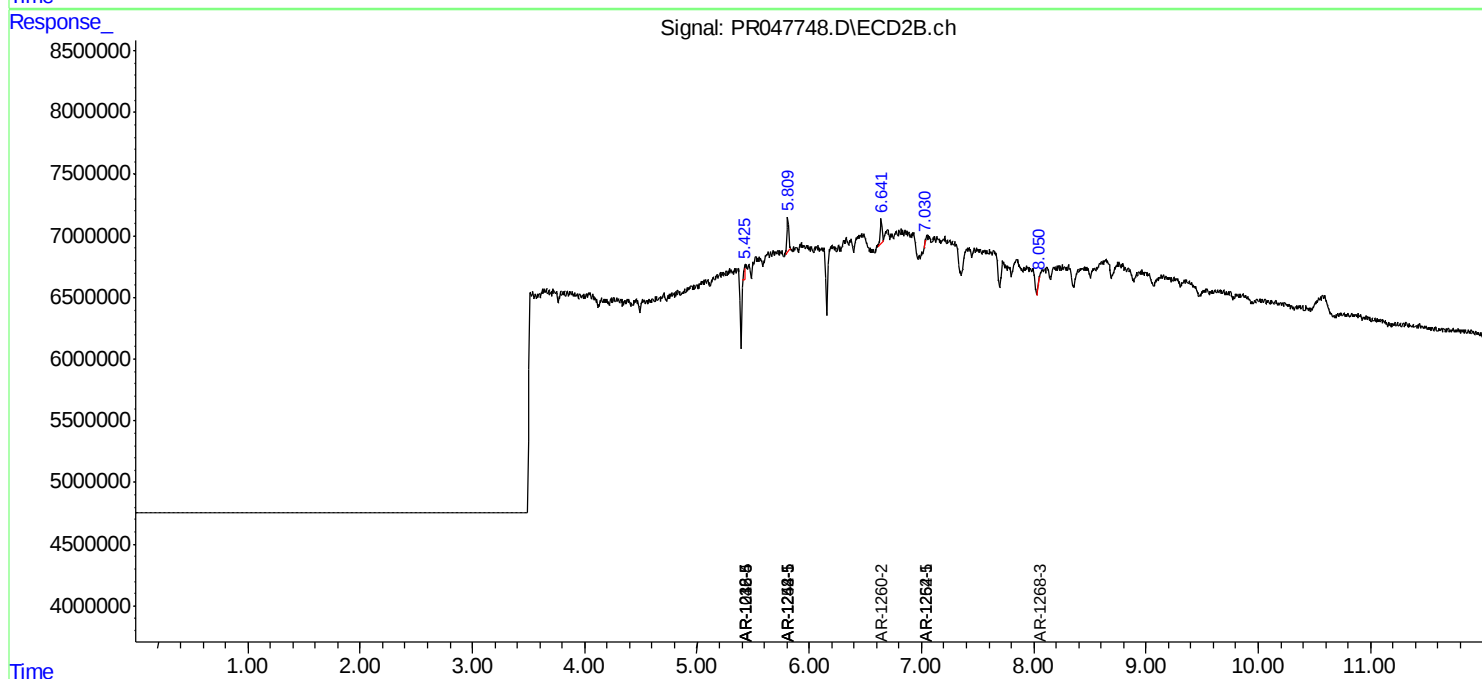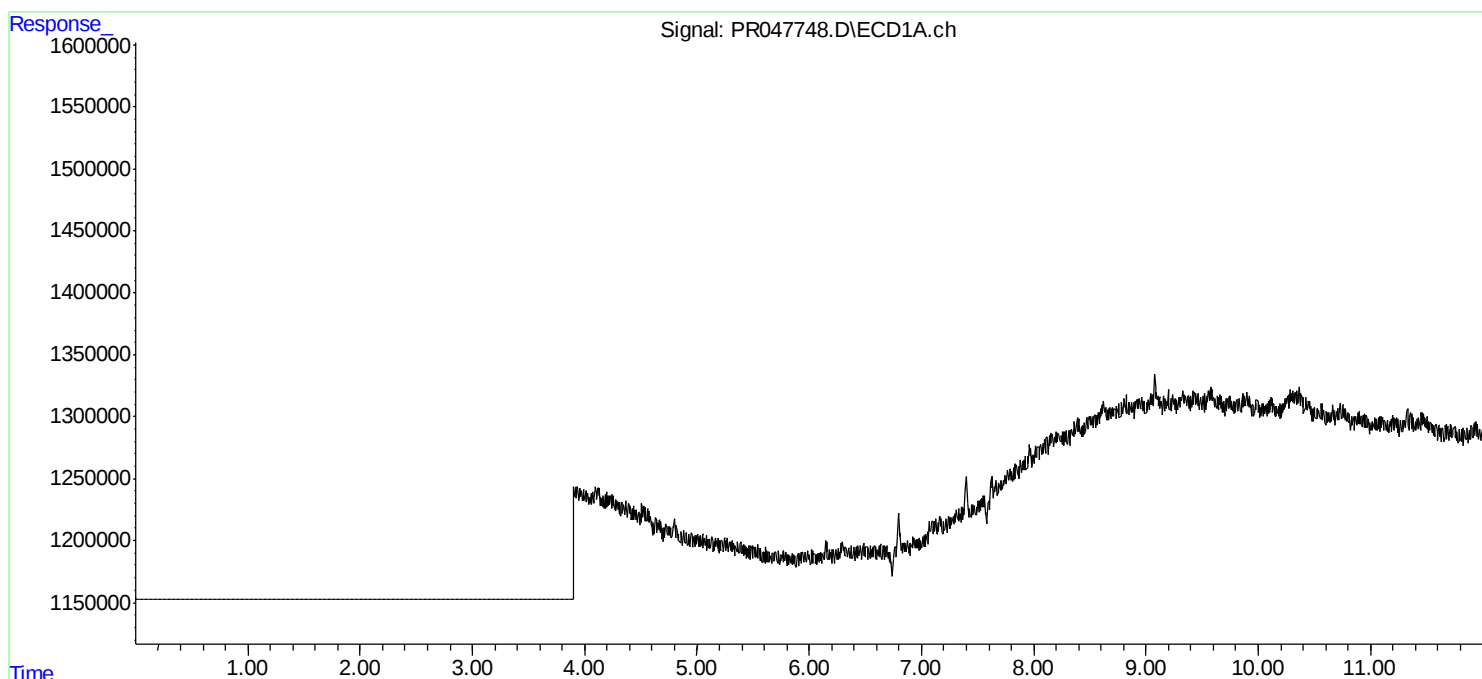


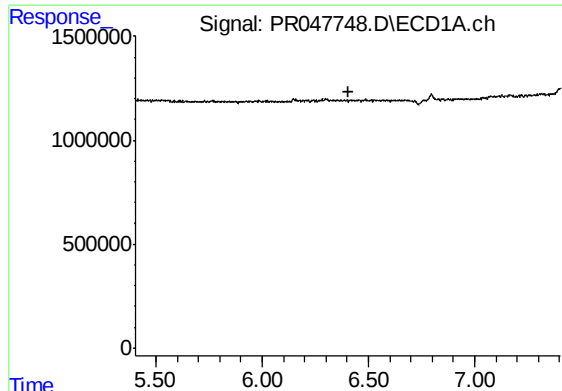

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

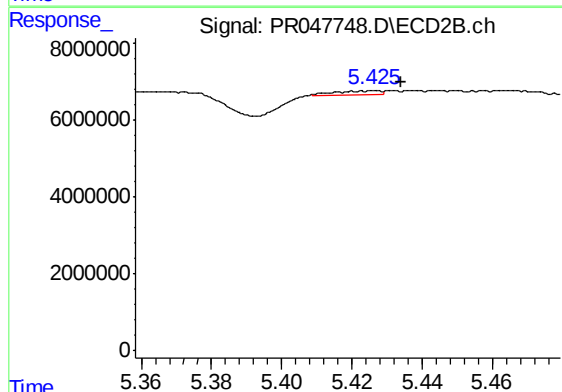


#7 AR-1016-5

R.T.: 5.426 min
Delta R.T.: -0.008 min
Response: 933948
Conc: 7.88 ng/ml

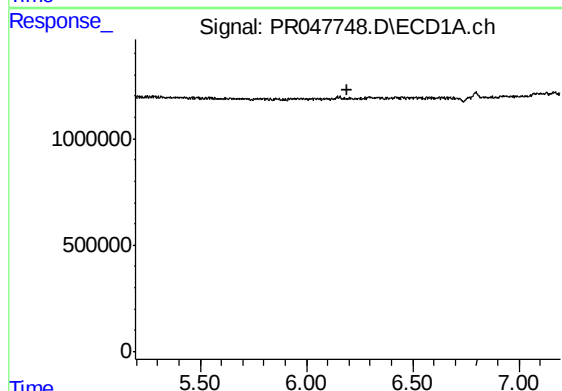


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.195 min
Response: 0
Conc: N.D.

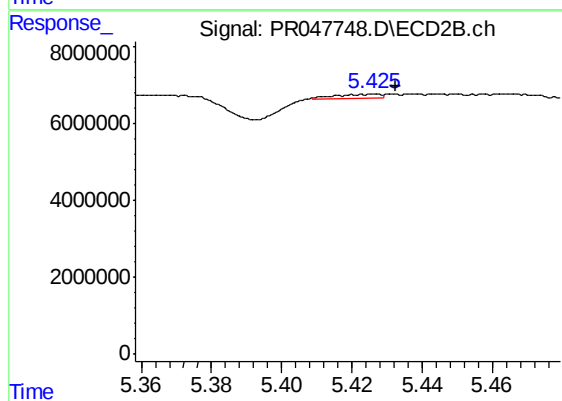

#15 AR-1232-5


R.T.: 5.426 min
Delta R.T.: -0.006 min
Response: 933948
Conc: 19.03 ng/ml

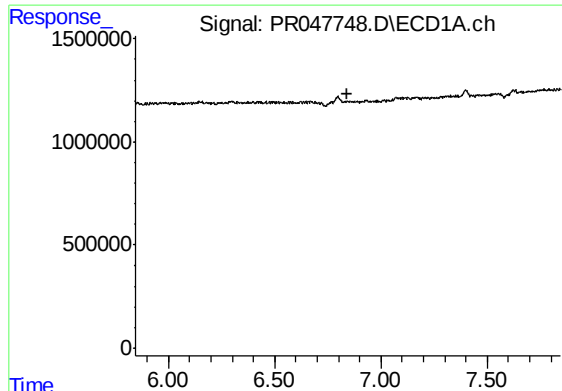

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

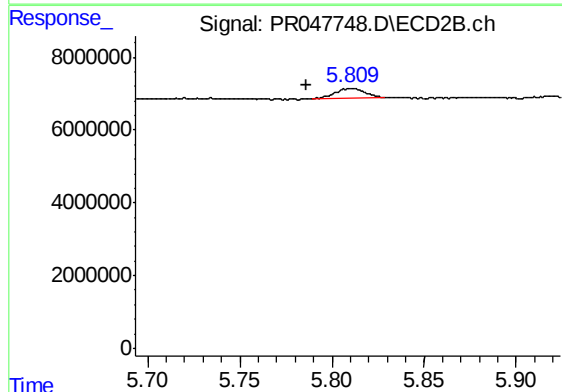


#20 AR-1242-5

R.T.: 5.810 min
Delta R.T.: 0.024 min
Response: 3084740
Conc: 21.74 ng/ml

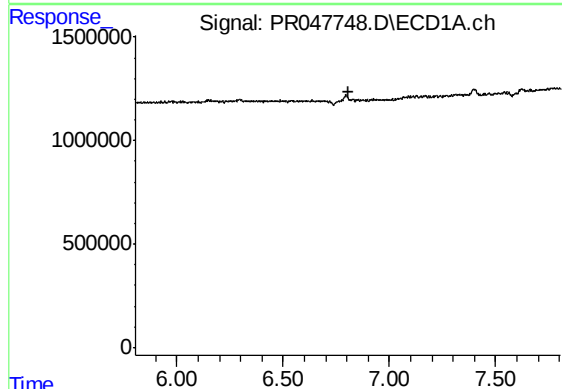


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.805 min
Response: 0
Conc: N.D.

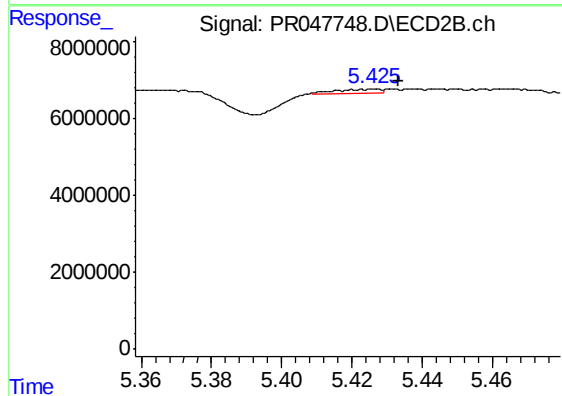

#24 AR-1248-4


R.T.: 5.426 min
Delta R.T.: -0.007 min
Response: 933948
Conc: 6.08 ng/ml

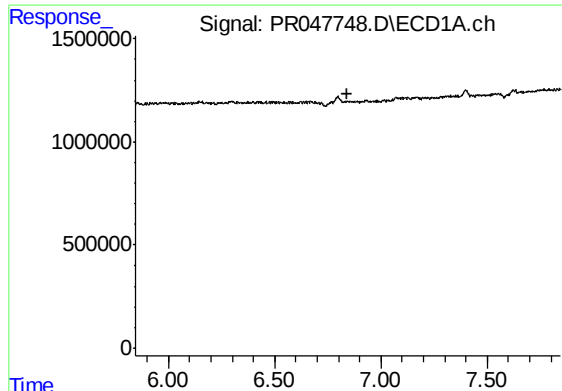

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

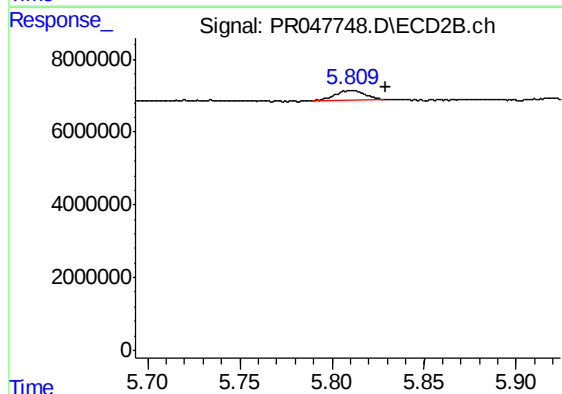


#25 AR-1248-5

R.T.: 5.810 min
Delta R.T.: -0.019 min
Response: 3084740
Conc: 14.33 ng/ml

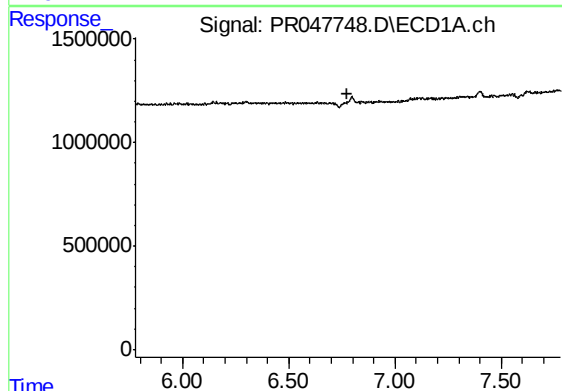


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.778 min
Response: 0
Conc: N.D.

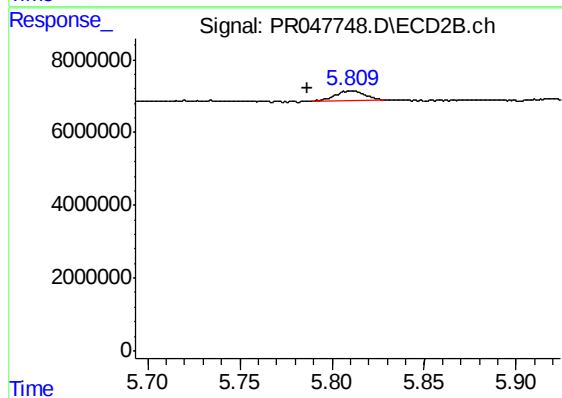

#26 AR-1254-1


R.T.: 5.810 min
Delta R.T.: 0.024 min
Response: 3084740
Conc: 13.00 ng/ml

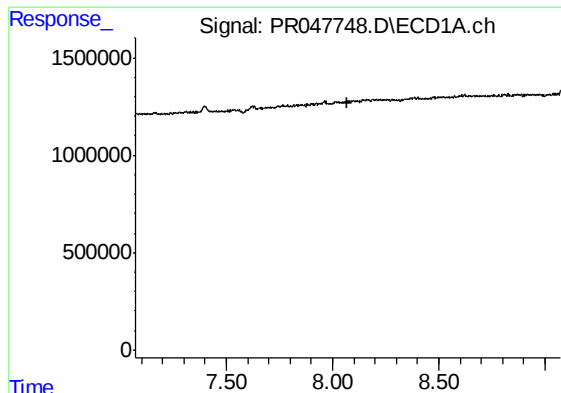

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

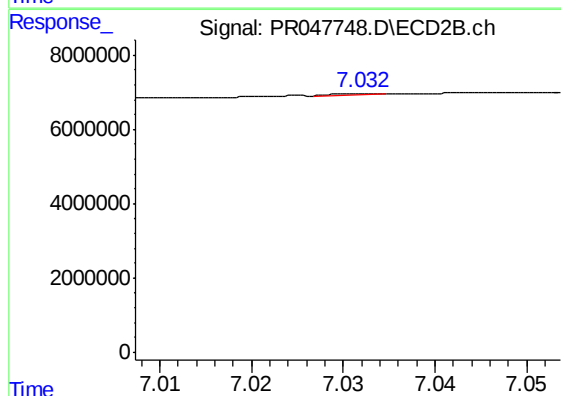


#30 AR-1254-5

R.T.: 7.032 min
Delta R.T.: 0.044 min
Response: 96515
Conc: 0.16 ng/ml

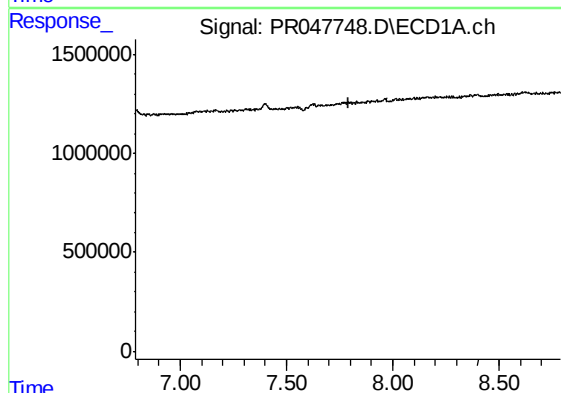


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.789 min
Response: 0
Conc: N.D.

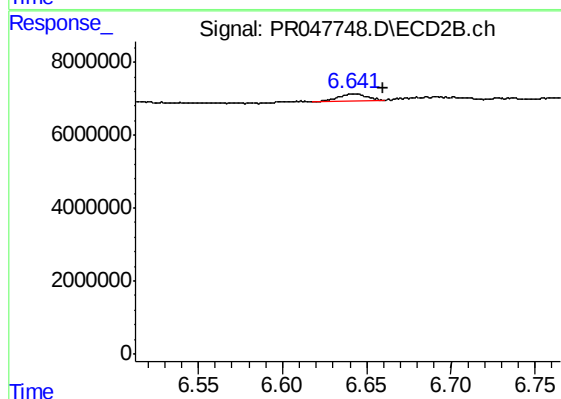

#32 AR-1260-2


R.T.: 6.641 min
Delta R.T.: -0.018 min
Response: 2181522
Conc: 3.71 ng/ml

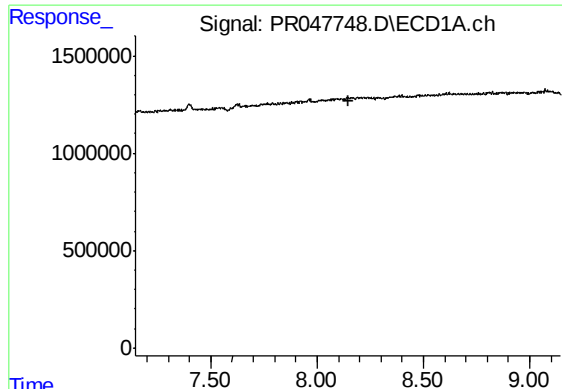

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 8.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

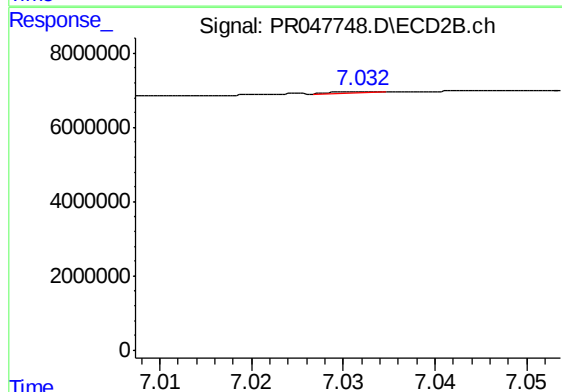


#36 AR-1262-1

R.T.: 7.032 min
Delta R.T.: 0.046 min
Response: 96515
Conc: 0.29 ng/ml

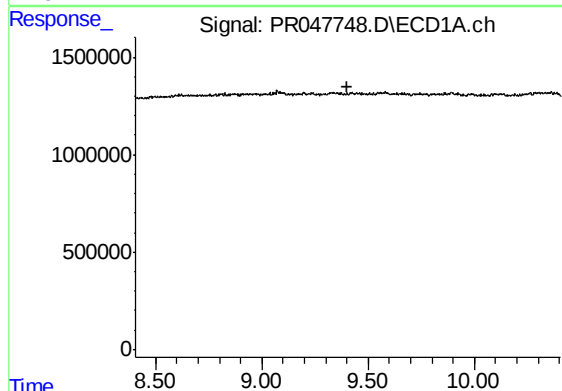

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.405 min
Response: 0
Conc: N.D.

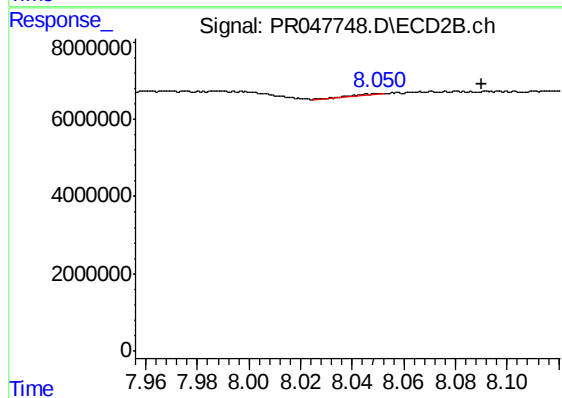

#43 AR-1268-3

R.T.: 8.050 min
Delta R.T.: -0.040 min
Response: 114009
Conc: 0.05 ng/ml