

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101822\
 Data File : PR057464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2022 15:35
 Operator : AJ\MA
 Sample : N5172-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 BU-02-101722

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/19/2022
 Supervised By :Ankita Jodhani 10/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 01:48:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 13 04:58:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.610	2.880	63079936	30922054	18.216m	21.948m
2) SA Decachlor...	9.489	8.076	47504865	31736985	18.049	17.212

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101822\
Data File : PR057464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2022 15:35
Operator : AJ\MA
Sample : N5172-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
BU-02-101722


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/19/2022
Supervised By :Ankita Jodhani 10/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:48:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 13 04:58:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

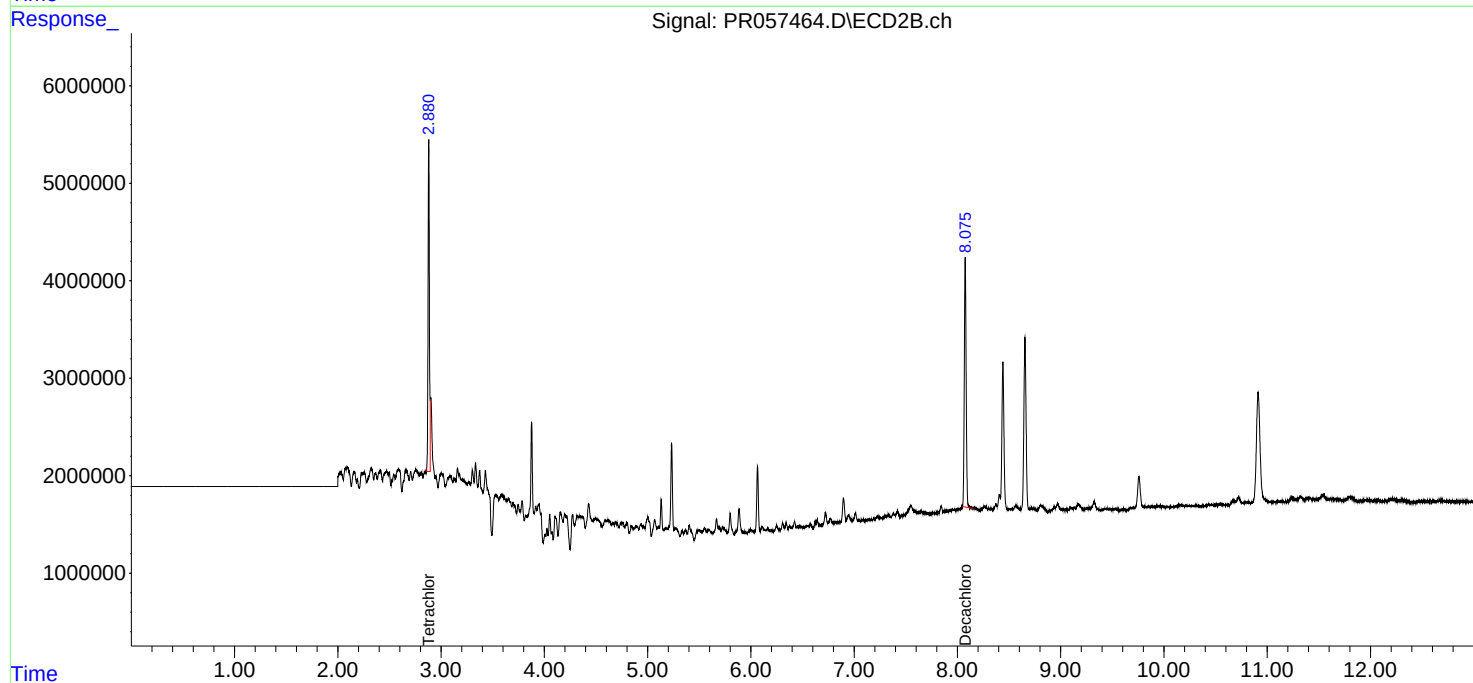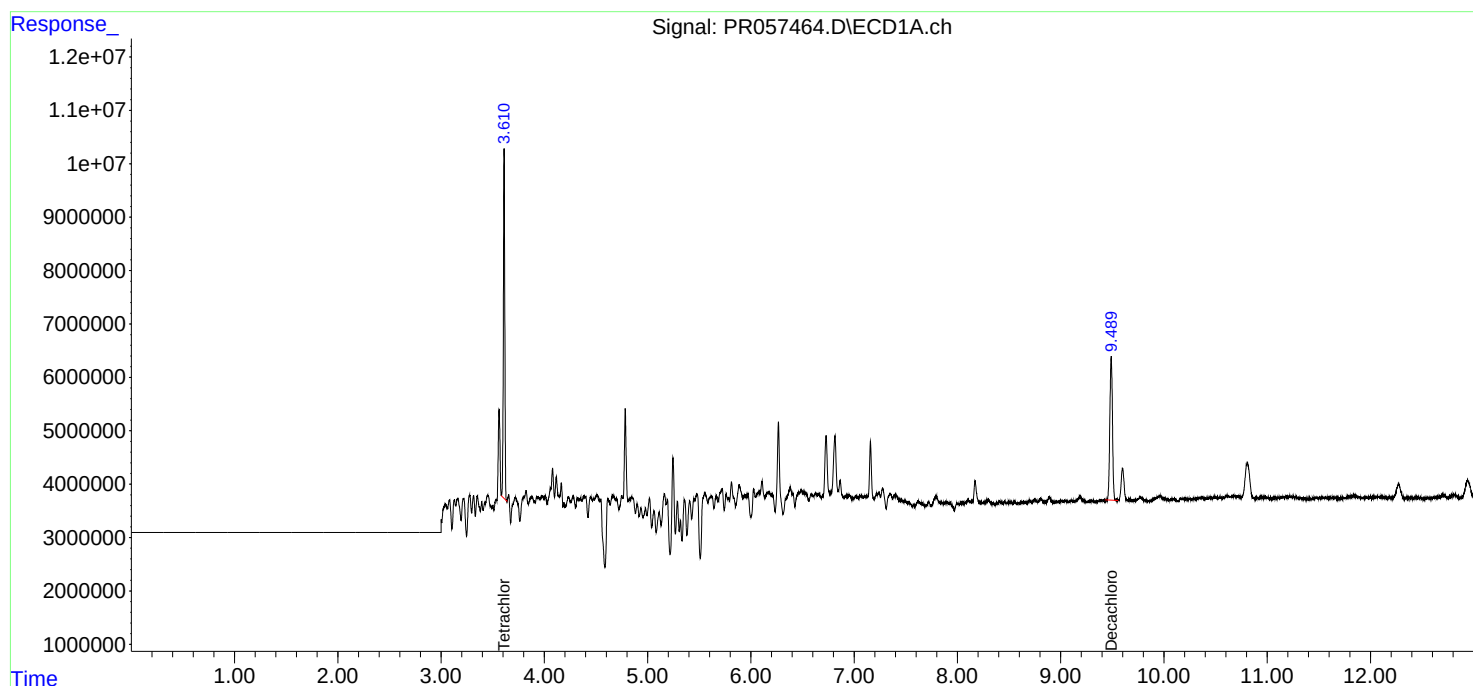

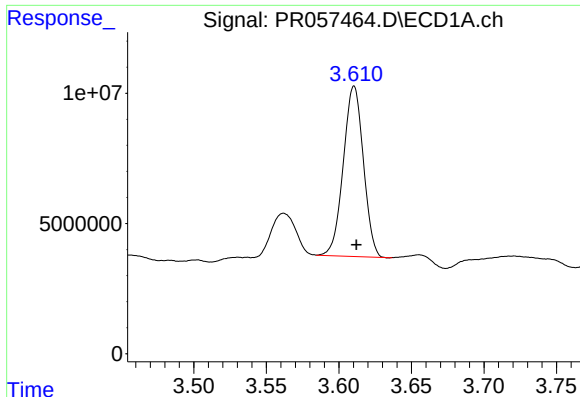


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.002 min
Response: 63079936
Conc: 18.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
BU-02-101722


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/19/2022
Supervised By :Ankita Jodhani 10/19/2022

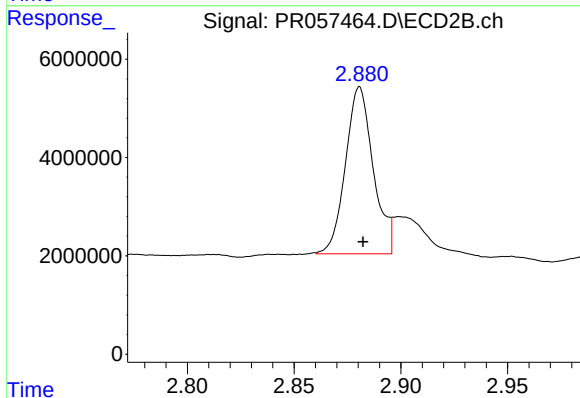


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: -0.002 min
Response: 30922054
Conc: 21.95 ng/ml m

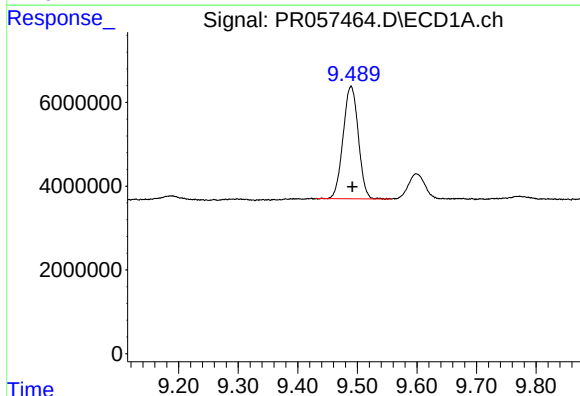

#2 Decachlorobiphenyl

R.T.: 9.489 min
Delta R.T.: -0.002 min
Response: 47504865
Conc: 18.05 ng/ml

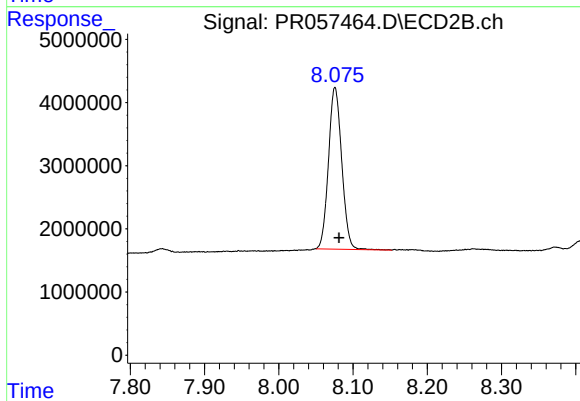

#2 Decachlorobiphenyl

R.T.: 8.076 min
Delta R.T.: -0.005 min
Response: 31736985
Conc: 17.21 ng/ml