

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101824\
 Data File : PR068815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 17:26
 Operator : AJ\MA
 Sample : P4413-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 KR-SS27

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/18/2024
 Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 02:43:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 13:42:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.645	2.977	14410784	86210820	15.370m	15.495m
2) SA Decachlor...	9.537	8.265	8576489	50636656	14.863	11.870

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101824\
Data File : PR068815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 17:26
Operator : AJ\MA
Sample : P4413-09
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
KR-SS27


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 02:43:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 13:42:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

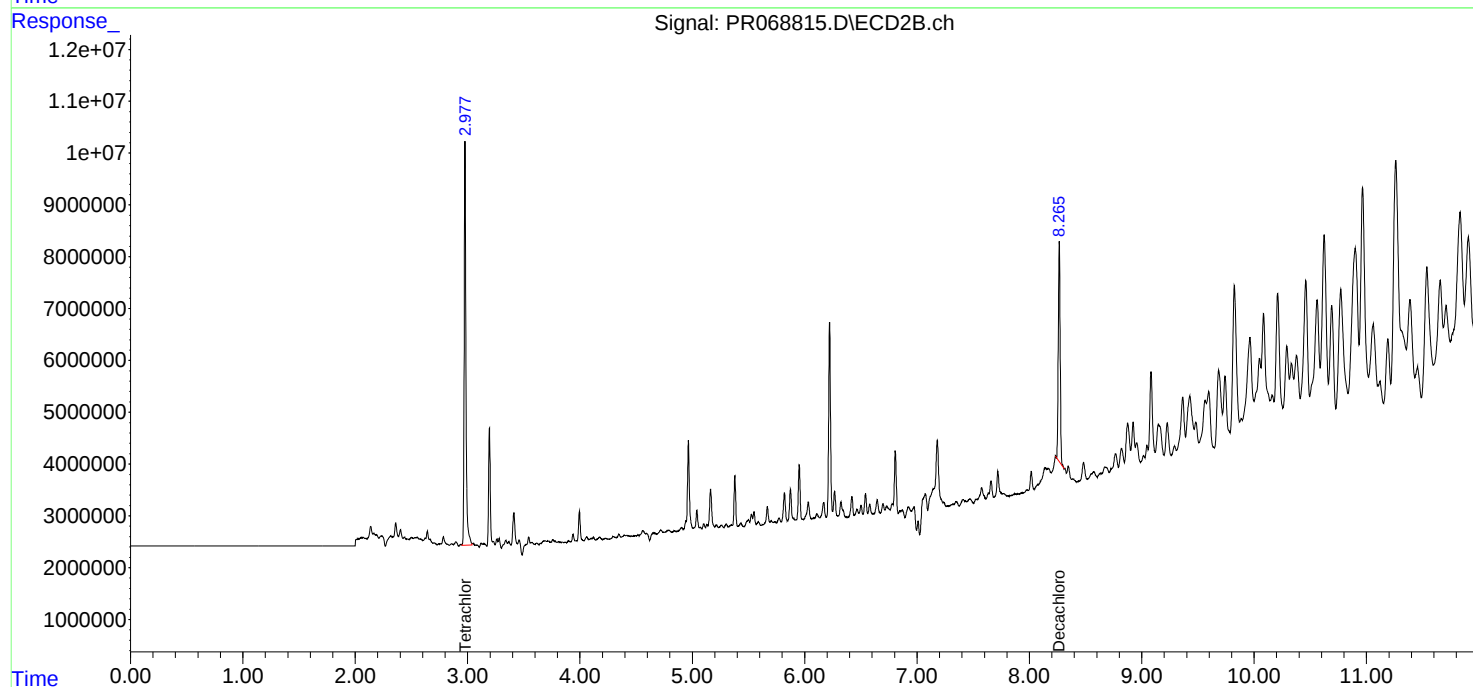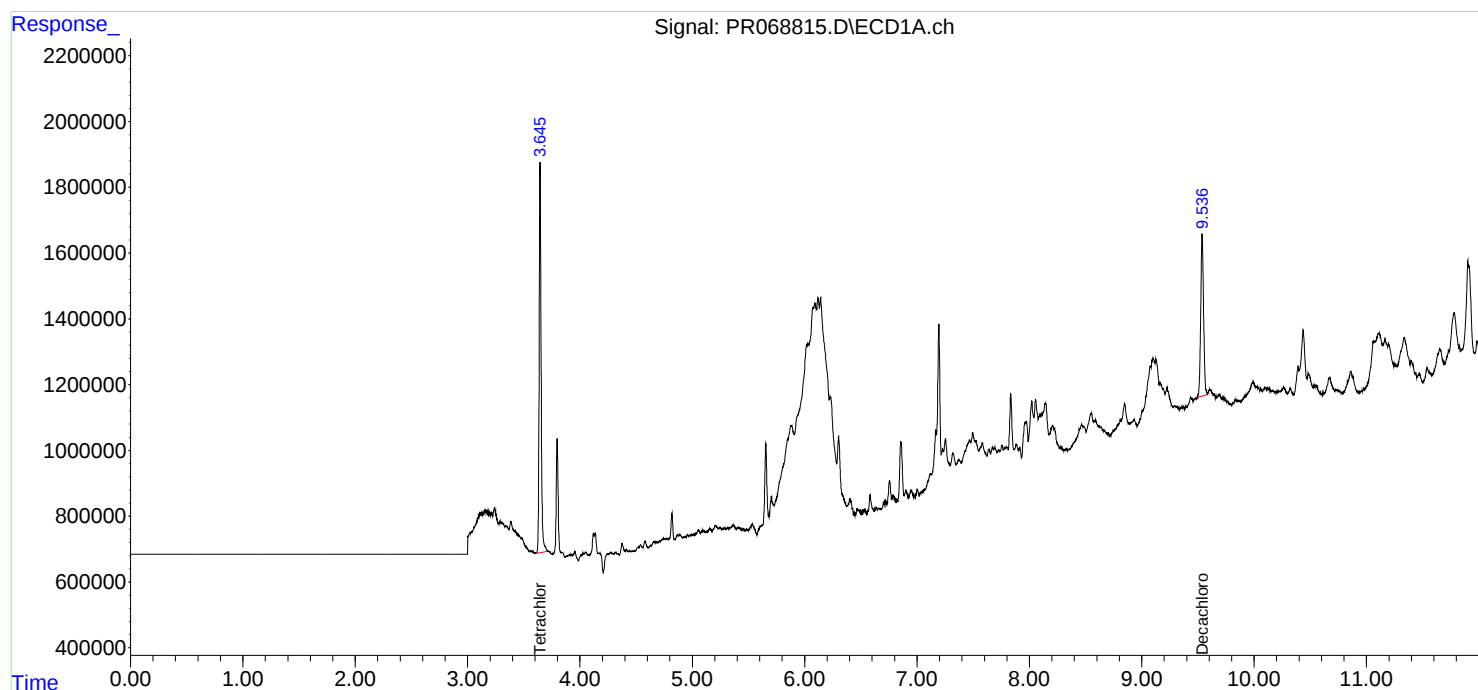

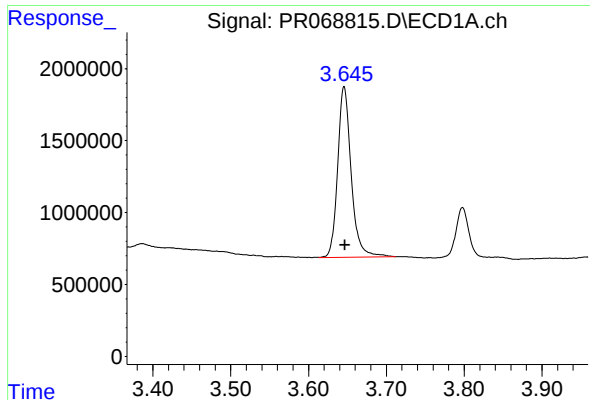


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.002 min
Response: 14410784
Conc: 15.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
KR-SS27


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :Ankita Jodhani 10/18/2024

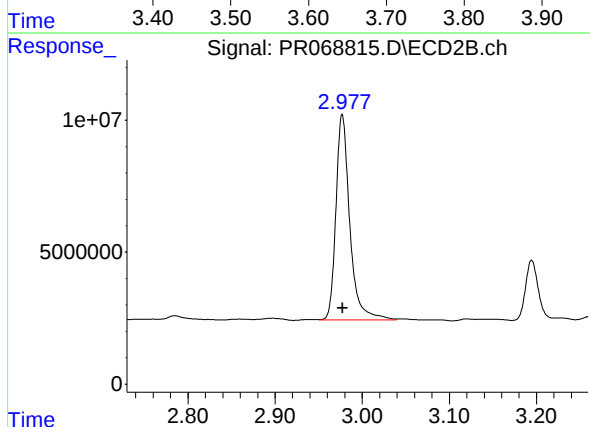


#1 Tetrachloro-m-xylene

R.T.: 2.977 min
Delta R.T.: -0.001 min
Response: 86210820
Conc: 15.50 ng/ml

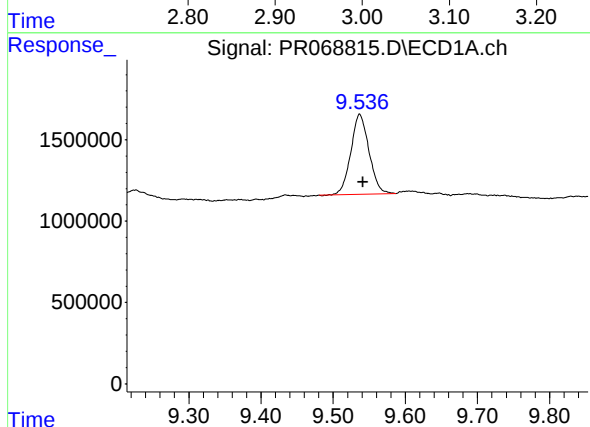

#2 Decachlorobiphenyl

R.T.: 9.537 min
Delta R.T.: -0.005 min
Response: 8576489
Conc: 14.86 ng/ml

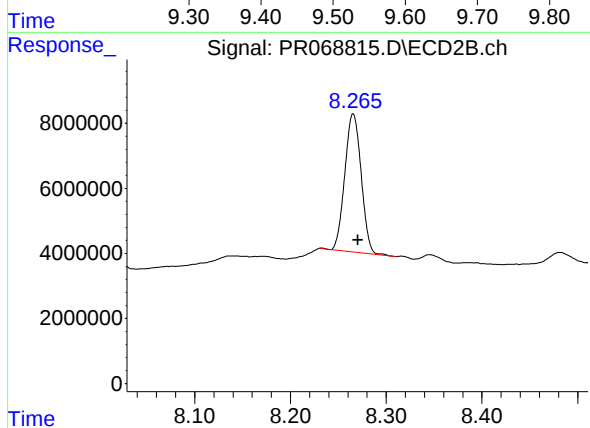

#2 Decachlorobiphenyl

R.T.: 8.265 min
Delta R.T.: -0.005 min
Response: 50636656
Conc: 11.87 ng/ml