

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101824\
 Data File : PR068821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 20:22
 Operator : AJ\MA
 Sample : P4413-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 KR-SS33

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/18/2024
 Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 02:02:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 13:42:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.646	2.977	13571995	79383814	14.475	14.268
2) SA Decachlor...	9.536	8.266	9717443	57953801	16.841	13.585m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR101824\
Data File : PR068821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 20:22
Operator : AJ\MA
Sample : P4413-15
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
KR-SS33


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 02:02:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101624.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 13:42:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

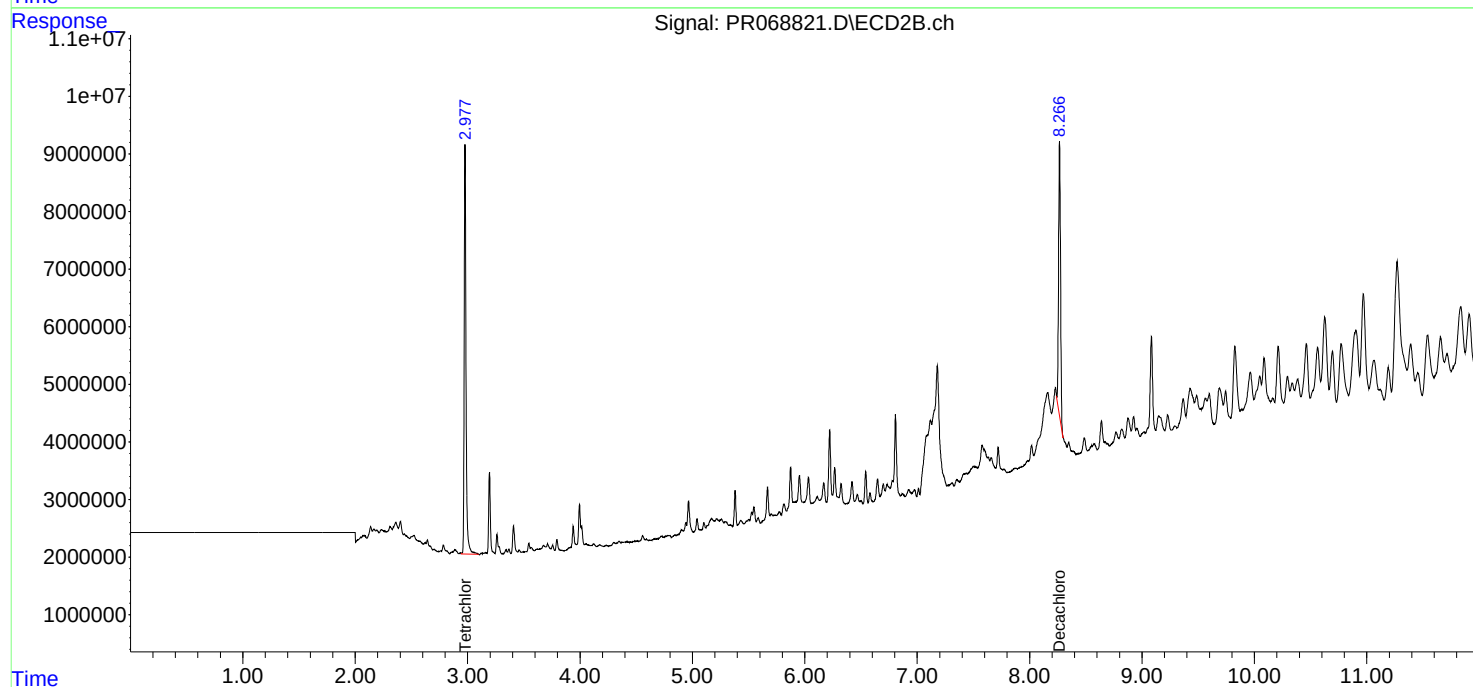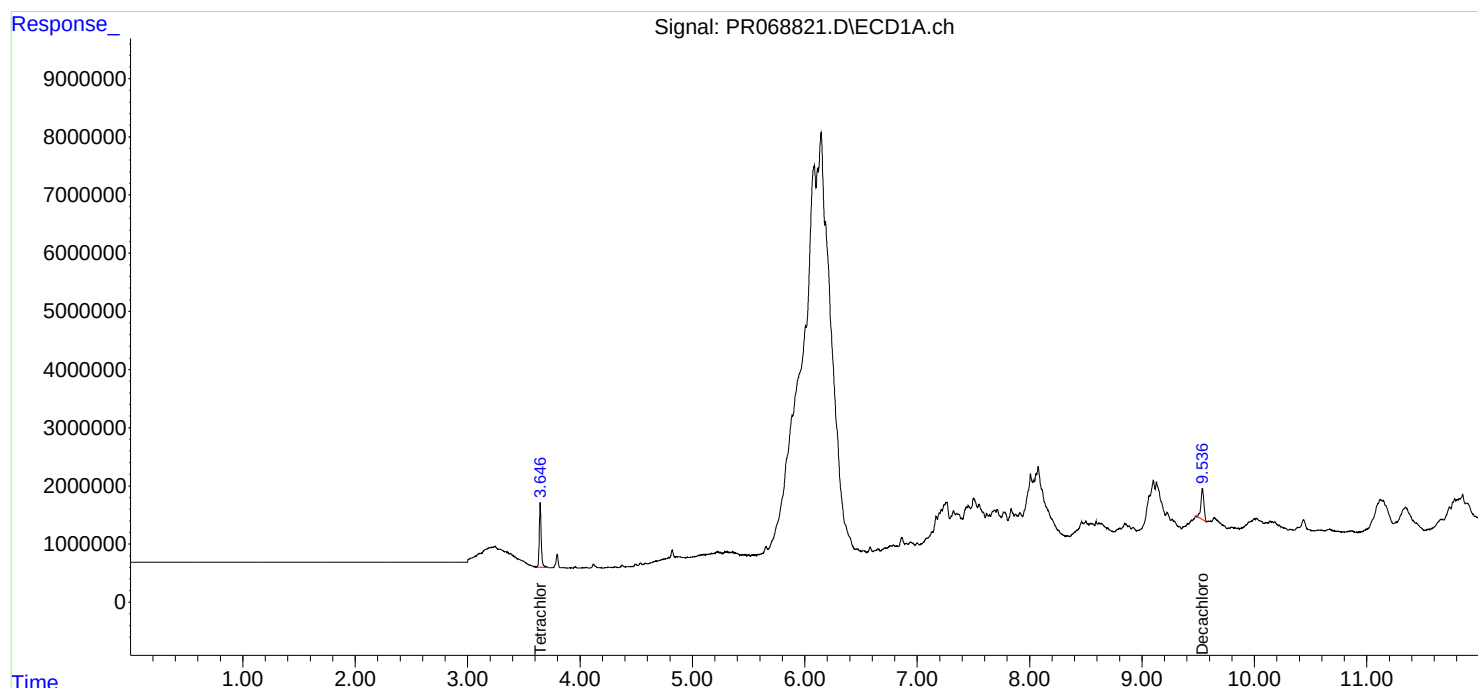

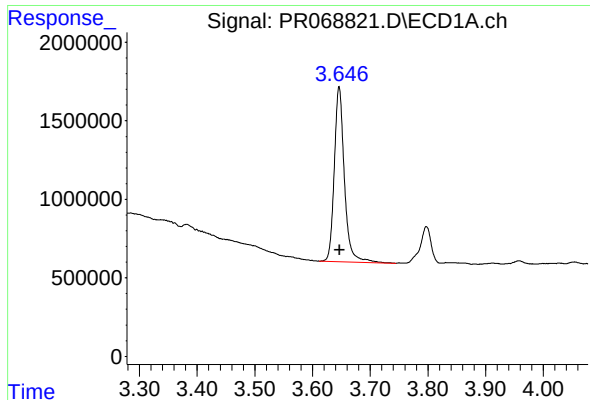


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 13571995
Conc: 14.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
KR-SS33


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :Ankita Jodhani 10/18/2024

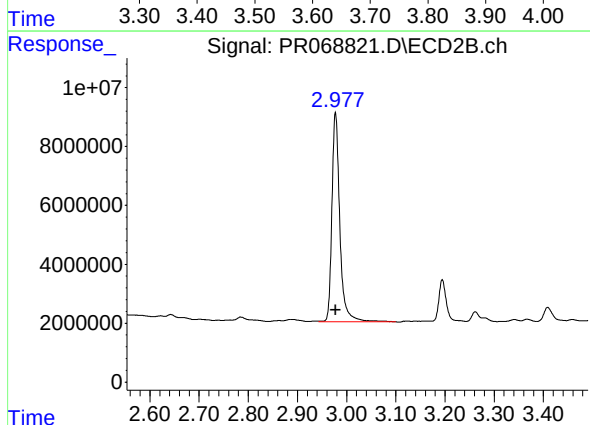


#1 Tetrachloro-m-xylene

R.T.: 2.977 min
Delta R.T.: 0.000 min
Response: 79383814
Conc: 14.27 ng/ml

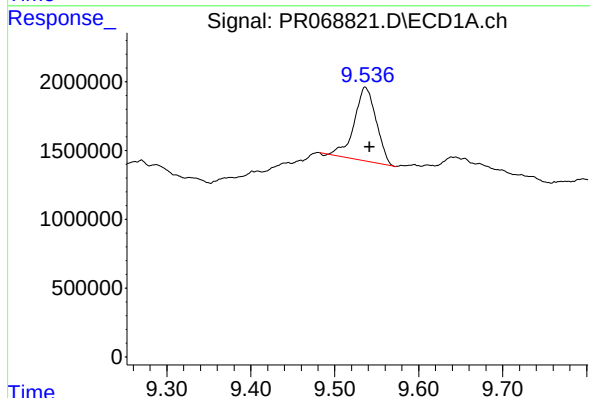

#2 Decachlorobiphenyl

R.T.: 9.536 min
Delta R.T.: -0.005 min
Response: 9717443
Conc: 16.84 ng/ml

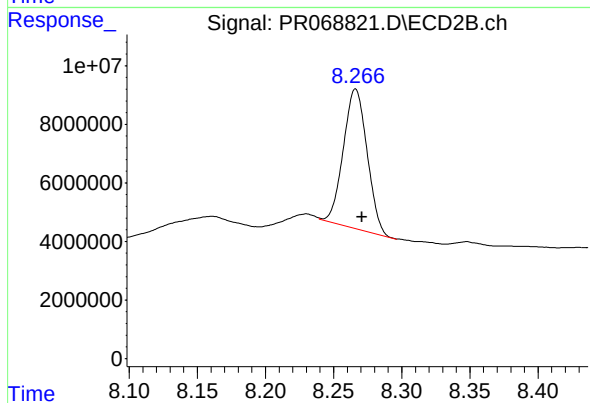

#2 Decachlorobiphenyl

R.T.: 8.266 min
Delta R.T.: -0.005 min
Response: 57953801
Conc: 13.59 ng/ml m