

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102220\
 Data File : PR047982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2020 02:49
 Operator : AJ\MA
 Sample : L4451-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1


Instrument :
 ECD_R
 ClientSampled :
 C0AG2

Manual Integrations
 APPROVED

mohammad
 10/26/2020 8:26:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 03:26:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102120CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 21 10:52:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

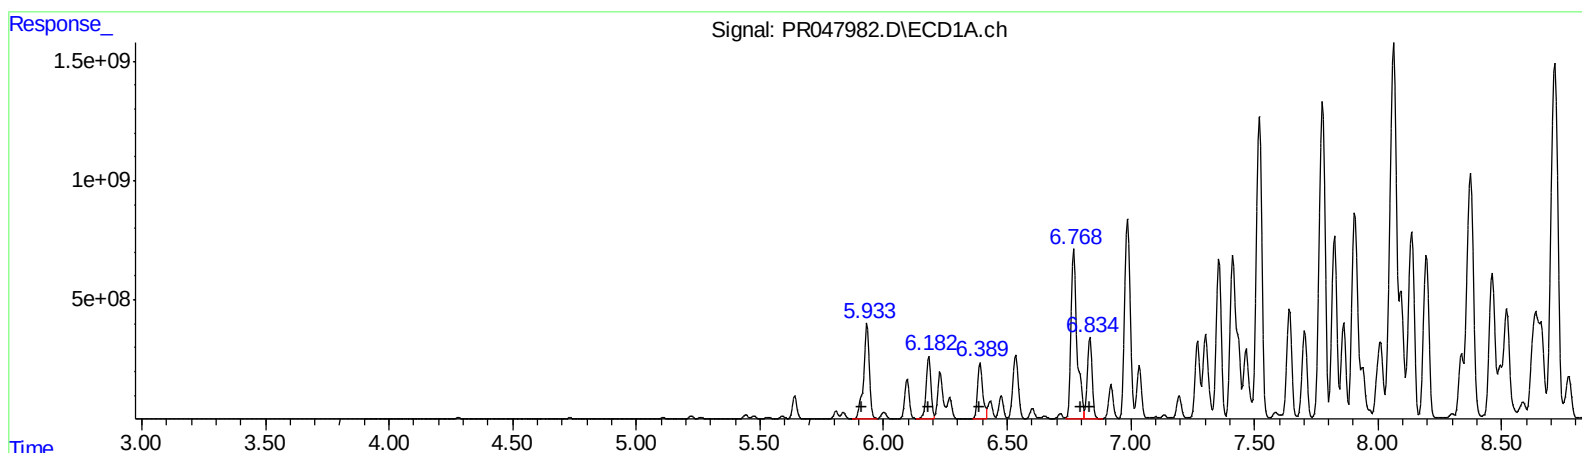

(21) AR-1248-1 (L5)
 R.T. Response Conc
 5.93 6385025377 136334.96
 6.18 3524575213 52631.99
 6.39 3377931280 45458.68
 6.77 12005147392 133243.04
 6.83 4571920400 52935.50

(21) AR-1248-1 #2 (L5)
 R.T. Response Conc
 4.99 7626811966 167114.20
 5.21 2747734975 47671.70
 5.25 2714096728 38214.86
 5.43 3952452487 40116.16
 5.82 6728676731 44652.50

QEdit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102220\
Data File : PR047982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2020 02:49
Operator : AJ\MA
Sample : L4451-08
Misc :
ALS Vial : 32 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampled :
C0AG2

Manual Integrations
APPROVED

mohammad
10/26/2020 8:26:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 03:26:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102120CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 21 10:52:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

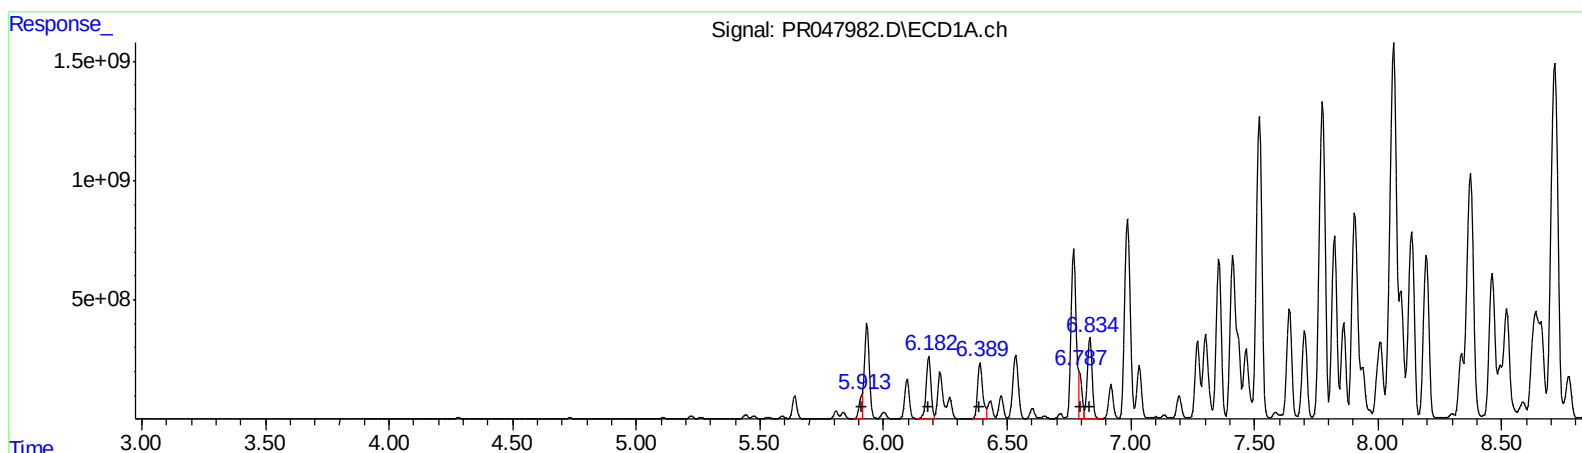

(21) AR-1248-1 #2 (L5)
R.T. Response Conc
5.91 830834627 17740.23
6.18 3524575213 52631.99
6.39 3377931280 45458.68
6.79 1908619945 21183.44
6.83 4571920400 52935.50

(21) AR-1248-1 #2 (L5)
R.T. Response Conc
4.98 853828063 18708.58
5.21 2747734975 47671.70
5.25 2714096728 38214.86
5.43 3952452487 40116.16
5.82 6728676731 44652.50

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102220\
 Data File : PR047982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2020 02:49
 Operator : AJ\MA
 Sample : L4451-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 C0AG2

Manual Integrations
 APPROVED

mohammad
 10/26/2020 8:26:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 03:26:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102120CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 21 10:52:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.730	3.883	44894134	59549125	24.853	22.051
2) SA Decachlor...	10.662	8.976	96129641	573.2E6	47.726	51.232
Target Compounds						
21) L5 AR-1248-1	5.913	4.979	830.8E6	853.8E6	17740.228m	18708.576m
22) L5 AR-1248-2	6.183	5.212	3524.6E6	2747.7E6	52631.990	47671.700
23) L5 AR-1248-3	6.390	5.254	3377.9E6	2714.1E6	45458.685	38214.860
24) L5 AR-1248-4	6.787	5.429	1908.6E6	3952.5E6	21183.440m	40116.163 #
25) L5 AR-1248-5	6.834	5.824	4571.9E6	6728.7E6	52935.497	44652.496
31) L7 AR-1260-1	7.520	6.473	20047.0E6	36905.2E6	195391.321	208176.445
32) L7 AR-1260-2	7.775	6.676	22324.9E6	57042.4E6	175953.241	94751.747 #
33) L7 AR-1260-3	8.136	6.823	13101.2E6	47995.5E6	135319.853	129751.737
34) L7 AR-1260-4	8.374	7.298	19589.5E6	46712.3E6	179030.782	103195.086 #
35) L7 AR-1260-5	8.714	7.550	29373.7E6	98939.6E6	129258.058	52516.380 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 10/26/20