

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102423\
 Data File : PR064225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 15:53
 Operator : AJ\MA
 Sample : 04987-14
 Misc :
 ALS Vial : 51 Sample Multiplier: 1


Instrument :
 ECD_R
 ClientSampleId :
 PCB-GCP2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:38:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 13 05:04:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Reviewed By :Yogesh Patel 10/25/2023
 Supervised By :Ankita Jodhani 10/25/2023

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

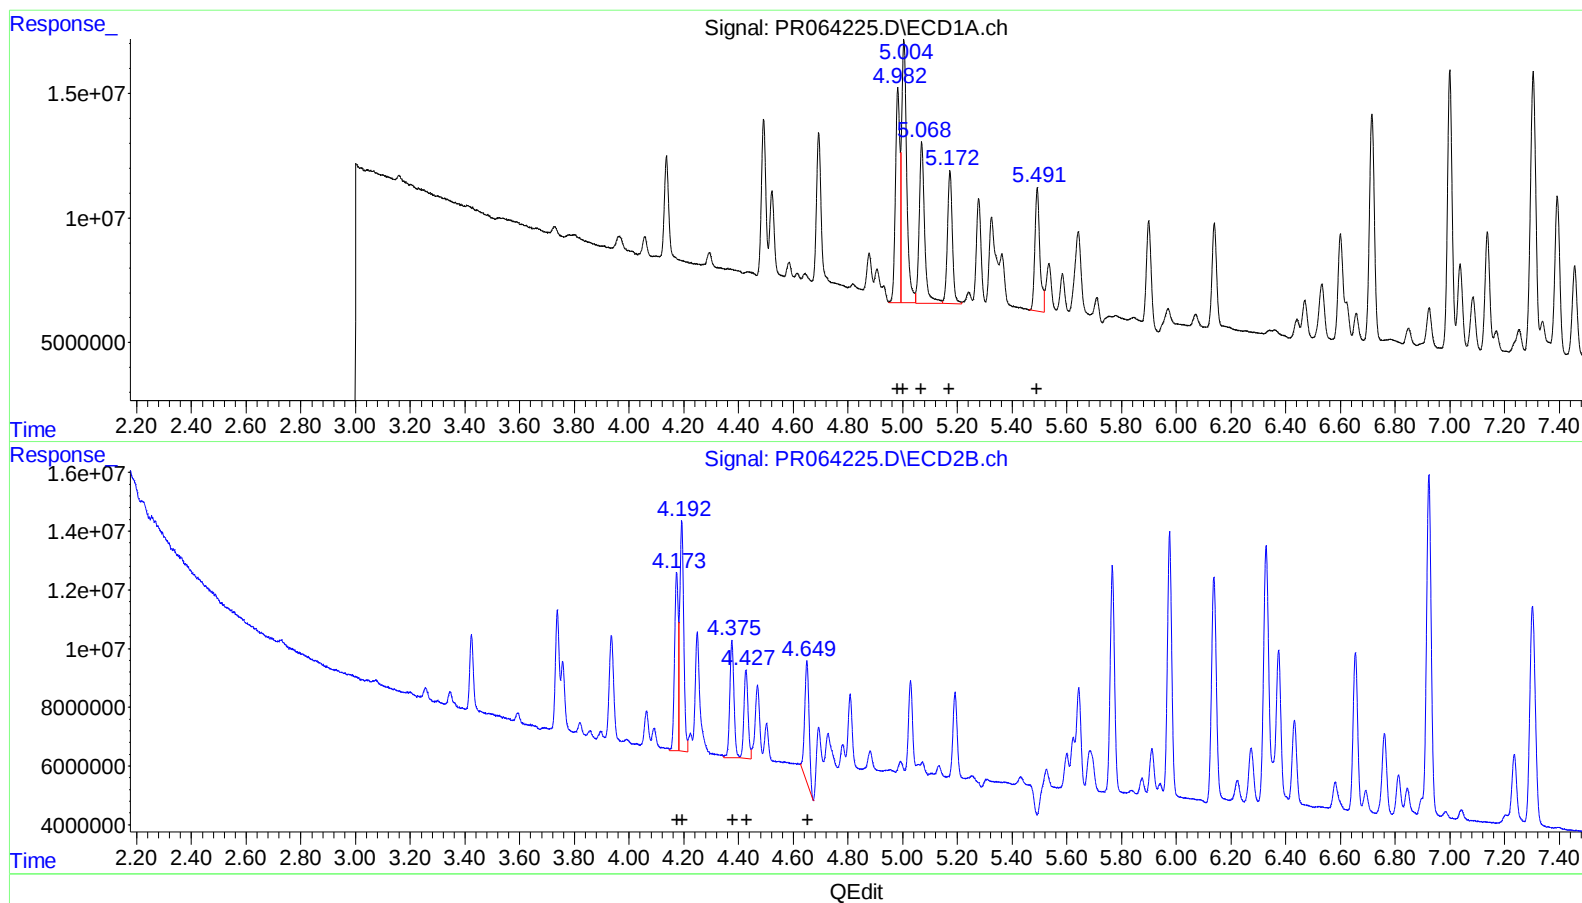

(3) AR-1016-1 (L1)
 R.T. Response Conc
 4.98 94240224 438.10
 5.00 139129267 424.61
 5.07 88085156 425.80
 5.17 66163117 406.20
 5.49 62746051 386.00

(3) AR-1016-1 #2 (L1)
 R.T. Response Conc
 4.17 56496487 388.64
 4.19 79306529 396.72
 4.38 41249897 374.18
 4.43 31913397 368.78
 4.65 46496605 406.98

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102423\
Data File : PR064225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 15:53
Operator : AJ\MA
Sample : 04987-14
Misc :
ALS Vial : 51 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
PCB-GCP2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:38:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

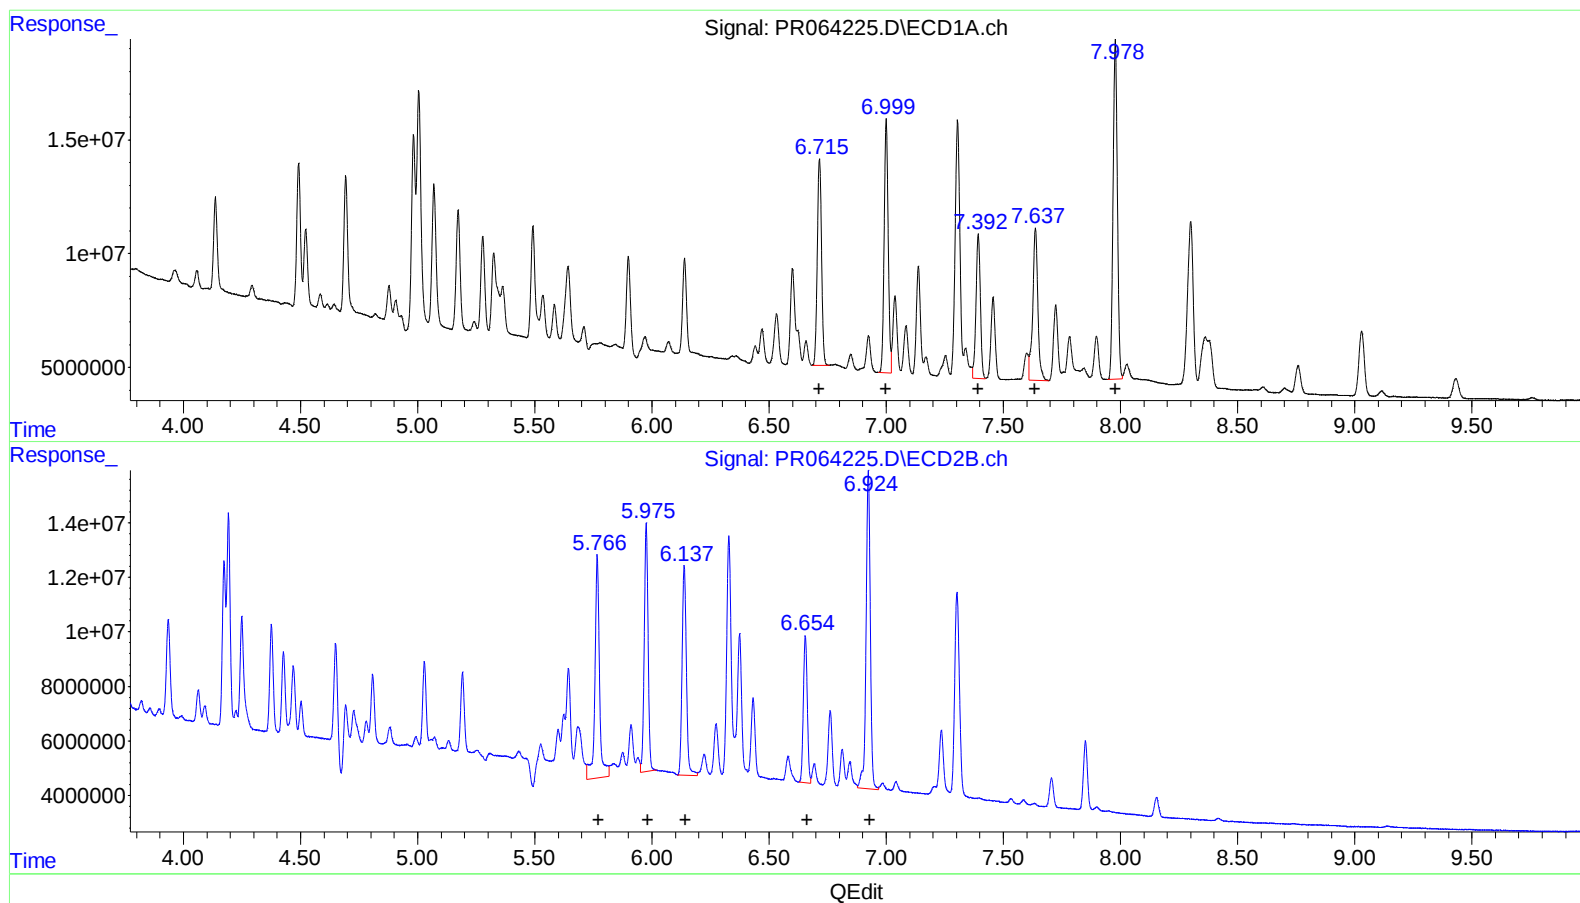

(31) AR-1260-1 (L7)
R.T. Response Conc
6.72 114286855 384.54
7.00 133089906 384.85
7.39 81689780 317.95
7.64 101269133 358.32
7.98 190833164 353.47

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
5.77 112386878 500.54
5.98 103148021 391.15
6.14 98424212 389.23
6.65 63310557 320.92
6.92 147727619 347.89

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102423\
Data File : PR064225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 15:53
Operator : AJ\MA
Sample : 04987-14
Misc :
ALS Vial : 51 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
PCB-GCP2-BLANK-SPIKE

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:38:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

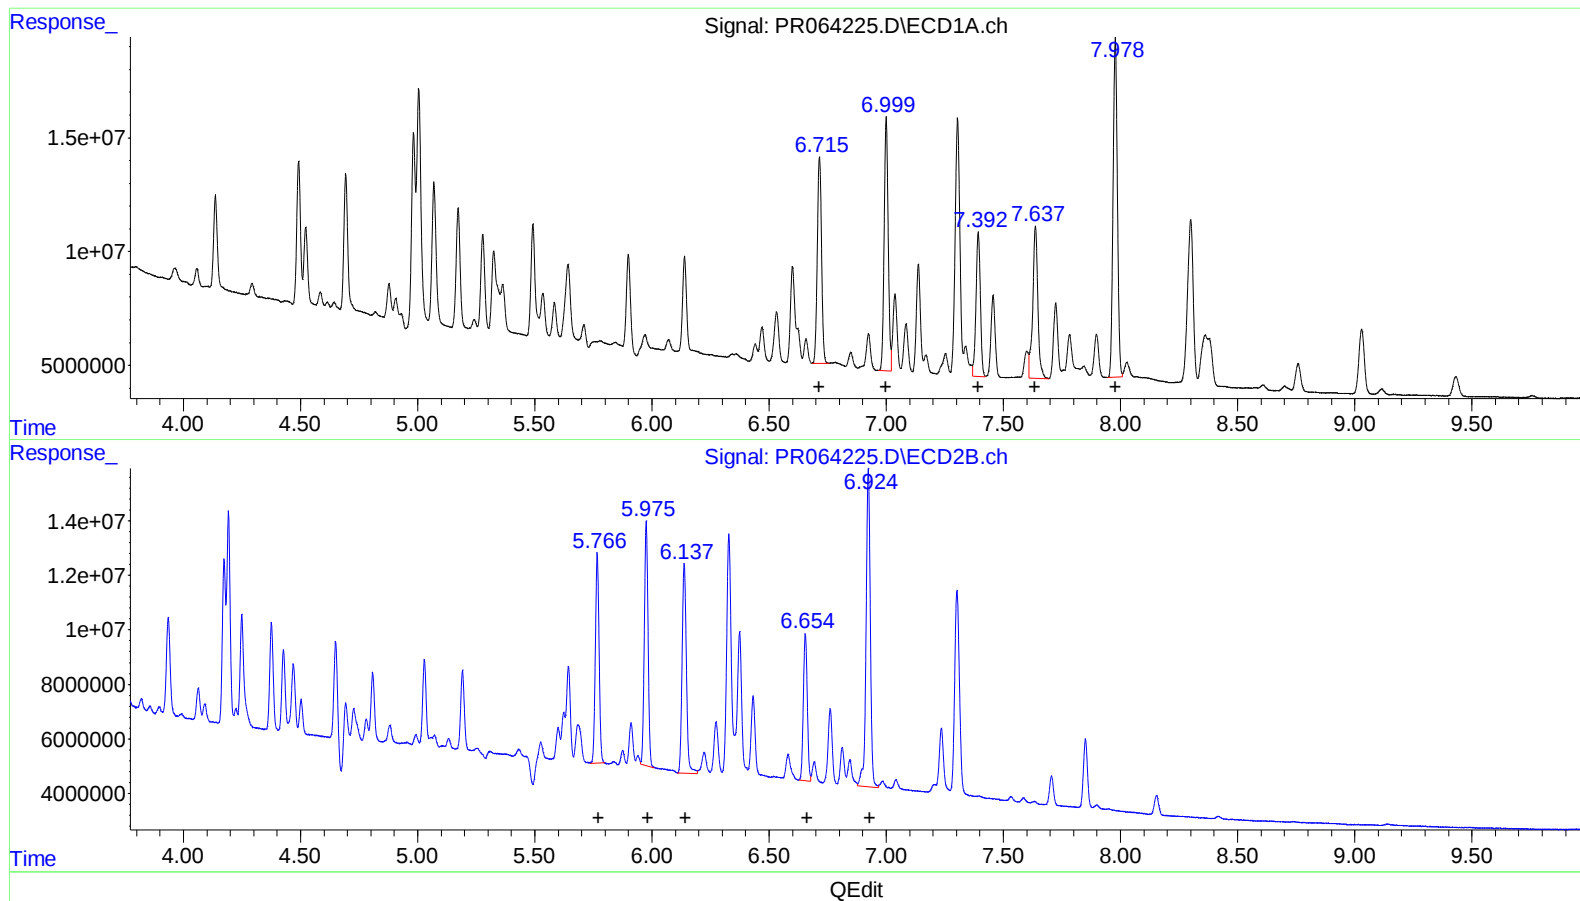

(31) AR-1260-1 (L7)
R.T. Response Conc
6.72 114286855 384.54
7.00 133089906 384.85
7.39 81689780 317.95
7.64 101269133 358.32
7.98 190833164 353.47

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
5.77 84989612 378.52
5.98 99010180 375.45
6.14 98424212 389.23
6.65 63310557 320.92
6.92 147727619 347.89